

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029467.D
 Acq On : 14 Jun 2022 16:07
 Operator : JC/MD
 Sample : N3254-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029467.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	53	rVB	133746	132334	11.02%	1.467%
2	1.666	91	95	103	rVB	109148	129324	10.77%	1.434%
3	2.306	194	200	212	rBV	217764	350702	29.20%	3.888%
4	2.501	228	232	237	rBV3	596	1236	0.10%	0.014%
5	2.629	251	253	255	rBV2	301	304	0.03%	0.003%
6	2.708	262	266	269	rBV2	657	928	0.08%	0.010%
7	2.794	275	280	285	rVB3	3002	5318	0.44%	0.059%
8	2.946	295	305	319	rBV	49253	113028	9.41%	1.253%
9	3.056	321	323	327	rVB2	532	415	0.03%	0.005%
10	3.135	335	336	340	rBV3	274	281	0.02%	0.003%
11	3.410	379	381	384	rBV2	217	260	0.02%	0.003%
12	3.538	401	402	407	rVB2	277	325	0.03%	0.004%
13	3.580	407	409	410	rBV	270	226	0.02%	0.003%
14	3.592	410	411	414	rVV2	396	287	0.02%	0.003%
15	3.635	416	418	420	rBV2	246	233	0.02%	0.003%
16	3.678	423	425	430	rVB3	257	344	0.03%	0.004%
17	3.714	430	431	435	rBV3	248	333	0.03%	0.004%
18	3.848	451	453	456	rVB3	359	439	0.04%	0.005%
19	3.928	463	466	470	rVB2	221	341	0.03%	0.004%
20	4.208	509	512	513	rVB2	229	227	0.02%	0.003%
21	4.312	527	529	534	rBV2	290	477	0.04%	0.005%
22	4.354	534	536	538	rBV2	434	343	0.03%	0.004%
23	4.464	543	554	566	rBV	116324	329679	27.45%	3.655%
24	4.928	629	630	634	rVB3	411	390	0.03%	0.004%
25	4.982	637	639	641	rBV	499	629	0.05%	0.007%
26	5.062	641	652	670	rVV	152618	471206	39.23%	5.224%
27	5.269	683	686	688	rBV2	378	474	0.04%	0.005%
28	5.397	699	707	713	rBV5	1629	4482	0.37%	0.050%
29	5.555	726	733	746	rBV6	2915	8398	0.70%	0.093%
30	5.659	746	750	752	rBV2	254	271	0.02%	0.003%
31	5.824	773	777	778	rVB3	375	397	0.03%	0.004%
32	5.976	789	802	817	rBV2	402770	1201163	100.00%	13.316%
33	6.190	834	837	840	rVB2	405	469	0.04%	0.005%
34	6.275	849	851	852	rBV	398	298	0.02%	0.003%
35	6.354	862	864	866	rBV	318	374	0.03%	0.004%
36	6.476	881	884	886	rBV3	280	365	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029467.D
 Acq On : 14 Jun 2022 16:07
 Operator : JC/MD
 Sample : N3254-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	6.763	922	931	947	rBV	271294	641051	53.37%	7.107%
38	6.945	960	961	966	rBV	299	276	0.02%	0.003%
39	7.128	983	991	1002	rVB5	20637	48649	4.05%	0.539%
40	7.311	1012	1021	1034	rBV	247701	535738	44.60%	5.939%
41	7.482	1046	1049	1053	rVV3	705	1133	0.09%	0.013%
42	7.543	1055	1059	1064	rBV3	263	534	0.04%	0.006%
43	7.622	1070	1072	1077	rVB	287	412	0.03%	0.005%
44	7.701	1082	1085	1088	rBV3	347	481	0.04%	0.005%
45	7.762	1094	1095	1098	rBV2	346	290	0.02%	0.003%
46	7.811	1100	1103	1104	rBV3	341	315	0.03%	0.003%
47	7.915	1117	1120	1121	rBV2	289	290	0.02%	0.003%
48	7.939	1123	1124	1128	rVV4	545	718	0.06%	0.008%
49	8.165	1159	1161	1163	rBV	348	351	0.03%	0.004%
50	8.244	1171	1174	1175	rBV2	274	247	0.02%	0.003%
51	8.262	1175	1177	1179	rVB2	335	248	0.02%	0.003%
52	8.329	1181	1188	1202	rBV	158111	263545	21.94%	2.922%
53	8.494	1211	1215	1218	rVB2	490	636	0.05%	0.007%
54	8.579	1225	1229	1233	rBV5	2120	3237	0.27%	0.036%
55	8.652	1233	1241	1249	rVV	595609	922293	76.78%	10.225%
56	8.726	1249	1253	1259	rVB	7955	13033	1.09%	0.144%
57	8.951	1283	1290	1302	rBV	114727	168483	14.03%	1.868%
58	9.274	1340	1343	1347	rVB5	2502	3437	0.29%	0.038%
59	9.390	1356	1362	1378	rBV	491335	729831	60.76%	8.091%
60	9.701	1408	1413	1417	rBV2	10281	13417	1.12%	0.149%
61	9.780	1424	1426	1430	rVB3	282	312	0.03%	0.003%
62	10.055	1466	1471	1478	rBV	554729	748278	62.30%	8.296%
63	10.305	1509	1512	1516	rBV2	1379	1952	0.16%	0.022%
64	10.384	1522	1525	1526	rBV	444	351	0.03%	0.004%
65	10.524	1546	1548	1550	rBV	172	223	0.02%	0.002%
66	10.756	1584	1586	1590	rVB2	397	443	0.04%	0.005%
67	10.817	1594	1596	1599	rVB2	266	234	0.02%	0.003%
68	10.914	1611	1612	1614	rBV	403	283	0.02%	0.003%
69	11.006	1626	1627	1629	rBV2	377	282	0.02%	0.003%
70	11.122	1642	1646	1652	rVB2	4408	5839	0.49%	0.065%
71	11.195	1652	1658	1666	rBV	508486	646115	53.79%	7.163%
72	11.384	1686	1689	1692	rBV2	679	513	0.04%	0.006%
73	11.481	1697	1705	1707	rBV4	1806	3097	0.26%	0.034%
74	11.615	1723	1727	1728	rBV2	662	747	0.06%	0.008%
75	11.719	1740	1744	1746	rBV3	684	1054	0.09%	0.012%
76	11.749	1746	1749	1755	rVB3	4317	5342	0.44%	0.059%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029467.D
 Acq On : 14 Jun 2022 16:07
 Operator : JC/MD
 Sample : N3254-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	11.932	1774	1779	1783	rBV4	1814	2533	0.21%	0.028%
78	12.024	1789	1794	1804	rBV	579370	707281	58.88%	7.841%
79	12.152	1813	1815	1823	rVB3	3709	3708	0.31%	0.041%
80	12.323	1836	1843	1849	rBV	623212	775530	64.56%	8.598%
81	12.487	1865	1870	1872	rVB3	881	1445	0.12%	0.016%
82	12.591	1885	1887	1889	rVB	398	232	0.02%	0.003%
83	12.627	1892	1893	1895	rVV2	550	404	0.03%	0.004%
84	12.664	1897	1899	1902	rVV	902	872	0.07%	0.010%
85	12.768	1912	1916	1919	rBV3	586	736	0.06%	0.008%
86	12.950	1944	1946	1948	rBV2	232	271	0.02%	0.003%
87	13.011	1954	1956	1959	rVB2	332	272	0.02%	0.003%
88	13.054	1959	1963	1964	rBV2	651	651	0.05%	0.007%
89	13.310	2004	2005	2007	rBV	358	270	0.02%	0.003%
90	13.511	2036	2038	2041	rBV	265	370	0.03%	0.004%
91	14.030	2121	2123	2124	rBV	364	305	0.03%	0.003%
92	14.048	2124	2126	2127	rVB	503	328	0.03%	0.004%
93	14.133	2134	2140	2143	rBV2	1463	2673	0.22%	0.030%
94	14.603	2216	2217	2218	rBV	516	237	0.02%	0.003%
95	14.749	2240	2241	2243	rBV2	410	366	0.03%	0.004%
96	14.786	2245	2247	2249	rVV2	418	312	0.03%	0.003%
97	14.859	2258	2259	2261	rBV	538	370	0.03%	0.004%
98	14.920	2267	2269	2271	rBV2	513	479	0.04%	0.005%
99	16.212	2479	2481	2482	rBV	463	324	0.03%	0.004%
100	16.450	2518	2520	2522	rBV2	478	306	0.03%	0.003%




Sum of corrected areas: 9020285

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029467.D
Acq On : 14 Jun 2022 16:07
Operator : JC/MD
Sample : N3254-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

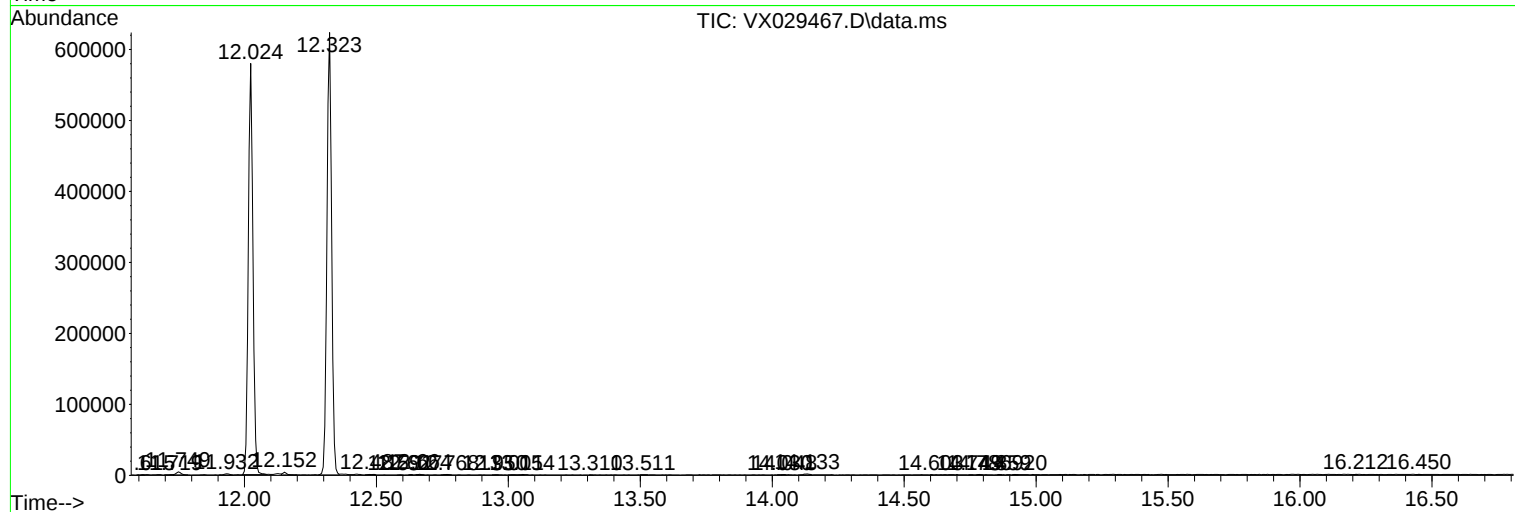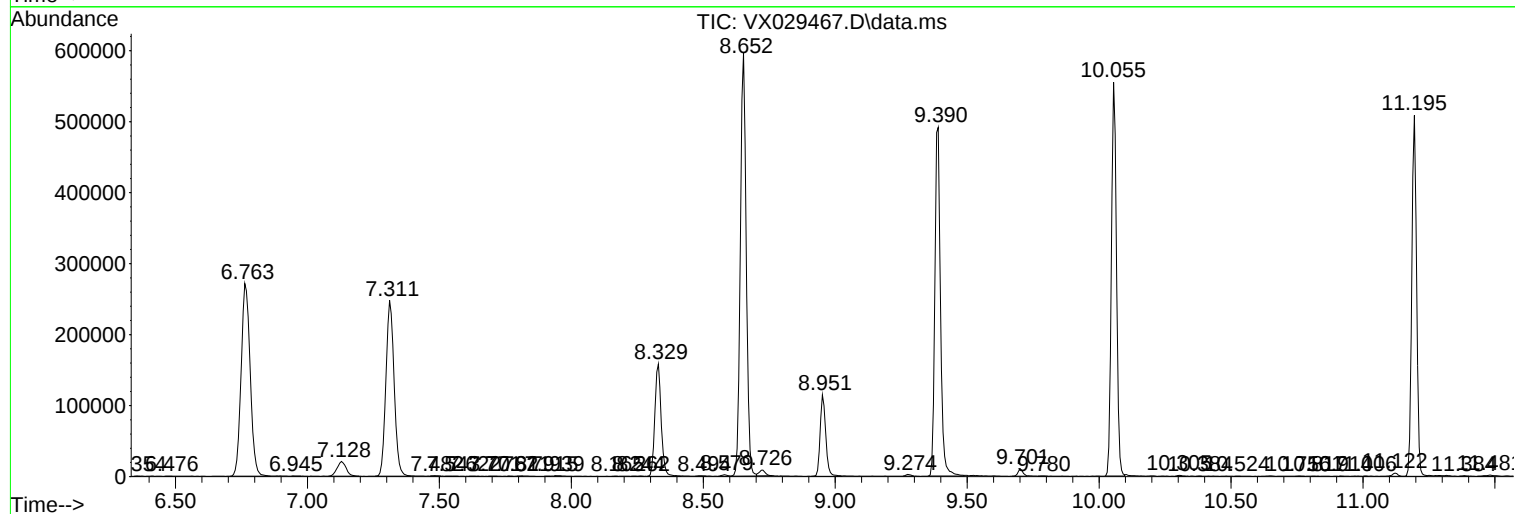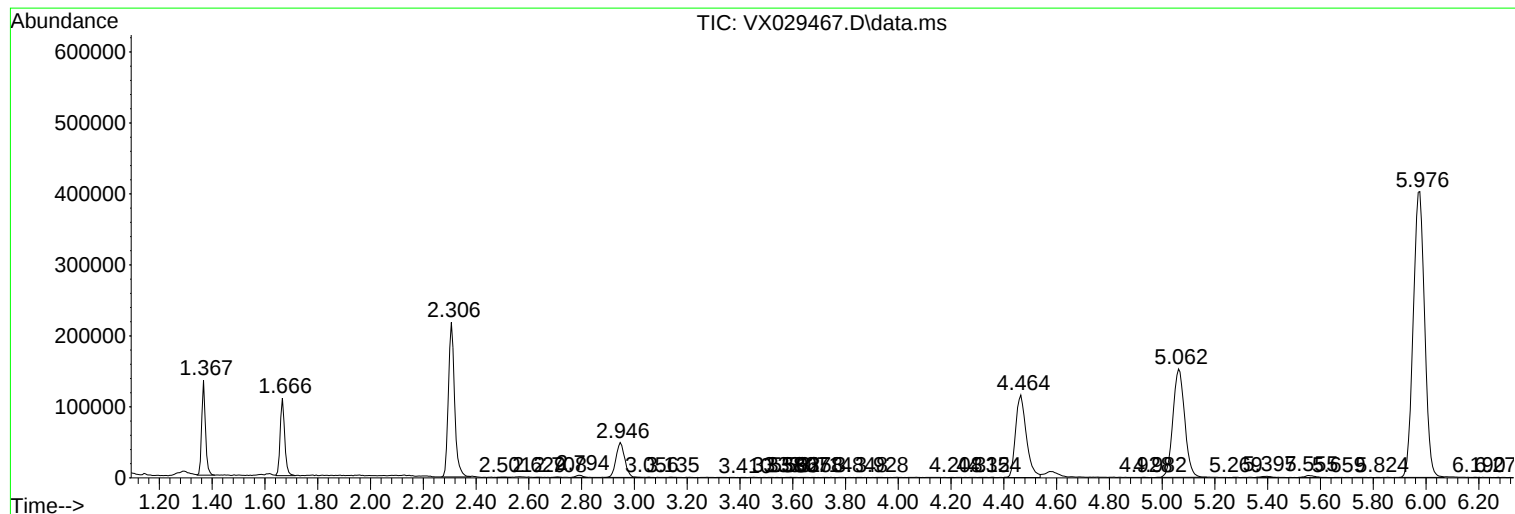

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029467.D
Acq On : 14 Jun 2022 16:07
Operator : JC/MD
Sample : N3254-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029467.D
Acq On : 14 Jun 2022 16:07
Operator : JC/MD
Sample : N3254-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------