

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029468.D
 Acq On : 14 Jun 2022 16:30
 Operator : JC/MD
 Sample : N3249-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M

Title : VOC Analysis

Signal : TIC: VX029468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.295	27	34	42	rBV4	6969	19074	1.39%	0.180%
2	1.368	42	46	57	rVB	186742	193283	14.13%	1.822%
3	1.666	90	95	103	rVB	137593	163262	11.93%	1.539%
4	2.307	194	200	210	rBV	306964	481753	35.22%	4.541%
5	2.386	210	213	220	rVB	3846	5867	0.43%	0.055%
6	2.483	226	229	230	rBV2	400	380	0.03%	0.004%
7	2.703	261	265	271	rBV3	905	1563	0.11%	0.015%
8	2.941	299	304	308	rBV3	748	1457	0.11%	0.014%
9	3.020	315	317	319	rBV	253	270	0.02%	0.003%
10	3.099	324	330	335	rVV4	2343	4914	0.36%	0.046%
11	3.319	364	366	372	rBV3	510	662	0.05%	0.006%
12	3.611	406	414	425	rVV	40076	93119	6.81%	0.878%
13	3.727	429	433	437	rBV2	173	275	0.02%	0.003%
14	3.879	454	458	459	rBV3	207	293	0.02%	0.003%
15	4.001	474	478	480	rVB	239	305	0.02%	0.003%
16	4.026	480	482	484	rBV2	345	378	0.03%	0.004%
17	4.257	518	520	526	rBV2	202	355	0.03%	0.003%
18	4.367	534	538	540	rVB2	348	427	0.03%	0.004%
19	4.465	540	554	571	rBV2	117868	433429	31.68%	4.086%
20	4.709	593	594	596	rBV2	269	265	0.02%	0.002%
21	5.062	639	652	669	rBV	174080	537071	39.26%	5.063%
22	5.233	678	680	684	rBV2	381	515	0.04%	0.005%
23	5.282	684	688	690	rBV2	313	492	0.04%	0.005%
24	5.397	700	707	711	rBV6	1981	4305	0.31%	0.041%
25	5.519	725	727	728	rBV	391	237	0.02%	0.002%
26	5.556	728	733	739	rVV3	1783	3786	0.28%	0.036%
27	5.897	788	789	790	rBV	429	275	0.02%	0.003%
28	5.977	790	802	818	rVV2	462800	1367935	100.00%	12.895%
29	6.147	829	830	832	rBV	330	338	0.02%	0.003%
30	6.324	857	859	861	rBV2	387	365	0.03%	0.003%
31	6.397	869	871	874	rVB2	315	267	0.02%	0.003%
32	6.458	878	881	882	rBV	349	396	0.03%	0.004%
33	6.513	887	890	892	rVB	309	261	0.02%	0.002%
34	6.763	921	931	949	rBV	337421	801918	58.62%	7.559%
35	6.952	960	962	965	rVB	460	424	0.03%	0.004%
36	6.976	965	966	969	rBV2	463	501	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029468.D
 Acq On : 14 Jun 2022 16:30
 Operator : JC/MD
 Sample : N3249-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.068	979	981	983	rVV2	378	402	0.03%	0.004%
38	7.129	983	991	1004	rVV4	25288	58630	4.29%	0.553%
39	7.312	1012	1021	1037	rVV	278064	597372	43.67%	5.631%
40	7.629	1072	1073	1076	rBV2	253	296	0.02%	0.003%
41	7.690	1078	1083	1087	rVV2	1092	1969	0.14%	0.019%
42	7.818	1100	1104	1107	rBV3	554	815	0.06%	0.008%
43	7.891	1114	1116	1117	rVB	493	269	0.02%	0.003%
44	7.909	1117	1119	1120	rBV	319	294	0.02%	0.003%
45	7.928	1120	1122	1123	rBV	333	235	0.02%	0.002%
46	8.220	1168	1170	1175	rVB2	294	348	0.03%	0.003%
47	8.269	1175	1178	1180	rBV2	308	430	0.03%	0.004%
48	8.330	1181	1188	1199	rBV	178374	290207	21.21%	2.736%
49	8.482	1211	1213	1215	rBV2	364	317	0.02%	0.003%
50	8.653	1234	1241	1248	rBV	723094	1147659	83.90%	10.819%
51	8.720	1249	1252	1263	rVV	10314	18777	1.37%	0.177%
52	8.952	1285	1290	1304	rVB	124030	182021	13.31%	1.716%
53	9.141	1320	1321	1323	rBV	432	288	0.02%	0.003%
54	9.275	1339	1343	1347	rVV3	3285	4745	0.35%	0.045%
55	9.336	1352	1353	1356	rBV2	293	254	0.02%	0.002%
56	9.385	1356	1361	1381	rBV	461909	694094	50.74%	6.543%
57	9.805	1428	1430	1432	rBV	273	242	0.02%	0.002%
58	9.866	1436	1440	1442	rVB3	359	499	0.04%	0.005%
59	10.055	1465	1471	1485	rBV	700598	934399	68.31%	8.808%
60	10.208	1492	1496	1499	rVB4	869	1231	0.09%	0.012%
61	10.305	1508	1512	1519	rVB4	1578	2414	0.18%	0.023%
62	10.579	1556	1557	1560	rBV3	345	294	0.02%	0.003%
63	10.647	1565	1568	1569	rBV2	634	569	0.04%	0.005%
64	10.964	1618	1620	1623	rBV3	471	569	0.04%	0.005%
65	11.122	1642	1646	1650	rVB2	5812	7564	0.55%	0.071%
66	11.195	1652	1658	1666	rBV	508304	652510	47.70%	6.151%
67	11.378	1686	1688	1691	rBV2	510	406	0.03%	0.004%
68	11.476	1698	1704	1712	rVB7	2188	5340	0.39%	0.050%
69	11.549	1712	1716	1722	rBV5	685	1182	0.09%	0.011%
70	11.628	1725	1729	1734	rVV5	693	1346	0.10%	0.013%
71	11.683	1736	1738	1741	rVV2	802	995	0.07%	0.009%
72	11.713	1741	1743	1745	rVV	966	890	0.07%	0.008%
73	11.750	1745	1749	1754	rVB3	5314	7183	0.53%	0.068%
74	11.841	1760	1764	1769	rBV3	1442	1798	0.13%	0.017%
75	11.939	1775	1780	1783	rVV2	2506	3252	0.24%	0.031%
76	12.024	1789	1794	1804	rBV	752758	909723	66.50%	8.576%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029468.D
 Acq On : 14 Jun 2022 16:30
 Operator : JC/MD
 Sample : N3249-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.226	1826	1827	1828	rBV	655	383	0.03%	0.004%
78	12.268	1831	1834	1835	rBV	560	618	0.05%	0.006%
79	12.323	1836	1843	1852	rVV	743406	943149	68.95%	8.891%
80	12.427	1857	1860	1863	rVB3	2007	2500	0.18%	0.024%
81	12.585	1881	1886	1887	rVB2	289	334	0.02%	0.003%
82	12.658	1896	1898	1902	rBV3	870	1234	0.09%	0.012%
83	12.768	1912	1916	1918	rVB2	606	709	0.05%	0.007%
84	12.817	1922	1924	1925	rBV	230	237	0.02%	0.002%
85	12.853	1929	1930	1935	rBV3	340	539	0.04%	0.005%
86	12.988	1949	1952	1954	rBV	409	337	0.02%	0.003%
87	13.055	1961	1963	1969	rVB3	1188	1390	0.10%	0.013%
88	13.195	1984	1986	1988	rVB	436	319	0.02%	0.003%
89	13.384	2013	2017	2019	rBV	211	239	0.02%	0.002%
90	13.591	2049	2051	2053	rBV2	378	335	0.02%	0.003%
91	13.786	2079	2083	2084	rBV3	477	614	0.04%	0.006%
92	13.969	2112	2113	2116	rBV2	345	350	0.03%	0.003%
93	14.018	2120	2121	2123	rBV	379	243	0.02%	0.002%
94	14.067	2127	2129	2133	rBV2	310	380	0.03%	0.004%
95	14.231	2154	2156	2157	rBV2	347	336	0.02%	0.003%
96	14.347	2174	2175	2177	rVB	477	267	0.02%	0.003%
97	14.371	2177	2179	2181	rBV2	342	331	0.02%	0.003%
98	14.536	2204	2206	2209	rBV2	456	434	0.03%	0.004%
99	14.585	2212	2214	2215	rVV	464	259	0.02%	0.002%
100	14.628	2219	2221	2225	rBV	446	446	0.03%	0.004%

Sum of corrected areas: 10608228




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029468.D
Acq On : 14 Jun 2022 16:30
Operator : JC/MD
Sample : N3249-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

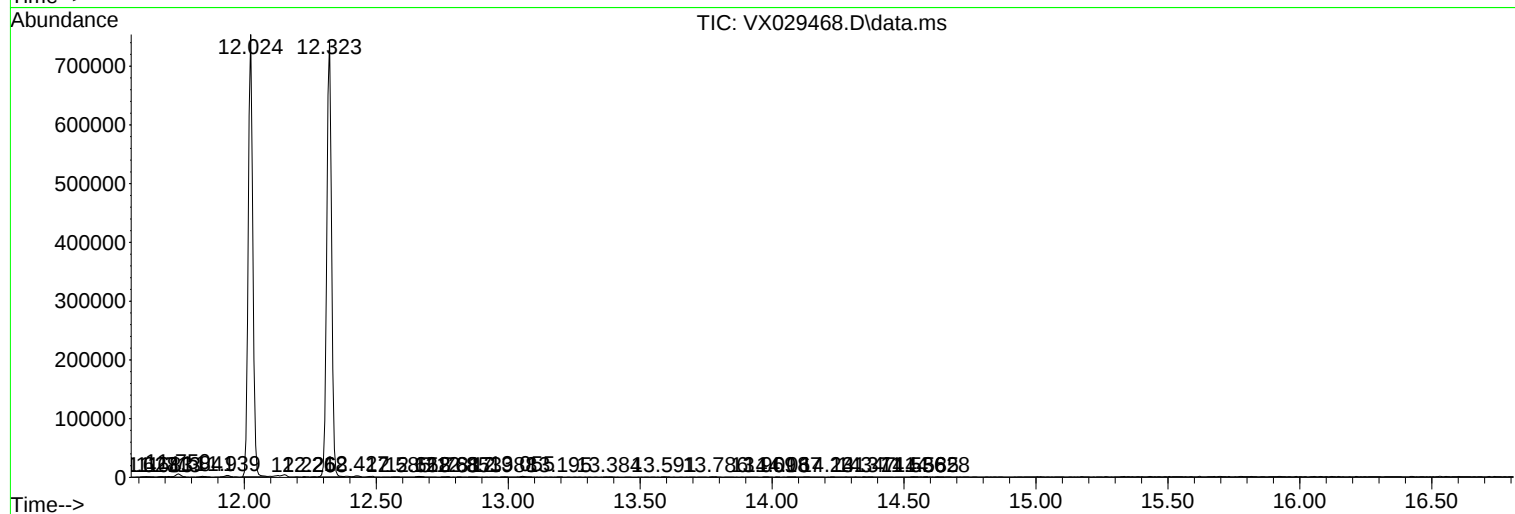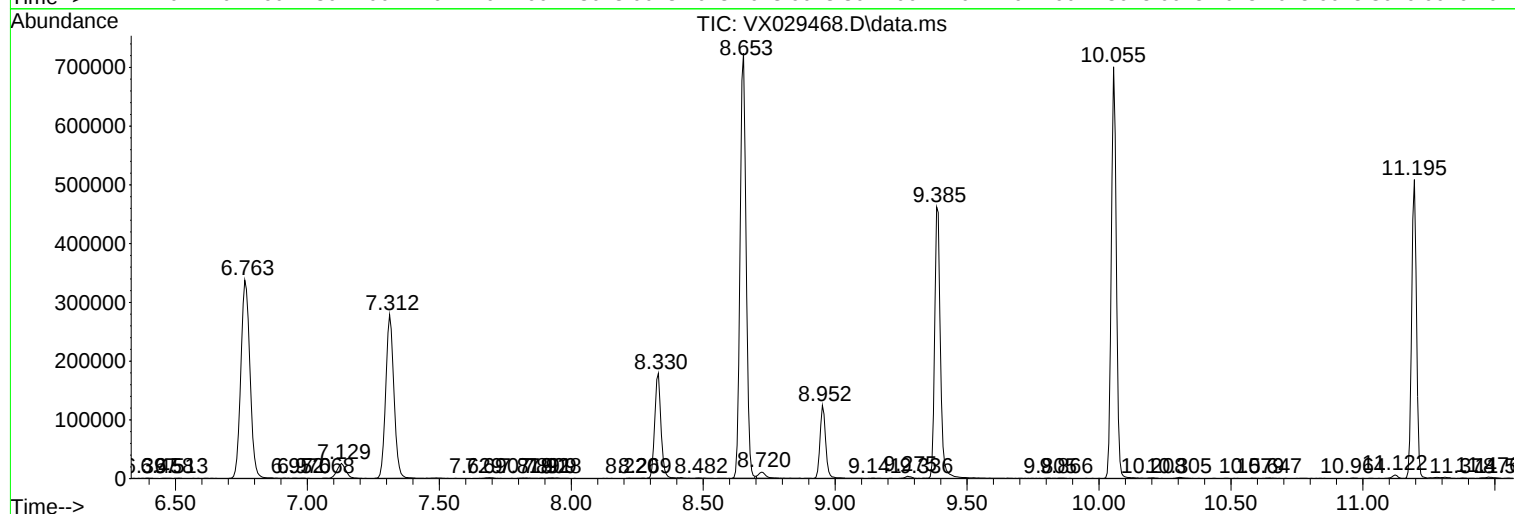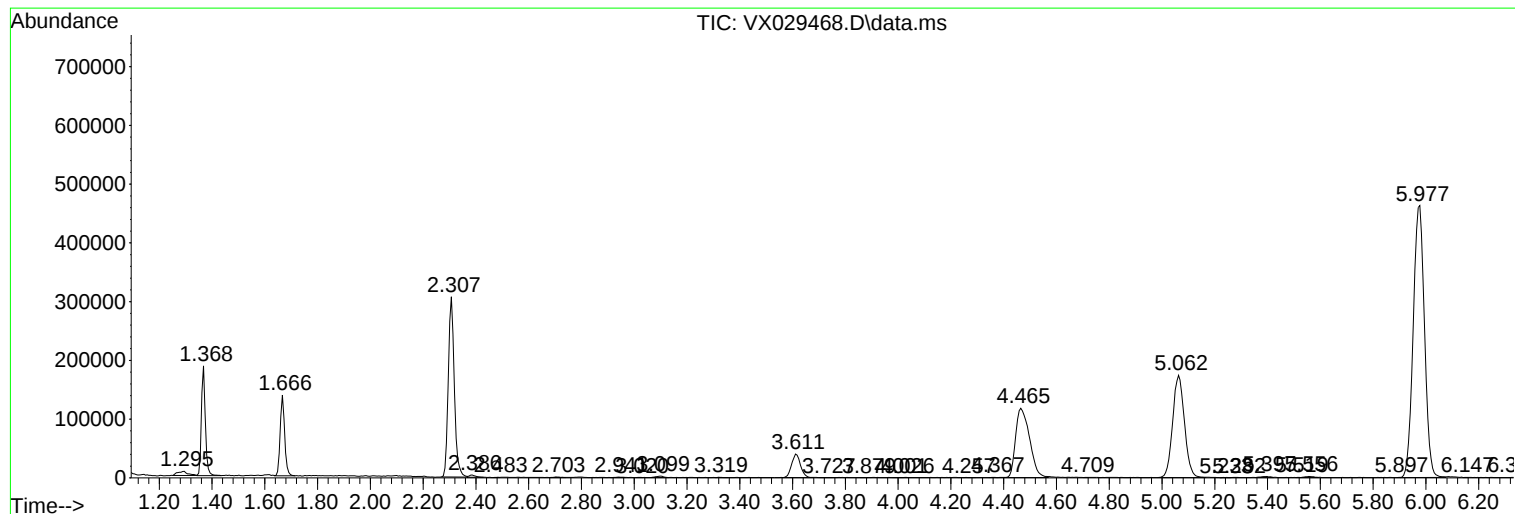

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029468.D
Acq On : 14 Jun 2022 16:30
Operator : JC/MD
Sample : N3249-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029468.D
Acq On : 14 Jun 2022 16:30
Operator : JC/MD
Sample : N3249-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------