

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029471.D
 Acq On : 14 Jun 2022 17:40
 Operator : JC/MD
 Sample : N3249-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029471.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB	179779	184452	13.66%	1.764%
2	1.666	91	95	105	rVB	135978	161750	11.98%	1.547%
3	2.306	194	200	211	rBV	300377	480649	35.59%	4.598%
4	2.508	228	233	241	rVB2	4084	7209	0.53%	0.069%
5	2.703	262	265	266	rBV2	796	816	0.06%	0.008%
6	2.788	272	279	286	rBV5	2984	5812	0.43%	0.056%
7	2.947	298	305	318	rVB	7813	18875	1.40%	0.181%
8	3.099	325	330	342	rVB5	3573	9048	0.67%	0.087%
9	3.361	369	373	376	rBV	357	476	0.04%	0.005%
10	3.428	380	384	386	rBV2	504	652	0.05%	0.006%
11	3.526	399	400	403	rBV	300	407	0.03%	0.004%
12	3.617	412	415	421	rVB2	1031	1478	0.11%	0.014%
13	3.678	423	425	429	rBV3	373	376	0.03%	0.004%
14	3.812	442	447	448	rBV2	300	376	0.03%	0.004%
15	4.068	486	489	491	rBV2	252	345	0.03%	0.003%
16	4.233	513	516	517	rBV2	285	368	0.03%	0.004%
17	4.465	544	554	568	rBV	108837	320996	23.77%	3.071%
18	4.904	621	626	635	rBV5	1173	2950	0.22%	0.028%
19	5.062	639	652	668	rBV	173224	535744	39.67%	5.125%
20	5.391	700	706	712	rBV6	1442	3808	0.28%	0.036%
21	5.471	714	719	727	rVB4	1888	5424	0.40%	0.052%
22	5.556	727	733	739	rVB3	1286	2706	0.20%	0.026%
23	5.678	747	753	760	rBV6	1070	2541	0.19%	0.024%
24	5.977	789	802	818	rBV2	450277	1350337	100.00%	12.917%
25	6.269	847	850	851	rVB2	394	291	0.02%	0.003%
26	6.355	862	864	865	rVB	442	276	0.02%	0.003%
27	6.763	922	931	946	rBV	322242	767215	56.82%	7.339%
28	6.909	953	955	961	rVB3	427	611	0.05%	0.006%
29	7.129	981	991	1001	rVV4	25444	57752	4.28%	0.552%
30	7.312	1012	1021	1032	rBV	272616	590912	43.76%	5.653%
31	7.501	1050	1052	1055	rVB2	757	662	0.05%	0.006%
32	7.580	1063	1065	1068	rVB2	454	337	0.02%	0.003%
33	7.623	1068	1072	1075	rBV3	312	518	0.04%	0.005%
34	7.757	1091	1094	1096	rBV3	324	390	0.03%	0.004%
35	7.830	1099	1106	1111	rBV5	1407	2975	0.22%	0.028%
36	7.903	1117	1118	1120	rBV2	382	285	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029471.D
 Acq On : 14 Jun 2022 17:40
 Operator : JC/MD
 Sample : N3249-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.940	1120	1124	1125	rBV4	494	612	0.05%	0.006%
38	8.238	1170	1173	1175	rBV2	246	367	0.03%	0.004%
39	8.330	1181	1188	1204	rBV	173373	294939	21.84%	2.821%
40	8.586	1224	1230	1234	rBV2	2806	5087	0.38%	0.049%
41	8.653	1234	1241	1248	rVV	726884	1135447	84.09%	10.862%
42	8.726	1248	1253	1262	rVB2	13671	25369	1.88%	0.243%
43	8.952	1285	1290	1304	rVV	123372	182668	13.53%	1.747%
44	9.074	1309	1310	1314	rBV	341	256	0.02%	0.002%
45	9.159	1320	1324	1329	rVB4	2324	2944	0.22%	0.028%
46	9.275	1339	1343	1349	rBV2	6610	9449	0.70%	0.090%
47	9.336	1349	1353	1356	rBV2	207	268	0.02%	0.003%
48	9.384	1356	1361	1380	rBV	484004	712084	52.73%	6.812%
49	9.616	1392	1399	1404	rBV5	1378	2729	0.20%	0.026%
50	9.695	1410	1412	1421	rBV3	1205	2323	0.17%	0.022%
51	9.866	1437	1440	1441	rVV3	302	283	0.02%	0.003%
52	9.897	1441	1445	1448	rVB3	238	363	0.03%	0.003%
53	9.970	1453	1457	1460	rBV2	259	285	0.02%	0.003%
54	10.055	1465	1471	1484	rBV	664686	900890	66.72%	8.618%
55	10.201	1490	1495	1499	rBV	6504	9087	0.67%	0.087%
56	10.305	1506	1512	1522	rBV	7893	12102	0.90%	0.116%
57	10.659	1564	1570	1578	rVB3	8662	17340	1.28%	0.166%
58	10.805	1590	1594	1598	rVB5	978	1286	0.10%	0.012%
59	10.963	1616	1620	1625	rVB	7807	9660	0.72%	0.092%
60	11.031	1628	1631	1634	rBV3	372	558	0.04%	0.005%
61	11.085	1637	1640	1641	rBV2	464	437	0.03%	0.004%
62	11.122	1641	1646	1652	rVB3	4377	6099	0.45%	0.058%
63	11.195	1652	1658	1664	rBV	503783	653032	48.36%	6.247%
64	11.451	1697	1700	1707	rBV	7900	11511	0.85%	0.110%
65	11.549	1713	1716	1723	rVB4	681	866	0.06%	0.008%
66	11.616	1723	1727	1733	rBV5	389	865	0.06%	0.008%
67	11.719	1741	1744	1745	rBV3	502	549	0.04%	0.005%
68	11.750	1745	1749	1756	rVB2	11378	15986	1.18%	0.153%
69	11.841	1761	1764	1768	rVB2	1322	1451	0.11%	0.014%
70	11.933	1773	1779	1782	rBV3	2661	3422	0.25%	0.033%
71	11.969	1782	1785	1789	rVV2	8041	9833	0.73%	0.094%
72	12.024	1789	1794	1806	rVB	716465	889456	65.87%	8.509%
73	12.152	1813	1815	1819	rVB2	3935	3470	0.26%	0.033%
74	12.262	1831	1833	1836	rBV3	600	443	0.03%	0.004%
75	12.323	1837	1843	1851	rVV	736851	943241	69.85%	9.023%
76	12.427	1857	1860	1864	rVB4	1642	2483	0.18%	0.024%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029471.D
 Acq On : 14 Jun 2022 17:40
 Operator : JC/MD
 Sample : N3249-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.475	1864	1868	1875	rVB5	999	2402	0.18%	0.023%
78	12.628	1892	1893	1895	rVV	501	315	0.02%	0.003%
79	12.664	1897	1899	1903	rVB4	1217	1102	0.08%	0.011%
80	12.768	1912	1916	1920	rVB	757	1015	0.08%	0.010%
81	12.866	1930	1932	1936	rVB3	399	446	0.03%	0.004%
82	12.945	1943	1945	1953	rVB4	1234	1566	0.12%	0.015%
83	13.006	1953	1955	1958	rVB2	325	278	0.02%	0.003%
84	13.048	1958	1962	1966	rBV4	890	1493	0.11%	0.014%
85	13.079	1966	1967	1969	rBV2	369	267	0.02%	0.003%
86	13.116	1969	1973	1977	rVB	8207	10054	0.74%	0.096%
87	13.201	1985	1987	1990	rBV2	219	285	0.02%	0.003%
88	13.250	1994	1995	1998	rBV2	219	262	0.02%	0.003%
89	13.554	2041	2045	2046	rBV	288	398	0.03%	0.004%
90	13.591	2046	2051	2056	rVB	10181	12648	0.94%	0.121%
91	13.707	2069	2070	2072	rVB	520	328	0.02%	0.003%
92	13.780	2077	2082	2087	rVV	11261	14048	1.04%	0.134%
93	13.920	2103	2105	2108	rBV2	279	313	0.02%	0.003%
94	13.963	2108	2112	2117	rVV2	10306	12007	0.89%	0.115%
95	14.134	2136	2140	2146	rVB	1961	2753	0.20%	0.026%
96	14.243	2156	2158	2160	rBV2	471	437	0.03%	0.004%
97	14.475	2194	2196	2197	rBV2	500	306	0.02%	0.003%
98	14.615	2215	2219	2221	rBV3	433	537	0.04%	0.005%
99	15.219	2316	2318	2321	rBV3	405	425	0.03%	0.004%
100	15.438	2352	2354	2356	rBV3	577	592	0.04%	0.006%




Sum of corrected areas: 10453636

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029471.D
Acq On : 14 Jun 2022 17:40
Operator : JC/MD
Sample : N3249-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

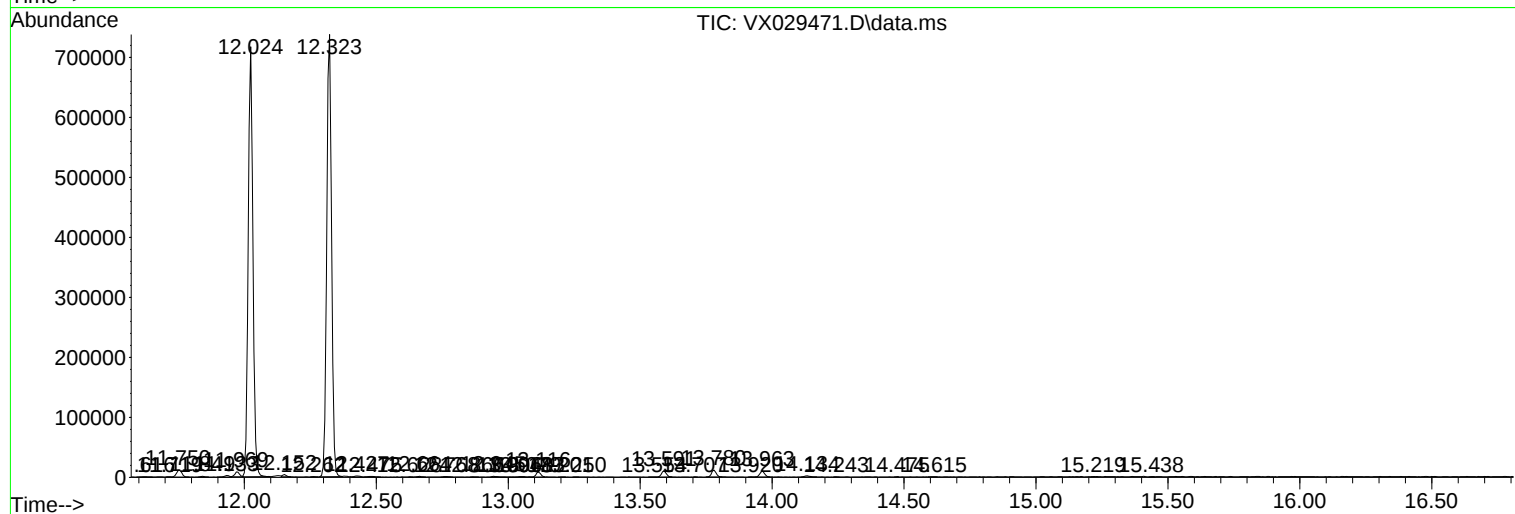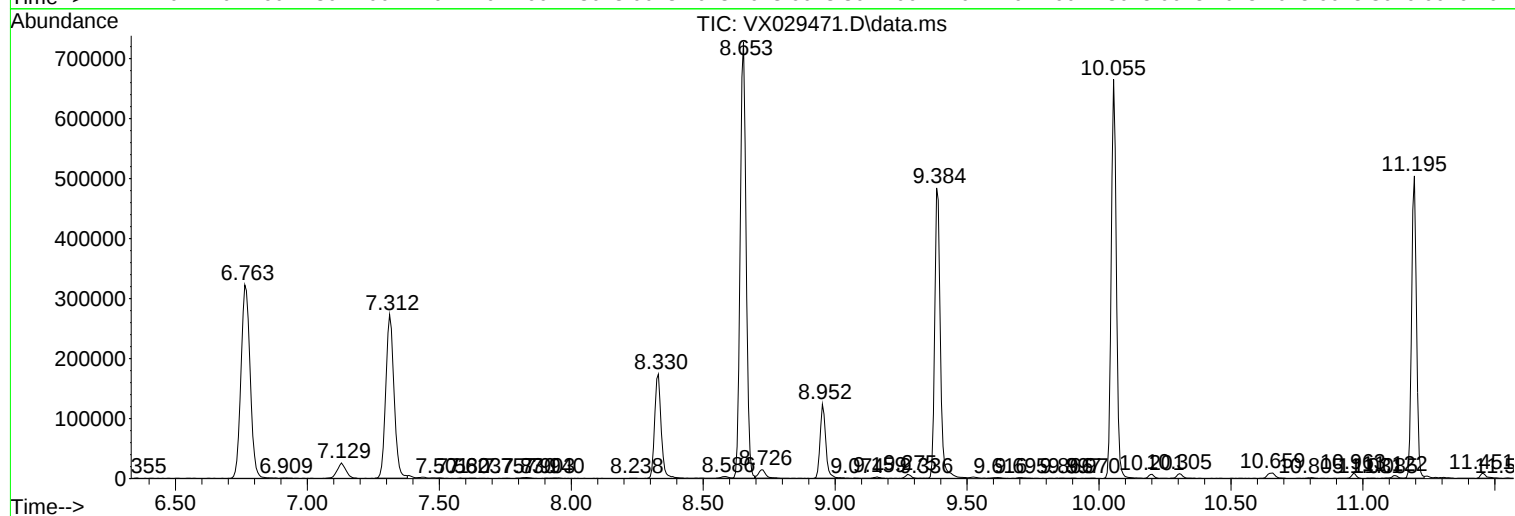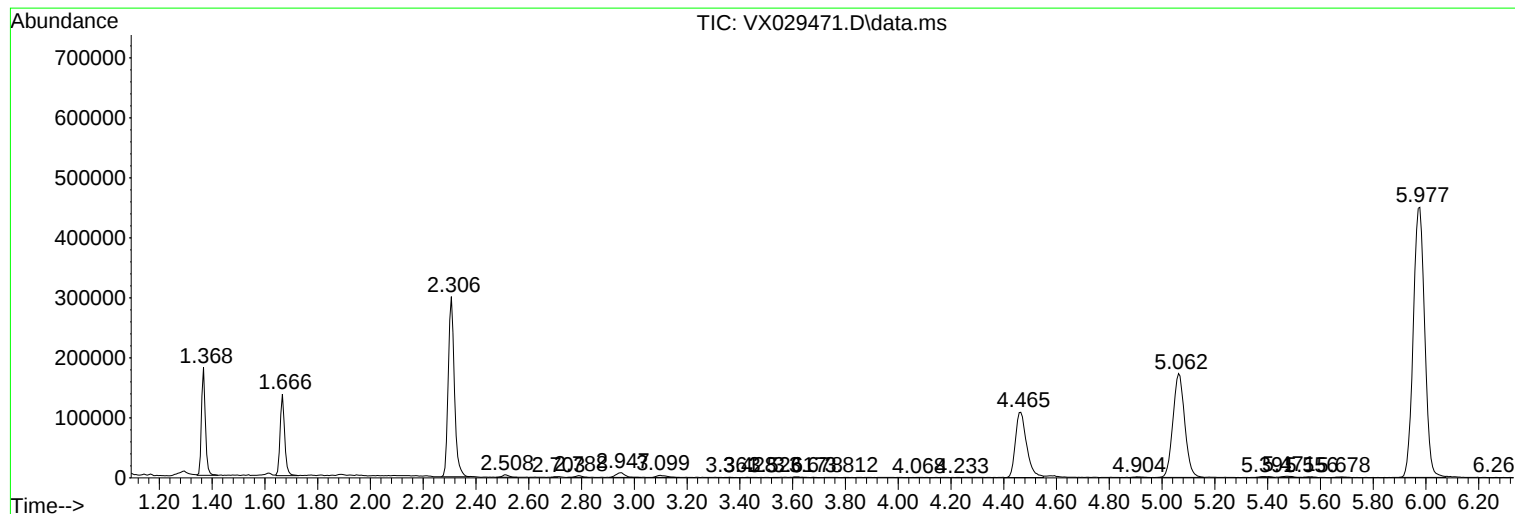

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029471.D
Acq On : 14 Jun 2022 17:40
Operator : JC/MD
Sample : N3249-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029471.D
Acq On : 14 Jun 2022 17:40
Operator : JC/MD
Sample : N3249-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc