

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029472.D
 Acq On : 14 Jun 2022 18:04
 Operator : JC/MD
 Sample : N3311-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0E07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029472.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rVB	184464	186277	13.62%	1.789%
2	1.666	90	95	104	rBV	134023	161301	11.79%	1.549%
3	2.306	194	200	210	rBV	302418	475789	34.78%	4.569%
4	2.465	224	226	228	rVB2	551	402	0.03%	0.004%
5	2.514	229	234	238	rBV	1600	2658	0.19%	0.026%
6	2.788	276	279	284	rVB4	1231	2401	0.18%	0.023%
7	2.849	285	289	293	rBV2	285	448	0.03%	0.004%
8	2.965	300	308	310	rBV4	1000	2509	0.18%	0.024%
9	3.062	322	324	326	rBV2	478	561	0.04%	0.005%
10	3.087	326	328	329	rBV2	709	494	0.04%	0.005%
11	3.446	384	387	388	rBV	358	419	0.03%	0.004%
12	3.501	391	396	397	rVB2	312	497	0.04%	0.005%
13	3.514	397	398	400	rBV	431	331	0.02%	0.003%
14	3.666	422	423	428	rVB2	326	340	0.02%	0.003%
15	4.111	494	496	499	rVB2	305	268	0.02%	0.003%
16	4.178	504	507	508	rBV2	376	303	0.02%	0.003%
17	4.465	545	554	577	rBV	114498	336104	24.57%	3.228%
18	4.788	604	607	609	rBV3	387	325	0.02%	0.003%
19	4.934	627	631	635	rBV4	362	726	0.05%	0.007%
20	5.062	640	652	670	rBV	176443	544500	39.81%	5.229%
21	5.367	700	702	703	rBV	513	545	0.04%	0.005%
22	5.470	714	719	720	rBV4	570	785	0.06%	0.008%
23	5.562	726	734	742	rVB5	1159	3188	0.23%	0.031%
24	5.647	746	748	751	rVB2	429	361	0.03%	0.003%
25	5.678	751	753	754	rBV2	514	445	0.03%	0.004%
26	5.873	784	785	788	rBV2	378	338	0.02%	0.003%
27	5.976	789	802	817	rBV2	463802	1367808	100.00%	13.136%
28	6.190	834	837	840	rVB3	331	399	0.03%	0.004%
29	6.275	849	851	856	rBV3	259	412	0.03%	0.004%
30	6.458	879	881	885	rBV2	242	279	0.02%	0.003%
31	6.513	885	890	892	rBV2	216	350	0.03%	0.003%
32	6.543	892	895	900	rBV3	452	589	0.04%	0.006%
33	6.769	922	932	948	rBV	326796	791757	57.89%	7.604%
34	7.129	982	991	1002	rVV5	22013	53378	3.90%	0.513%
35	7.312	1011	1021	1032	rBV	275331	600155	43.88%	5.764%
36	7.495	1046	1051	1054	rVB3	723	1005	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029472.D
 Acq On : 14 Jun 2022 18:04
 Operator : JC/MD
 Sample : N3311-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0E07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.641	1073	1075	1078	rVB2	445	379	0.03%	0.004%
38	7.665	1078	1079	1081	rBV	265	250	0.02%	0.002%
39	7.732	1089	1090	1093	rBV2	372	408	0.03%	0.004%
40	7.933	1120	1123	1128	rBV2	620	1190	0.09%	0.011%
41	8.281	1177	1180	1181	rBV2	228	247	0.02%	0.002%
42	8.330	1181	1188	1203	rVV	179690	295093	21.57%	2.834%
43	8.482	1211	1213	1214	rBV	450	273	0.02%	0.003%
44	8.574	1227	1228	1231	rVB3	302	268	0.02%	0.003%
45	8.653	1234	1241	1248	rBV	734191	1133698	82.88%	10.888%
46	8.720	1249	1252	1259	rVB	10537	17625	1.29%	0.169%
47	8.952	1285	1290	1299	rBV	122061	182742	13.36%	1.755%
48	9.122	1316	1318	1321	rBV	400	359	0.03%	0.003%
49	9.275	1339	1343	1349	rVB3	3004	4598	0.34%	0.044%
50	9.384	1356	1361	1376	rBV	491698	730420	53.40%	7.015%
51	9.708	1412	1414	1417	rVB2	476	316	0.02%	0.003%
52	9.787	1424	1427	1428	rBV	270	251	0.02%	0.002%
53	10.055	1465	1471	1484	rBV	699094	919758	67.24%	8.833%
54	10.195	1492	1494	1502	rVB3	2057	2899	0.21%	0.028%
55	10.256	1502	1504	1505	rVV	328	271	0.02%	0.003%
56	10.305	1509	1512	1518	rVB4	2795	3824	0.28%	0.037%
57	10.555	1552	1553	1559	rVB3	312	430	0.03%	0.004%
58	10.659	1565	1570	1574	rVB5	1807	3411	0.25%	0.033%
59	10.713	1574	1579	1581	rVB2	400	551	0.04%	0.005%
60	10.756	1581	1586	1588	rBV2	373	556	0.04%	0.005%
61	10.896	1607	1609	1610	rBV2	254	260	0.02%	0.002%
62	10.963	1617	1620	1624	rBV2	1444	1630	0.12%	0.016%
63	11.085	1637	1640	1641	rBV2	403	345	0.03%	0.003%
64	11.122	1642	1646	1652	rVB	4461	5793	0.42%	0.056%
65	11.195	1652	1658	1665	rBV	541686	673759	49.26%	6.471%
66	11.274	1669	1671	1673	rBV2	697	500	0.04%	0.005%
67	11.463	1698	1702	1703	rBV2	1140	1497	0.11%	0.014%
68	11.549	1714	1716	1721	rVB3	733	793	0.06%	0.008%
69	11.628	1727	1729	1735	rVV4	415	462	0.03%	0.004%
70	11.677	1735	1737	1742	rVV2	555	1109	0.08%	0.011%
71	11.719	1742	1744	1745	rVV2	643	494	0.04%	0.005%
72	11.756	1745	1750	1755	rVB3	6371	8842	0.65%	0.085%
73	11.835	1760	1763	1768	rVB4	1167	1532	0.11%	0.015%
74	11.939	1773	1780	1782	rBV3	2313	3296	0.24%	0.032%
75	11.975	1782	1786	1788	rBV3	2096	2534	0.19%	0.024%
76	12.024	1789	1794	1807	rVV	732638	906062	66.24%	8.702%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029472.D
 Acq On : 14 Jun 2022 18:04
 Operator : JC/MD
 Sample : N3311-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0E07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.323	1836	1843	1850	rBV	759239	942369	68.90%	9.051%
78	12.427	1857	1860	1864	rVB4	1417	1731	0.13%	0.017%
79	12.597	1886	1888	1891	rBV2	427	386	0.03%	0.004%
80	12.805	1920	1922	1923	rBV2	287	260	0.02%	0.002%
81	12.975	1947	1950	1952	rBV2	520	582	0.04%	0.006%
82	13.054	1961	1963	1967	rVB3	1037	1112	0.08%	0.011%
83	13.091	1967	1969	1970	rBV	303	276	0.02%	0.003%
84	13.115	1970	1973	1977	rVB2	1917	2600	0.19%	0.025%
85	13.268	1993	1998	1999	rBV2	275	453	0.03%	0.004%
86	13.591	2047	2051	2054	rBV3	2484	3286	0.24%	0.032%
87	13.652	2059	2061	2065	rVB3	354	348	0.03%	0.003%
88	13.749	2075	2077	2078	rBV	355	254	0.02%	0.002%
89	13.780	2078	2082	2090	rVB	2338	3305	0.24%	0.032%
90	13.963	2108	2112	2117	rVB5	2542	2900	0.21%	0.028%
91	14.079	2129	2131	2134	rBV2	313	388	0.03%	0.004%
92	14.134	2137	2140	2143	rVB3	1129	1511	0.11%	0.015%
93	14.164	2143	2145	2148	rVB2	367	320	0.02%	0.003%
94	14.188	2148	2149	2152	rBV	468	475	0.03%	0.005%
95	14.609	2216	2218	2221	rVB2	495	363	0.03%	0.003%
96	14.640	2221	2223	2224	rBV2	426	267	0.02%	0.003%
97	14.658	2224	2226	2229	rBV2	445	536	0.04%	0.005%
98	15.066	2291	2293	2296	rVB2	623	632	0.05%	0.006%
99	15.091	2296	2297	2299	rBV	517	472	0.03%	0.005%
100	16.237	2483	2485	2486	rBV	519	326	0.02%	0.003%




Sum of corrected areas: 10412324

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029472.D
Acq On : 14 Jun 2022 18:04
Operator : JC/MD
Sample : N3311-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0E07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

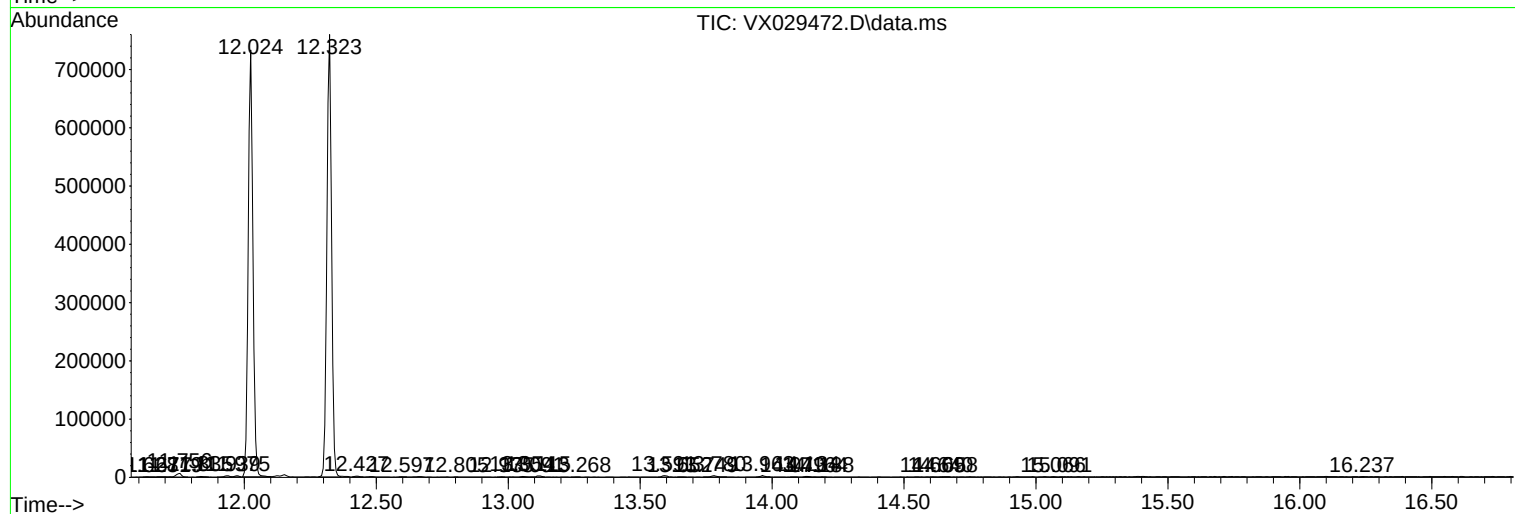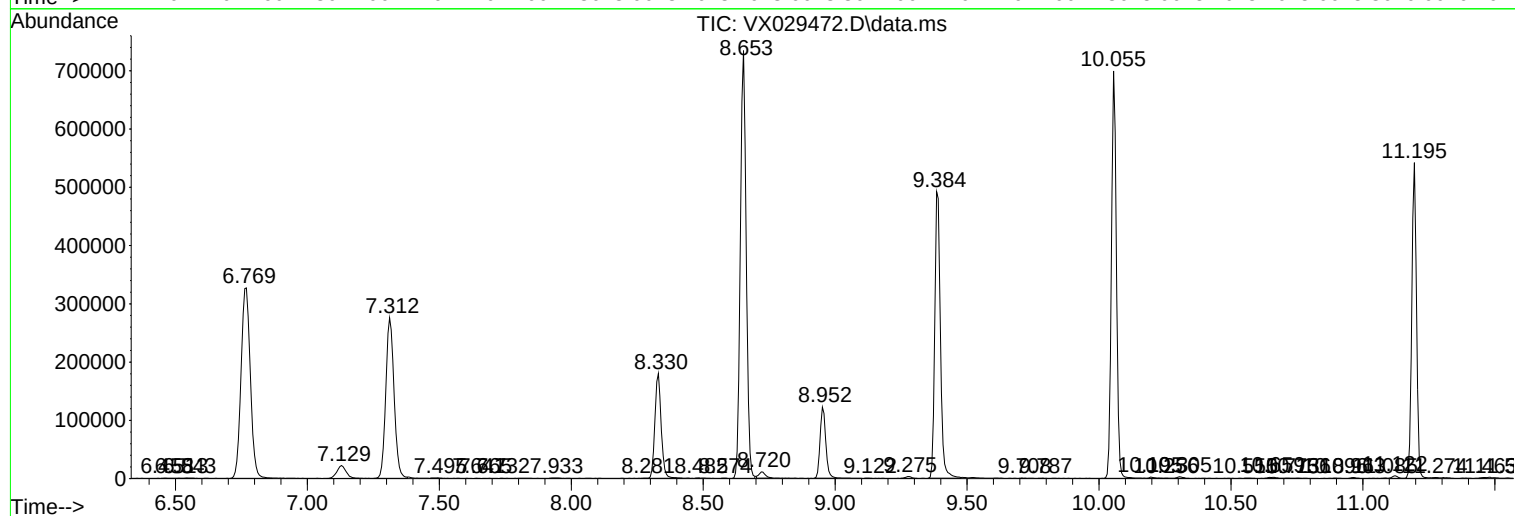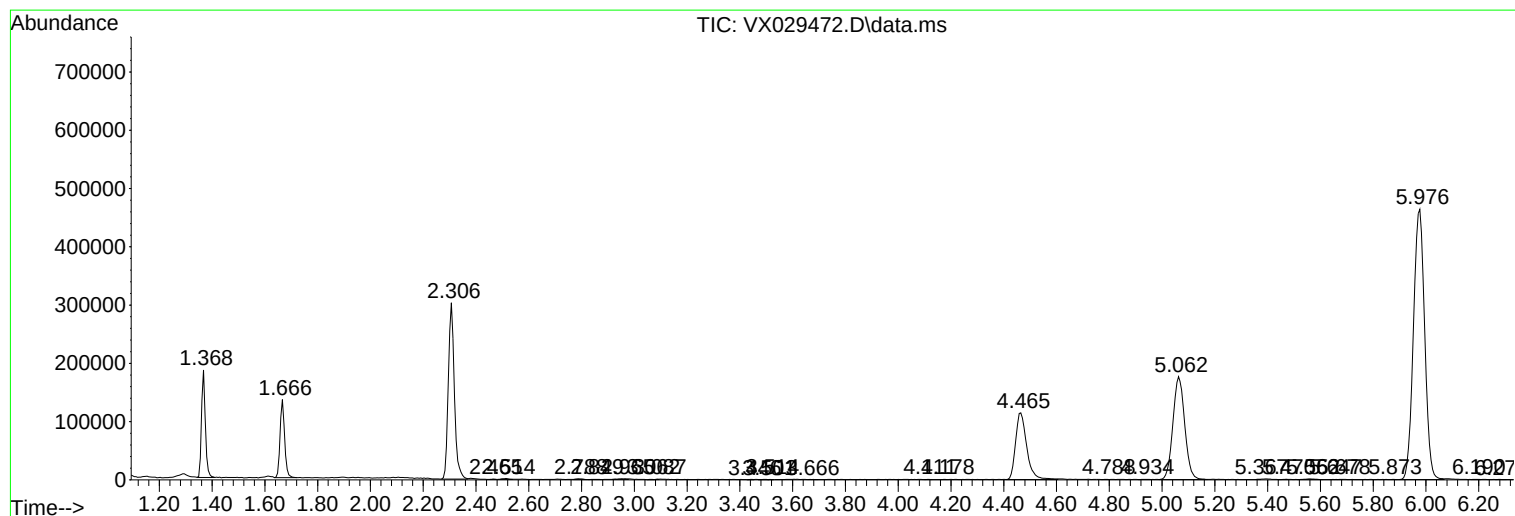

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029472.D
Acq On : 14 Jun 2022 18:04
Operator : JC/MD
Sample : N3311-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0E07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029472.D
Acq On : 14 Jun 2022 18:04
Operator : JC/MD
Sample : N3311-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0E07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc