

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029473.D
 Acq On : 14 Jun 2022 18:27
 Operator : JC/MD
 Sample : N3311-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M

Title : VOC Analysis

Signal : TIC: VX029473.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	56	rVB	178900	181148	13.74%	1.785%
2	1.666	91	95	105	rVB	129179	154000	11.68%	1.517%
3	2.306	194	200	210	rBV	290628	457209	34.69%	4.505%
4	2.392	210	214	218	rVB	3254	5068	0.38%	0.050%
5	2.562	236	242	254	rVB3	7541	22183	1.68%	0.219%
6	2.794	275	280	285	rVB2	3779	6362	0.48%	0.063%
7	2.946	299	305	314	rVB2	4555	10415	0.79%	0.103%
8	3.087	326	328	335	rVV2	679	870	0.07%	0.009%
9	3.154	338	339	343	rBV3	432	448	0.03%	0.004%
10	3.611	412	414	417	rBV2	242	268	0.02%	0.003%
11	3.897	459	461	463	rBV3	264	320	0.02%	0.003%
12	4.458	544	553	572	rBV	111131	321304	24.38%	3.166%
13	5.062	640	652	668	rBV	169441	519632	39.42%	5.120%
14	5.318	691	694	695	rBV2	277	307	0.02%	0.003%
15	5.373	698	703	704	rBV3	555	745	0.06%	0.007%
16	5.476	717	720	721	rBV2	378	367	0.03%	0.004%
17	5.556	729	733	738	rBV4	1066	1852	0.14%	0.018%
18	5.659	749	750	753	rBV3	382	417	0.03%	0.004%
19	5.970	790	801	818	rBV2	445215	1318146	100.00%	12.988%
20	6.299	852	855	857	rVB2	240	308	0.02%	0.003%
21	6.373	866	867	870	rVB3	544	345	0.03%	0.003%
22	6.763	922	931	948	rBV	331554	793223	60.18%	7.816%
23	6.897	951	953	956	rBV3	476	678	0.05%	0.007%
24	6.970	961	965	966	rVV2	234	261	0.02%	0.003%
25	6.988	966	968	972	rVB2	483	453	0.03%	0.004%
26	7.135	982	992	1001	rBV3	21057	53014	4.02%	0.522%
27	7.312	1013	1021	1039	rBV	265867	581060	44.08%	5.725%
28	7.647	1070	1076	1077	rBV2	298	421	0.03%	0.004%
29	7.732	1086	1090	1093	rBV3	257	462	0.04%	0.005%
30	7.763	1093	1095	1098	rVV2	440	497	0.04%	0.005%
31	7.811	1101	1103	1105	rBV2	519	530	0.04%	0.005%
32	7.854	1108	1110	1112	rBV2	385	271	0.02%	0.003%
33	7.946	1121	1125	1131	rVB4	967	1592	0.12%	0.016%
34	8.031	1136	1139	1140	rBV	314	279	0.02%	0.003%
35	8.092	1147	1149	1152	rVB2	288	353	0.03%	0.003%
36	8.189	1160	1165	1167	rBV3	271	469	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029473.D
 Acq On : 14 Jun 2022 18:27
 Operator : JC/MD
 Sample : N3311-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	8.330	1181	1188	1201	rBV	171620	281419	21.35%	2.773%
38	8.482	1211	1213	1217	rBV3	536	541	0.04%	0.005%
39	8.573	1225	1228	1231	rBV3	338	501	0.04%	0.005%
40	8.653	1234	1241	1248	rBV	704362	1101828	83.59%	10.856%
41	8.720	1250	1252	1257	rVB	9787	13627	1.03%	0.134%
42	8.866	1271	1276	1279	rBV3	374	581	0.04%	0.006%
43	8.951	1284	1290	1300	rBV	116207	174939	13.27%	1.724%
44	9.275	1339	1343	1349	rVB3	2878	3692	0.28%	0.036%
45	9.384	1356	1361	1376	rBV	476203	705723	53.54%	6.953%
46	9.750	1419	1421	1424	rVB2	321	271	0.02%	0.003%
47	10.055	1465	1471	1487	rBV	690508	920826	69.86%	9.073%
48	10.201	1491	1495	1500	rVB3	1389	2407	0.18%	0.024%
49	10.250	1500	1503	1506	rBV3	584	719	0.05%	0.007%
50	10.305	1508	1512	1519	rVV2	1854	3165	0.24%	0.031%
51	10.433	1529	1533	1534	rBV3	201	296	0.02%	0.003%
52	10.591	1556	1559	1561	rBV2	380	401	0.03%	0.004%
53	10.646	1564	1568	1571	rBV5	1262	2078	0.16%	0.020%
54	10.750	1583	1585	1588	rVB2	458	493	0.04%	0.005%
55	10.872	1603	1605	1607	rBV2	328	293	0.02%	0.003%
56	10.963	1617	1620	1621	rBV2	677	776	0.06%	0.008%
57	11.036	1627	1632	1633	rBV	613	777	0.06%	0.008%
58	11.067	1636	1637	1639	rBV2	357	290	0.02%	0.003%
59	11.085	1639	1640	1643	rVV3	427	567	0.04%	0.006%
60	11.122	1643	1646	1652	rVB2	4840	5803	0.44%	0.057%
61	11.195	1652	1658	1670	rBV	504213	640473	48.59%	6.310%
62	11.280	1670	1672	1673	rBV2	673	540	0.04%	0.005%
63	11.378	1686	1688	1691	rBV2	546	531	0.04%	0.005%
64	11.475	1698	1704	1712	rVB7	1355	3993	0.30%	0.039%
65	11.542	1712	1715	1717	rBV3	556	668	0.05%	0.007%
66	11.713	1740	1743	1744	rBV3	466	477	0.04%	0.005%
67	11.750	1745	1749	1755	rVB2	5053	7415	0.56%	0.073%
68	11.805	1755	1758	1759	rBV2	285	280	0.02%	0.003%
69	11.841	1761	1764	1768	rVB3	1321	1555	0.12%	0.015%
70	11.933	1776	1779	1783	rVB3	1824	2305	0.17%	0.023%
71	11.975	1783	1786	1789	rBV2	1192	1073	0.08%	0.011%
72	12.024	1789	1794	1806	rBV	749632	898815	68.19%	8.856%
73	12.152	1813	1815	1819	rVB3	4088	3966	0.30%	0.039%
74	12.219	1824	1826	1831	rVB3	1638	2083	0.16%	0.021%
75	12.262	1831	1833	1835	rBV2	749	549	0.04%	0.005%
76	12.323	1836	1843	1851	rBV	737661	911118	69.12%	8.977%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029473.D
 Acq On : 14 Jun 2022 18:27
 Operator : JC/MD
 Sample : N3311-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.463	1863	1866	1868	rBV2	406	555	0.04%	0.005%
78	12.481	1868	1869	1870	rBV	801	355	0.03%	0.003%
79	12.548	1878	1880	1881	rBV	344	275	0.02%	0.003%
80	12.670	1896	1900	1905	rVB2	1062	1627	0.12%	0.016%
81	12.975	1948	1950	1952	rBV2	350	333	0.03%	0.003%
82	13.054	1960	1963	1966	rBV4	964	1016	0.08%	0.010%
83	13.115	1970	1973	1977	rVB2	1356	1480	0.11%	0.015%
84	13.152	1977	1979	1983	rBV3	357	396	0.03%	0.004%
85	13.286	2000	2001	2005	rVB	338	248	0.02%	0.002%
86	13.463	2026	2030	2031	rBV	320	315	0.02%	0.003%
87	13.591	2048	2051	2058	rVB3	1627	2173	0.16%	0.021%
88	13.664	2059	2063	2066	rVB2	394	399	0.03%	0.004%
89	13.737	2073	2075	2076	rBV	356	285	0.02%	0.003%
90	13.780	2080	2082	2086	rVB3	1012	1309	0.10%	0.013%
91	13.963	2109	2112	2116	rVB3	1076	1334	0.10%	0.013%
92	14.030	2121	2123	2125	rBV	529	466	0.04%	0.005%
93	14.072	2128	2130	2132	rVB	310	244	0.02%	0.002%
94	14.097	2132	2134	2135	rBV2	357	330	0.03%	0.003%
95	14.133	2137	2140	2144	rVB3	1105	1528	0.12%	0.015%
96	14.371	2177	2179	2182	rBV2	322	287	0.02%	0.003%
97	14.688	2229	2231	2232	rVB	394	251	0.02%	0.002%
98	14.707	2232	2234	2235	rBV2	420	346	0.03%	0.003%
99	14.877	2260	2262	2263	rBV2	543	285	0.02%	0.003%
100	15.060	2290	2292	2294	rBV	506	370	0.03%	0.004%

Sum of corrected areas: 10149338




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029473.D
Acq On : 14 Jun 2022 18:27
Operator : JC/MD
Sample : N3311-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

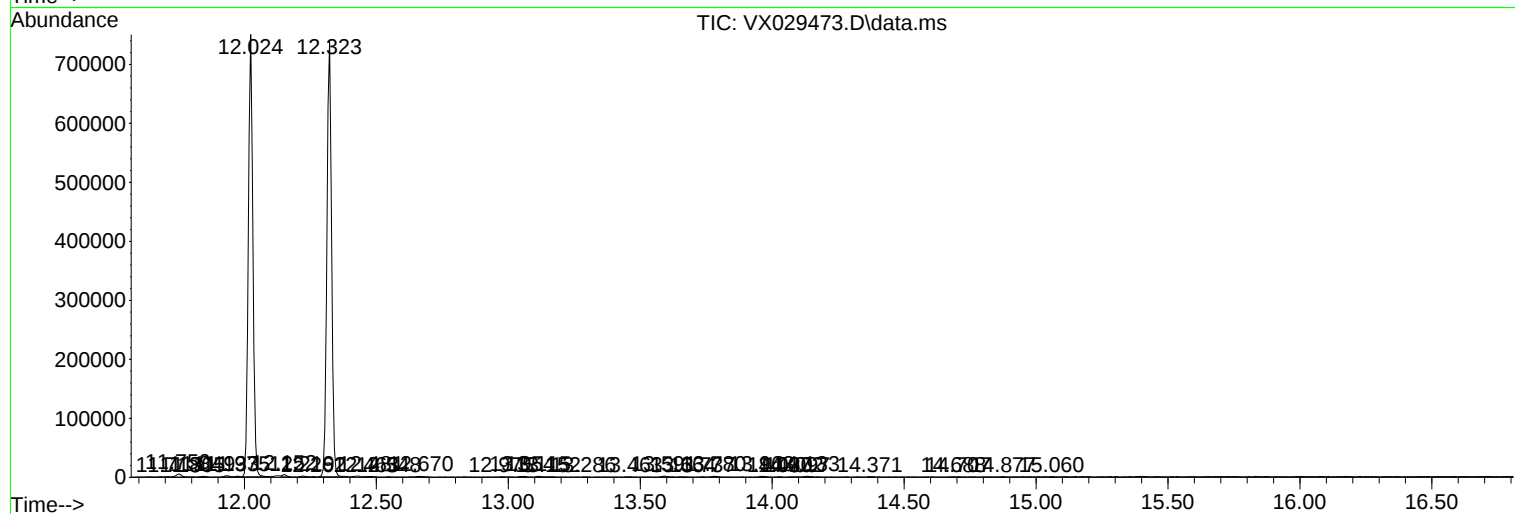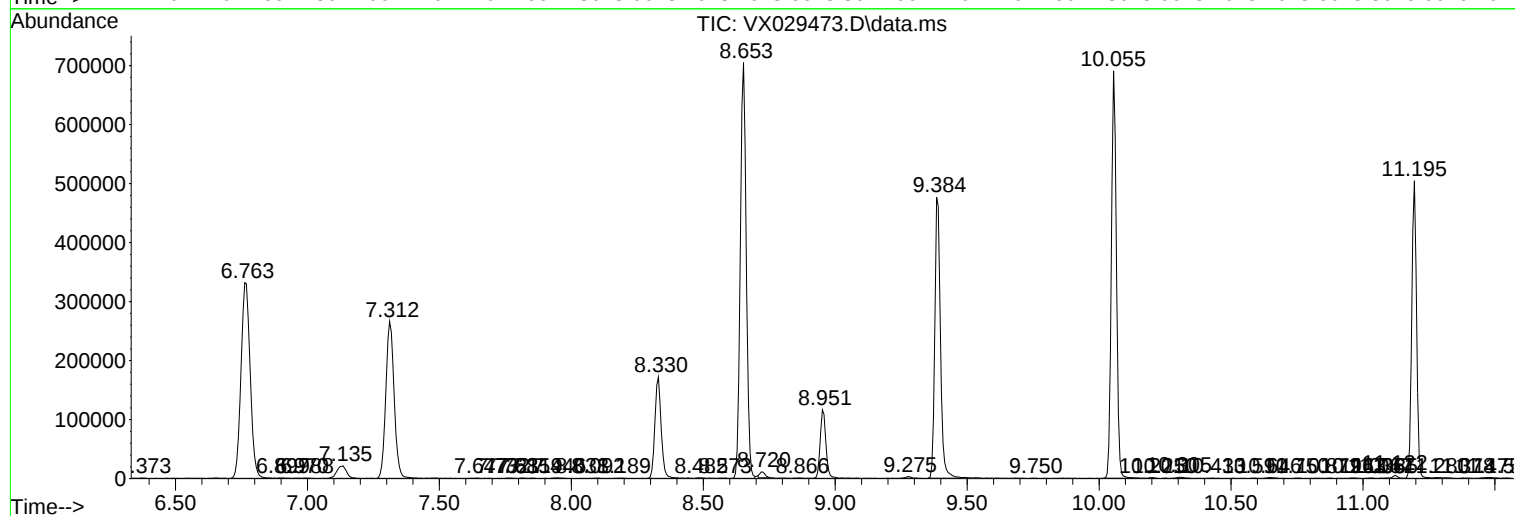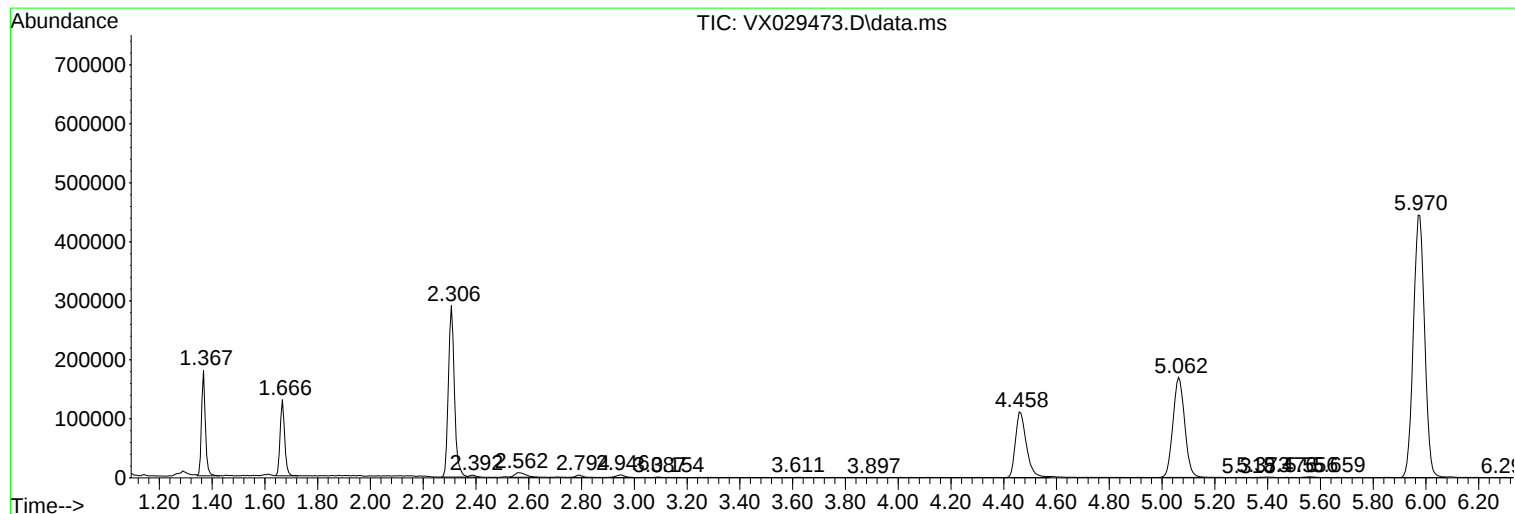

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029473.D
Acq On : 14 Jun 2022 18:27
Operator : JC/MD
Sample : N3311-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029473.D
Acq On : 14 Jun 2022 18:27
Operator : JC/MD
Sample : N3311-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc