

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029476.D
 Acq On : 14 Jun 2022 19:37
 Operator : JC/MD
 Sample : N3313-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YB7L3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M

Title : VOC Analysis

Signal : TIC: VX029476.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	56	rVB	185421	187211	3.02%	1.093%
2	1.666	91	95	103	rVB	132404	157767	2.55%	0.921%
3	2.306	194	200	212	rBV2	338674	617908	9.97%	3.607%
4	2.751	272	273	274	rBV	404	224	0.00%	0.001%
5	2.953	297	306	315	rVB2	6058	13939	0.22%	0.081%
6	3.093	327	329	333	rVB3	546	537	0.01%	0.003%
7	3.190	342	345	346	rBV2	444	465	0.01%	0.003%
8	3.611	409	414	422	rVB3	3422	6853	0.11%	0.040%
9	3.721	430	432	435	rBV2	307	249	0.00%	0.001%
10	3.757	437	438	441	rVB2	306	249	0.00%	0.001%
11	3.788	441	443	447	rBV2	246	360	0.01%	0.002%
12	3.879	456	458	461	rBV2	330	291	0.00%	0.002%
13	3.971	471	473	477	rVB	284	341	0.01%	0.002%
14	4.062	486	488	490	rBV2	365	321	0.01%	0.002%
15	4.178	506	507	510	rBV2	273	270	0.00%	0.002%
16	4.239	515	517	519	rBV2	397	346	0.01%	0.002%
17	4.343	531	534	535	rBV2	242	277	0.00%	0.002%
18	4.355	535	536	539	rVB	371	258	0.00%	0.002%
19	4.391	539	542	544	rBV2	460	470	0.01%	0.003%
20	4.464	544	554	571	rBV	112911	336128	5.42%	1.962%
21	4.781	605	606	608	rVB2	337	242	0.00%	0.001%
22	4.885	620	623	626	rBV2	337	416	0.01%	0.002%
23	5.062	638	652	669	rBV	172895	543772	8.77%	3.174%
24	5.367	698	702	703	rBV2	541	676	0.01%	0.004%
25	5.397	703	707	714	rVB3	1047	2185	0.04%	0.013%
26	5.470	717	719	722	rVB3	338	304	0.00%	0.002%
27	5.556	726	733	735	rBV4	1559	2580	0.04%	0.015%
28	5.653	745	749	750	rBV2	370	354	0.01%	0.002%
29	5.757	764	766	769	rVB2	386	470	0.01%	0.003%
30	5.793	769	772	777	rVB2	409	698	0.01%	0.004%
31	5.836	777	779	780	rBV	308	264	0.00%	0.002%
32	5.976	789	802	816	rBV2	458946	1360730	21.95%	7.943%
33	6.397	869	871	875	rBV2	428	581	0.01%	0.003%
34	6.556	892	897	900	rBV2	430	816	0.01%	0.005%
35	6.653	911	913	914	rBV	347	257	0.00%	0.002%
36	6.763	922	931	946	rBV	326753	790316	12.75%	4.613%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029476.D
 Acq On : 14 Jun 2022 19:37
 Operator : JC/MD
 Sample : N3313-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YB7L3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.129	980	991	1012	rBV	2900672	6198781	100.00%	36.185%
38	7.311	1013	1021	1036	rVB	268900	595077	9.60%	3.474%
39	7.476	1046	1048	1053	rVB3	498	565	0.01%	0.003%
40	7.659	1076	1078	1079	rBV	415	287	0.00%	0.002%
41	7.696	1079	1084	1092	rBV4	1126	2419	0.04%	0.014%
42	7.824	1103	1105	1107	rBV2	707	694	0.01%	0.004%
43	7.939	1119	1124	1128	rBV6	622	1022	0.02%	0.006%
44	8.037	1138	1140	1143	rBV2	204	278	0.00%	0.002%
45	8.135	1155	1156	1159	rBV2	285	361	0.01%	0.002%
46	8.330	1181	1188	1200	rBV	178975	288389	4.65%	1.683%
47	8.653	1234	1241	1249	rVV	727188	1148086	18.52%	6.702%
48	8.726	1249	1253	1261	rVB	9897	17410	0.28%	0.102%
49	8.951	1284	1290	1305	rBV	122442	180706	2.92%	1.055%
50	9.159	1320	1324	1330	rVB4	1841	2949	0.05%	0.017%
51	9.275	1337	1343	1352	rBV	321287	462073	7.45%	2.697%
52	9.384	1356	1361	1379	rBV	477880	716118	11.55%	4.180%
53	9.671	1404	1408	1411	rBV3	339	575	0.01%	0.003%
54	10.000	1459	1462	1465	rBV	312	361	0.01%	0.002%
55	10.055	1465	1471	1481	rBV	698613	924745	14.92%	5.398%
56	10.201	1491	1495	1498	rBV3	855	948	0.02%	0.006%
57	10.311	1508	1513	1517	rVB2	1782	2924	0.05%	0.017%
58	10.482	1540	1541	1542	rBV	378	220	0.00%	0.001%
59	10.811	1594	1595	1599	rBV2	229	299	0.00%	0.002%
60	10.860	1601	1603	1607	rBV	268	357	0.01%	0.002%
61	11.000	1624	1626	1629	rBV2	393	297	0.00%	0.002%
62	11.030	1629	1631	1632	rVV2	335	240	0.00%	0.001%
63	11.079	1638	1639	1641	rBV	438	346	0.01%	0.002%
64	11.122	1641	1646	1652	rVB	4674	5929	0.10%	0.035%
65	11.195	1652	1658	1665	rBV	531055	657890	10.61%	3.840%
66	11.433	1695	1697	1698	rBV	510	429	0.01%	0.003%
67	11.481	1702	1705	1712	rVB4	1385	2366	0.04%	0.014%
68	11.683	1734	1738	1741	rBV3	573	828	0.01%	0.005%
69	11.713	1741	1743	1744	rVV	832	613	0.01%	0.004%
70	11.750	1744	1749	1755	rVB4	4147	6508	0.10%	0.038%
71	11.847	1761	1765	1769	rVB3	1031	1382	0.02%	0.008%
72	11.878	1769	1770	1773	rBV2	304	260	0.00%	0.002%
73	11.933	1775	1779	1783	rBV4	2906	4160	0.07%	0.024%
74	11.981	1783	1787	1788	rVB	594	599	0.01%	0.003%
75	12.024	1789	1794	1806	rVB	750334	908785	14.66%	5.305%
76	12.225	1823	1827	1830	rBV3	2222	3254	0.05%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029476.D
 Acq On : 14 Jun 2022 19:37
 Operator : JC/MD
 Sample : N3313-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YB7L3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.323	1837	1843	1852	rVB	752715	944650	15.24%	5.514%
78	12.426	1857	1860	1865	rVB4	1866	2296	0.04%	0.013%
79	12.475	1866	1868	1876	rVB2	1039	1521	0.02%	0.009%
80	12.548	1879	1880	1882	rBV	375	293	0.00%	0.002%
81	12.579	1882	1885	1886	rBV2	395	388	0.01%	0.002%
82	12.628	1890	1893	1895	rBV3	585	589	0.01%	0.003%
83	12.658	1896	1898	1903	rVB4	1213	1404	0.02%	0.008%
84	12.774	1915	1917	1919	rVB2	447	343	0.01%	0.002%
85	12.792	1919	1920	1921	rBV	359	230	0.00%	0.001%
86	12.859	1927	1931	1937	rVB4	2967	3785	0.06%	0.022%
87	13.048	1959	1962	1968	rVB3	762	1326	0.02%	0.008%
88	13.097	1968	1970	1971	rBV	371	292	0.00%	0.002%
89	13.115	1971	1973	1976	rVB3	692	694	0.01%	0.004%
90	13.176	1982	1983	1985	rVB	363	233	0.00%	0.001%
91	13.256	1992	1996	1998	rVB2	398	528	0.01%	0.003%
92	13.377	2014	2016	2017	rBV2	307	244	0.00%	0.001%
93	13.426	2022	2024	2027	rBV2	266	296	0.00%	0.002%
94	13.591	2049	2051	2055	rVV2	498	680	0.01%	0.004%
95	13.640	2057	2059	2060	rBV	347	278	0.00%	0.002%
96	13.902	2100	2102	2104	rBV2	309	324	0.01%	0.002%
97	14.005	2118	2119	2121	rBV	562	286	0.00%	0.002%
98	14.731	2236	2238	2241	rBV2	492	522	0.01%	0.003%
99	15.517	2365	2367	2369	rBV2	723	667	0.01%	0.004%
100	16.737	2565	2567	2568	rBV	595	300	0.00%	0.002%




Sum of corrected areas: 17130824

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029476.D
Acq On : 14 Jun 2022 19:37
Operator : JC/MD
Sample : N3313-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YB7L3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

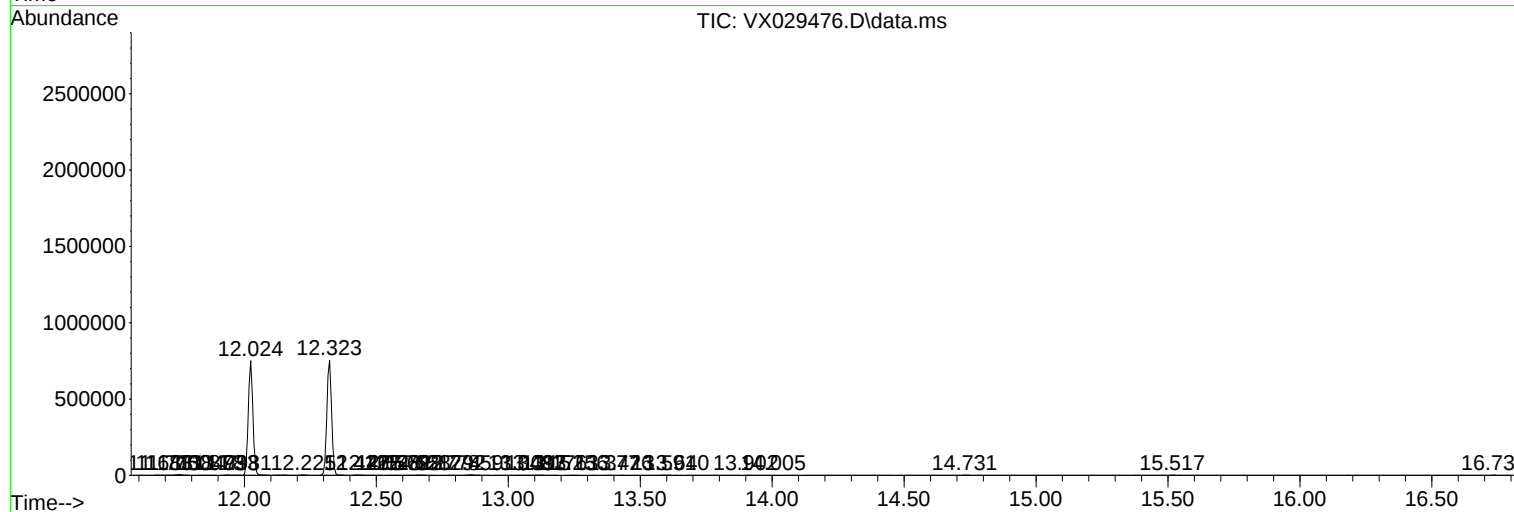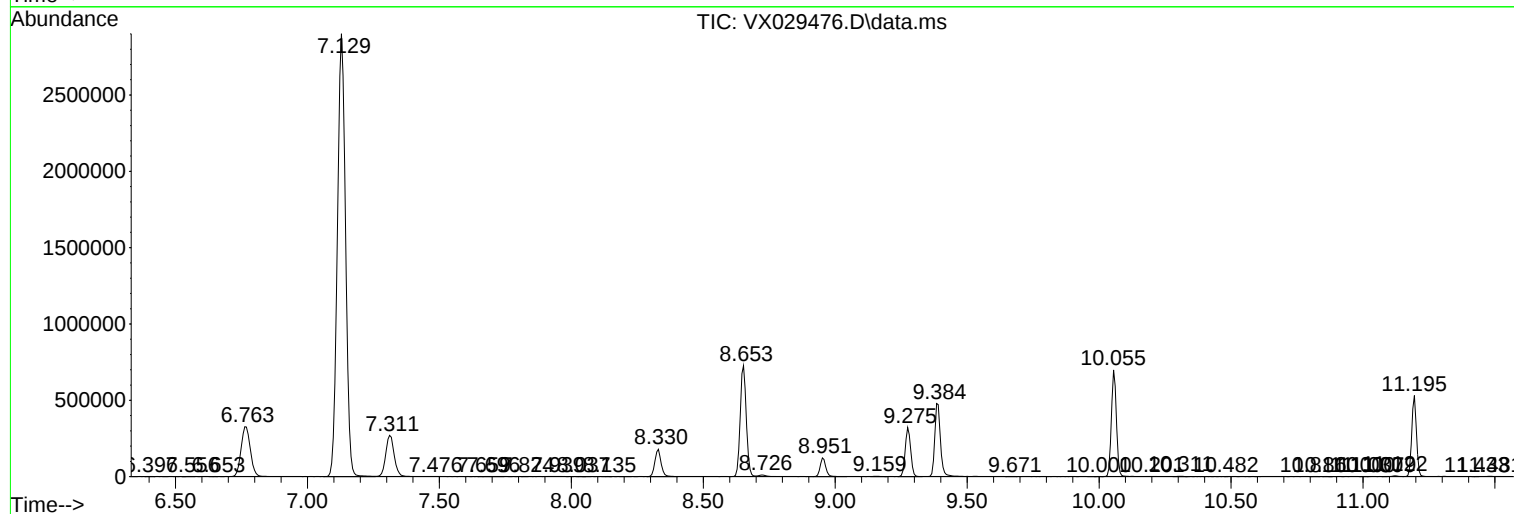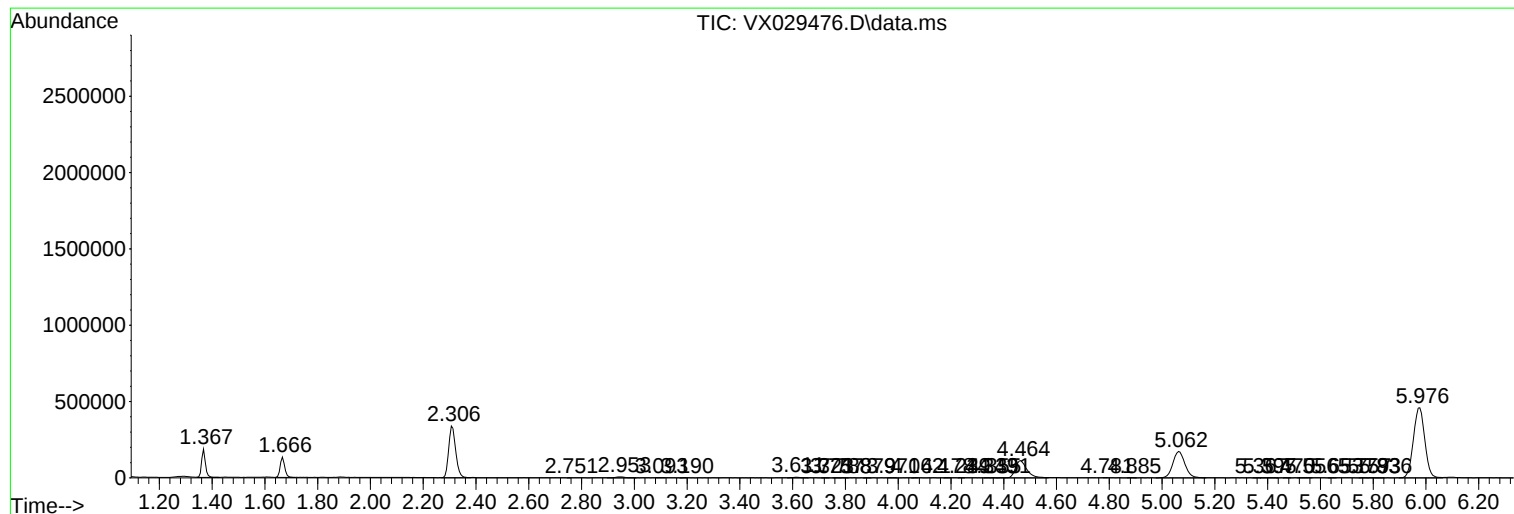

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029476.D
Acq On : 14 Jun 2022 19:37
Operator : JC/MD
Sample : N3313-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YB7L3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029476.D
Acq On : 14 Jun 2022 19:37
Operator : JC/MD
Sample : N3313-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YB7L3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc