

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029477.D
 Acq On : 14 Jun 2022 20:00
 Operator : JC/MD
 Sample : N3313-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YB7L4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029477.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	182029	182434	7.23%	1.394%
2	1.666	91	95	104	rVB	132554	158147	6.26%	1.208%
3	2.307	193	200	210	rBV2	308587	507983	20.12%	3.881%
4	2.624	250	252	256	rVB2	468	569	0.02%	0.004%
5	2.709	263	266	269	rVV2	557	602	0.02%	0.005%
6	2.788	277	279	283	rVB3	1030	1381	0.05%	0.011%
7	2.831	283	286	288	rBV2	255	307	0.01%	0.002%
8	2.886	293	295	297	rVV2	430	334	0.01%	0.003%
9	2.947	300	305	315	rVB	4290	8787	0.35%	0.067%
10	3.239	349	353	354	rBV2	418	297	0.01%	0.002%
11	3.288	358	361	363	rBV2	357	309	0.01%	0.002%
12	3.593	407	411	412	rBV	462	644	0.03%	0.005%
13	3.605	412	413	421	rVB3	820	1600	0.06%	0.012%
14	3.697	426	428	431	rBV2	407	462	0.02%	0.004%
15	3.971	469	473	476	rBV2	240	422	0.02%	0.003%
16	4.355	534	536	539	rVB2	504	376	0.01%	0.003%
17	4.459	544	553	568	rBV	110046	318943	12.63%	2.437%
18	4.660	584	586	587	rVB2	519	286	0.01%	0.002%
19	5.062	640	652	668	rBV	171408	540862	21.42%	4.132%
20	5.367	696	702	703	rBV2	431	580	0.02%	0.004%
21	5.562	726	734	744	rBV4	1516	4366	0.17%	0.033%
22	5.666	749	751	756	rBV3	397	690	0.03%	0.005%
23	5.977	789	802	820	rBV2	460792	1356494	53.73%	10.364%
24	6.214	838	841	844	rBV3	471	567	0.02%	0.004%
25	6.257	847	848	852	rVV2	365	461	0.02%	0.004%
26	6.330	856	860	861	rVV2	313	318	0.01%	0.002%
27	6.416	871	874	877	rBV2	360	469	0.02%	0.004%
28	6.452	877	880	881	rBV2	401	383	0.02%	0.003%
29	6.562	894	898	900	rBV2	382	493	0.02%	0.004%
30	6.763	919	931	941	rBV	312552	749247	29.68%	5.724%
31	7.129	981	991	1011	rBV	1155940	2524490	100.00%	19.287%
32	7.312	1012	1021	1038	rVB	271014	595039	23.57%	4.546%
33	7.549	1059	1060	1062	rBV2	387	350	0.01%	0.003%
34	7.574	1062	1064	1066	rVB	384	278	0.01%	0.002%
35	7.665	1077	1079	1082	rBV2	283	281	0.01%	0.002%
36	7.696	1082	1084	1088	rVV3	638	817	0.03%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029477.D
 Acq On : 14 Jun 2022 20:00
 Operator : JC/MD
 Sample : N3313-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YB7L4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.940	1119	1124	1130	rBV4	886	1947	0.08%	0.015%
38	8.001	1132	1134	1136	rVB	390	284	0.01%	0.002%
39	8.110	1149	1152	1154	rBV2	326	398	0.02%	0.003%
40	8.196	1164	1166	1171	rVB2	229	344	0.01%	0.003%
41	8.330	1182	1188	1201	rVV	175904	285929	11.33%	2.185%
42	8.494	1211	1215	1218	rVB4	528	761	0.03%	0.006%
43	8.574	1226	1228	1229	rBV2	448	363	0.01%	0.003%
44	8.653	1233	1241	1249	rBV	733418	1137351	45.05%	8.689%
45	8.726	1249	1253	1261	rVB2	10310	17249	0.68%	0.132%
46	8.891	1278	1280	1282	rBV	297	277	0.01%	0.002%
47	8.952	1285	1290	1304	rVV	121531	182338	7.22%	1.393%
48	9.092	1309	1313	1315	rBV2	249	347	0.01%	0.003%
49	9.159	1320	1324	1327	rVB4	709	854	0.03%	0.007%
50	9.275	1337	1343	1355	rBV	251993	371434	14.71%	2.838%
51	9.385	1356	1361	1376	rVV	482163	712162	28.21%	5.441%
52	9.525	1380	1384	1395	rVB2	8304	14074	0.56%	0.108%
53	9.598	1395	1396	1399	rBV2	505	338	0.01%	0.003%
54	9.683	1408	1410	1414	rVB3	399	544	0.02%	0.004%
55	9.726	1414	1417	1420	rBV	396	552	0.02%	0.004%
56	9.756	1420	1422	1423	rBV	307	259	0.01%	0.002%
57	9.945	1452	1453	1456	rBV	377	284	0.01%	0.002%
58	10.055	1465	1471	1484	rBV	675013	880156	34.86%	6.724%
59	10.244	1500	1502	1505	rVB3	387	378	0.01%	0.003%
60	10.311	1508	1513	1516	rVB3	1468	2305	0.09%	0.018%
61	10.744	1581	1584	1585	rBV2	403	345	0.01%	0.003%
62	10.970	1618	1621	1626	rBV3	738	829	0.03%	0.006%
63	11.043	1630	1633	1634	rBV	503	377	0.01%	0.003%
64	11.073	1636	1638	1639	rBV	330	267	0.01%	0.002%
65	11.122	1642	1646	1652	rVB	4097	5101	0.20%	0.039%
66	11.195	1652	1658	1667	rBV	518966	659633	26.13%	5.040%
67	11.378	1686	1688	1689	rBV	411	299	0.01%	0.002%
68	11.482	1698	1705	1707	rBV5	1572	3112	0.12%	0.024%
69	11.549	1713	1716	1719	rVB2	875	779	0.03%	0.006%
70	11.628	1726	1729	1732	rBV4	517	727	0.03%	0.006%
71	11.713	1740	1743	1744	rBV	701	771	0.03%	0.006%
72	11.756	1746	1750	1754	rVB3	4062	5825	0.23%	0.045%
73	11.841	1762	1764	1768	rBV2	424	595	0.02%	0.005%
74	11.933	1775	1779	1783	rBV2	5878	7181	0.28%	0.055%
75	12.024	1789	1794	1805	rBV	688016	859055	34.03%	6.563%
76	12.152	1813	1815	1821	rVB3	2969	3414	0.14%	0.026%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029477.D
 Acq On : 14 Jun 2022 20:00
 Operator : JC/MD
 Sample : N3313-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YB7L4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.219	1823	1826	1830	rVB3	1498	2055	0.08%	0.016%
78	12.323	1836	1843	1852	rBV	752718	943109	37.36%	7.205%
79	12.427	1857	1860	1865	rVV5	1605	2340	0.09%	0.018%
80	12.475	1867	1868	1873	rVB5	934	1213	0.05%	0.009%
81	12.518	1873	1875	1877	rBV3	326	282	0.01%	0.002%
82	12.597	1886	1888	1891	rVB2	475	474	0.02%	0.004%
83	12.628	1891	1893	1895	rBV	451	514	0.02%	0.004%
84	12.664	1895	1899	1901	rVB3	693	939	0.04%	0.007%
85	12.860	1926	1931	1938	rBV	7973	10733	0.43%	0.082%
86	13.109	1970	1972	1977	rBV3	627	727	0.03%	0.006%
87	13.426	2022	2024	2027	rVB2	288	260	0.01%	0.002%
88	13.591	2048	2051	2056	rBV2	509	841	0.03%	0.006%
89	13.689	2064	2067	2070	rBV3	1104	1309	0.05%	0.010%
90	13.853	2091	2094	2097	rBV3	402	525	0.02%	0.004%
91	13.914	2102	2104	2105	rBV	278	286	0.01%	0.002%
92	13.957	2110	2111	2115	rVB3	462	469	0.02%	0.004%
93	14.262	2159	2161	2163	rVB	412	307	0.01%	0.002%
94	14.445	2189	2191	2192	rBV	442	342	0.01%	0.003%
95	15.255	2322	2324	2328	rBV2	476	602	0.02%	0.005%
96	15.390	2345	2346	2348	rBV2	572	309	0.01%	0.002%
97	15.664	2389	2391	2394	rBV3	551	526	0.02%	0.004%
98	16.115	2464	2465	2468	rBV3	468	415	0.02%	0.003%
99	16.237	2484	2485	2486	rBV	603	305	0.01%	0.002%
100	16.438	2515	2518	2519	rBV2	640	717	0.03%	0.005%




Sum of corrected areas: 13088905

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029477.D
Acq On : 14 Jun 2022 20:00
Operator : JC/MD
Sample : N3313-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YB7L4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

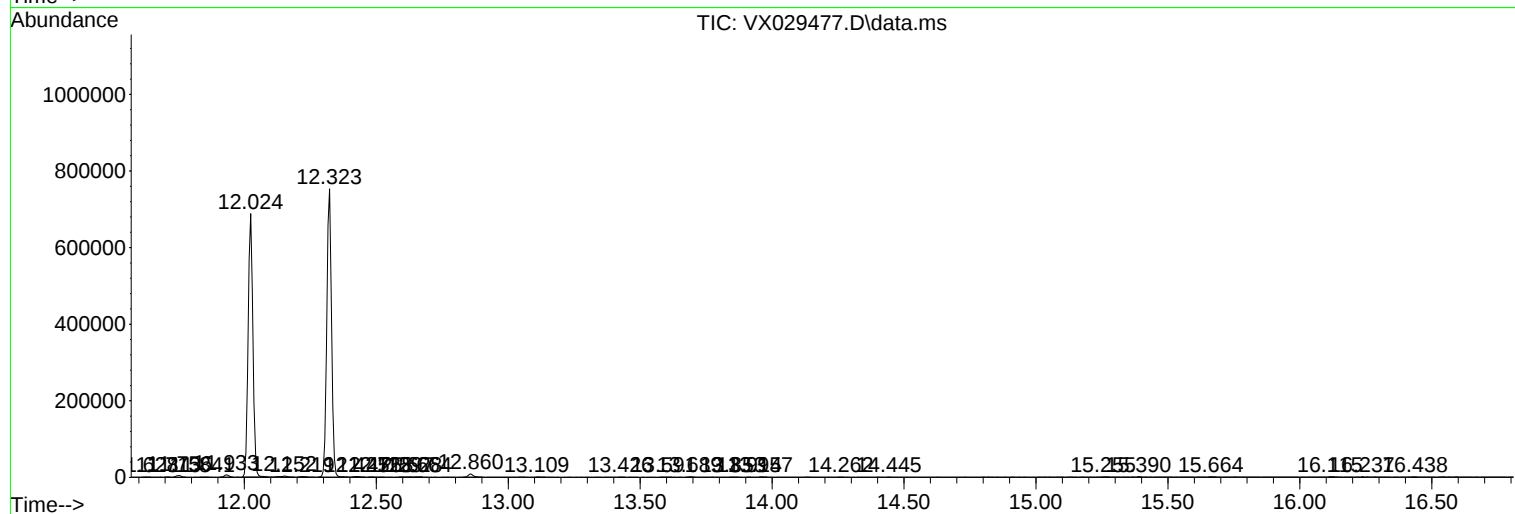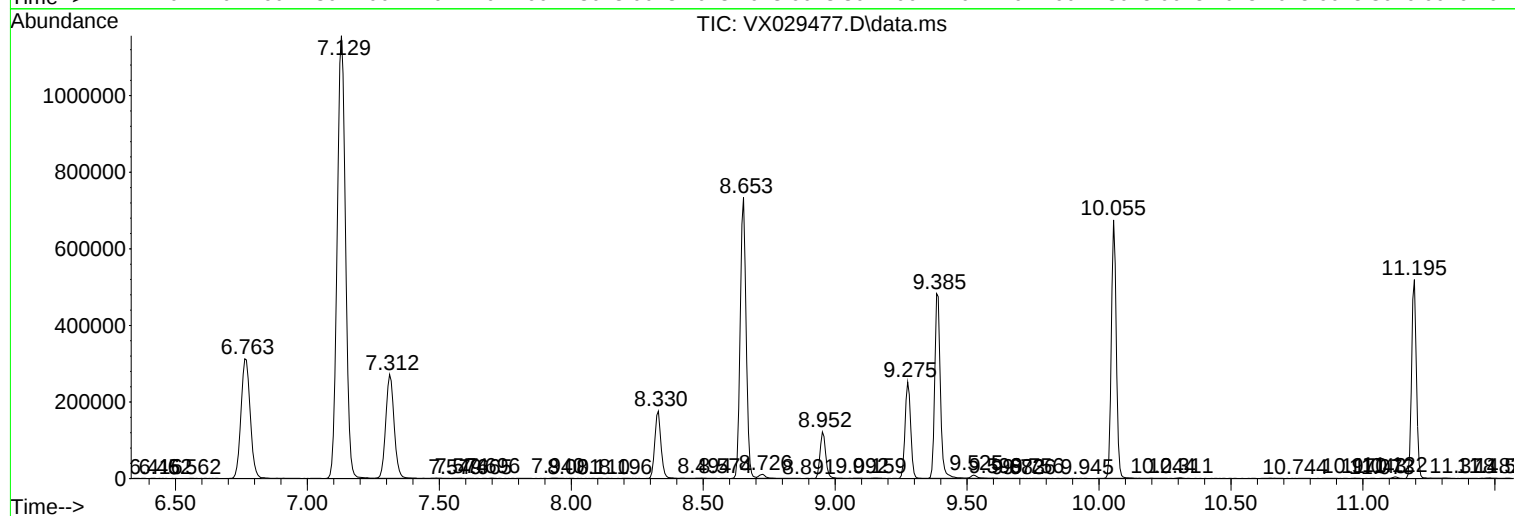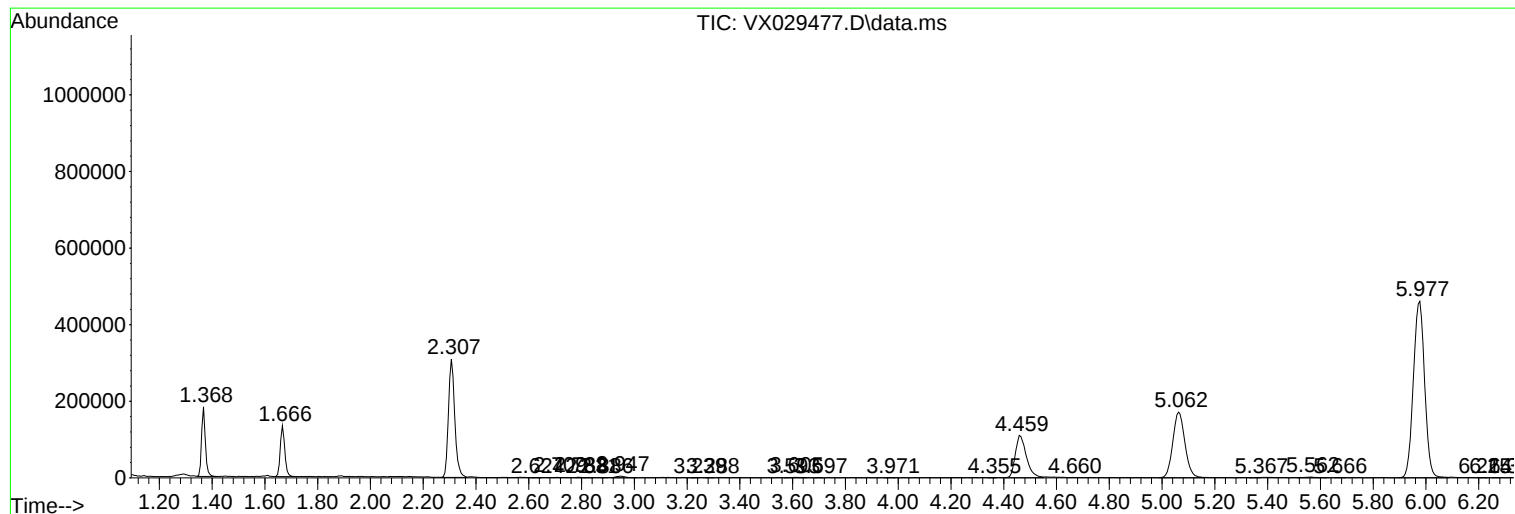

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029477.D
Acq On : 14 Jun 2022 20:00
Operator : JC/MD
Sample : N3313-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YB7L4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029477.D
Acq On : 14 Jun 2022 20:00
Operator : JC/MD
Sample : N3313-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YB7L4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc