

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029479.D
 Acq On : 14 Jun 2022 20:47
 Operator : JC/MD
 Sample : N3313-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YB7L6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029479.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	58	rVB	175644	179907	6.32%	1.359%
2	1.666	91	95	103	rVB	132698	157962	5.55%	1.194%
3	2.306	193	200	211	rBV2	303693	501433	17.61%	3.789%
4	2.465	225	226	227	rBV	536	287	0.01%	0.002%
5	2.782	275	278	287	rVB5	670	1458	0.05%	0.011%
6	2.898	296	297	299	rBV	430	293	0.01%	0.002%
7	2.940	299	304	314	rVV2	3230	7521	0.26%	0.057%
8	3.038	318	320	323	rVB2	464	399	0.01%	0.003%
9	3.081	323	327	328	rBV2	474	383	0.01%	0.003%
10	3.099	328	330	335	rBV2	590	982	0.03%	0.007%
11	3.581	405	409	410	rBV2	387	400	0.01%	0.003%
12	3.611	410	414	421	rVB4	839	1742	0.06%	0.013%
13	3.891	457	460	463	rBV	354	381	0.01%	0.003%
14	3.946	465	469	470	rBV2	329	475	0.02%	0.004%
15	4.148	500	502	508	rBV2	479	451	0.02%	0.003%
16	4.465	544	554	568	rBV	107729	316341	11.11%	2.390%
17	4.806	609	610	612	rVB	413	265	0.01%	0.002%
18	4.910	624	627	629	rBV3	422	474	0.02%	0.004%
19	5.062	639	652	674	rBV2	172468	539532	18.94%	4.077%
20	5.550	729	732	733	rBV2	846	846	0.03%	0.006%
21	5.684	751	754	759	rBV3	372	684	0.02%	0.005%
22	5.970	788	801	817	rBV2	453042	1335102	46.88%	10.089%
23	6.763	922	931	948	rBV	311778	733366	25.75%	5.542%
24	7.129	981	991	1013	rVV	1313590	2848099	100.00%	21.521%
25	7.312	1013	1021	1035	rVB	265633	583665	20.49%	4.410%
26	7.482	1045	1049	1052	rBV6	798	1109	0.04%	0.008%
27	7.696	1081	1084	1086	rVV3	605	754	0.03%	0.006%
28	7.720	1086	1088	1090	rVB3	460	313	0.01%	0.002%
29	7.818	1101	1104	1106	rBV2	561	653	0.02%	0.005%
30	7.940	1121	1124	1128	rVV2	790	1029	0.04%	0.008%
31	8.031	1137	1139	1142	rBV2	282	330	0.01%	0.002%
32	8.232	1170	1172	1174	rVB2	322	266	0.01%	0.002%
33	8.269	1174	1178	1180	rVB2	282	386	0.01%	0.003%
34	8.330	1180	1188	1204	rBV	169899	281620	9.89%	2.128%
35	8.488	1212	1214	1218	rBV4	680	1081	0.04%	0.008%
36	8.653	1234	1241	1249	rBV	712361	1115862	39.18%	8.432%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029479.D
 Acq On : 14 Jun 2022 20:47
 Operator : JC/MD
 Sample : N3313-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YB7L6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	8.720	1249	1252	1260	rVV	9924	17413	0.61%	0.132%
38	8.848	1270	1273	1277	rBV4	334	632	0.02%	0.005%
39	8.952	1284	1290	1299	rBV	118740	172804	6.07%	1.306%
40	9.159	1321	1324	1329	rVV2	582	834	0.03%	0.006%
41	9.275	1337	1343	1353	rVB	265633	378900	13.30%	2.863%
42	9.384	1356	1361	1379	rBV	470990	693578	24.35%	5.241%
43	9.525	1380	1384	1391	rVB3	9720	14429	0.51%	0.109%
44	9.823	1431	1433	1437	rVB2	318	389	0.01%	0.003%
45	9.884	1442	1443	1446	rVV	377	275	0.01%	0.002%
46	10.055	1465	1471	1487	rBV	644265	858512	30.14%	6.487%
47	10.195	1491	1494	1501	rVB4	872	1423	0.05%	0.011%
48	10.250	1501	1503	1507	rVB2	485	470	0.02%	0.004%
49	10.305	1507	1512	1516	rBV3	1997	2710	0.10%	0.020%
50	10.537	1547	1550	1553	rBV2	225	356	0.01%	0.003%
51	10.646	1566	1568	1573	rVV4	889	976	0.03%	0.007%
52	10.762	1584	1587	1589	rVB2	362	376	0.01%	0.003%
53	10.860	1601	1603	1608	rVB2	661	850	0.03%	0.006%
54	11.030	1626	1631	1633	rBV3	333	477	0.02%	0.004%
55	11.055	1633	1635	1638	rBV2	316	297	0.01%	0.002%
56	11.122	1642	1646	1652	rVB2	3859	4873	0.17%	0.037%
57	11.195	1652	1658	1668	rBV	508818	645540	22.67%	4.878%
58	11.305	1673	1676	1679	rBV4	879	1130	0.04%	0.009%
59	11.390	1688	1690	1691	rBV	609	361	0.01%	0.003%
60	11.457	1698	1701	1702	rBV2	625	718	0.03%	0.005%
61	11.506	1708	1709	1711	rVB	871	456	0.02%	0.003%
62	11.549	1714	1716	1717	rVV3	405	333	0.01%	0.003%
63	11.591	1719	1723	1725	rBV2	357	517	0.02%	0.004%
64	11.683	1735	1738	1740	rBV3	722	695	0.02%	0.005%
65	11.750	1745	1749	1757	rVB2	3805	5877	0.21%	0.044%
66	11.933	1775	1779	1784	rBV2	6571	8517	0.30%	0.064%
67	11.975	1784	1786	1788	rVB2	996	808	0.03%	0.006%
68	12.024	1788	1794	1805	rBV	706826	851230	29.89%	6.432%
69	12.219	1822	1826	1833	rBV5	2506	4079	0.14%	0.031%
70	12.323	1837	1843	1851	rVV	745281	917416	32.21%	6.932%
71	12.475	1863	1868	1872	rVB4	928	1513	0.05%	0.011%
72	12.530	1872	1877	1880	rBV4	439	616	0.02%	0.005%
73	12.573	1882	1884	1885	rBV2	444	386	0.01%	0.003%
74	12.603	1887	1889	1891	rVB	780	517	0.02%	0.004%
75	12.664	1897	1899	1903	rBV2	921	882	0.03%	0.007%
76	12.762	1913	1915	1917	rBV2	405	448	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029479.D
 Acq On : 14 Jun 2022 20:47
 Operator : JC/MD
 Sample : N3313-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YB7L6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.859	1926	1931	1938	rVB2	10320	13171	0.46%	0.100%
78	12.963	1945	1948	1951	rBV2	363	445	0.02%	0.003%
79	13.054	1961	1963	1966	rVB4	938	984	0.03%	0.007%
80	13.085	1966	1968	1970	rVB2	497	367	0.01%	0.003%
81	13.115	1970	1973	1976	rBV3	770	796	0.03%	0.006%
82	13.439	2024	2026	2030	rBV2	324	374	0.01%	0.003%
83	13.628	2053	2057	2059	rBV2	251	393	0.01%	0.003%
84	13.695	2064	2068	2073	rBV4	1532	1913	0.07%	0.014%
85	13.786	2081	2083	2089	rVB4	579	754	0.03%	0.006%
86	13.835	2089	2091	2094	rVB	367	371	0.01%	0.003%
87	13.865	2094	2096	2098	rBV2	614	414	0.01%	0.003%
88	14.030	2121	2123	2125	rBV2	275	278	0.01%	0.002%
89	14.073	2129	2130	2134	rBV2	407	594	0.02%	0.004%
90	14.134	2137	2140	2143	rVV3	525	682	0.02%	0.005%
91	14.213	2151	2153	2155	rBV	338	457	0.02%	0.003%
92	14.451	2189	2192	2193	rBV2	292	268	0.01%	0.002%
93	14.621	2217	2220	2221	rBV2	304	326	0.01%	0.002%
94	14.963	2274	2276	2278	rBV	525	324	0.01%	0.002%
95	14.987	2278	2280	2282	rBV2	446	311	0.01%	0.002%
96	15.152	2305	2307	2308	rBV	600	565	0.02%	0.004%
97	15.194	2312	2314	2316	rBV	543	398	0.01%	0.003%
98	15.700	2395	2397	2399	rBV3	605	411	0.01%	0.003%
99	15.737	2401	2403	2404	rBV	582	359	0.01%	0.003%
100	16.078	2458	2459	2461	rVB2	768	357	0.01%	0.003%




Sum of corrected areas: 13233776

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029479.D
Acq On : 14 Jun 2022 20:47
Operator : JC/MD
Sample : N3313-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YB7L6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

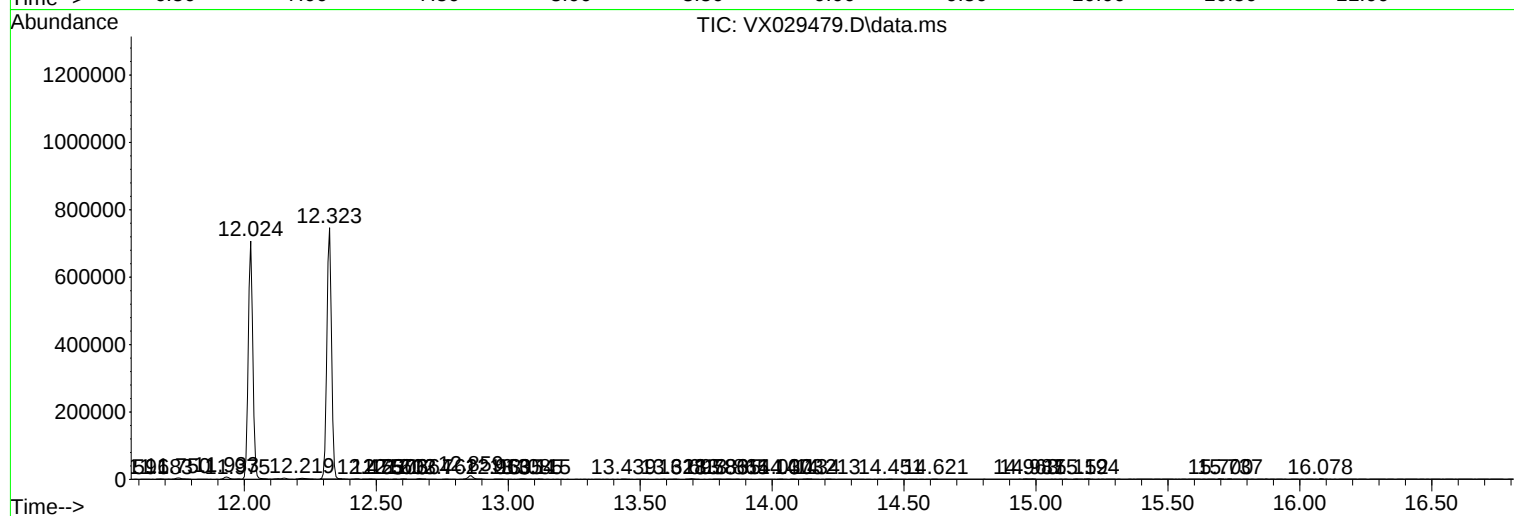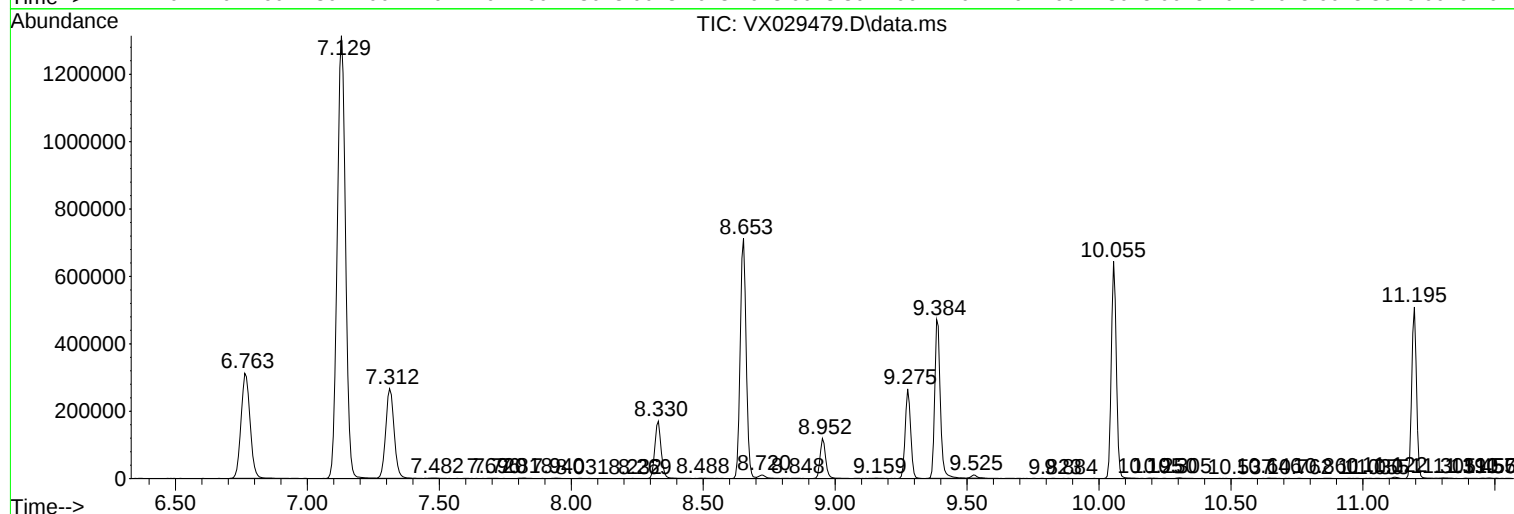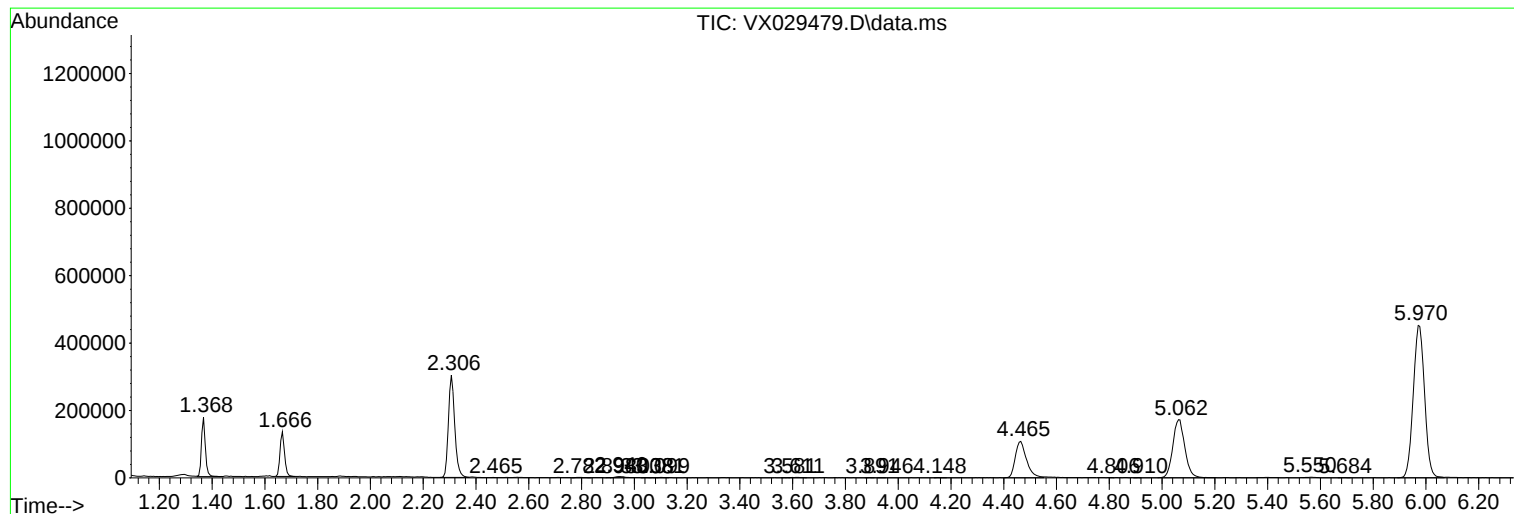

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029479.D
Acq On : 14 Jun 2022 20:47
Operator : JC/MD
Sample : N3313-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YB7L6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029479.D
Acq On : 14 Jun 2022 20:47
Operator : JC/MD
Sample : N3313-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YB7L6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
