

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029482.D
 Acq On : 14 Jun 2022 21:56
 Operator : JC/MD
 Sample : VX0614WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK662

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029482.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	57	rVB	193634	194516	14.04%	1.839%
2	1.666	91	95	101	rVB	139711	159976	11.54%	1.512%
3	2.306	193	200	211	rBV	309844	492068	35.51%	4.652%
4	2.501	230	232	233	rBV2	723	586	0.04%	0.006%
5	2.648	254	256	257	rBV	374	293	0.02%	0.003%
6	2.794	276	280	284	rVB5	1555	2600	0.19%	0.025%
7	2.867	291	292	295	rVB	270	220	0.02%	0.002%
8	2.946	295	305	314	rBV2	22886	52797	3.81%	0.499%
9	3.062	321	324	325	rBV2	292	265	0.02%	0.003%
10	3.099	326	330	335	rVV3	658	986	0.07%	0.009%
11	3.379	375	376	378	rBV	239	245	0.02%	0.002%
12	3.520	396	399	401	rVB3	187	224	0.02%	0.002%
13	3.568	404	407	409	rBV2	276	325	0.02%	0.003%
14	3.611	412	414	416	rBV2	327	302	0.02%	0.003%
15	3.751	435	437	441	rVB2	278	218	0.02%	0.002%
16	4.306	527	528	531	rVB2	525	334	0.02%	0.003%
17	4.385	539	541	543	rBV2	259	289	0.02%	0.003%
18	4.464	545	554	568	rBV	114721	332612	24.00%	3.144%
19	4.739	597	599	602	rVB2	420	347	0.03%	0.003%
20	5.062	640	652	671	rBV	177848	545176	39.34%	5.154%
21	5.227	676	679	680	rBV2	306	284	0.02%	0.003%
22	5.385	702	705	711	rBV4	636	1108	0.08%	0.010%
23	5.464	716	718	720	rBV2	508	497	0.04%	0.005%
24	5.483	720	721	724	rVB3	590	405	0.03%	0.004%
25	5.544	728	731	735	rBV4	787	1127	0.08%	0.011%
26	5.678	751	753	757	rVB2	378	352	0.03%	0.003%
27	5.757	762	766	767	rBV	292	371	0.03%	0.004%
28	5.861	779	783	784	rBV2	253	309	0.02%	0.003%
29	5.976	789	802	818	rBV2	475064	1385850	100.00%	13.102%
30	6.220	838	842	843	rVB2	326	317	0.02%	0.003%
31	6.348	860	863	865	rBV	360	398	0.03%	0.004%
32	6.409	870	873	874	rBV	232	244	0.02%	0.002%
33	6.464	879	882	885	rBV3	486	678	0.05%	0.006%
34	6.537	892	894	898	rBV3	393	611	0.04%	0.006%
35	6.684	914	918	919	rVB2	281	266	0.02%	0.003%
36	6.763	922	931	952	rBV	328613	791407	57.11%	7.482%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029482.D
 Acq On : 14 Jun 2022 21:56
 Operator : JC/MD
 Sample : VX0614WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK662

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	6.897	952	953	957	rVB2	520	302	0.02%	0.003%
38	7.013	971	972	974	rVB2	450	265	0.02%	0.003%
39	7.129	982	991	1000	rVV3	39721	92176	6.65%	0.871%
40	7.312	1012	1021	1037	rBV	273856	605101	43.66%	5.721%
41	7.610	1068	1070	1073	rVB	264	264	0.02%	0.002%
42	7.696	1082	1084	1089	rVB2	484	556	0.04%	0.005%
43	7.738	1089	1091	1093	rBV	391	420	0.03%	0.004%
44	7.818	1100	1104	1108	rVB2	534	971	0.07%	0.009%
45	7.946	1120	1125	1127	rVV4	962	1211	0.09%	0.011%
46	8.135	1155	1156	1161	rBV2	237	256	0.02%	0.002%
47	8.330	1181	1188	1200	rVV	171584	287502	20.75%	2.718%
48	8.494	1213	1215	1220	rVB4	621	688	0.05%	0.007%
49	8.586	1228	1230	1233	rVB	821	542	0.04%	0.005%
50	8.653	1233	1241	1248	rBV	750550	1159695	83.68%	10.964%
51	8.726	1249	1253	1257	rVB2	9456	16093	1.16%	0.152%
52	8.951	1284	1290	1302	rBV	120598	180649	13.04%	1.708%
53	9.122	1316	1318	1321	rVB2	314	248	0.02%	0.002%
54	9.275	1340	1343	1348	rVB4	3273	4896	0.35%	0.046%
55	9.384	1356	1361	1383	rVV	492609	736843	53.17%	6.966%
56	9.653	1403	1405	1407	rVB2	470	277	0.02%	0.003%
57	9.677	1407	1409	1410	rBV2	323	219	0.02%	0.002%
58	9.707	1410	1414	1417	rBV3	1559	2013	0.15%	0.019%
59	9.872	1440	1441	1444	rBV2	596	306	0.02%	0.003%
60	10.055	1465	1471	1479	rBV	682346	926530	66.86%	8.759%
61	10.201	1492	1495	1498	rVB	1027	1136	0.08%	0.011%
62	10.305	1509	1512	1518	rVB3	2166	3520	0.25%	0.033%
63	10.433	1531	1533	1537	rBV2	214	353	0.03%	0.003%
64	10.518	1545	1547	1549	rBV	276	234	0.02%	0.002%
65	10.573	1554	1556	1559	rVB3	339	398	0.03%	0.004%
66	10.604	1559	1561	1564	rBV	412	433	0.03%	0.004%
67	10.640	1564	1567	1568	rBV2	1254	1097	0.08%	0.010%
68	10.768	1582	1588	1590	rVV2	311	618	0.04%	0.006%
69	10.805	1592	1594	1596	rVB2	328	244	0.02%	0.002%
70	10.963	1617	1620	1625	rBV3	1093	1295	0.09%	0.012%
71	11.122	1642	1646	1650	rVB3	4334	6133	0.44%	0.058%
72	11.195	1652	1658	1667	rBV	527074	670816	48.40%	6.342%
73	11.451	1697	1700	1701	rBV2	808	827	0.06%	0.008%
74	11.542	1712	1715	1720	rVB4	622	1122	0.08%	0.011%
75	11.597	1722	1724	1725	rVV	446	376	0.03%	0.004%
76	11.628	1725	1729	1730	rVV2	544	731	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029482.D
 Acq On : 14 Jun 2022 21:56
 Operator : JC/MD
 Sample : VX0614WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK662

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	11.683	1734	1738	1740	rVV	875	970	0.07%	0.009%
78	11.719	1740	1744	1746	rVV4	957	1767	0.13%	0.017%
79	11.750	1746	1749	1755	rVB2	6070	7779	0.56%	0.074%
80	11.847	1761	1765	1768	rBV2	954	1335	0.10%	0.013%
81	11.933	1776	1779	1783	rBV3	1891	2432	0.18%	0.023%
82	11.975	1783	1786	1789	rBV3	1688	2125	0.15%	0.020%
83	12.024	1789	1794	1805	rBV	737967	909507	65.63%	8.598%
84	12.122	1808	1810	1812	rBV	1004	1013	0.07%	0.010%
85	12.323	1837	1843	1851	rBV	771203	957973	69.13%	9.057%
86	12.475	1865	1868	1874	rVB4	948	1830	0.13%	0.017%
87	12.664	1896	1899	1904	rVB4	929	1256	0.09%	0.012%
88	12.878	1933	1934	1936	rBV	367	231	0.02%	0.002%
89	12.945	1941	1945	1947	rBV2	391	668	0.05%	0.006%
90	13.048	1960	1962	1967	rVB2	734	958	0.07%	0.009%
91	13.115	1970	1973	1981	rVB3	1698	1967	0.14%	0.019%
92	13.530	2037	2041	2043	rBV2	289	434	0.03%	0.004%
93	13.591	2048	2051	2056	rVB2	1959	2248	0.16%	0.021%
94	13.749	2074	2077	2079	rBV2	408	346	0.02%	0.003%
95	13.780	2079	2082	2085	rVV2	1708	2209	0.16%	0.021%
96	13.963	2109	2112	2116	rVB4	1396	1671	0.12%	0.016%
97	14.133	2136	2140	2143	rVB	1601	1893	0.14%	0.018%
98	14.432	2187	2189	2190	rBV2	450	457	0.03%	0.004%
99	14.822	2251	2253	2255	rVB	513	271	0.02%	0.003%
100	15.036	2285	2288	2289	rBV2	374	416	0.03%	0.004%




Sum of corrected areas: 10577715

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029482.D
Acq On : 14 Jun 2022 21:56
Operator : JC/MD
Sample : VX0614WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK662

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

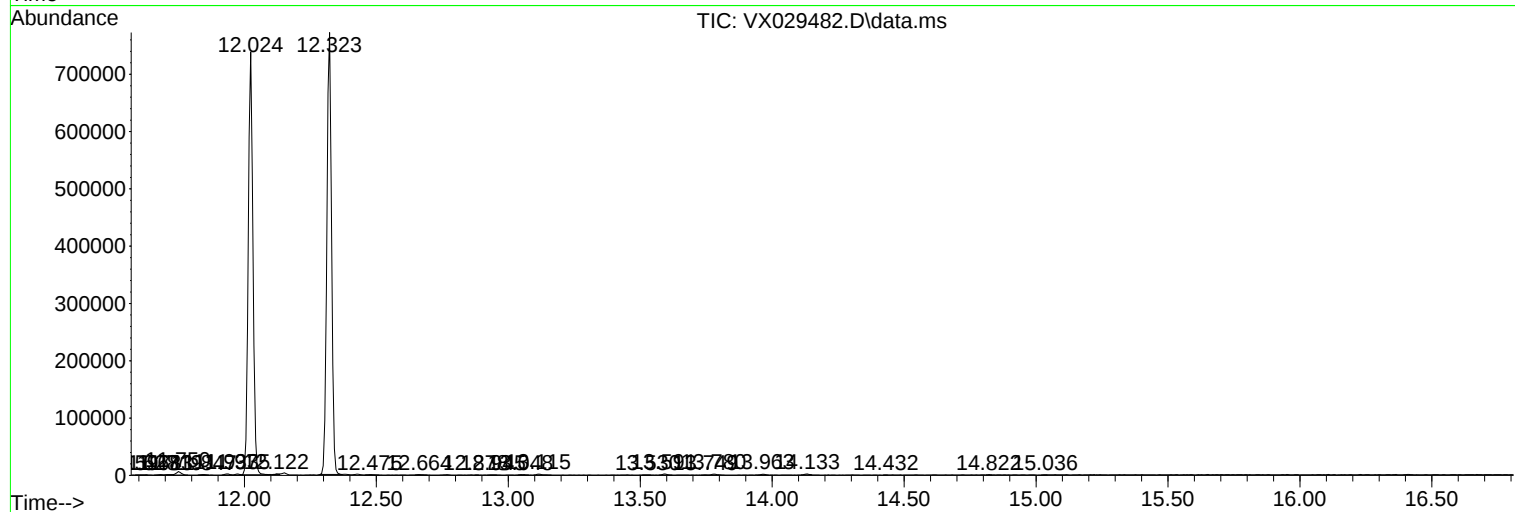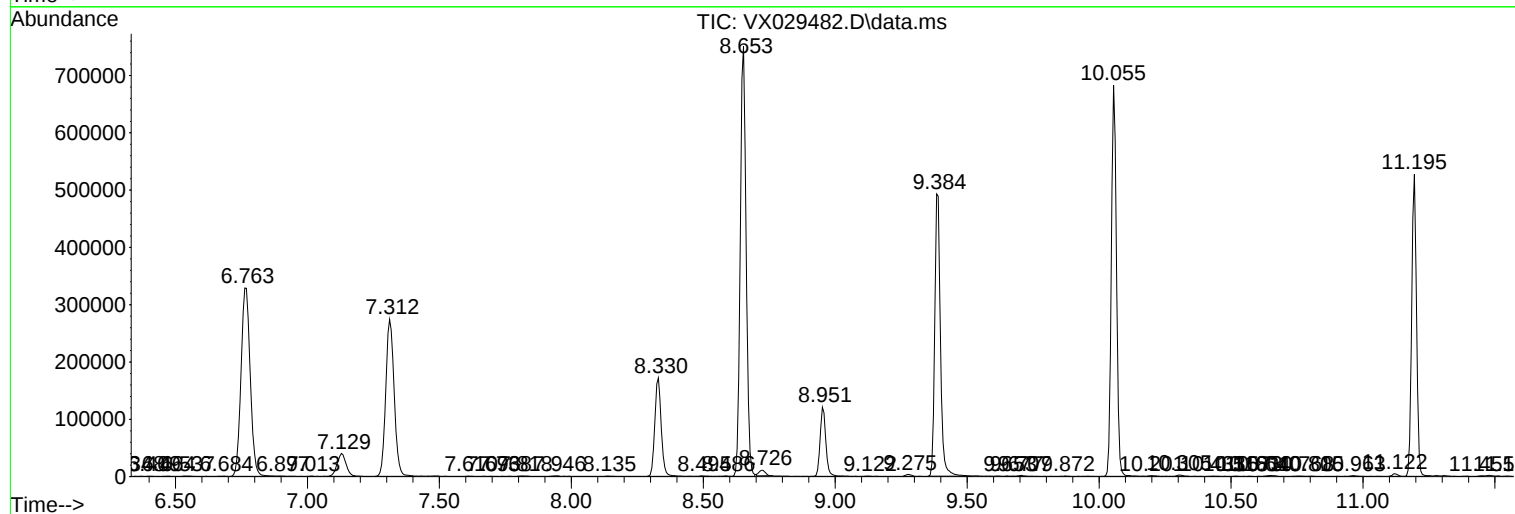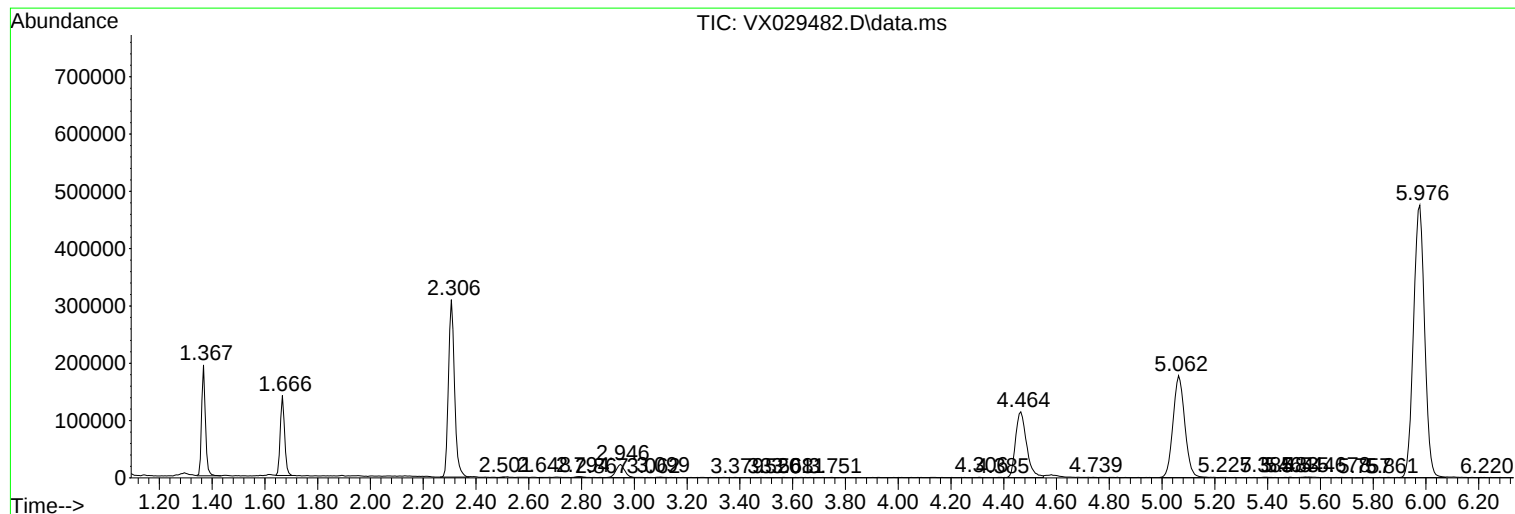

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029482.D
Acq On : 14 Jun 2022 21:56
Operator : JC/MD
Sample : VX0614WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK662

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029482.D
Acq On : 14 Jun 2022 21:56
Operator : JC/MD
Sample : VX0614WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK662

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------