

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029483.D
 Acq On : 14 Jun 2022 22:20
 Operator : JC/MD
 Sample : VX0614MBL02
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK663

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029483.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	176768	179157	13.40%	1.753%
2	1.453	57	60	63	rBV	11324	12118	0.91%	0.119%
3	1.666	91	95	106	rVB	130422	156390	11.70%	1.530%
4	2.306	194	200	210	rBV	290736	464577	34.75%	4.547%
5	2.386	210	213	223	rVB	6299	10983	0.82%	0.107%
6	2.514	230	234	237	rBV	881	1423	0.11%	0.014%
7	2.575	237	244	247	rBV4	1131	2741	0.21%	0.027%
8	2.715	263	267	273	rVB5	812	1120	0.08%	0.011%
9	2.947	297	305	316	rVB	8651	19609	1.47%	0.192%
10	3.069	323	325	327	rBV2	257	262	0.02%	0.003%
11	3.422	381	383	388	rBV3	346	652	0.05%	0.006%
12	3.477	390	392	394	rBV	410	370	0.03%	0.004%
13	3.672	421	424	427	rBV2	269	363	0.03%	0.004%
14	3.837	448	451	453	rBV2	300	421	0.03%	0.004%
15	3.946	466	469	474	rVB2	357	560	0.04%	0.005%
16	4.068	486	489	490	rBV	262	214	0.02%	0.002%
17	4.459	544	553	567	rBV	107078	313558	23.45%	3.069%
18	4.800	607	609	611	rBV2	361	207	0.02%	0.002%
19	4.824	611	613	615	rBV2	343	252	0.02%	0.002%
20	4.904	625	626	629	rBV	459	366	0.03%	0.004%
21	5.062	639	652	668	rBV	171812	527599	39.46%	5.163%
22	5.330	693	696	697	rVB	251	197	0.01%	0.002%
23	5.532	727	729	730	rBV	404	365	0.03%	0.004%
24	5.617	741	743	744	rVB	357	205	0.02%	0.002%
25	5.635	744	746	747	rBV	276	235	0.02%	0.002%
26	5.861	781	783	784	rBV	352	190	0.01%	0.002%
27	5.977	789	802	819	rVV2	449916	1336921	100.00%	13.084%
28	6.397	869	871	873	rVB2	276	235	0.02%	0.002%
29	6.422	873	875	878	rBV	284	312	0.02%	0.003%
30	6.537	893	894	901	rBV2	350	575	0.04%	0.006%
31	6.763	922	931	947	rVV	328172	785934	58.79%	7.691%
32	6.952	961	962	965	rBV2	315	322	0.02%	0.003%
33	7.037	975	976	980	rBV3	224	203	0.02%	0.002%
34	7.129	983	991	1003	rVB4	35900	83906	6.28%	0.821%
35	7.245	1008	1010	1012	rBV2	423	354	0.03%	0.003%
36	7.312	1012	1021	1037	rBV	271798	584384	43.71%	5.719%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029483.D
 Acq On : 14 Jun 2022 22:20
 Operator : JC/MD
 Sample : VX0614MBL02
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK663

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.488	1045	1050	1053	rVB3	762	1198	0.09%	0.012%
38	7.940	1120	1124	1126	rBV3	517	750	0.06%	0.007%
39	7.958	1126	1127	1130	rVB3	594	483	0.04%	0.005%
40	8.147	1157	1158	1161	rBV	187	244	0.02%	0.002%
41	8.214	1165	1169	1173	rVB3	414	644	0.05%	0.006%
42	8.330	1181	1188	1197	rBV	163423	274348	20.52%	2.685%
43	8.586	1227	1230	1233	rVB2	409	481	0.04%	0.005%
44	8.653	1233	1241	1248	rBV	732511	1118818	83.69%	10.949%
45	8.726	1249	1253	1258	rVB	9634	15841	1.18%	0.155%
46	8.952	1285	1290	1301	rBV	119416	171701	12.84%	1.680%
47	9.110	1312	1316	1318	rVB3	364	388	0.03%	0.004%
48	9.226	1334	1335	1337	rBV2	283	193	0.01%	0.002%
49	9.281	1339	1344	1353	rVB5	3562	5853	0.44%	0.057%
50	9.384	1356	1361	1380	rBV	465987	709106	53.04%	6.940%
51	9.628	1399	1401	1403	rBV2	286	227	0.02%	0.002%
52	9.744	1414	1420	1422	rBV3	316	537	0.04%	0.005%
53	9.762	1422	1423	1426	rVB	377	218	0.02%	0.002%
54	9.890	1442	1444	1445	rBV	277	226	0.02%	0.002%
55	10.055	1465	1471	1485	rBV	684233	917154	68.60%	8.976%
56	10.305	1509	1512	1519	rVB2	2476	3175	0.24%	0.031%
57	10.427	1530	1532	1533	rBV2	300	197	0.01%	0.002%
58	10.659	1564	1570	1579	rVB5	1035	2193	0.16%	0.021%
59	10.738	1581	1583	1584	rBV5	362	305	0.02%	0.003%
60	10.793	1590	1592	1594	rBV2	268	229	0.02%	0.002%
61	10.872	1603	1605	1608	rBV2	228	262	0.02%	0.003%
62	10.970	1617	1621	1625	rBV3	762	1138	0.09%	0.011%
63	11.031	1630	1631	1634	rVV	239	219	0.02%	0.002%
64	11.122	1642	1646	1650	rVB2	4831	5730	0.43%	0.056%
65	11.195	1652	1658	1666	rBV	517678	647517	48.43%	6.337%
66	11.409	1691	1693	1695	rBV3	372	400	0.03%	0.004%
67	11.476	1697	1704	1708	rBV5	1364	2884	0.22%	0.028%
68	11.549	1714	1716	1724	rVB3	478	725	0.05%	0.007%
69	11.610	1724	1726	1729	rBV	239	312	0.02%	0.003%
70	11.634	1729	1730	1733	rVB	383	312	0.02%	0.003%
71	11.671	1733	1736	1737	rBV	462	443	0.03%	0.004%
72	11.756	1745	1750	1754	rVB3	3866	5259	0.39%	0.051%
73	11.841	1761	1764	1768	rVB4	603	849	0.06%	0.008%
74	11.933	1774	1779	1783	rBV2	2020	2830	0.21%	0.028%
75	11.969	1783	1785	1789	rVV3	908	1262	0.09%	0.012%
76	12.024	1789	1794	1806	rVB	729844	894041	66.87%	8.749%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029483.D
 Acq On : 14 Jun 2022 22:20
 Operator : JC/MD
 Sample : VX0614MBL02
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK663

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.152	1813	1815	1818	rVB2	3514	3041	0.23%	0.030%
78	12.219	1822	1826	1832	rBV	3601	5241	0.39%	0.051%
79	12.323	1835	1843	1851	rBV	741052	921985	68.96%	9.023%
80	12.469	1865	1867	1868	rBV	542	385	0.03%	0.004%
81	12.591	1885	1887	1889	rVB2	386	333	0.02%	0.003%
82	12.664	1896	1899	1903	rVB2	709	807	0.06%	0.008%
83	12.817	1922	1924	1926	rVB	638	283	0.02%	0.003%
84	12.896	1934	1937	1940	rBV2	337	421	0.03%	0.004%
85	12.957	1944	1947	1948	rBV	185	240	0.02%	0.002%
86	13.116	1970	1973	1977	rVB5	1034	1292	0.10%	0.013%
87	13.298	2002	2003	2005	rVB	369	187	0.01%	0.002%
88	13.445	2026	2027	2030	rVB2	431	380	0.03%	0.004%
89	13.481	2030	2033	2035	rBV2	317	338	0.03%	0.003%
90	13.591	2047	2051	2054	rBV3	1050	1305	0.10%	0.013%
91	13.731	2072	2074	2075	rVB2	267	185	0.01%	0.002%
92	13.750	2075	2077	2078	rBV	370	356	0.03%	0.003%
93	13.780	2080	2082	2089	rVB3	935	1316	0.10%	0.013%
94	13.835	2089	2091	2095	rBV2	283	349	0.03%	0.003%
95	13.963	2109	2112	2115	rBV2	988	1161	0.09%	0.011%
96	13.993	2115	2117	2120	rBV2	412	294	0.02%	0.003%
97	14.085	2130	2132	2133	rVB2	377	204	0.02%	0.002%
98	14.134	2134	2140	2144	rVB4	581	1044	0.08%	0.010%
99	15.457	2354	2357	2360	rBV4	531	830	0.06%	0.008%
100	16.042	2452	2453	2455	rBV	599	351	0.03%	0.003%


Sum of corrected areas: 10218300

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029483.D
Acq On : 14 Jun 2022 22:20
Operator : JC/MD
Sample : VX0614MBL02
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK663

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

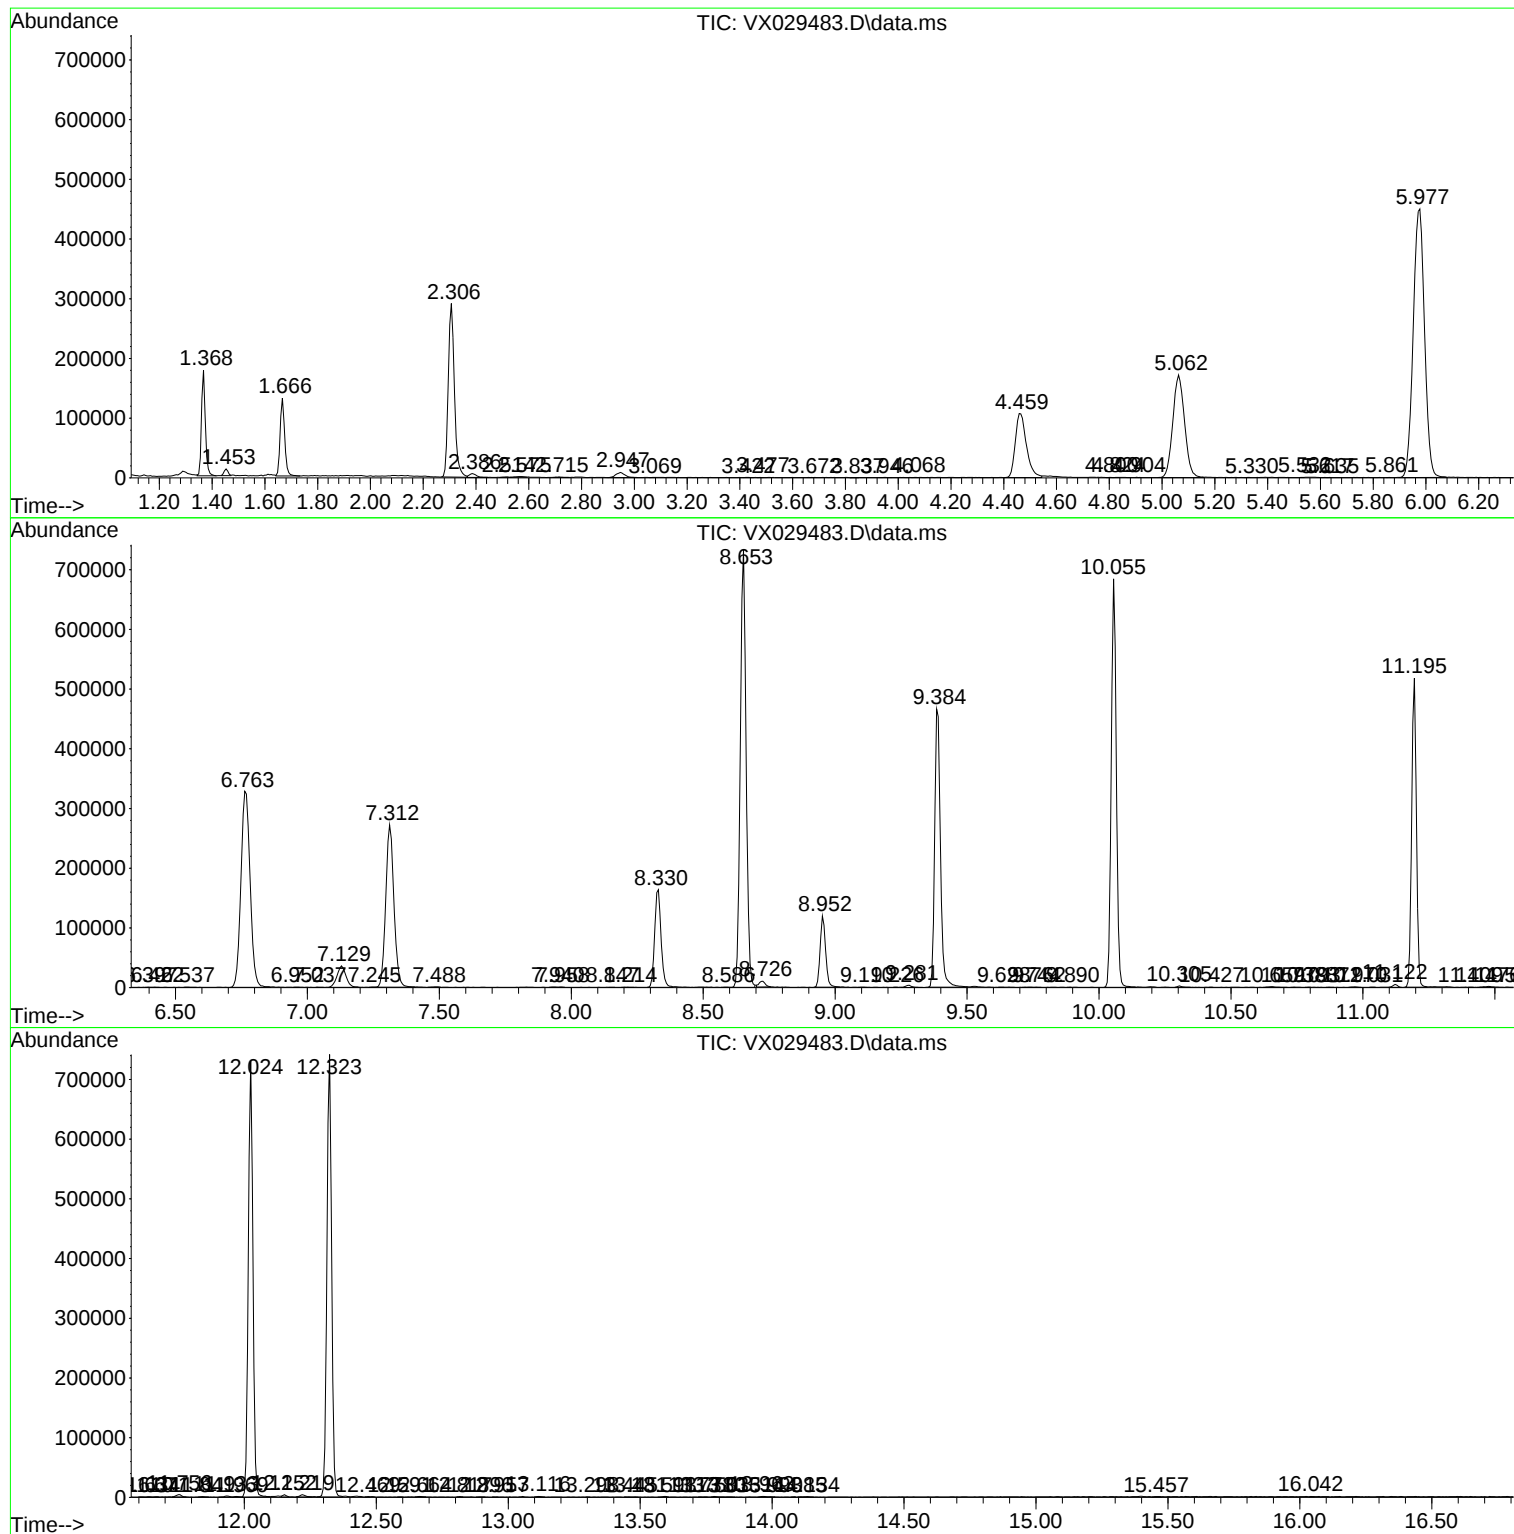

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029483.D
Acq On : 14 Jun 2022 22:20
Operator : JC/MD
Sample : VX0614MBL02
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK663

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029483.D
Acq On : 14 Jun 2022 22:20
Operator : JC/MD
Sample : VX0614MBL02
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK663

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc