

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029484.D
 Acq On : 14 Jun 2022 22:43
 Operator : JC/MD
 Sample : N3313-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YB7N2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029484.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB	180979	182625	13.69%	1.793%
2	1.453	57	60	66	rVV	10627	11609	0.87%	0.114%
3	1.666	91	95	101	rVB	130815	149328	11.20%	1.466%
4	2.307	194	200	210	rBV	295149	465927	34.94%	4.575%
5	2.392	210	214	220	rVB	5879	9716	0.73%	0.095%
6	2.477	226	228	229	rBV	642	292	0.02%	0.003%
7	2.947	297	305	315	rBV2	7150	16625	1.25%	0.163%
8	3.252	353	355	358	rVB2	414	403	0.03%	0.004%
9	3.380	374	376	379	rBV2	231	319	0.02%	0.003%
10	3.422	381	383	385	rBV	287	266	0.02%	0.003%
11	3.471	389	391	394	rVV3	276	301	0.02%	0.003%
12	3.672	422	424	426	rBV	302	290	0.02%	0.003%
13	3.953	468	470	472	rBV	387	276	0.02%	0.003%
14	4.007	478	479	483	rBV2	259	338	0.03%	0.003%
15	4.135	495	500	502	rBV2	366	605	0.05%	0.006%
16	4.251	516	519	523	rBV	281	365	0.03%	0.004%
17	4.318	527	530	532	rVB	321	342	0.03%	0.003%
18	4.355	534	536	539	rBV2	340	290	0.02%	0.003%
19	4.465	543	554	568	rBV	110470	322290	24.17%	3.165%
20	4.727	596	597	599	rBV	416	291	0.02%	0.003%
21	5.062	640	652	668	rBV2	170319	528816	39.65%	5.193%
22	5.330	694	696	699	rBV2	362	296	0.02%	0.003%
23	5.538	726	730	731	rBV3	364	461	0.03%	0.005%
24	5.562	731	734	738	rVB3	706	978	0.07%	0.010%
25	5.727	760	761	765	rBV2	340	411	0.03%	0.004%
26	5.830	776	778	781	rBV	290	340	0.03%	0.003%
27	5.977	788	802	820	rBV2	446797	1333621	100.00%	13.095%
28	6.135	826	828	830	rVB2	406	266	0.02%	0.003%
29	6.160	830	832	834	rVV	334	269	0.02%	0.003%
30	6.202	837	839	841	rBV	452	359	0.03%	0.004%
31	6.531	891	893	896	rBV2	359	357	0.03%	0.004%
32	6.635	908	910	912	rBV3	425	447	0.03%	0.004%
33	6.763	921	931	948	rBV	320803	778995	58.41%	7.649%
34	7.129	982	991	1001	rBV4	29733	71363	5.35%	0.701%
35	7.312	1012	1021	1037	rBV	269571	584287	43.81%	5.737%
36	7.489	1045	1050	1055	rBV4	527	1225	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029484.D
 Acq On : 14 Jun 2022 22:43
 Operator : JC/MD
 Sample : N3313-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YB7N2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.556	1058	1061	1064	rBV2	360	602	0.05%	0.006%
38	7.665	1078	1079	1084	rBV2	227	360	0.03%	0.004%
39	7.818	1101	1104	1105	rBV	611	612	0.05%	0.006%
40	7.946	1121	1125	1127	rBV3	613	858	0.06%	0.008%
41	8.037	1138	1140	1143	rVB3	307	315	0.02%	0.003%
42	8.110	1149	1152	1157	rBV2	453	733	0.05%	0.007%
43	8.330	1181	1188	1202	rBV	163132	275834	20.68%	2.708%
44	8.427	1202	1204	1206	rBV2	344	387	0.03%	0.004%
45	8.653	1234	1241	1249	rBV	708093	1111188	83.32%	10.911%
46	8.720	1249	1252	1261	rVV2	9815	17063	1.28%	0.168%
47	8.805	1265	1266	1269	rVB2	447	321	0.02%	0.003%
48	8.866	1273	1276	1278	rBV2	448	607	0.05%	0.006%
49	8.952	1285	1290	1302	rVB	117353	170316	12.77%	1.672%
50	9.196	1326	1330	1331	rBV2	328	421	0.03%	0.004%
51	9.275	1340	1343	1348	rVB3	2879	3964	0.30%	0.039%
52	9.385	1356	1361	1379	rBV	470972	711935	53.38%	6.991%
53	9.817	1428	1432	1436	rBV3	339	502	0.04%	0.005%
54	9.897	1443	1445	1448	rBV2	269	334	0.03%	0.003%
55	10.055	1465	1471	1485	rBV	685906	909533	68.20%	8.931%
56	10.201	1491	1495	1500	rVB2	1045	1691	0.13%	0.017%
57	10.244	1500	1502	1504	rVB2	416	311	0.02%	0.003%
58	10.269	1504	1506	1507	rBV	336	305	0.02%	0.003%
59	10.311	1509	1513	1518	rVB2	1802	2258	0.17%	0.022%
60	10.640	1564	1567	1569	rBV2	553	651	0.05%	0.006%
61	10.805	1591	1594	1596	rBV3	396	325	0.02%	0.003%
62	10.878	1605	1606	1609	rBV	343	270	0.02%	0.003%
63	10.945	1613	1617	1618	rBV	268	357	0.03%	0.004%
64	11.024	1626	1630	1631	rBV2	341	435	0.03%	0.004%
65	11.122	1641	1646	1652	rBV2	4475	5761	0.43%	0.057%
66	11.195	1652	1658	1669	rBV	522675	654405	49.07%	6.426%
67	11.360	1683	1685	1687	rBV2	323	311	0.02%	0.003%
68	11.451	1698	1700	1702	rBV3	675	858	0.06%	0.008%
69	11.549	1714	1716	1721	rVB3	694	990	0.07%	0.010%
70	11.610	1725	1726	1728	rVV2	401	282	0.02%	0.003%
71	11.683	1734	1738	1741	rVB3	577	775	0.06%	0.008%
72	11.713	1741	1743	1745	rBV2	585	614	0.05%	0.006%
73	11.750	1745	1749	1755	rVB2	4886	6519	0.49%	0.064%
74	11.848	1761	1765	1768	rBV2	1183	1550	0.12%	0.015%
75	11.933	1775	1779	1783	rBV3	2050	3031	0.23%	0.030%
76	11.969	1783	1785	1789	rBV3	769	669	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029484.D
 Acq On : 14 Jun 2022 22:43
 Operator : JC/MD
 Sample : N3313-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YB7N2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.024	1789	1794	1806	rBV	734289	894480	67.07%	8.783%
78	12.152	1813	1815	1819	rVB2	3197	2791	0.21%	0.027%
79	12.219	1822	1826	1831	rVB4	1684	2621	0.20%	0.026%
80	12.262	1831	1833	1835	rBV2	585	534	0.04%	0.005%
81	12.323	1837	1843	1851	rBV	718284	917076	68.77%	9.005%
82	12.482	1864	1869	1872	rBV5	1010	1435	0.11%	0.014%
83	12.561	1879	1882	1884	rBV2	416	480	0.04%	0.005%
84	12.634	1892	1894	1896	rBV2	458	479	0.04%	0.005%
85	12.664	1896	1899	1902	rBV3	959	1363	0.10%	0.013%
86	12.762	1913	1915	1916	rBV	384	280	0.02%	0.003%
87	12.969	1945	1949	1952	rBV2	545	770	0.06%	0.008%
88	13.055	1961	1963	1970	rVB4	998	1228	0.09%	0.012%
89	13.116	1970	1973	1976	rBV2	568	697	0.05%	0.007%
90	13.439	2024	2026	2029	rBV2	213	303	0.02%	0.003%
91	13.536	2040	2042	2044	rVB	421	277	0.02%	0.003%
92	13.567	2044	2047	2049	rBV2	293	454	0.03%	0.004%
93	13.591	2049	2051	2054	rVV2	707	670	0.05%	0.007%
94	13.780	2081	2082	2086	rBV3	836	914	0.07%	0.009%
95	13.963	2110	2112	2117	rVB3	580	818	0.06%	0.008%
96	14.134	2136	2140	2142	rBV3	506	754	0.06%	0.007%
97	14.884	2260	2263	2266	rBV3	590	923	0.07%	0.009%
98	15.457	2355	2357	2360	rBV3	512	512	0.04%	0.005%
99	15.633	2384	2386	2388	rBV2	397	327	0.02%	0.003%
100	15.920	2432	2433	2437	rBV	612	592	0.04%	0.006%




Sum of corrected areas: 10184020

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029484.D
Acq On : 14 Jun 2022 22:43
Operator : JC/MD
Sample : N3313-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YB7N2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

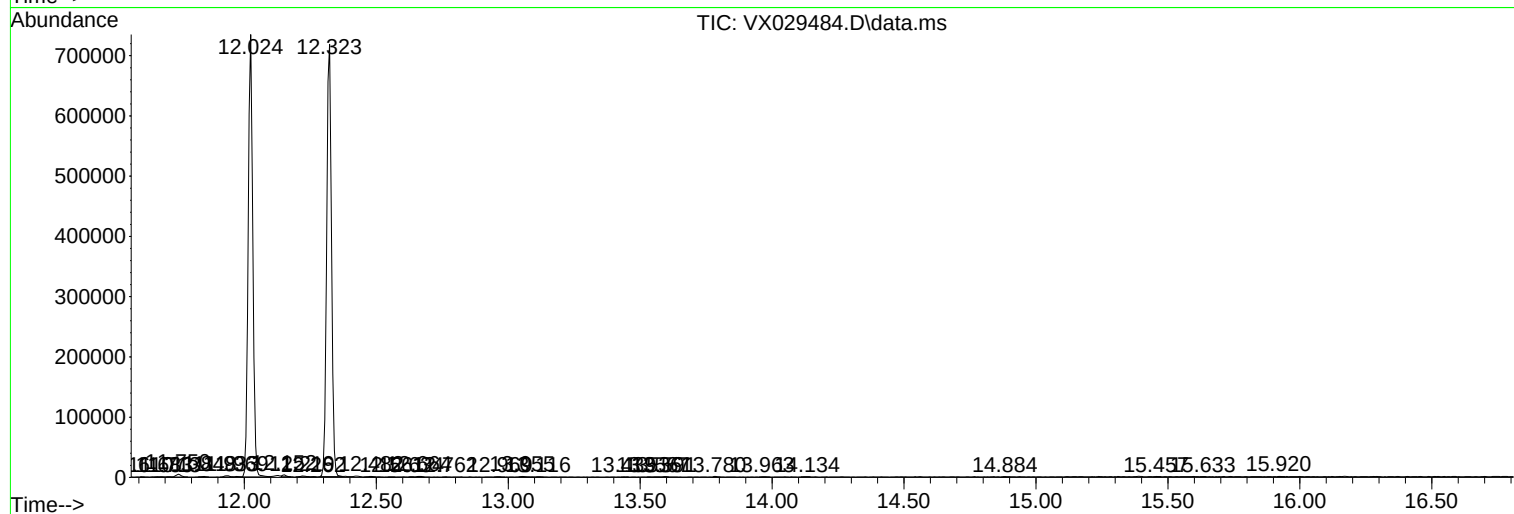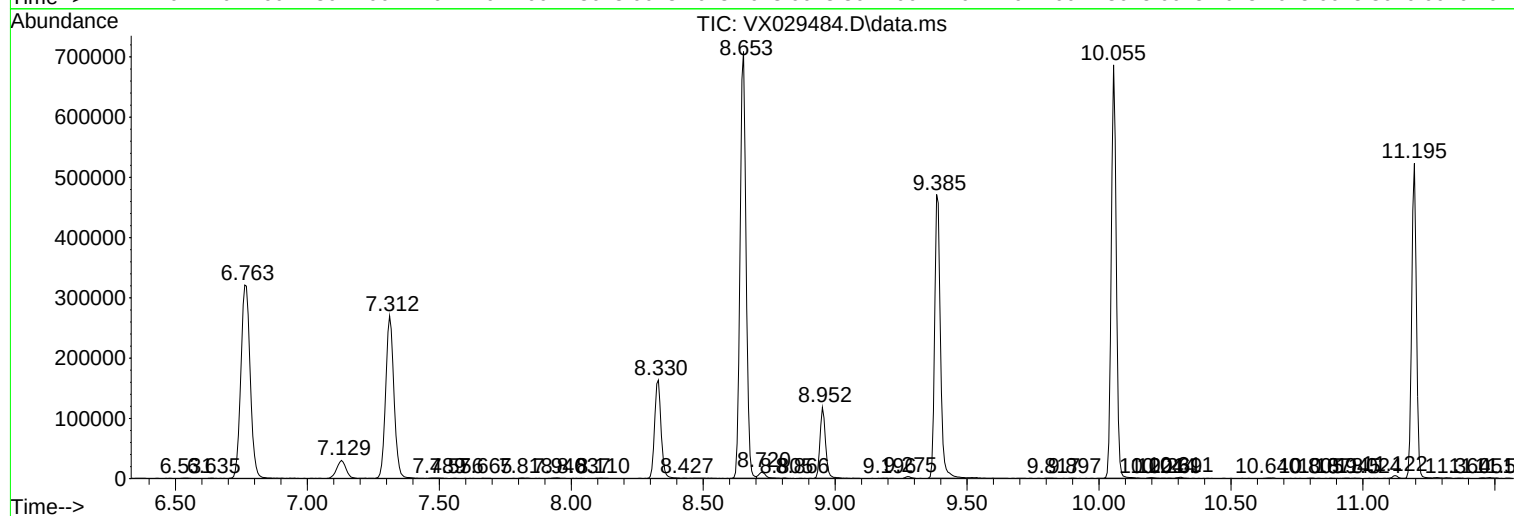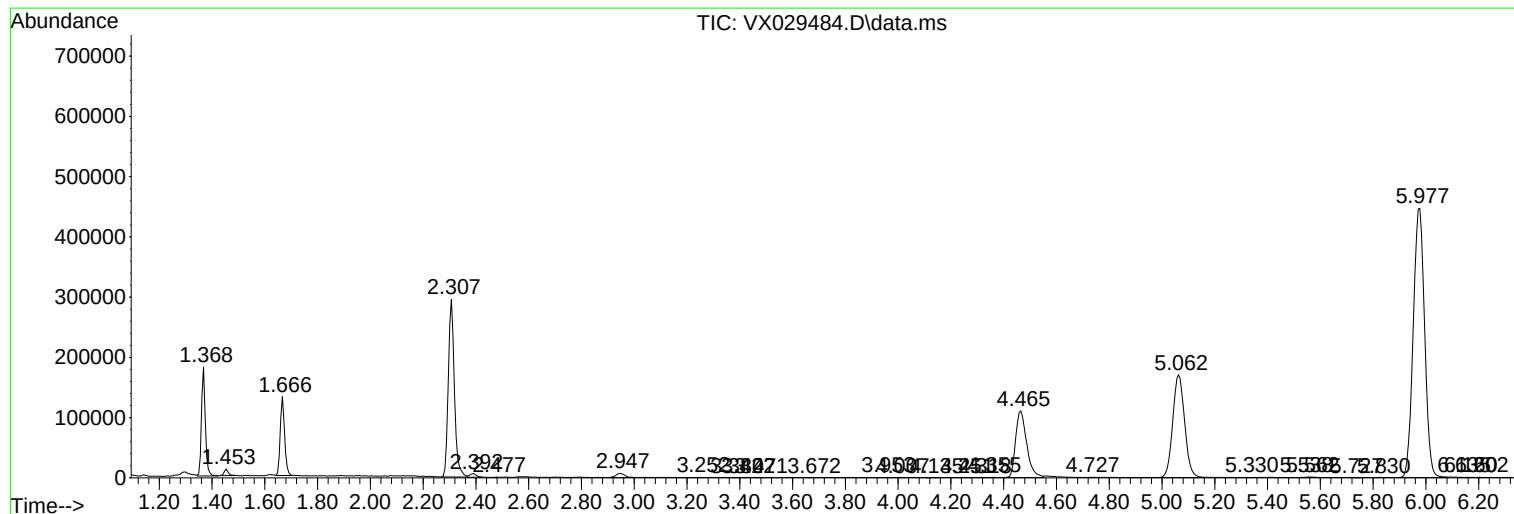

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029484.D
Acq On : 14 Jun 2022 22:43
Operator : JC/MD
Sample : N3313-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YB7N2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029484.D
Acq On : 14 Jun 2022 22:43
Operator : JC/MD
Sample : N3313-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YB7N2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------