

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029485.D
 Acq On : 14 Jun 2022 23:06
 Operator : JC/MD
 Sample : N3313-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YB7N3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M

Title : VOC Analysis

Signal : TIC: VX029485.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	56	rVB	181664	181954	13.37%	1.809%
2	1.453	57	60	68	rVB	14282	15866	1.17%	0.158%
3	1.666	91	95	105	rVB	137072	161080	11.83%	1.601%
4	2.306	194	200	210	rBV	297213	476199	34.98%	4.734%
5	2.385	210	213	223	rVB	6395	11053	0.81%	0.110%
6	2.507	229	233	236	rBV2	559	889	0.07%	0.009%
7	2.550	238	240	241	rBV2	906	814	0.06%	0.008%
8	2.788	276	279	284	rVB4	716	1435	0.11%	0.014%
9	2.873	290	293	294	rBV2	362	334	0.02%	0.003%
10	2.946	298	305	316	rVB	9394	21256	1.56%	0.211%
11	3.093	327	329	330	rBV2	448	396	0.03%	0.004%
12	3.184	341	344	346	rVB2	411	328	0.02%	0.003%
13	3.251	354	355	358	rBV2	319	271	0.02%	0.003%
14	3.471	389	391	393	rVB	413	293	0.02%	0.003%
15	3.501	393	396	399	rVB3	290	311	0.02%	0.003%
16	3.727	430	433	436	rVB3	263	380	0.03%	0.004%
17	3.757	436	438	439	rBV	316	265	0.02%	0.003%
18	3.897	458	461	462	rBV2	282	264	0.02%	0.003%
19	4.013	478	480	482	rVV	336	287	0.02%	0.003%
20	4.196	506	510	511	rBV3	206	249	0.02%	0.002%
21	4.336	532	533	537	rBV2	240	278	0.02%	0.003%
22	4.464	545	554	568	rBV	112899	323996	23.80%	3.221%
23	4.745	599	600	605	rVB2	416	465	0.03%	0.005%
24	4.903	623	626	628	rBV2	205	260	0.02%	0.003%
25	4.946	632	633	636	rBV	287	266	0.02%	0.003%
26	5.062	640	652	671	rBV	173675	537355	39.48%	5.342%
27	5.385	701	705	706	rBV3	518	520	0.04%	0.005%
28	5.562	725	734	735	rBV3	812	1587	0.12%	0.016%
29	5.970	789	801	818	rBV2	458381	1361223	100.00%	13.531%
30	6.183	834	836	837	rBV	309	304	0.02%	0.003%
31	6.269	847	850	852	rVB2	286	244	0.02%	0.002%
32	6.336	859	861	863	rBV2	362	301	0.02%	0.003%
33	6.464	878	882	884	rBV2	350	421	0.03%	0.004%
34	6.763	920	931	947	rBV	294851	702570	51.61%	6.984%
35	7.037	975	976	979	rBV2	479	474	0.03%	0.005%
36	7.128	982	991	1002	rVV5	27310	67593	4.97%	0.672%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029485.D
 Acq On : 14 Jun 2022 23:06
 Operator : JC/MD
 Sample : N3313-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YB7N3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.208	1002	1004	1008	rVB3	356	441	0.03%	0.004%
38	7.311	1010	1021	1034	rBV	274269	599674	44.05%	5.961%
39	7.482	1047	1049	1053	rVB	649	761	0.06%	0.008%
40	7.616	1069	1071	1077	rVB2	340	471	0.03%	0.005%
41	7.939	1123	1124	1126	rBV	486	264	0.02%	0.003%
42	8.244	1170	1174	1177	rBV2	271	426	0.03%	0.004%
43	8.329	1181	1188	1201	rVV	169234	279762	20.55%	2.781%
44	8.561	1223	1226	1227	rBV2	234	254	0.02%	0.003%
45	8.653	1234	1241	1248	rBV	734869	1130623	83.06%	11.239%
46	8.726	1249	1253	1258	rVB	10078	16170	1.19%	0.161%
47	8.890	1279	1280	1284	rVB2	298	267	0.02%	0.003%
48	8.951	1285	1290	1300	rBV	121851	174103	12.79%	1.731%
49	9.280	1340	1344	1348	rVV6	2605	4033	0.30%	0.040%
50	9.384	1356	1361	1382	rBV	483059	727511	53.45%	7.232%
51	10.055	1465	1471	1480	rBV	606144	807737	59.34%	8.029%
52	10.201	1492	1495	1498	rVB3	621	566	0.04%	0.006%
53	10.311	1508	1513	1517	rVV4	1947	2653	0.19%	0.026%
54	10.427	1530	1532	1535	rVB2	297	273	0.02%	0.003%
55	10.463	1535	1538	1541	rBV2	235	383	0.03%	0.004%
56	10.561	1552	1554	1558	rBV	187	256	0.02%	0.003%
57	10.652	1567	1569	1572	rVB3	633	561	0.04%	0.006%
58	10.756	1584	1586	1588	rBV2	320	310	0.02%	0.003%
59	10.878	1605	1606	1609	rBV2	365	440	0.03%	0.004%
60	10.939	1613	1616	1618	rBV2	262	377	0.03%	0.004%
61	11.122	1642	1646	1650	rVB	4488	5608	0.41%	0.056%
62	11.195	1652	1658	1666	rBV	525472	662956	48.70%	6.590%
63	11.384	1686	1689	1691	rBV	553	621	0.05%	0.006%
64	11.408	1691	1693	1696	rVB2	387	437	0.03%	0.004%
65	11.451	1697	1700	1701	rBV	424	442	0.03%	0.004%
66	11.481	1702	1705	1709	rVB	1283	1730	0.13%	0.017%
67	11.548	1714	1716	1719	rVB2	518	406	0.03%	0.004%
68	11.615	1725	1727	1729	rBV2	277	310	0.02%	0.003%
69	11.676	1736	1737	1741	rVB2	421	315	0.02%	0.003%
70	11.707	1741	1742	1745	rVV	462	488	0.04%	0.005%
71	11.750	1745	1749	1755	rVB3	4971	6374	0.47%	0.063%
72	11.841	1762	1764	1769	rVB3	820	995	0.07%	0.010%
73	11.939	1775	1780	1783	rBV5	2063	3176	0.23%	0.032%
74	11.969	1783	1785	1788	rVB4	925	1068	0.08%	0.011%
75	12.024	1788	1794	1804	rBV	641187	791197	58.12%	7.865%
76	12.219	1821	1826	1832	rBV4	4657	8078	0.59%	0.080%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029485.D
 Acq On : 14 Jun 2022 23:06
 Operator : JC/MD
 Sample : N3313-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YB7N3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.323	1836	1843	1851	rBV	747364	940680	69.11%	9.351%
78	12.426	1858	1860	1864	rVB4	1592	1861	0.14%	0.018%
79	12.481	1866	1869	1873	rVB4	1016	1329	0.10%	0.013%
80	12.579	1884	1885	1888	rVB2	365	320	0.02%	0.003%
81	12.627	1891	1893	1896	rBV2	385	400	0.03%	0.004%
82	12.664	1896	1899	1909	rVB5	1119	2430	0.18%	0.024%
83	12.737	1909	1911	1912	rBV2	372	362	0.03%	0.004%
84	12.816	1922	1924	1926	rBV	372	392	0.03%	0.004%
85	12.859	1928	1931	1934	rBV4	486	665	0.05%	0.007%
86	13.012	1953	1956	1958	rBV3	276	354	0.03%	0.004%
87	13.054	1958	1963	1965	rVV3	776	885	0.07%	0.009%
88	13.115	1971	1973	1976	rVB3	280	283	0.02%	0.003%
89	13.335	2007	2009	2011	rVB	479	298	0.02%	0.003%
90	13.450	2024	2028	2029	rBV2	287	321	0.02%	0.003%
91	13.469	2029	2031	2035	rVB	380	328	0.02%	0.003%
92	13.597	2049	2052	2054	rVB2	667	693	0.05%	0.007%
93	13.780	2080	2082	2085	rVB2	713	531	0.04%	0.005%
94	13.987	2114	2116	2119	rBV2	288	274	0.02%	0.003%
95	14.048	2124	2126	2127	rBV2	354	332	0.02%	0.003%
96	14.127	2137	2139	2144	rVV2	871	1224	0.09%	0.012%
97	14.408	2183	2185	2188	rBV2	364	477	0.04%	0.005%
98	14.481	2195	2197	2200	rBV2	299	241	0.02%	0.002%
99	15.328	2334	2336	2337	rBV2	587	345	0.03%	0.003%
100	15.377	2343	2344	2346	rBV	789	632	0.05%	0.006%




Sum of corrected areas: 10059955

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029485.D
Acq On : 14 Jun 2022 23:06
Operator : JC/MD
Sample : N3313-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YB7N3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

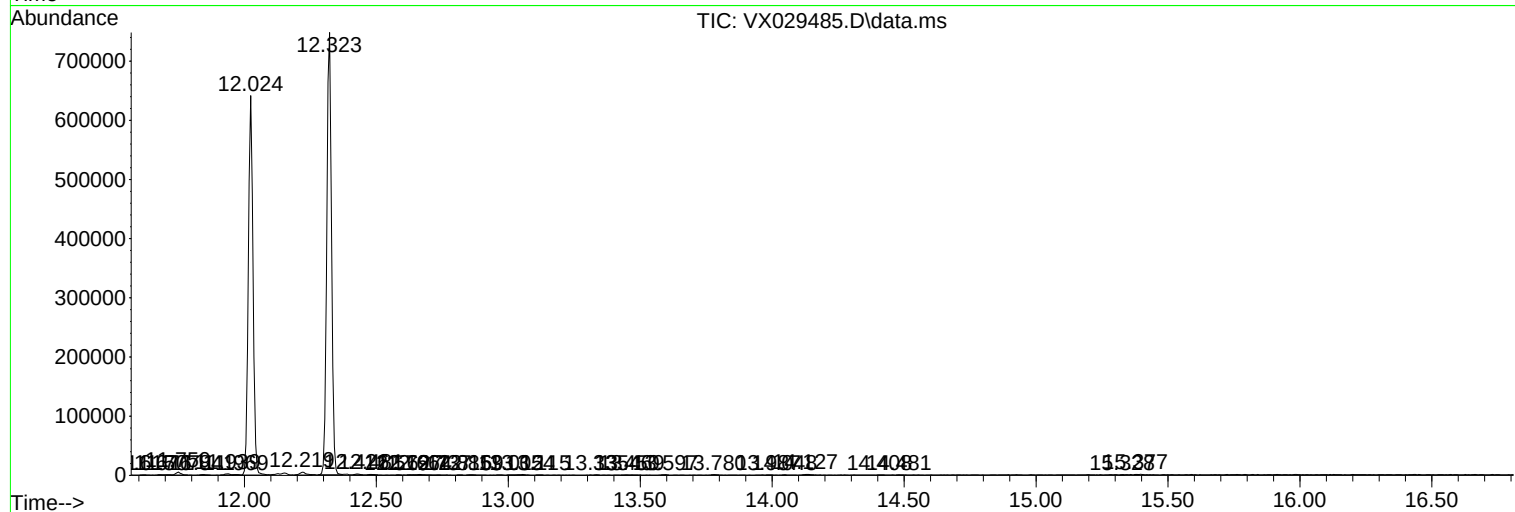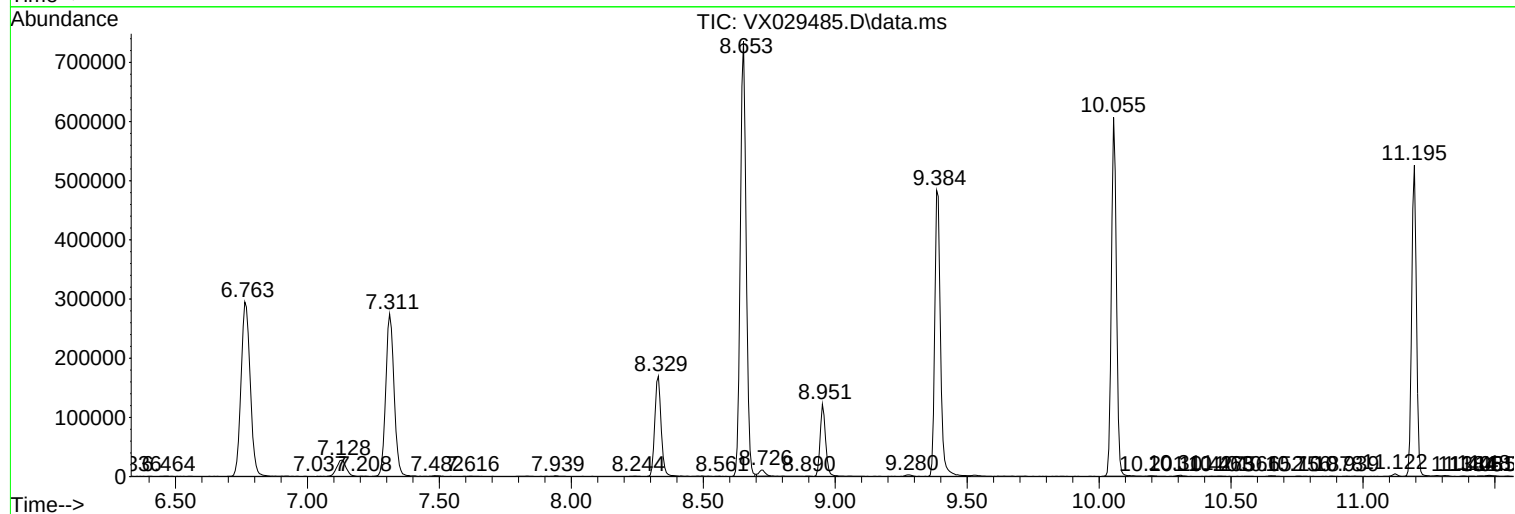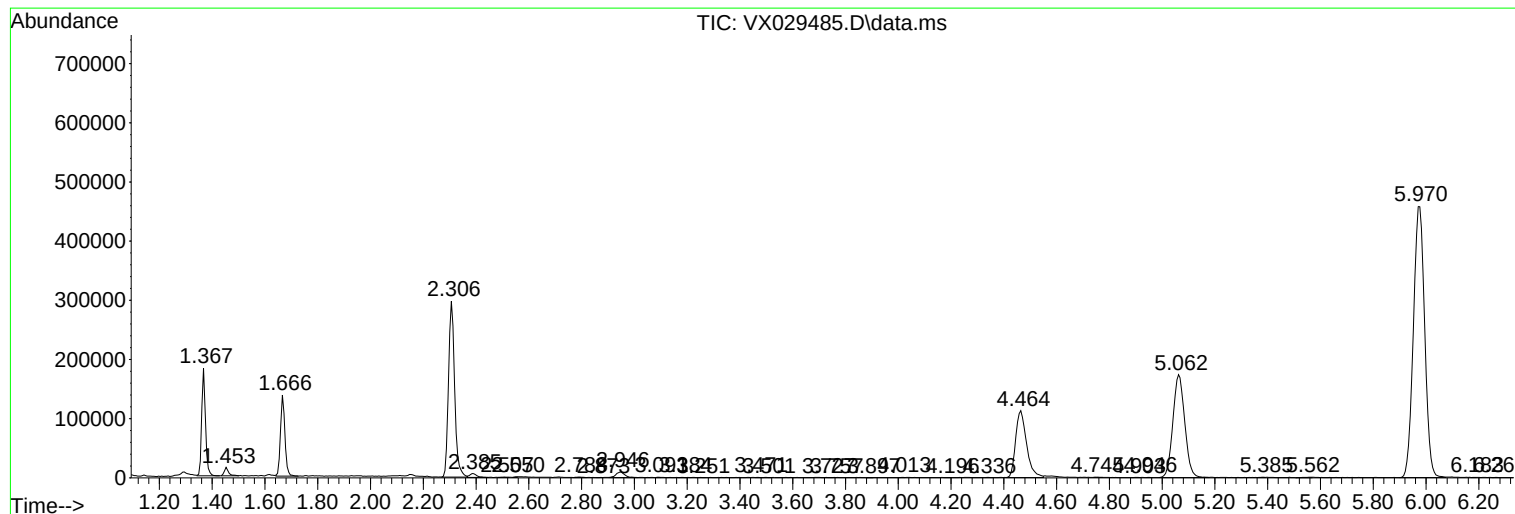

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029485.D
Acq On : 14 Jun 2022 23:06
Operator : JC/MD
Sample : N3313-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YB7N3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029485.D
Acq On : 14 Jun 2022 23:06
Operator : JC/MD
Sample : N3313-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YB7N3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc