

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029486.D
 Acq On : 14 Jun 2022 23:29
 Operator : JC/MD
 Sample : N3313-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M

Title : VOC Analysis

Signal : TIC: VX029486.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	53	rVB	182561	180061	13.23%	1.762%
2	1.666	91	95	103	rVB	136206	159248	11.70%	1.559%
3	2.306	194	200	211	rBV	297343	470109	34.54%	4.601%
4	2.636	252	254	255	rBV	289	220	0.02%	0.002%
5	2.715	262	267	274	rBV4	767	1338	0.10%	0.013%
6	2.788	276	279	285	rVB3	1243	1990	0.15%	0.019%
7	2.940	298	304	319	rVB	12821	31275	2.30%	0.306%
8	3.172	341	342	344	rBV2	339	341	0.03%	0.003%
9	3.221	348	350	352	rVV	369	275	0.02%	0.003%
10	3.245	352	354	355	rVV	364	267	0.02%	0.003%
11	3.282	358	360	361	rVV2	245	221	0.02%	0.002%
12	3.337	367	369	371	rVV2	342	332	0.02%	0.003%
13	3.398	378	379	382	rVV2	304	238	0.02%	0.002%
14	3.605	411	413	414	rBV	275	214	0.02%	0.002%
15	3.654	419	421	424	rVB2	304	256	0.02%	0.003%
16	3.708	428	430	433	rVB2	338	301	0.02%	0.003%
17	3.837	449	451	453	rVV	386	279	0.02%	0.003%
18	3.879	455	458	461	rBV	210	378	0.03%	0.004%
19	3.958	467	471	473	rBV2	327	525	0.04%	0.005%
20	4.464	545	554	568	rBV	108437	316702	23.27%	3.100%
21	4.714	593	595	597	rBV2	379	290	0.02%	0.003%
22	5.062	640	652	671	rBV	172123	534223	39.25%	5.228%
23	5.385	700	705	708	rBV3	592	1128	0.08%	0.011%
24	5.556	728	733	738	rVV5	647	1520	0.11%	0.015%
25	5.720	759	760	762	rBV2	334	244	0.02%	0.002%
26	5.867	780	784	786	rBV2	306	452	0.03%	0.004%
27	5.976	786	802	821	rBV2	459621	1361129	100.00%	13.321%
28	6.275	849	851	856	rVB2	471	645	0.05%	0.006%
29	6.318	856	858	859	rBV2	305	229	0.02%	0.002%
30	6.360	862	865	866	rBV2	415	397	0.03%	0.004%
31	6.385	866	869	872	rVB3	495	582	0.04%	0.006%
32	6.428	872	876	877	rBV	230	322	0.02%	0.003%
33	6.501	886	888	892	rVB2	224	308	0.02%	0.003%
34	6.556	895	897	901	rVB2	482	440	0.03%	0.004%
35	6.763	920	931	946	rBV	320656	765869	56.27%	7.495%
36	7.049	976	978	979	rBV2	349	284	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029486.D
 Acq On : 14 Jun 2022 23:29
 Operator : JC/MD
 Sample : N3313-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.129	982	991	1002	rVV4	25170	60204	4.42%	0.589%
38	7.238	1007	1009	1010	rBV	286	245	0.02%	0.002%
39	7.312	1013	1021	1035	rBV	273635	590227	43.36%	5.776%
40	7.482	1045	1049	1055	rBV4	882	1704	0.13%	0.017%
41	7.580	1062	1065	1067	rVV2	244	241	0.02%	0.002%
42	7.629	1071	1073	1078	rVV2	301	351	0.03%	0.003%
43	7.818	1100	1104	1110	rVB3	611	1168	0.09%	0.011%
44	7.860	1110	1111	1115	rBV2	186	269	0.02%	0.003%
45	7.939	1120	1124	1129	rBV3	874	1561	0.11%	0.015%
46	8.013	1134	1136	1137	rVB2	359	218	0.02%	0.002%
47	8.037	1137	1140	1142	rBV2	246	321	0.02%	0.003%
48	8.330	1181	1188	1200	rBV	165338	277691	20.40%	2.718%
49	8.586	1224	1230	1232	rBV3	409	769	0.06%	0.008%
50	8.653	1234	1241	1248	rVV	724734	1133607	83.28%	11.094%
51	8.720	1249	1252	1263	rVV3	10401	19077	1.40%	0.187%
52	8.951	1285	1290	1299	rBV	117607	171969	12.63%	1.683%
53	9.275	1340	1343	1348	rVB3	2520	3771	0.28%	0.037%
54	9.384	1356	1361	1377	rBV	470931	713300	52.41%	6.981%
55	9.701	1410	1413	1418	rVB2	2037	2435	0.18%	0.024%
56	9.915	1446	1448	1454	rBV2	273	404	0.03%	0.004%
57	10.055	1466	1471	1488	rVB	670356	891525	65.50%	8.725%
58	10.244	1500	1502	1504	rBV	330	306	0.02%	0.003%
59	10.305	1509	1512	1516	rVB2	1923	2150	0.16%	0.021%
60	10.396	1524	1527	1528	rBV2	259	226	0.02%	0.002%
61	10.530	1547	1549	1551	rVB2	266	225	0.02%	0.002%
62	10.555	1551	1553	1555	rVB2	243	212	0.02%	0.002%
63	10.640	1565	1567	1569	rBV2	405	433	0.03%	0.004%
64	10.750	1583	1585	1587	rBV	559	362	0.03%	0.004%
65	10.847	1600	1601	1603	rBV2	406	285	0.02%	0.003%
66	10.872	1603	1605	1607	rVB2	303	312	0.02%	0.003%
67	10.963	1617	1620	1627	rVB3	438	709	0.05%	0.007%
68	11.122	1642	1646	1651	rVB3	4543	5720	0.42%	0.056%
69	11.195	1652	1658	1666	rBV	535856	657875	48.33%	6.438%
70	11.451	1697	1700	1702	rBV2	821	1081	0.08%	0.011%
71	11.488	1702	1706	1707	rVB3	955	1255	0.09%	0.012%
72	11.549	1713	1716	1718	rBV3	593	579	0.04%	0.006%
73	11.622	1725	1728	1729	rBV	382	352	0.03%	0.003%
74	11.677	1735	1737	1741	rBV3	548	572	0.04%	0.006%
75	11.713	1741	1743	1744	rVV2	409	306	0.02%	0.003%
76	11.750	1745	1749	1757	rVB4	3981	6007	0.44%	0.059%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029486.D
 Acq On : 14 Jun 2022 23:29
 Operator : JC/MD
 Sample : N3313-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	11.890	1769	1772	1775	rVB	252	273	0.02%	0.003%
78	11.933	1775	1779	1782	rBV	2521	2761	0.20%	0.027%
79	11.969	1782	1785	1789	rBV2	547	756	0.06%	0.007%
80	12.024	1789	1794	1806	rBV	713244	874269	64.23%	8.556%
81	12.128	1807	1811	1812	rBV3	1322	1491	0.11%	0.015%
82	12.323	1836	1843	1851	rBV	753443	942693	69.26%	9.226%
83	12.481	1865	1869	1873	rVB3	717	1123	0.08%	0.011%
84	12.597	1884	1888	1889	rBV3	282	332	0.02%	0.003%
85	12.664	1896	1899	1901	rBV2	850	1180	0.09%	0.012%
86	12.768	1913	1916	1921	rVB4	877	1305	0.10%	0.013%
87	12.847	1927	1929	1932	rBV3	282	394	0.03%	0.004%
88	13.012	1955	1956	1958	rBV2	275	232	0.02%	0.002%
89	13.054	1961	1963	1967	rVB3	867	865	0.06%	0.008%
90	13.121	1970	1974	1976	rBV2	453	585	0.04%	0.006%
91	13.591	2048	2051	2054	rBV2	762	848	0.06%	0.008%
92	13.701	2066	2069	2073	rBV	396	423	0.03%	0.004%
93	13.957	2109	2111	2114	rVB3	491	509	0.04%	0.005%
94	14.133	2135	2140	2144	rVB	2025	2723	0.20%	0.027%
95	14.450	2189	2192	2193	rVB2	390	331	0.02%	0.003%
96	14.902	2264	2266	2267	rBV	485	280	0.02%	0.003%
97	14.944	2272	2273	2276	rBV	367	238	0.02%	0.002%
98	15.731	2400	2402	2405	rVB2	773	761	0.06%	0.007%
99	15.932	2434	2435	2437	rBV2	651	321	0.02%	0.003%
100	16.103	2461	2463	2464	rBV2	725	489	0.04%	0.005%




Sum of corrected areas: 10217838

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029486.D
Acq On : 14 Jun 2022 23:29
Operator : JC/MD
Sample : N3313-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

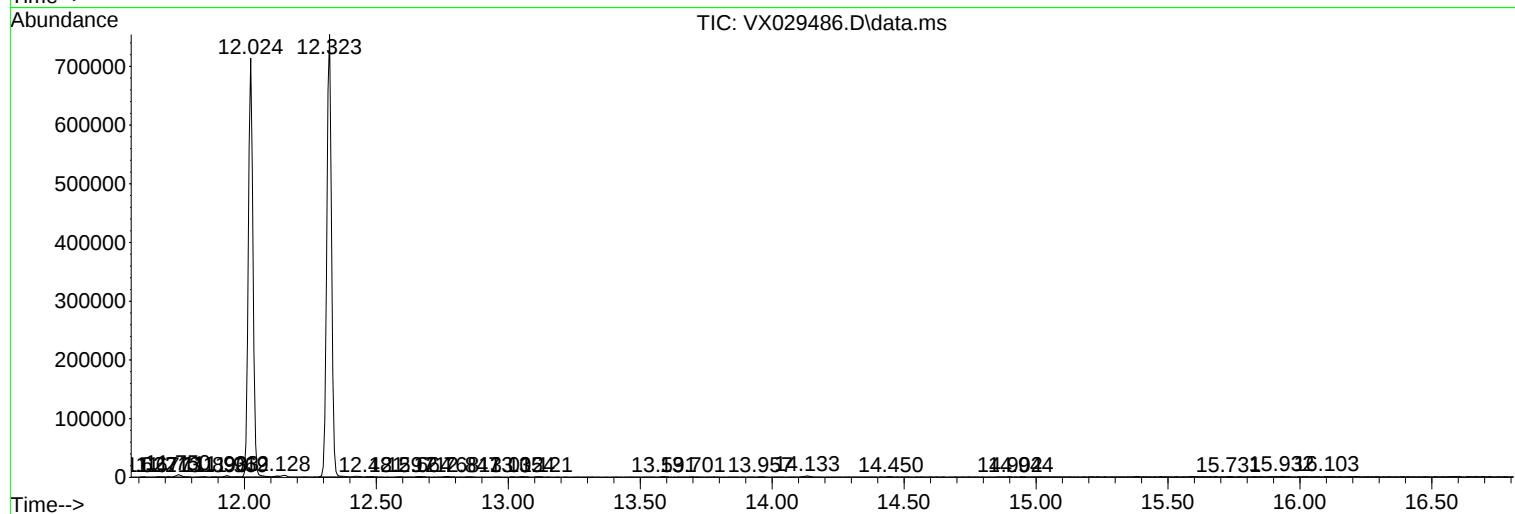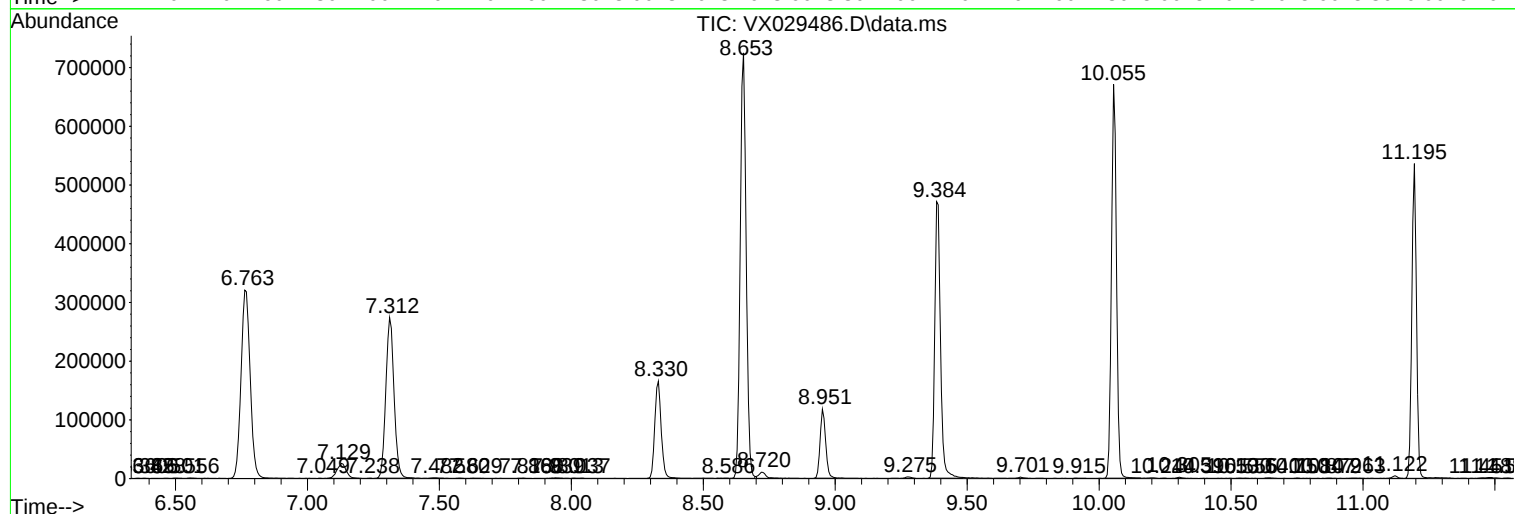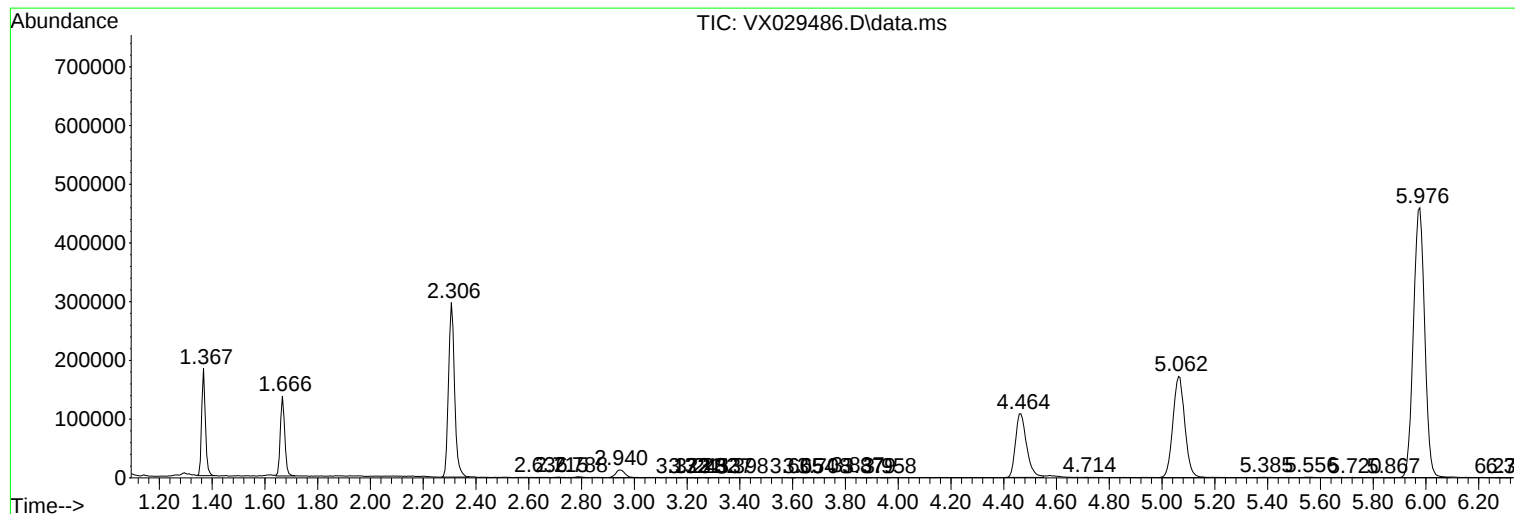

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029486.D
Acq On : 14 Jun 2022 23:29
Operator : JC/MD
Sample : N3313-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029486.D
Acq On : 14 Jun 2022 23:29
Operator : JC/MD
Sample : N3313-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc