

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029487.D
 Acq On : 14 Jun 2022 23:53
 Operator : JC/MD
 Sample : N3248-20 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	56	rVB	176471	178761	13.39%	1.476%
2	1.666	91	95	105	rVB	123266	146725	10.99%	1.211%
3	2.306	194	200	212	rBV	290808	468479	35.08%	3.868%
4	2.788	275	279	284	rVB4	2163	3596	0.27%	0.030%
5	2.885	292	295	297	rBV2	318	365	0.03%	0.003%
6	2.946	297	305	316	rVB	26989	62320	4.67%	0.515%
7	3.093	323	329	337	rVV2	6405	11828	0.89%	0.098%
8	3.190	344	345	348	rBV2	299	320	0.02%	0.003%
9	3.422	380	383	386	rVB	439	375	0.03%	0.003%
10	3.464	386	390	391	rBV2	288	305	0.02%	0.003%
11	3.611	405	414	425	rBV	40216	94529	7.08%	0.780%
12	4.391	538	542	543	rBV	403	571	0.04%	0.005%
13	4.489	545	558	582	rVV2	415929	1335053	99.98%	11.022%
14	4.812	609	611	613	rBV2	390	461	0.03%	0.004%
15	4.873	619	621	624	rBV2	289	352	0.03%	0.003%
16	5.062	638	652	671	rBV	170728	530203	39.71%	4.377%
17	5.391	692	706	720	rBV	213202	664814	49.79%	5.489%
18	5.525	725	728	729	rBV2	381	386	0.03%	0.003%
19	5.604	739	741	745	rVB2	259	302	0.02%	0.002%
20	5.702	753	757	761	rVB3	316	491	0.04%	0.004%
21	5.976	789	802	818	rBV2	447793	1335274	100.00%	11.024%
22	6.360	862	865	866	rBV2	455	391	0.03%	0.003%
23	6.379	866	868	869	rVB	475	328	0.02%	0.003%
24	6.403	869	872	873	rBV2	319	347	0.03%	0.003%
25	6.470	882	883	889	rVB2	305	434	0.03%	0.004%
26	6.537	891	894	896	rBV2	442	320	0.02%	0.003%
27	6.677	914	917	920	rBV2	284	435	0.03%	0.004%
28	6.763	920	931	945	rBV	312845	747490	55.98%	6.171%
29	7.128	982	991	1002	rVV4	28806	70761	5.30%	0.584%
30	7.238	1006	1009	1013	rBV3	274	453	0.03%	0.004%
31	7.311	1013	1021	1034	rBV	267722	585245	43.83%	4.832%
32	7.476	1045	1048	1053	rBV4	980	1919	0.14%	0.016%
33	7.640	1073	1075	1080	rVV	269	324	0.02%	0.003%
34	7.708	1084	1086	1090	rBV2	273	354	0.03%	0.003%
35	7.817	1100	1104	1107	rBV2	427	659	0.05%	0.005%
36	7.939	1120	1124	1128	rBV5	715	1354	0.10%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029487.D
 Acq On : 14 Jun 2022 23:53
 Operator : JC/MD
 Sample : N3248-20 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	8.085	1146	1148	1150	rBV2	288	319	0.02%	0.003%
38	8.329	1181	1188	1200	rVV	170436	274732	20.57%	2.268%
39	8.652	1234	1241	1248	rBV	727760	1102363	82.56%	9.101%
40	8.720	1248	1252	1259	rVB2	15997	26937	2.02%	0.222%
41	8.951	1284	1290	1301	rBV	116869	178413	13.36%	1.473%
42	9.152	1320	1323	1328	rVB4	1315	1786	0.13%	0.015%
43	9.274	1338	1343	1349	rVB	17519	26902	2.01%	0.222%
44	9.390	1356	1362	1378	rBV	487681	722938	54.14%	5.969%
45	9.841	1433	1436	1438	rBV	334	398	0.03%	0.003%
46	10.006	1460	1463	1465	rBV2	376	391	0.03%	0.003%
47	10.055	1465	1471	1481	rBV	639953	869783	65.14%	7.181%
48	10.201	1492	1495	1499	rVB	2838	3843	0.29%	0.032%
49	10.305	1506	1512	1519	rBV	8717	13188	0.99%	0.109%
50	10.359	1519	1521	1526	rVB3	1168	1318	0.10%	0.011%
51	10.524	1545	1548	1551	rBV2	334	359	0.03%	0.003%
52	10.585	1555	1558	1563	rVV2	721	1167	0.09%	0.010%
53	10.646	1563	1568	1576	rVB	7524	11712	0.88%	0.097%
54	10.756	1583	1586	1587	rBV2	617	570	0.04%	0.005%
55	10.780	1588	1590	1595	rVB3	2190	2504	0.19%	0.021%
56	10.853	1599	1602	1606	rBV3	1858	2651	0.20%	0.022%
57	10.939	1614	1616	1617	rBV2	415	326	0.02%	0.003%
58	10.969	1617	1621	1623	rVB	1211	1205	0.09%	0.010%
59	11.091	1637	1641	1643	rBV2	492	690	0.05%	0.006%
60	11.122	1643	1646	1651	rVB2	5139	6432	0.48%	0.053%
61	11.195	1652	1658	1669	rBV	524065	659658	49.40%	5.446%
62	11.311	1673	1677	1684	rVB2	3387	5885	0.44%	0.049%
63	11.384	1684	1689	1691	rBV	9705	14286	1.07%	0.118%
64	11.457	1697	1701	1704	rBV	8836	12245	0.92%	0.101%
65	11.615	1723	1727	1733	rVV	9285	12221	0.92%	0.101%
66	11.676	1735	1737	1741	rBV3	595	720	0.05%	0.006%
67	11.719	1741	1744	1745	rBV2	732	817	0.06%	0.007%
68	11.756	1745	1750	1757	rVB2	26383	33362	2.50%	0.275%
69	11.841	1761	1764	1767	rBV4	976	1546	0.12%	0.013%
70	11.938	1776	1780	1783	rBV5	2947	4317	0.32%	0.036%
71	11.969	1783	1785	1789	rVV3	2537	2754	0.21%	0.023%
72	12.024	1789	1794	1800	rVV	706143	854453	63.99%	7.055%
73	12.091	1801	1805	1808	rVV	13660	18290	1.37%	0.151%
74	12.146	1812	1814	1823	rVB4	3714	5768	0.43%	0.048%
75	12.243	1823	1830	1833	rBV4	5618	9119	0.68%	0.075%
76	12.323	1837	1843	1850	rVB	746861	933907	69.94%	7.711%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029487.D
 Acq On : 14 Jun 2022 23:53
 Operator : JC/MD
 Sample : N3248-20 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.426	1857	1860	1863	rVB3	1772	1912	0.14%	0.016%
78	12.469	1863	1867	1874	rVB3	2639	4135	0.31%	0.034%
79	12.548	1874	1880	1887	rBV7	4023	8743	0.65%	0.072%
80	12.615	1888	1891	1896	rVB3	3297	3724	0.28%	0.031%
81	12.713	1903	1907	1916	rVB6	1618	3714	0.28%	0.031%
82	12.798	1916	1921	1923	rBV2	867	1105	0.08%	0.009%
83	12.853	1927	1930	1933	rVB3	1134	1207	0.09%	0.010%
84	12.920	1939	1941	1945	rVB2	1270	1353	0.10%	0.011%
85	12.963	1945	1948	1955	rVB3	3290	4200	0.31%	0.035%
86	13.048	1955	1962	1968	rBV5	1093	2306	0.17%	0.019%
87	13.286	1998	2001	2007	rVB3	2473	3528	0.26%	0.029%
88	13.426	2021	2024	2026	rVB2	440	483	0.04%	0.004%
89	13.475	2026	2032	2033	rBV2	324	390	0.03%	0.003%
90	13.585	2047	2050	2055	rBV4	993	1479	0.11%	0.012%
91	13.713	2069	2071	2073	rBV	426	361	0.03%	0.003%
92	13.774	2079	2081	2088	rVB2	964	1621	0.12%	0.013%
93	14.133	2137	2140	2144	rBV3	1328	1708	0.13%	0.014%
94	14.261	2159	2161	2164	rVB2	871	705	0.05%	0.006%
95	14.359	2175	2177	2179	rBV3	351	338	0.03%	0.003%
96	14.786	2246	2247	2250	rBV2	473	545	0.04%	0.004%
97	15.267	2325	2326	2328	rBV2	578	402	0.03%	0.003%
98	15.493	2361	2363	2367	rVB3	657	623	0.05%	0.005%
99	16.029	2449	2451	2452	rBV	575	395	0.03%	0.003%
100	16.377	2506	2508	2510	rBV	602	516	0.04%	0.004%




Sum of corrected areas: 12112092

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029487.D
Acq On : 14 Jun 2022 23:53
Operator : JC/MD
Sample : N3248-20 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

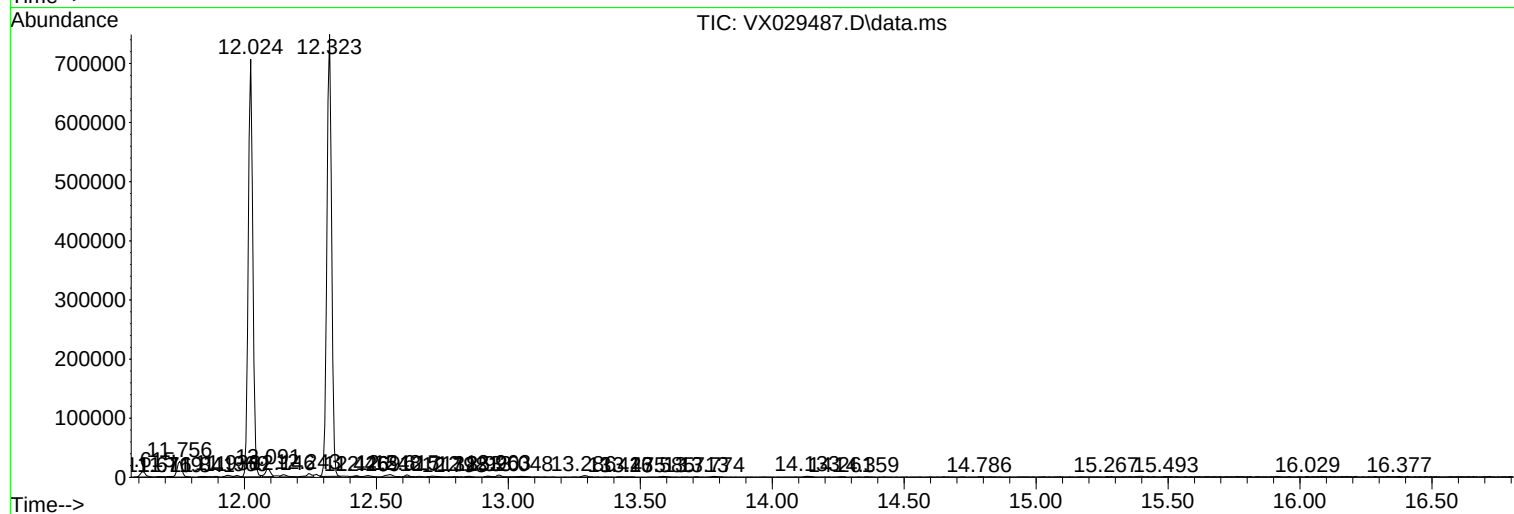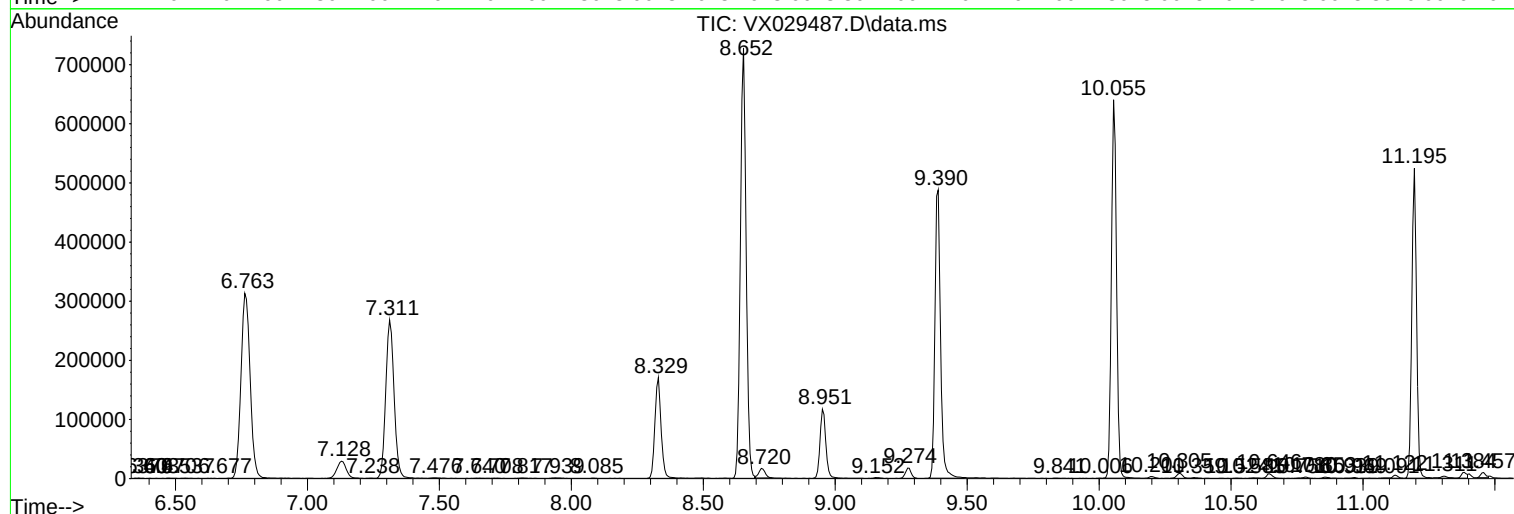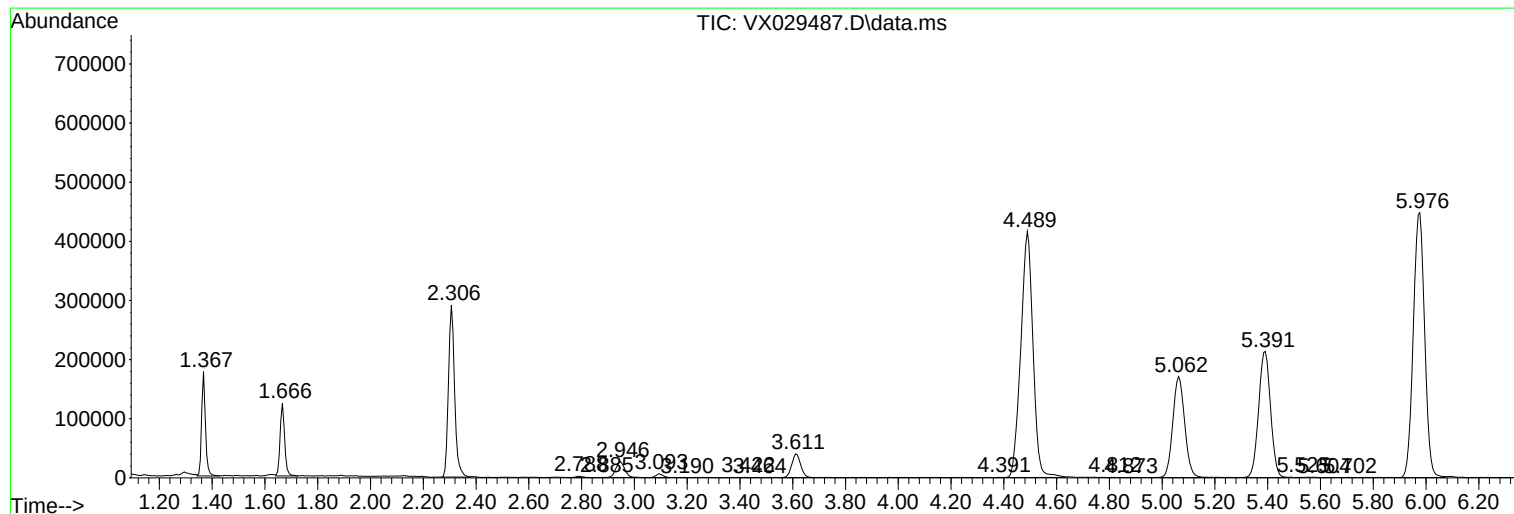

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029487.D
Acq On : 14 Jun 2022 23:53
Operator : JC/MD
Sample : N3248-20 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029487.D
Acq On : 14 Jun 2022 23:53
Operator : JC/MD
Sample : N3248-20 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc