

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029490.D
 Acq On : 15 Jun 2022 01:02
 Operator : JC/MD
 Sample : N3248-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rVB	172565	174436	5.57%	1.024%
2	1.666	91	95	102	rVB	130718	152335	4.86%	0.894%
3	2.306	194	200	211	rBV2	302178	523823	16.71%	3.075%
4	2.550	238	240	241	rBV	470	286	0.01%	0.002%
5	2.794	275	280	283	rBV4	1140	1838	0.06%	0.011%
6	2.940	301	304	307	rBV4	658	1075	0.03%	0.006%
7	3.093	323	329	340	rVB2	18191	36025	1.15%	0.211%
8	3.221	347	350	351	rBV2	395	298	0.01%	0.002%
9	3.343	368	370	371	rBV2	339	261	0.01%	0.002%
10	3.611	403	414	432	rVV	417113	973533	31.06%	5.715%
11	3.830	449	450	458	rVB3	357	571	0.02%	0.003%
12	3.885	458	459	462	rBV2	356	255	0.01%	0.001%
13	3.934	464	467	468	rBV2	315	349	0.01%	0.002%
14	3.983	474	475	479	rBV3	242	313	0.01%	0.002%
15	4.489	544	558	579	rBV2	990903	2899006	92.50%	17.018%
16	4.751	599	601	605	rBV3	384	297	0.01%	0.002%
17	4.910	624	627	628	rVB	300	268	0.01%	0.002%
18	4.928	628	630	631	rBV	395	284	0.01%	0.002%
19	5.062	638	652	671	rBV	167840	526643	16.80%	3.092%
20	5.275	685	687	690	rBV3	255	243	0.01%	0.001%
21	5.391	690	706	723	rBV	1002794	3134195	100.00%	18.398%
22	5.580	736	737	740	rVB2	754	435	0.01%	0.003%
23	5.666	748	751	752	rBV2	334	319	0.01%	0.002%
24	5.976	789	802	817	rBV2	444243	1310699	41.82%	7.694%
25	6.239	843	845	848	rVB	407	298	0.01%	0.002%
26	6.330	857	860	861	rBV2	414	425	0.01%	0.002%
27	6.507	888	889	891	rBV2	306	251	0.01%	0.001%
28	6.550	893	896	898	rBV3	399	483	0.02%	0.003%
29	6.763	922	931	944	rBV	326414	773458	24.68%	4.540%
30	7.049	976	978	980	rBV2	304	341	0.01%	0.002%
31	7.129	982	991	1003	rVB2	53907	123685	3.95%	0.726%
32	7.214	1003	1005	1007	rBV2	314	251	0.01%	0.001%
33	7.312	1012	1021	1037	rVV	264032	578752	18.47%	3.397%
34	7.946	1119	1125	1127	rBV3	954	1396	0.04%	0.008%
35	8.080	1145	1147	1153	rVB2	449	557	0.02%	0.003%
36	8.189	1162	1165	1167	rVB	489	487	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029490.D
 Acq On : 15 Jun 2022 01:02
 Operator : JC/MD
 Sample : N3248-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	8.220	1167	1170	1171	rBV	309	306	0.01%	0.002%
38	8.330	1181	1188	1200	rVV	167601	275326	8.78%	1.616%
39	8.653	1234	1241	1248	rBV	689976	1086514	34.67%	6.378%
40	8.720	1249	1252	1260	rVB	9681	16888	0.54%	0.099%
41	8.952	1283	1290	1303	rBV	124930	186778	5.96%	1.096%
42	9.043	1303	1305	1306	rVV2	688	472	0.02%	0.003%
43	9.061	1306	1308	1314	rVV3	571	700	0.02%	0.004%
44	9.110	1314	1316	1319	rVV2	315	345	0.01%	0.002%
45	9.159	1319	1324	1329	rVB4	3166	4248	0.14%	0.025%
46	9.275	1337	1343	1351	rVB	113324	165160	5.27%	0.970%
47	9.384	1356	1361	1376	rBV	466599	686680	21.91%	4.031%
48	9.927	1449	1450	1452	rVV	424	280	0.01%	0.002%
49	10.012	1459	1464	1465	rBV2	302	422	0.01%	0.002%
50	10.055	1465	1471	1485	rBV	674805	899233	28.69%	5.279%
51	10.201	1492	1495	1499	rVB3	760	1098	0.04%	0.006%
52	10.250	1502	1503	1505	rBV	514	296	0.01%	0.002%
53	10.305	1509	1512	1517	rVB2	1909	2549	0.08%	0.015%
54	10.512	1544	1546	1548	rVB2	293	259	0.01%	0.002%
55	10.561	1551	1554	1555	rBV	323	295	0.01%	0.002%
56	10.652	1565	1569	1574	rVB4	751	1036	0.03%	0.006%
57	10.756	1584	1586	1589	rVB2	502	379	0.01%	0.002%
58	10.854	1599	1602	1603	rBV2	264	245	0.01%	0.001%
59	10.921	1611	1613	1617	rVB	338	342	0.01%	0.002%
60	10.957	1617	1619	1622	rBV2	755	754	0.02%	0.004%
61	11.012	1626	1628	1630	rVB	547	363	0.01%	0.002%
62	11.091	1639	1641	1642	rBV	608	508	0.02%	0.003%
63	11.122	1642	1646	1650	rVB	4291	5480	0.17%	0.032%
64	11.195	1652	1658	1669	rBV	503254	647864	20.67%	3.803%
65	11.347	1682	1683	1686	rBV	503	329	0.01%	0.002%
66	11.384	1686	1689	1692	rBV2	700	869	0.03%	0.005%
67	11.451	1698	1700	1703	rBV4	1412	1812	0.06%	0.011%
68	11.555	1713	1717	1718	rBV2	567	662	0.02%	0.004%
69	11.616	1723	1727	1730	rBV4	1432	2028	0.06%	0.012%
70	11.671	1734	1736	1737	rVV	451	366	0.01%	0.002%
71	11.689	1737	1739	1741	rVV	779	679	0.02%	0.004%
72	11.707	1741	1742	1744	rVV	641	569	0.02%	0.003%
73	11.756	1746	1750	1755	rVB2	7686	10471	0.33%	0.061%
74	11.792	1755	1756	1760	rBV	320	421	0.01%	0.002%
75	11.841	1762	1764	1768	rVB2	1150	910	0.03%	0.005%
76	11.933	1776	1779	1783	rVB3	2040	2730	0.09%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029490.D
 Acq On : 15 Jun 2022 01:02
 Operator : JC/MD
 Sample : N3248-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	11.975	1783	1786	1788	rBV3	481	582	0.02%	0.003%
78	12.024	1788	1794	1802	rBV	717632	881631	28.13%	5.175%
79	12.225	1825	1827	1828	rBV2	442	263	0.01%	0.002%
80	12.250	1828	1831	1835	rVB3	2981	3684	0.12%	0.022%
81	12.323	1837	1843	1851	rVV	722132	909723	29.03%	5.340%
82	12.427	1857	1860	1865	rVB3	1915	2226	0.07%	0.013%
83	12.615	1889	1891	1892	rBV2	440	331	0.01%	0.002%
84	12.664	1896	1899	1901	rBV2	843	827	0.03%	0.005%
85	12.823	1923	1925	1927	rVB2	405	344	0.01%	0.002%
86	13.061	1959	1964	1965	rBV2	1092	1301	0.04%	0.008%
87	13.115	1971	1973	1975	rBV	528	332	0.01%	0.002%
88	13.475	2029	2032	2033	rBV2	230	272	0.01%	0.002%
89	13.493	2033	2035	2038	rVV2	289	373	0.01%	0.002%
90	13.731	2071	2074	2075	rBV2	313	315	0.01%	0.002%
91	13.780	2078	2082	2087	rVB3	1611	2103	0.07%	0.012%
92	13.884	2097	2099	2101	rBV2	311	263	0.01%	0.002%
93	14.127	2136	2139	2145	rVB2	858	1276	0.04%	0.007%
94	14.640	2220	2223	2228	rBV3	810	1405	0.04%	0.008%
95	14.713	2233	2235	2238	rVV2	624	587	0.02%	0.003%
96	14.743	2238	2240	2242	rVV	573	396	0.01%	0.002%
97	14.780	2242	2246	2247	rVB2	554	578	0.02%	0.003%
98	14.847	2256	2257	2260	rBV2	369	277	0.01%	0.002%
99	14.938	2270	2272	2273	rBV2	513	441	0.01%	0.003%
100	15.036	2285	2288	2291	rBV	606	721	0.02%	0.004%

Sum of corrected areas: 17035088




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029490.D
Acq On : 15 Jun 2022 01:02
Operator : JC/MD
Sample : N3248-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

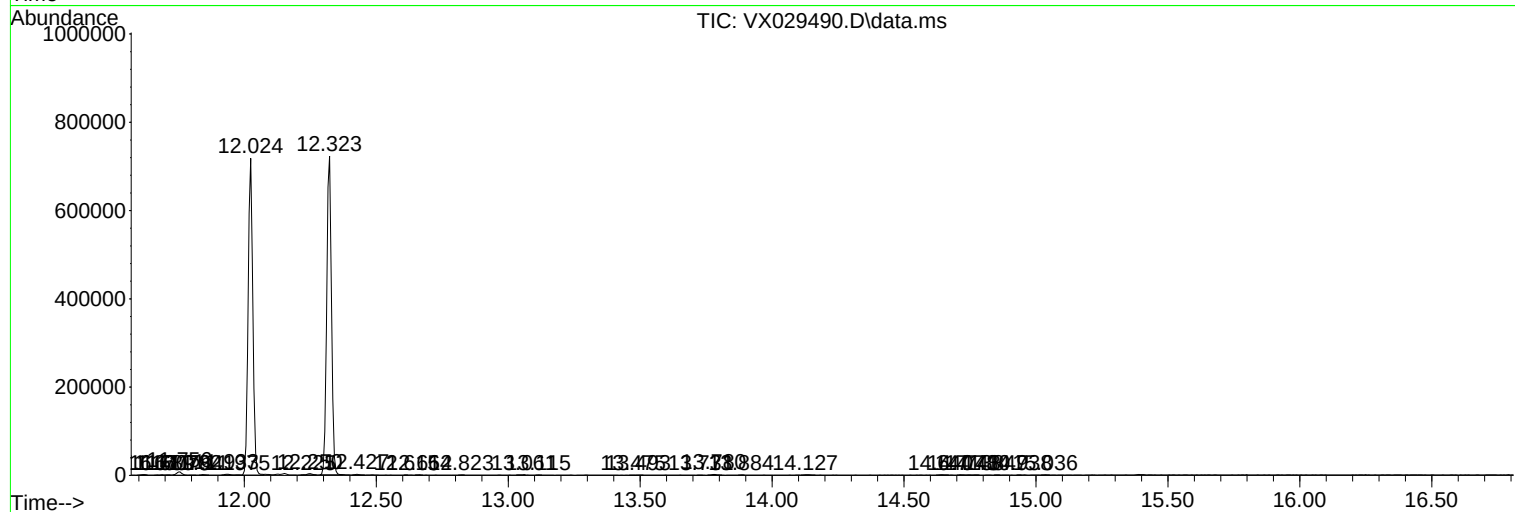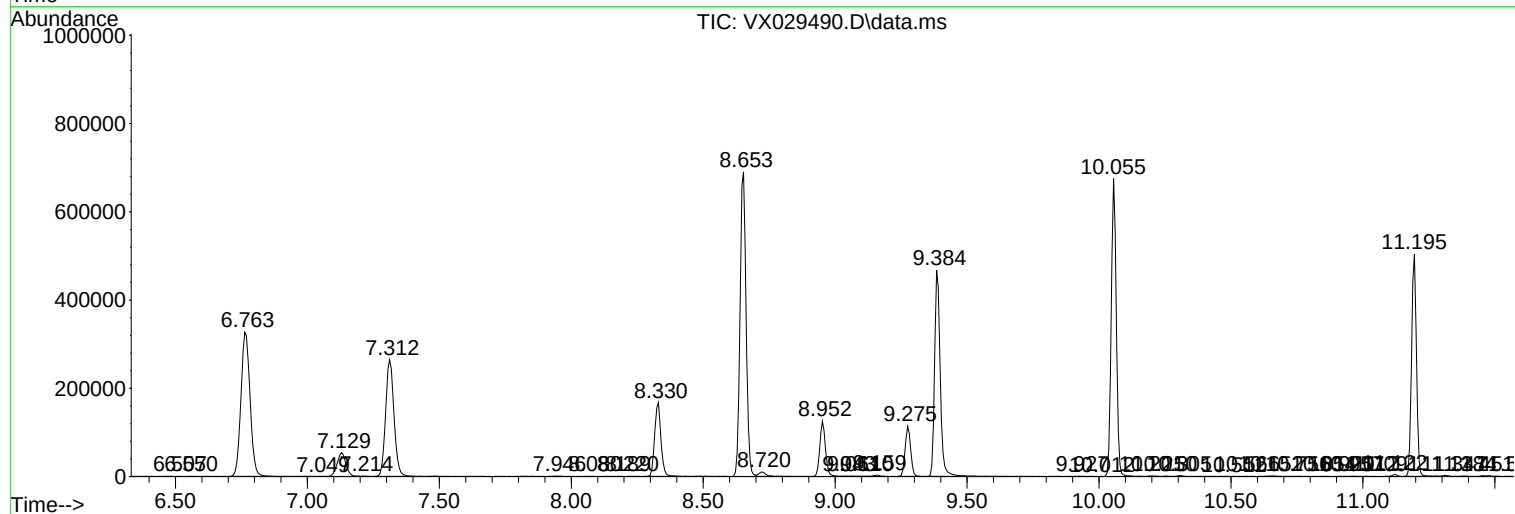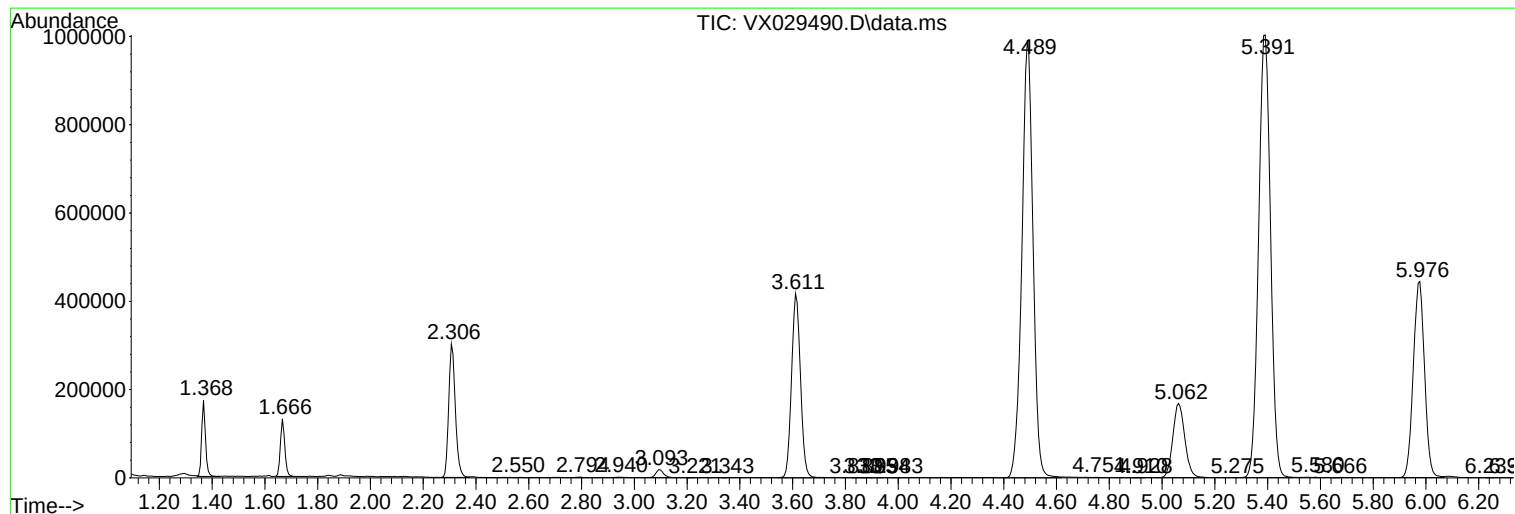

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029490.D
Acq On : 15 Jun 2022 01:02
Operator : JC/MD
Sample : N3248-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029490.D
Acq On : 15 Jun 2022 01:02
Operator : JC/MD
Sample : N3248-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc