

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029491.D
 Acq On : 15 Jun 2022 01:26
 Operator : JC/MD
 Sample : N3248-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029491.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rVB	176679	174218	13.20%	1.740%
2	1.666	91	95	103	rVB	133145	157791	11.96%	1.576%
3	2.307	194	200	211	rBV	286933	452205	34.27%	4.518%
4	2.654	255	257	260	rVB2	361	273	0.02%	0.003%
5	2.684	260	262	263	rBV	275	269	0.02%	0.003%
6	2.703	263	265	267	rBV3	464	510	0.04%	0.005%
7	2.788	274	279	286	rVB3	2155	4062	0.31%	0.041%
8	2.880	291	294	295	rVV3	293	285	0.02%	0.003%
9	2.947	295	305	314	rVV	21287	49799	3.77%	0.498%
10	3.184	342	344	346	rBV2	321	294	0.02%	0.003%
11	3.288	359	361	362	rBV	286	266	0.02%	0.003%
12	3.440	384	386	388	rVB	327	282	0.02%	0.003%
13	3.465	388	390	391	rBV2	376	308	0.02%	0.003%
14	3.575	405	408	410	rVB2	281	264	0.02%	0.003%
15	3.965	468	472	473	rBV2	281	358	0.03%	0.004%
16	4.026	478	482	483	rVV2	286	256	0.02%	0.003%
17	4.324	530	531	533	rBV	397	292	0.02%	0.003%
18	4.465	543	554	568	rBV	102540	306380	23.22%	3.061%
19	4.800	607	609	613	rBV	281	259	0.02%	0.003%
20	5.062	639	652	672	rBV	172588	529297	40.11%	5.288%
21	5.215	675	677	679	rVV2	452	382	0.03%	0.004%
22	5.385	700	705	709	rBV4	890	1707	0.13%	0.017%
23	5.507	723	725	728	rVB3	299	290	0.02%	0.003%
24	5.550	728	732	739	rBV3	542	1087	0.08%	0.011%
25	5.605	739	741	743	rBV2	271	282	0.02%	0.003%
26	5.970	789	801	819	rBV2	445042	1319600	100.00%	13.183%
27	6.300	851	855	858	rBV2	264	307	0.02%	0.003%
28	6.373	864	867	870	rVB	450	576	0.04%	0.006%
29	6.489	883	886	888	rBV2	233	259	0.02%	0.003%
30	6.592	899	903	905	rVB2	245	367	0.03%	0.004%
31	6.659	911	914	917	rVB3	258	363	0.03%	0.004%
32	6.690	917	919	922	rBV	233	309	0.02%	0.003%
33	6.763	922	931	948	rBV	314892	759753	57.57%	7.590%
34	7.129	982	991	1001	rBV5	18253	46195	3.50%	0.461%
35	7.312	1012	1021	1036	rBV2	264784	580852	44.02%	5.803%
36	7.482	1046	1049	1054	rBV3	936	1539	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029491.D
 Acq On : 15 Jun 2022 01:26
 Operator : JC/MD
 Sample : N3248-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.787	1094	1099	1100	rBV2	275	442	0.03%	0.004%
38	7.806	1100	1102	1105	rBV3	502	505	0.04%	0.005%
39	7.836	1105	1107	1115	rVB2	411	500	0.04%	0.005%
40	7.934	1121	1123	1125	rBV2	649	671	0.05%	0.007%
41	8.275	1176	1179	1181	rBV2	381	361	0.03%	0.004%
42	8.330	1181	1188	1201	rBV	163442	272247	20.63%	2.720%
43	8.482	1211	1213	1215	rBV2	458	347	0.03%	0.003%
44	8.580	1226	1229	1234	rBV3	507	740	0.06%	0.007%
45	8.653	1234	1241	1249	rBV	700289	1095072	82.99%	10.940%
46	8.726	1249	1253	1260	rVB	9934	16853	1.28%	0.168%
47	8.952	1284	1290	1301	rBV	113805	166975	12.65%	1.668%
48	9.116	1316	1317	1321	rBV3	267	270	0.02%	0.003%
49	9.214	1328	1333	1338	rBV3	379	671	0.05%	0.007%
50	9.275	1340	1343	1347	rBV2	2838	3869	0.29%	0.039%
51	9.385	1356	1361	1382	rBV	452739	674198	51.09%	6.735%
52	9.702	1410	1413	1421	rVB4	2009	3065	0.23%	0.031%
53	9.958	1454	1455	1458	rBV2	297	268	0.02%	0.003%
54	10.006	1460	1463	1465	rVB3	449	485	0.04%	0.005%
55	10.055	1465	1471	1485	rBV	679002	889506	67.41%	8.886%
56	10.201	1491	1495	1500	rVB4	597	934	0.07%	0.009%
57	10.305	1507	1512	1517	rBV3	1424	2507	0.19%	0.025%
58	10.409	1527	1529	1531	rBV	396	365	0.03%	0.004%
59	10.525	1547	1548	1550	rBV2	299	315	0.02%	0.003%
60	10.646	1564	1568	1572	rBV4	724	1083	0.08%	0.011%
61	10.720	1577	1580	1582	rBV	244	293	0.02%	0.003%
62	10.750	1582	1585	1588	rVB3	309	362	0.03%	0.004%
63	10.909	1608	1611	1617	rVB2	280	429	0.03%	0.004%
64	11.122	1642	1646	1652	rVB	4153	5302	0.40%	0.053%
65	11.195	1652	1658	1669	rBV	513995	647768	49.09%	6.471%
66	11.457	1695	1701	1702	rBV3	978	1149	0.09%	0.011%
67	11.476	1702	1704	1712	rVB5	1400	2754	0.21%	0.028%
68	11.549	1714	1716	1719	rVB3	488	428	0.03%	0.004%
69	11.677	1736	1737	1740	rBV3	423	420	0.03%	0.004%
70	11.719	1740	1744	1745	rVV3	562	610	0.05%	0.006%
71	11.750	1745	1749	1754	rVB2	5360	7126	0.54%	0.071%
72	11.841	1761	1764	1768	rVB3	979	1120	0.08%	0.011%
73	11.933	1775	1779	1783	rBV4	2135	2938	0.22%	0.029%
74	11.976	1783	1786	1788	rVV2	527	659	0.05%	0.007%
75	12.024	1788	1794	1806	rVV	718465	867371	65.73%	8.665%
76	12.128	1806	1811	1812	rVV4	1960	3321	0.25%	0.033%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029491.D
 Acq On : 15 Jun 2022 01:26
 Operator : JC/MD
 Sample : N3248-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.152	1812	1815	1819	rVV2	3520	4695	0.36%	0.047%
78	12.256	1831	1832	1834	rBV	394	291	0.02%	0.003%
79	12.323	1837	1843	1851	rVV	721447	919589	69.69%	9.187%
80	12.427	1857	1860	1865	rVB4	1499	1994	0.15%	0.020%
81	12.469	1865	1867	1868	rBV2	715	723	0.05%	0.007%
82	12.664	1896	1899	1902	rBV3	1034	1194	0.09%	0.012%
83	12.762	1913	1915	1922	rVB5	1265	1859	0.14%	0.019%
84	12.859	1929	1931	1935	rVV2	371	566	0.04%	0.006%
85	12.927	1938	1942	1945	rVB3	409	588	0.04%	0.006%
86	13.128	1972	1975	1979	rVB3	373	566	0.04%	0.006%
87	13.158	1979	1980	1983	rBV3	442	454	0.03%	0.005%
88	13.725	2071	2073	2075	rBV2	300	283	0.02%	0.003%
89	13.780	2079	2082	2087	rVB3	566	943	0.07%	0.009%
90	13.902	2101	2102	2106	rBV2	296	292	0.02%	0.003%
91	14.073	2128	2130	2134	rBV2	381	589	0.04%	0.006%
92	14.134	2134	2140	2146	rBV2	2500	4342	0.33%	0.043%
93	14.207	2149	2152	2154	rBV2	363	340	0.03%	0.003%
94	14.249	2157	2159	2160	rBV	301	266	0.02%	0.003%
95	14.286	2163	2165	2167	rBV	342	416	0.03%	0.004%
96	14.688	2229	2231	2233	rBV2	337	264	0.02%	0.003%
97	14.975	2276	2278	2281	rBV	581	452	0.03%	0.005%
98	15.133	2303	2304	2306	rBV	436	313	0.02%	0.003%
99	15.396	2342	2347	2354	rBV5	752	1934	0.15%	0.019%
100	16.633	2547	2550	2552	rBV4	783	1038	0.08%	0.010%




Sum of corrected areas: 10009826

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029491.D
Acq On : 15 Jun 2022 01:26
Operator : JC/MD
Sample : N3248-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

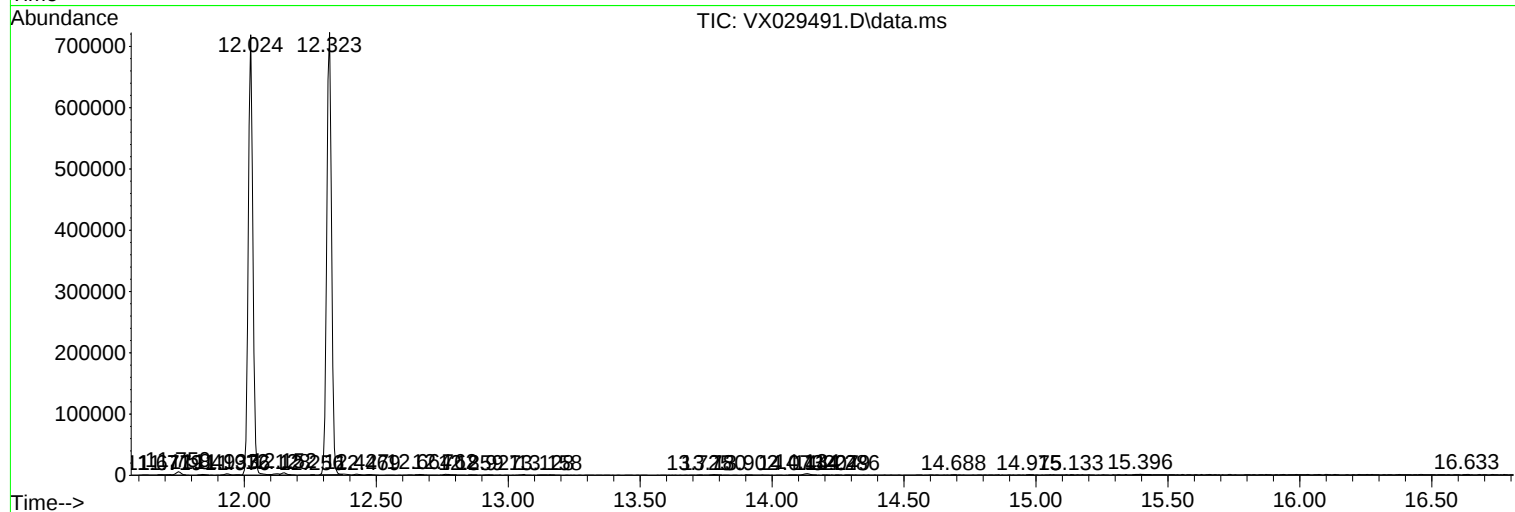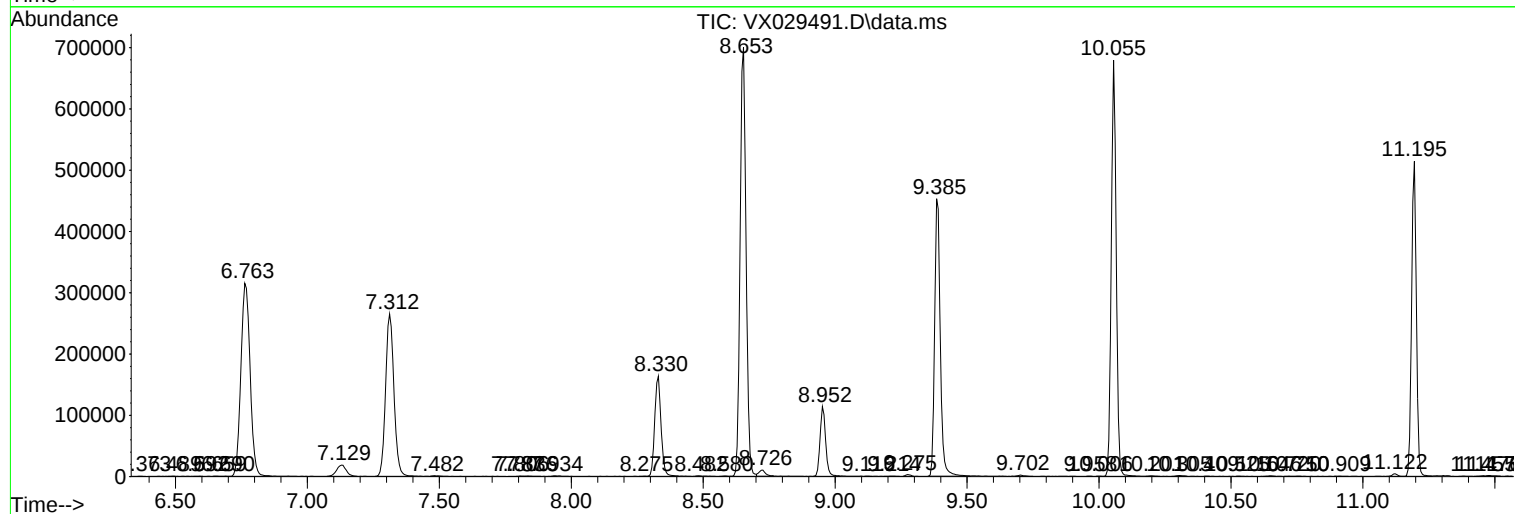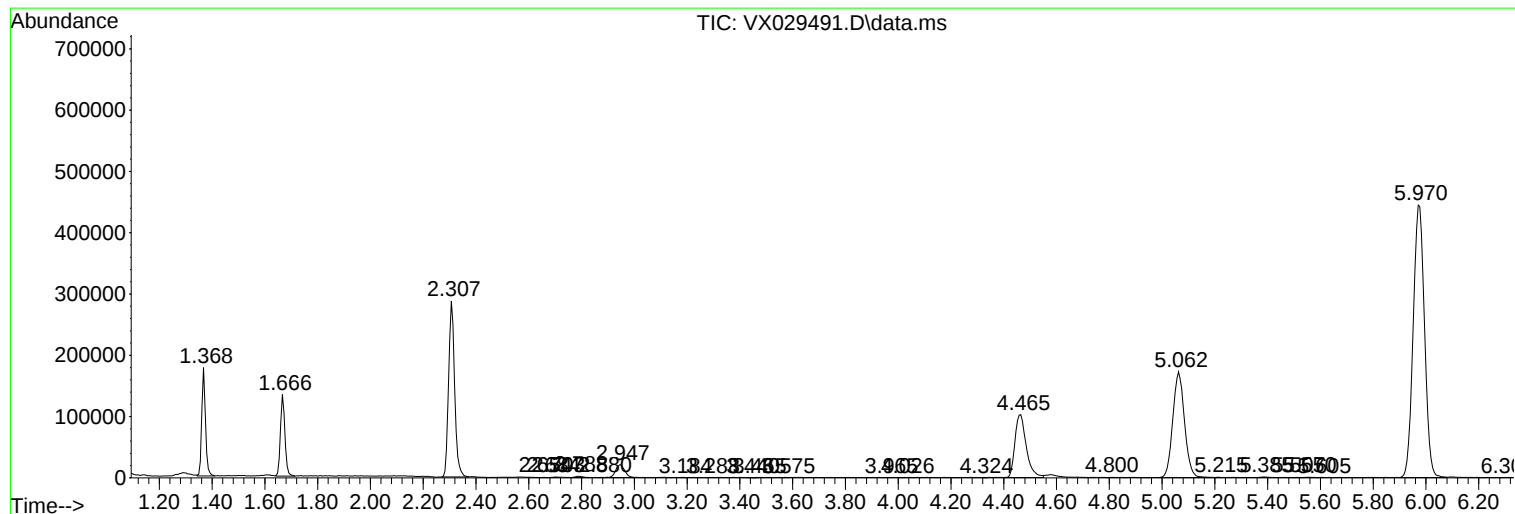

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029491.D
Acq On : 15 Jun 2022 01:26
Operator : JC/MD
Sample : N3248-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029491.D
Acq On : 15 Jun 2022 01:26
Operator : JC/MD
Sample : N3248-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc