
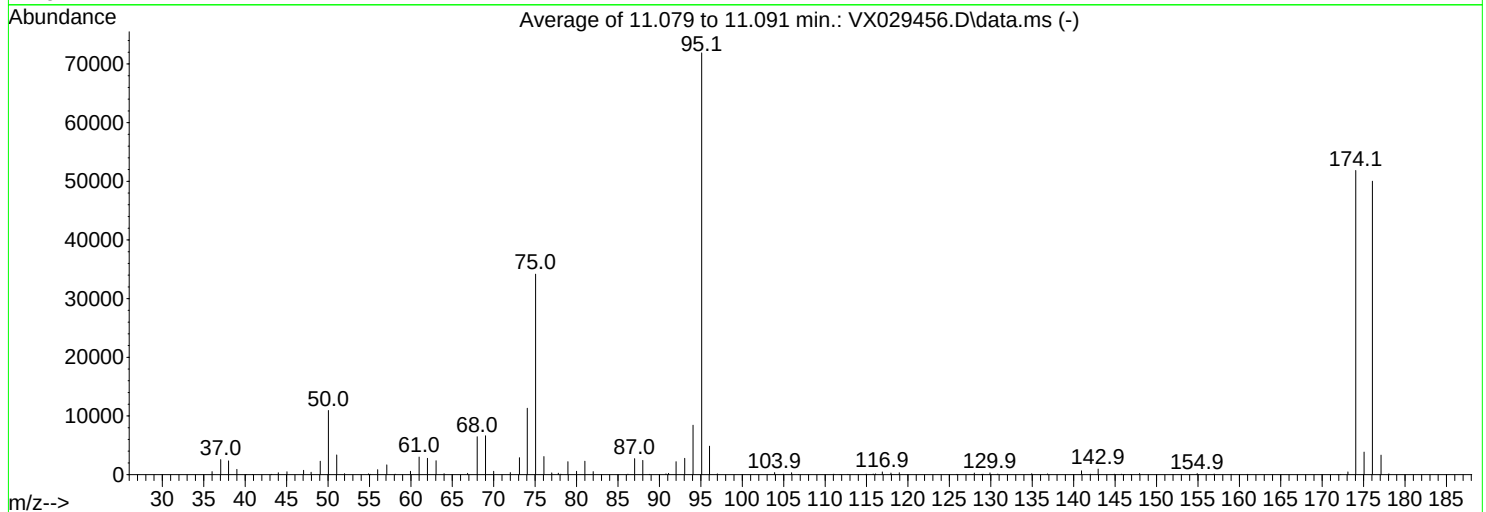


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029456.D
 Acq On : 14 Jun 2022 09:31
 Operator : JC/MD
 Sample : BFB637
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB637

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM061322WMA.M
 Title : VOC Analysis
 Last Update : Wed Jun 15 07:14:08 2022

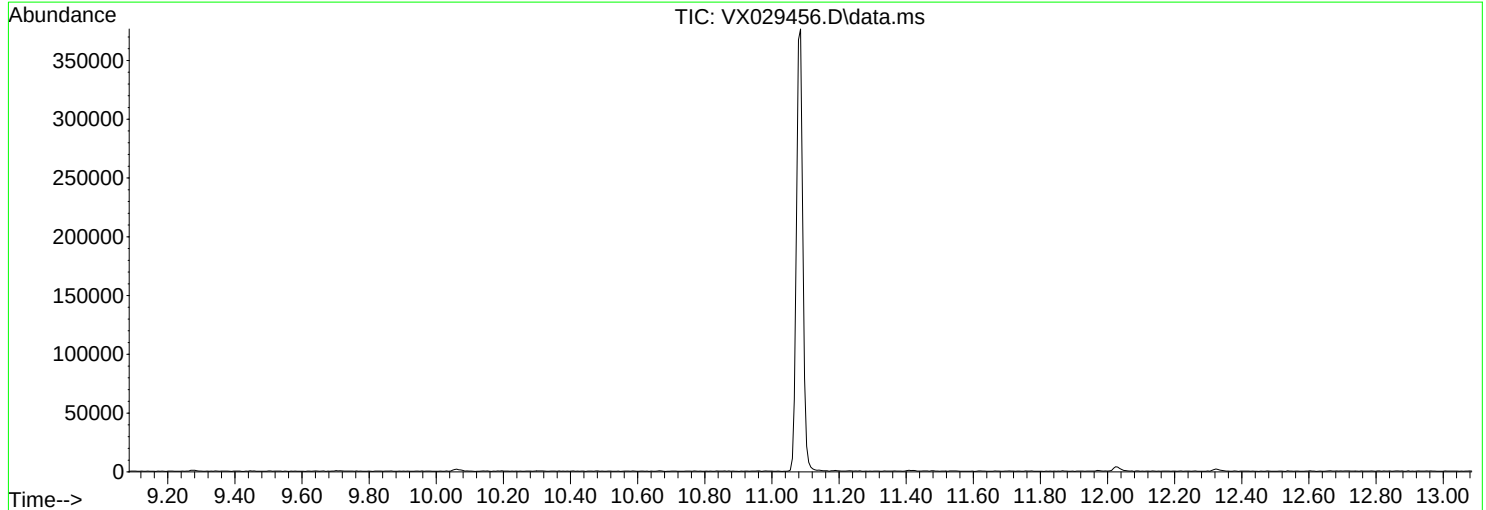

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	10927	PASS
75	95	30	80	47.5	34163	PASS
95	95	100	100	100.0	71893	PASS
96	95	5	9	6.8	4858	PASS
173	174	0.00	2	0.9	466	PASS
174	95	50	120	72.1	51848	PASS
175	174	5	9	7.4	3842	PASS
176	174	95	101	96.5	50013	PASS
177	176	5	9	6.7	3326	PASS

m/z	Abundance
40.00	357.0
44.00	218.0

Instrument :
MSVOA_X
ClientSampleId :
BFB637

m/z	Abundance
36.00	596.0
37.10	3354.0
38.00	2869.0
39.00	1151.0
40.00	406.0
44.00	587.0
45.10	669.0
47.10	1072.0
47.90	505.0
49.00	3243.0
50.10	14225.0
51.00	4273.0
52.00	163.0
54.90	251.0
56.00	1219.0
57.10	1743.0
58.20	135.0
60.00	686.0
61.00	3786.0
62.00	3266.0
63.10	2909.0
64.00	177.0
66.80	335.0
68.00	7866.0
69.00	8213.0
70.00	649.0
72.00	332.0
73.10	3321.0
74.00	14007.0
75.00	40768.0
76.00	3972.0
77.10	554.0
77.80	294.0
78.10	286.0
78.90	2609.0
80.00	620.0
81.00	2651.0
82.00	710.0
87.00	3023.0
88.00	2892.0
88.80	142.0
90.80	254.0
91.20	264.0
92.00	2793.0
93.00	3162.0
94.00	10078.0
95.10	83928.0
96.00	6449.0
97.00	223.0
103.90	360.0
105.00	73.0
105.90	461.0
106.80	59.0
111.10	74.0
112.70	84.0
116.10	327.0
117.00	548.0
118.00	370.0
118.90	428.0
125.90	58.0
128.10	297.0
128.90	72.0
129.10	74.0
129.80	373.0
131.00	88.0
134.90	168.0
136.80	95.0
141.00	834.0
142.00	90.0
142.90	1051.0
144.90	153.0
145.80	53.0
146.10	65.0
146.90	104.0
148.00	190.0
150.00	62.0
153.00	54.0
154.90	220.0
156.90	88.0
160.90	67.0
172.20	126.0
173.10	521.0
174.00	52824.0
175.10	4179.0
176.00	51560.0
177.10	3499.0
178.10	109.0

Instrument :
MSVOA_X
ClientSampleId :
BFB637

m/z	Abundance
36.00	705.0
37.00	2733.0
38.00	2696.0
39.00	1020.0
40.00	339.0
40.90	50.0
43.20	82.0
44.00	674.0
45.00	577.0
47.00	835.0
48.00	523.0
49.10	2188.0
50.00	12412.0
51.10	3964.0
52.00	248.0
55.10	188.0
56.00	940.0
57.10	1975.0
58.00	99.0
59.90	783.0
61.00	3590.0
62.00	3407.0
63.00	2729.0
64.00	245.0
66.90	266.0
68.00	7731.0
69.00	7466.0
70.10	681.0
72.00	513.0
73.10	3478.0
74.10	13045.0
75.10	39216.0
76.10	3447.0
76.90	389.0
77.80	347.0
79.00	2579.0
80.00	753.0
81.00	2624.0
82.00	579.0
83.00	59.0
86.20	120.0
87.00	3251.0
88.00	2979.0
91.00	394.0
92.00	2386.0
93.10	3312.0
94.10	9637.0
95.10	84192.0
96.10	5604.0
97.00	109.0
103.90	533.0
105.00	79.0
106.00	392.0
106.80	69.0
111.00	125.0
111.80	60.0
112.80	113.0
114.90	165.0
115.80	299.0
116.80	574.0
117.90	237.0
119.00	333.0
125.90	88.0
127.90	359.0
129.00	210.0
129.90	333.0
130.80	132.0
134.90	135.0
136.90	207.0
140.00	60.0
141.00	663.0
142.00	126.0
143.00	1070.0
144.90	111.0
145.80	148.0
147.90	205.0
150.00	55.0
152.00	106.0
153.10	78.0
155.00	217.0
156.90	154.0
159.00	88.0
161.00	94.0
171.90	105.0
173.10	640.0
174.10	62632.0
175.00	4341.0
176.00	58736.0
177.10	4359.0
178.00	170.0

Instrument :
MSVOA_X
ClientSampleId :
BFB637

m/z	Abundance
36.00	293.0
37.10	1603.0
38.10	1457.0
39.00	500.0
40.10	364.0
43.10	51.0
44.00	388.0
44.90	241.0
47.10	336.0
48.00	209.0
49.10	1470.0
50.00	6143.0
51.10	1830.0
52.00	65.0
54.90	129.0
56.00	405.0
57.10	1318.0
59.90	278.0
61.00	1650.0
62.00	1692.0
63.00	1459.0
64.10	103.0
66.80	76.0
68.00	3824.0
69.00	4241.0
69.90	384.0
72.10	213.0
73.00	1923.0
74.10	6950.0
75.00	22504.0
76.00	1807.0
77.80	99.0
79.00	1441.0
80.00	381.0
80.90	1575.0
82.00	284.0
86.20	107.0
87.10	1897.0
88.00	1459.0
90.80	175.0
92.00	1448.0
93.00	1876.0
94.10	5595.0
95.10	47560.0
96.10	2522.0
97.00	115.0
104.00	198.0
104.90	68.0
105.80	136.0
111.00	68.0
115.00	62.0
116.10	120.0
116.90	299.0
117.90	178.0
118.90	235.0
128.00	159.0
128.90	82.0
130.00	209.0
130.80	85.0
135.00	222.0
136.80	85.0
140.90	507.0
143.00	734.0
145.80	75.0
147.90	188.0
153.10	58.0
154.80	162.0
157.00	106.0
159.00	79.0
173.10	238.0
174.00	40088.0
175.00	3005.0
176.10	39744.0
177.00	2121.0
178.10	110.0

Instrument :
MSVOA_X
ClientSampleId :
BFB637