

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061424\
 Data File : VX041892.D
 Acq On : 14 Jun 2024 20:54
 Operator : JC/MD
 Sample : P2807-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 240606041-01

Quant Time: Jun 15 04:17:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X061424W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Sat Jun 15 04:02:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	4.897	128	31853	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	6.763	114	167797	30.000	ug/l	0.00
57) Chlorobenzene-d5	10.055	117	152205	30.000	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	5.958	65	63742	29.070	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	96.900%
60) 4-Bromofluorobenzene	11.079	95	64072	27.195	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	90.667%
63) Toluene-d8	8.647	98	197120	30.271	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	100.900%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061424\
Data File : VX041892.D
Acq On : 14 Jun 2024 20:54
Operator : JC/MD
Sample : P2807-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
240606041-01

Quant Time: Jun 15 04:17:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X061424W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Sat Jun 15 04:02:59 2024
Response via : Initial Calibration




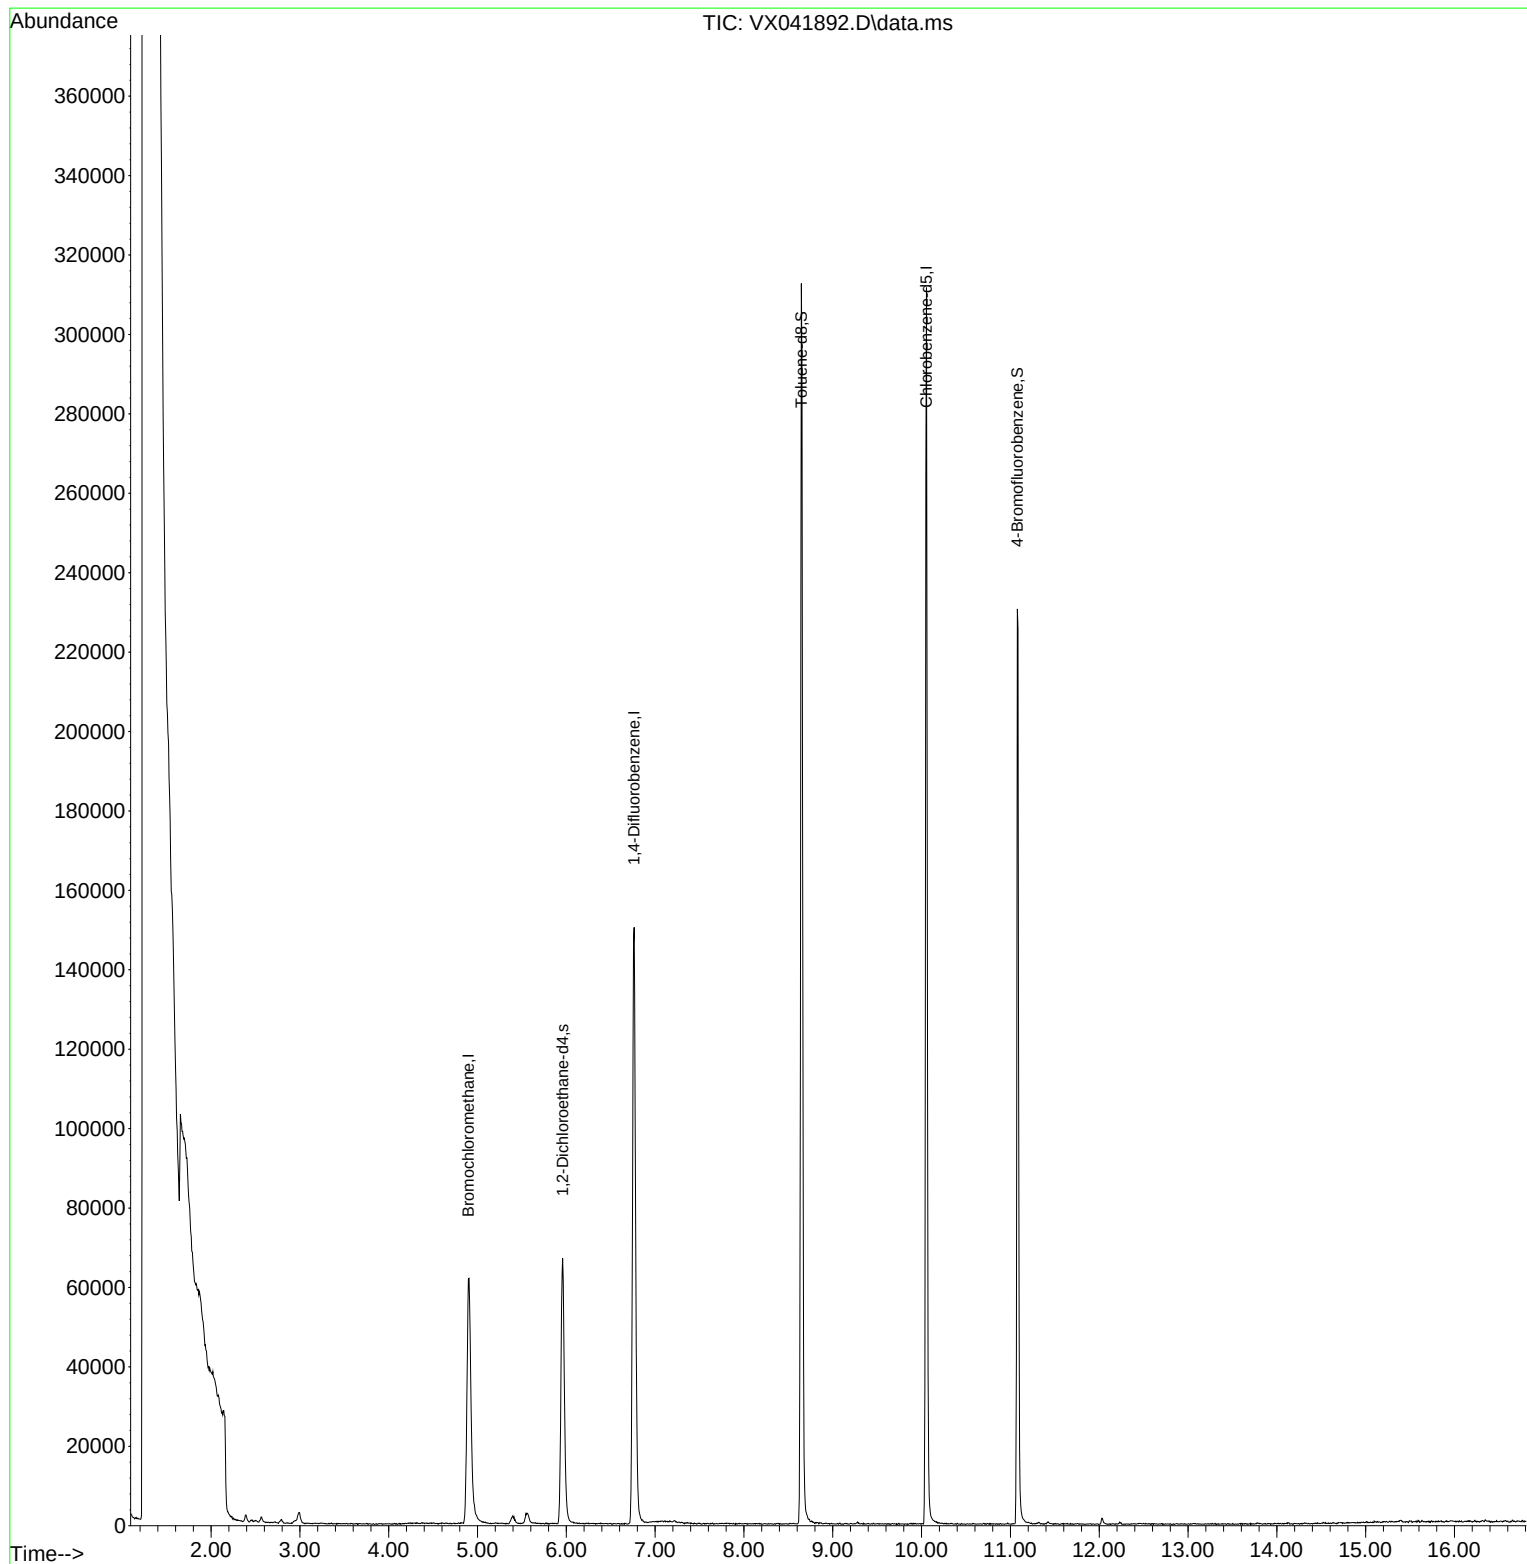


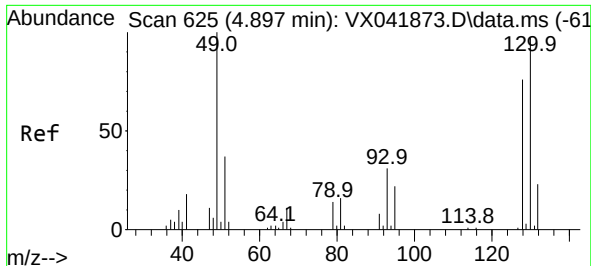

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 4.897 min Scan# 61
Delta R.T. 0.000 min
Lab File: VX041892.D
Acq: 14 Jun 2024 20:54




Instrument :
MSVOA_X
ClientSampleId :
240606041-01


Tgt Ion:128 Resp: 31853
Ion Ratio Lower Upper
128 100
49 137.5 0.0 338.5
130 131.3 0.0 324.5

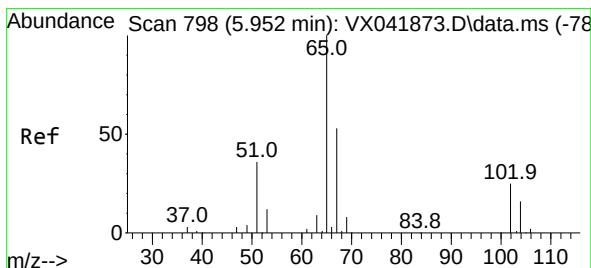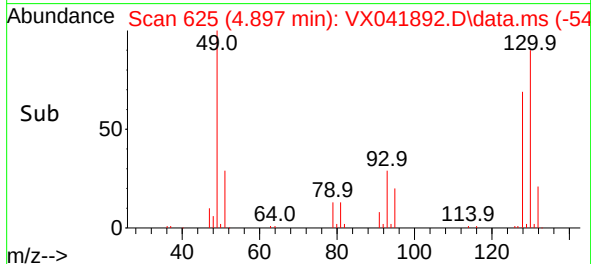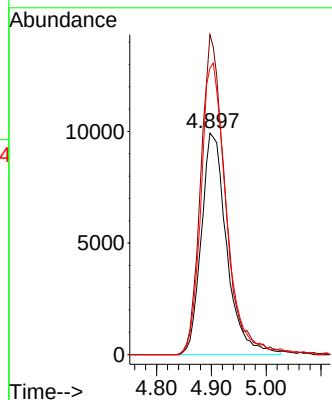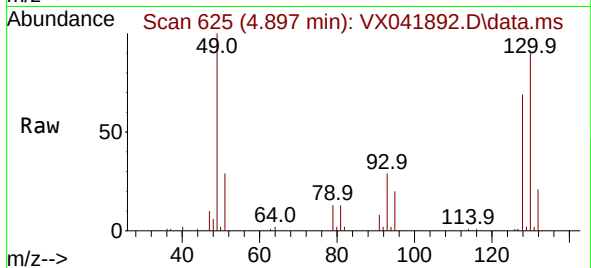

#27
1,2-Dichloroethane-d4
Concen: 29.070 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.006 min
Lab File: VX041892.D
Acq: 14 Jun 2024 20:54

Tgt Ion: 65 Resp: 63742
Ion Ratio Lower Upper
65 100
67 53.2 43.4 65.0

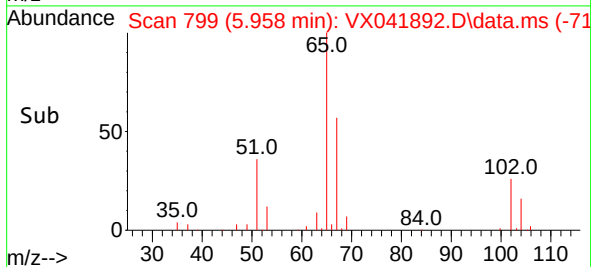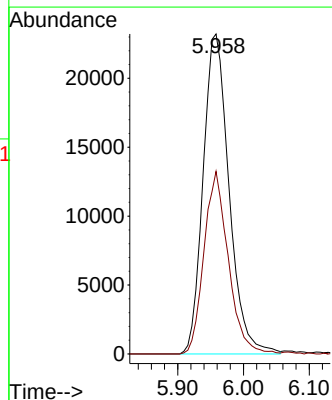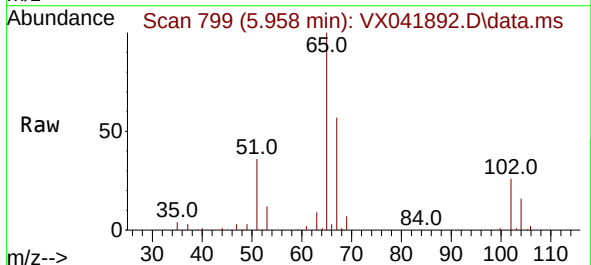

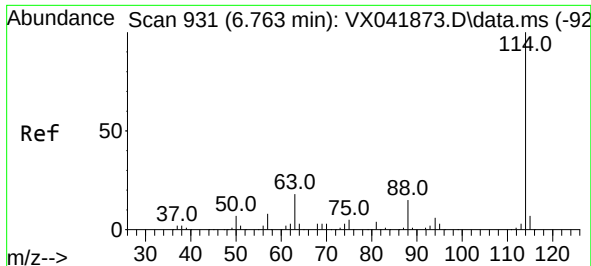

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 6.763 min Scan# 91

Delta R.T. -0.000 min

Lab File: VX041892.D

Acq: 14 Jun 2024 20:54

Instrument :

MSVOA_X

ClientSampleId :

240606041-01





Tgt Ion:114 Resp: 167797

Ion Ratio Lower Upper

114 100

63 18.2 14.6 21.8

88 15.2 11.8 17.8

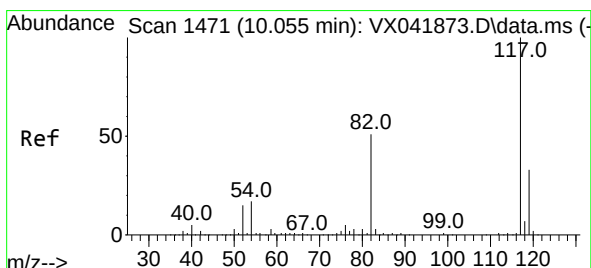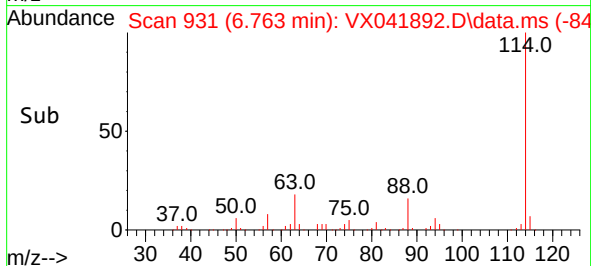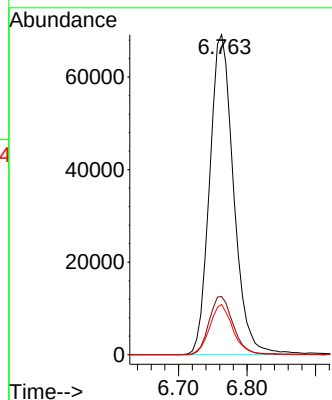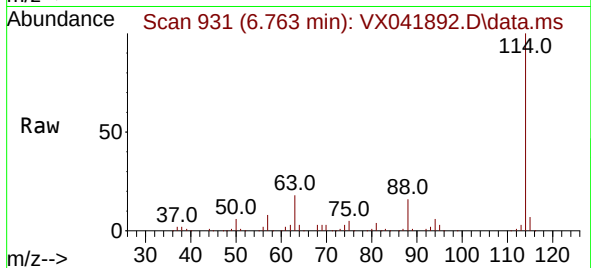

#57

Chlorobenzene-d5

Concen: 30.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX041892.D

Acq: 14 Jun 2024 20:54




Tgt Ion:117 Resp: 152205


Ion Ratio Lower Upper

117 100

82 51.4 41.1 61.7

119 32.7 26.1 39.1


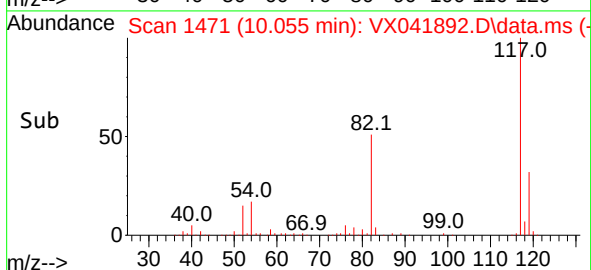
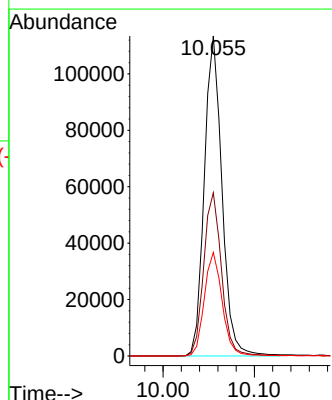
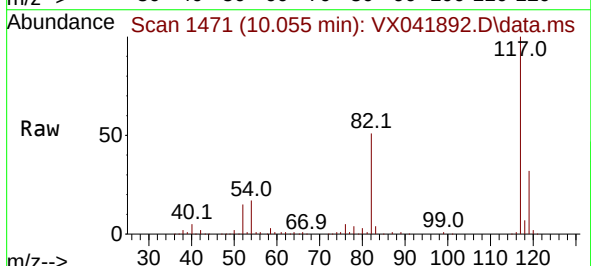


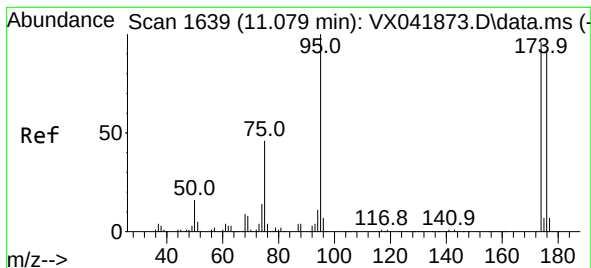

#60
4-Bromofluorobenzene
Concen: 27.195 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX041892.D
Acq: 14 Jun 2024 20:54

Instrument :
MSVOA_X
ClientSampleId :
240606041-01

Tgt Ion: 95 Resp: 64072
Ion Ratio Lower Upper
95 100
174 98.5 78.9 118.3
176 94.3 77.1 115.7

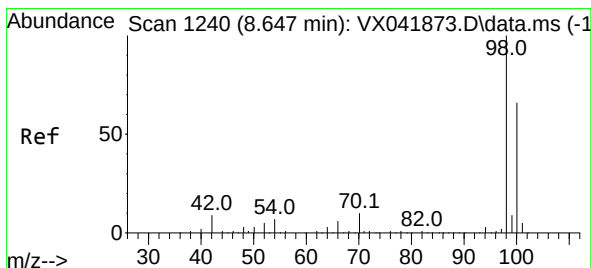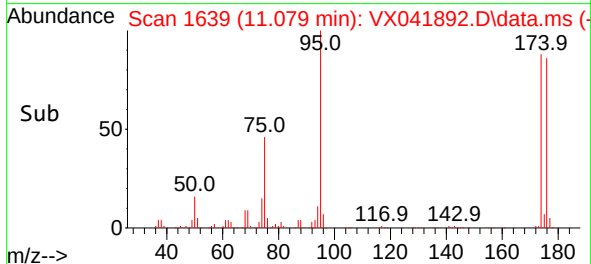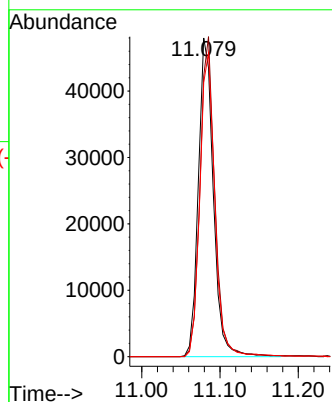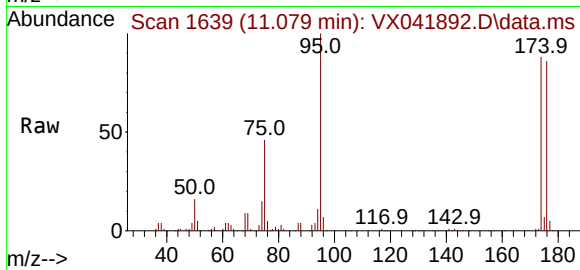

#63
Toluene-d8
Concen: 30.271 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX041892.D
Acq: 14 Jun 2024 20:54

Tgt Ion: 98 Resp: 197120
Ion Ratio Lower Upper
98 100
100 66.4 52.7 79.1

