
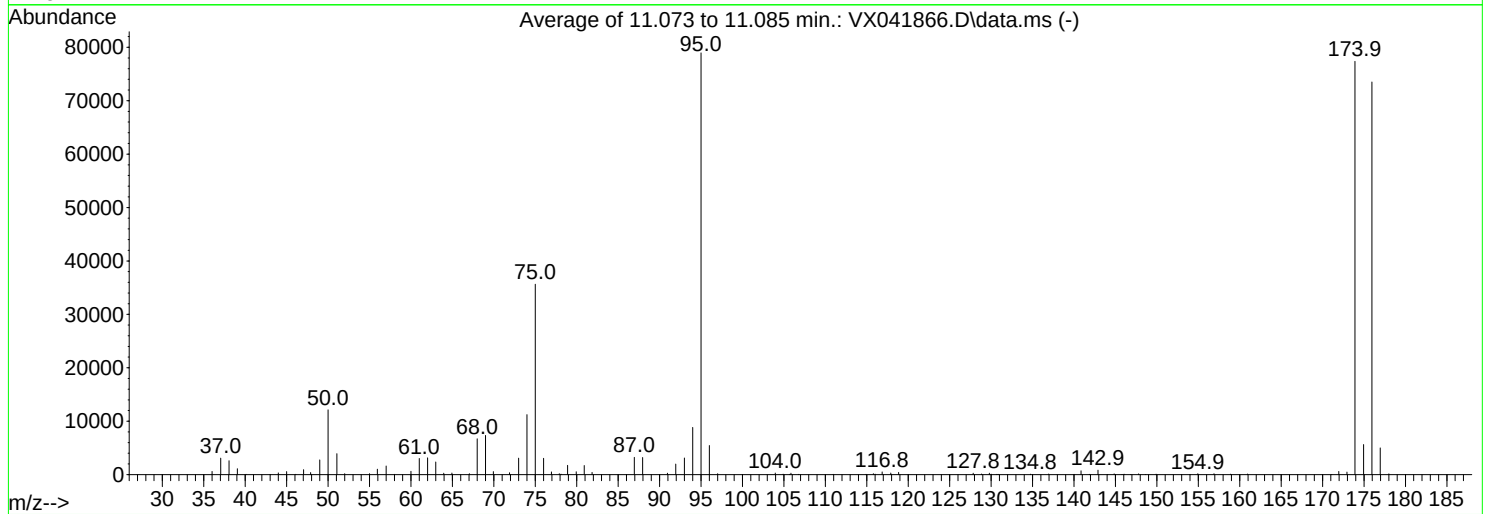


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061424\
Data File : VX041866.D
Acq On : 14 Jun 2024 08:02
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X061424W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Sat Jun 15 04:02:59 2024

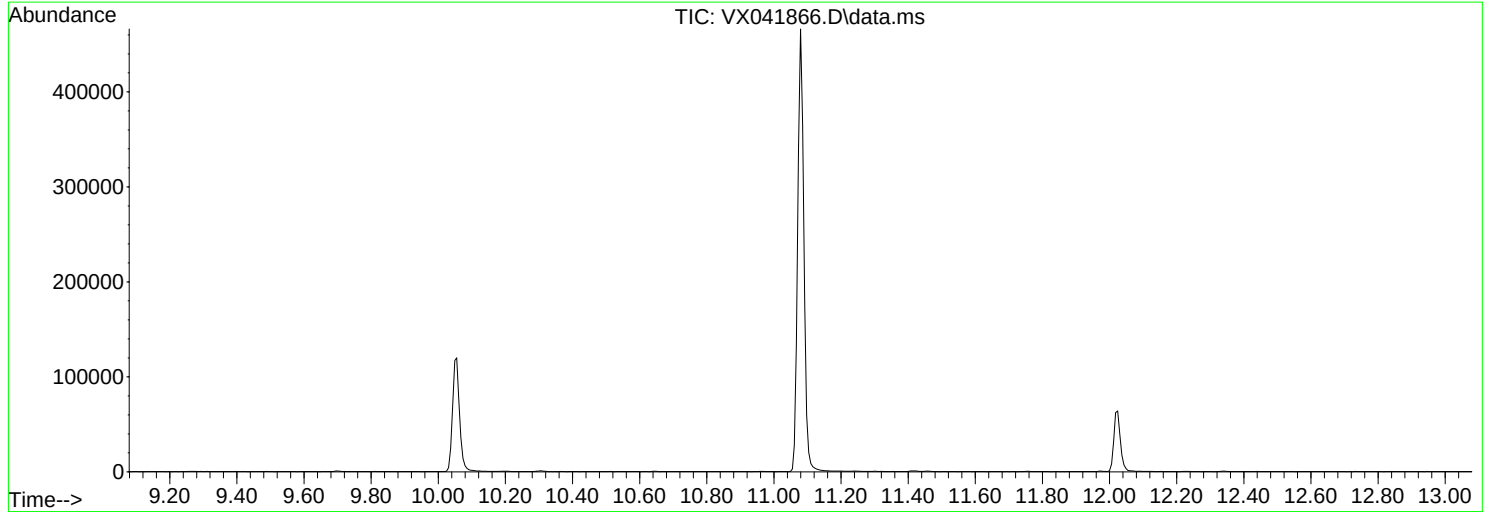

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.4	12135	PASS
75	95	30	60	45.1	35640	PASS
95	95	100	100	100.0	78957	PASS
96	95	5	9	6.9	5463	PASS
173	174	0.00	2	0.6	489	PASS
174	95	50	100	98.0	77371	PASS
175	174	5	9	7.3	5637	PASS
176	174	95	101	95.0	73499	PASS
177	176	5	9	6.8	5017	PASS