

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061521\
 Data File : VX022706.D
 Acq On : 15 Jun 2021 18:08
 Operator : JC/MD
 Sample : M2712-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP-1

Quant Time: Jun 16 05:27:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 10 12:20:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	59974	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	118798	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	106372	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	41653	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	50299	46.63	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	93.26%		
35) Dibromofluoromethane	5.397	113	35870	47.32	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	94.64%		
50) Toluene-d8	8.653	98	144176	48.25	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	96.50%		
62) 4-Bromofluorobenzene	11.085	95	51279	45.38	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	90.76%		
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.410	85	253	0.36	ug/l	98
4) Vinyl Chloride	1.374	62	9211	11.02	ug/l	99
5) Bromomethane	1.624	94	102	0.22	ug/l #	2
6) Chloroethane	1.691	64	2041	4.03	ug/l	97
10) Methyl Iodide	2.465	142	191	0.23	ug/l #	42
11) Tert butyl alcohol	2.971	59	87	0.35	ug/l #	73
12) 1,1-Dichloroethene	2.325	96	25333	34.79	ug/l	95
13) Acrolein	2.258	56	24	0.23	ug/l #	14
16) Acetone	2.392	43	815	1.69	ug/l #	83
20) Methylene Chloride	2.794	84	483	0.24	ug/l #	72
24) 1,1-Dichloroethane	3.617	63	32210	19.92	ug/l	99
27) cis-1,2-Dichloroethene	4.501	96	4981	5.07	ug/l	93
32) 1,1,1-Trichloroethane	5.397	97	5056	4.54	ug/l	96
36) 1,1-Dichloropropene	5.562	75	5846	4.94	ug/l #	49
38) Carbon Tetrachloride	5.562	117	7020	6.93	ug/l #	14
39) Methylcyclohexane	7.379	83	858	0.69	ug/l #	88
40) Benzene	6.044	78	1397	0.40	ug/l #	90
42) 1,2-Dichloroethane	6.099	62	2977	2.30	ug/l	88
43) Isopropyl Acetate	6.245	43	7928	3.34	ug/l #	57
44) Trichloroethene	7.129	130	596	0.72	ug/l	99
47) Bromodichloromethane	7.976	83	116	2.77	ug/l #	64
48) Methyl methacrylate	7.659	41	429	0.38	ug/l #	33
49) 1,4-Dioxane	7.665	88	13666	629.52	ug/l	99
51) 4-Methyl-2-Pentanone	8.653	43	774	0.51	ug/l #	1
53) t-1,3-Dichloropropene	8.976	75	26	3.28	ug/l #	44
58) 2-Chloroethyl Vinyl ether	7.970	63	399	0.49	ug/l #	45
76) 1,2,3-Trichloropropane	11.085	75	27964	25.32	ug/l #	39
81) trans-1,4-Dichloro-2-b...	11.085	75	27964	63.68	ug/l #	15
83) tert-Butylbenzene	11.719	119	900	0.34	ug/l	85
85) sec-Butylbenzene	11.896	105	1191	0.34	ug/l	93
86) p-Isopropyltoluene	12.250	119	939	0.33	ug/l	76
90) Hexachloroethane	12.701	117	1236	6.06	ug/l #	9
95) Naphthalene	13.780	128	199	1.53	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

MSVOA_X


ClientSampleId :

DUP-1






#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.000 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08

Instrument :
MSVOA_X
ClientSampleId :
DUP-1



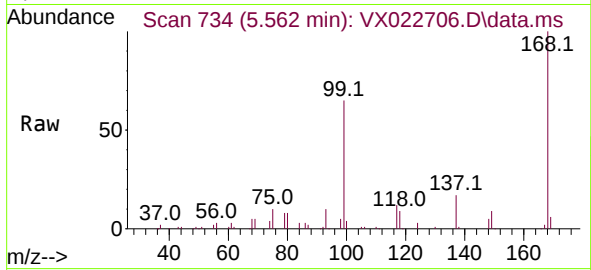



Tgt Ion:168 Resp: 59974
Ion Ratio Lower Upper
168 100
99 64.7 45.8 68.6

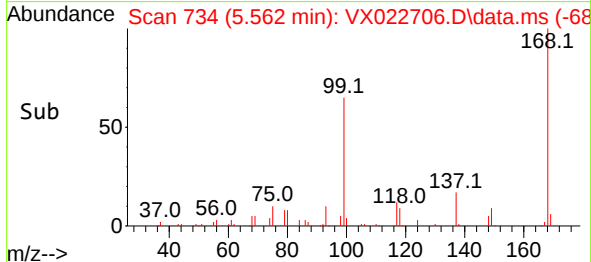

#2
Dichlorodifluoromethane
Concen: 0.36 ug/l
RT: 1.410 min Scan# 53
Delta R.T. 0.244 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08

Tgt Ion: 85 Resp: 253
Ion Ratio Lower Upper
85 100
87 34.2 16.4 49.2


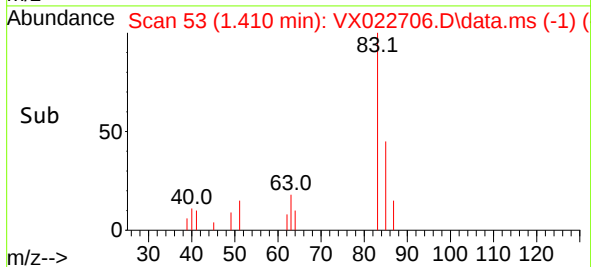

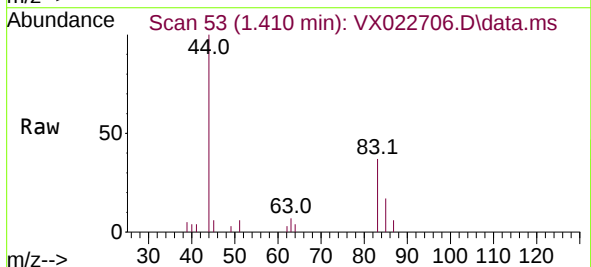


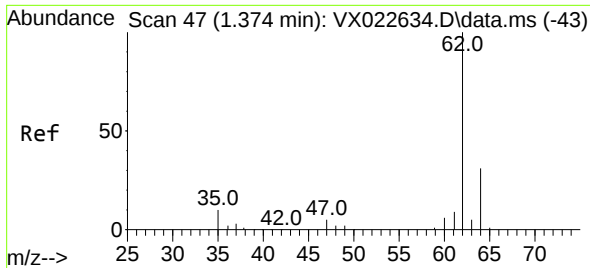

#4
 Vinyl Chloride
 Concen: 11.02 ug/l
 RT: 1.374 min Scan# 47
 Delta R.T. -0.000 min
 Lab File: VX022706.D
 Acq: 15 Jun 2021 18:08




Instrument :
 MSVOA_X
 ClientSampleID :
 DUP-1


Tgt Ion: 62 Resp: 9211
 Ion Ratio Lower Upper
 62 100
 64 31.7 25.7 38.5

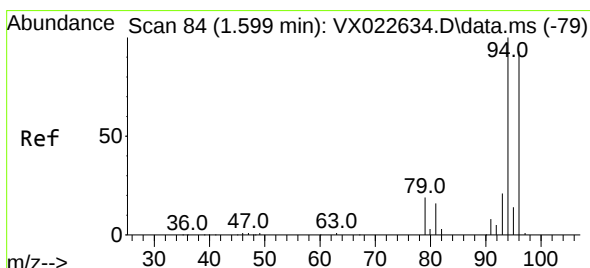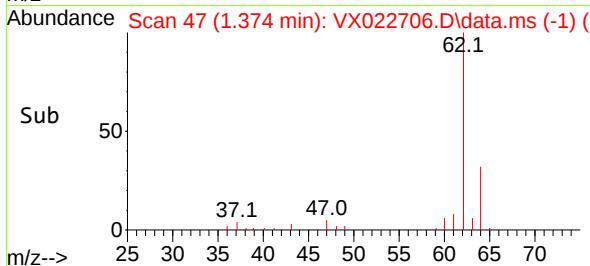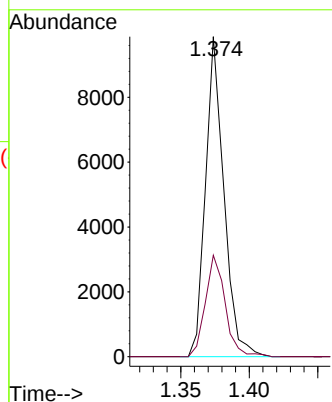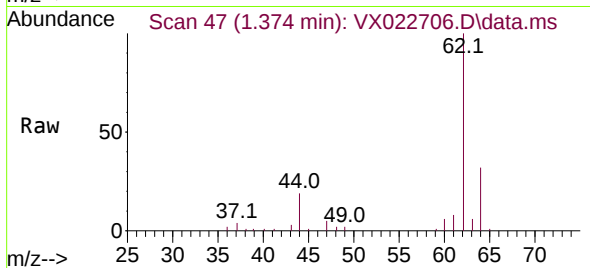

#5
 Bromomethane
 Concen: 0.22 ug/l
 RT: 1.624 min Scan# 88
 Delta R.T. 0.025 min
 Lab File: VX022706.D
 Acq: 15 Jun 2021 18:08

Tgt Ion: 94 Resp: 102
 Ion Ratio Lower Upper
 94 100
 96 0.0 76.4 114.6#


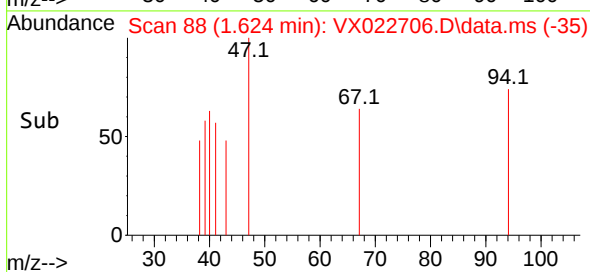
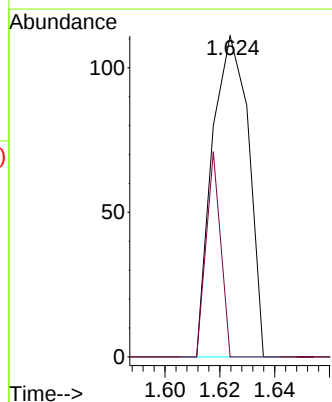
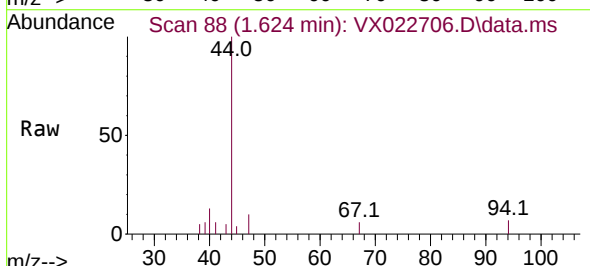


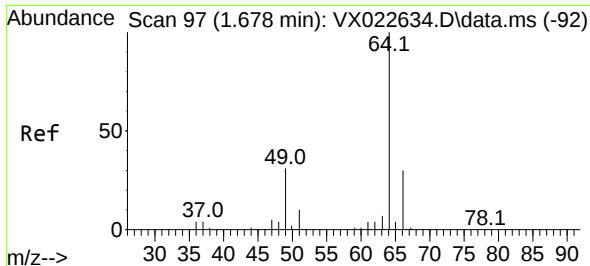

#6
Chloroethane
Concen: 4.03 ug/l
RT: 1.691 min Scan# 99
Delta R.T. 0.012 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08




Instrument :
MSVOA_X
ClientSampled :
DUP-1


Tgt Ion: 64 Resp: 2041
Ion Ratio Lower Upper
64 100
66 29.9 25.4 38.0

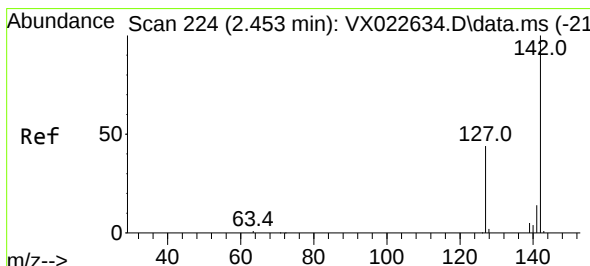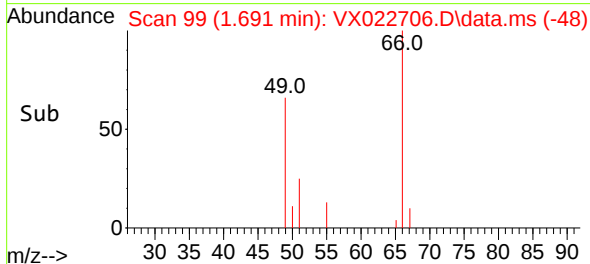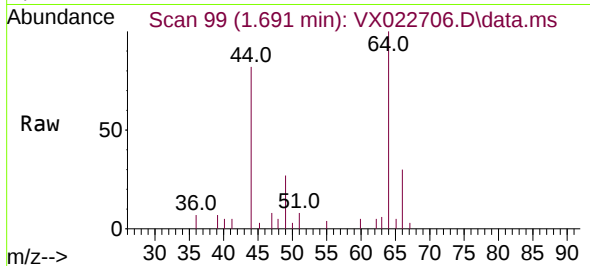

#10
Methyl Iodide
Concen: 0.23 ug/l
RT: 2.465 min Scan# 226
Delta R.T. 0.012 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08

Tgt Ion: 142 Resp: 191
Ion Ratio Lower Upper
142 100
127 0.0 33.3 49.9#
141 0.0 11.4 17.0#

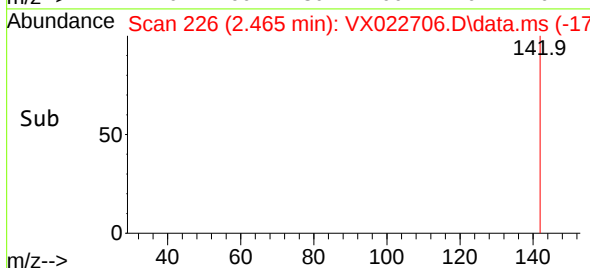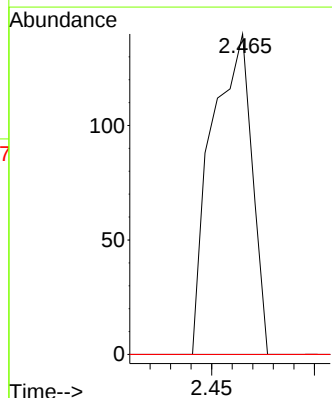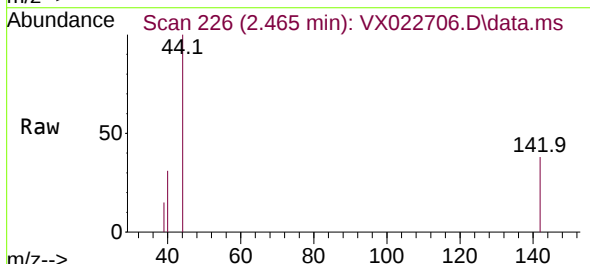




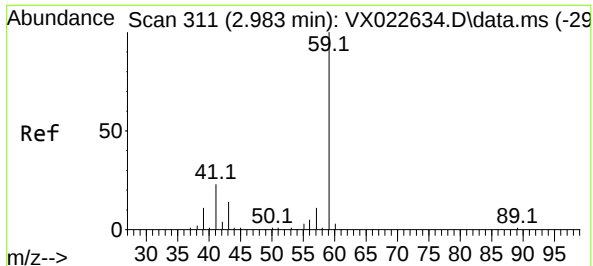


#11

Tert butyl alcohol
Concen: 0.35 ug/l
RT: 2.971 min Scan# 309
Delta R.T. -0.012 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08

Instrument :
MSVOA_X
ClientSampled :
DUP-1




Tgt Ion: 59 Resp: 87
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#

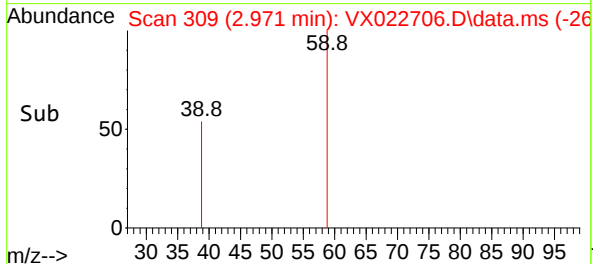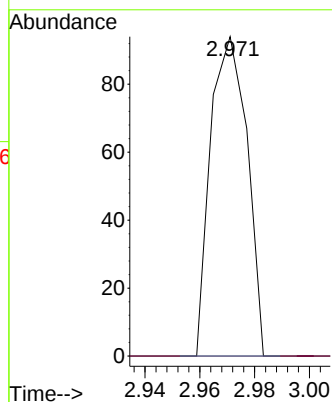


#12

1,1-Dichloroethene
Concen: 34.79 ug/l
RT: 2.325 min Scan# 203
Delta R.T. 0.006 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08

Tgt Ion: 96 Resp: 25333
Ion Ratio Lower Upper
96 100
61 164.5 124.6 187.0
98 62.0 50.6 76.0







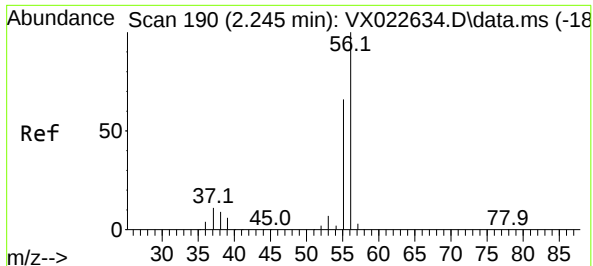

#13
Acrolein
Concen: 0.23 ug/l
RT: 2.258 min Scan# 192
Delta R.T. 0.019 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08




Instrument :
MSVOA_X
ClientSampled :
DUP-1


Tgt Ion: 56 Resp: 24
Ion Ratio Lower Upper
56 100
55 0.0 56.4 84.6#

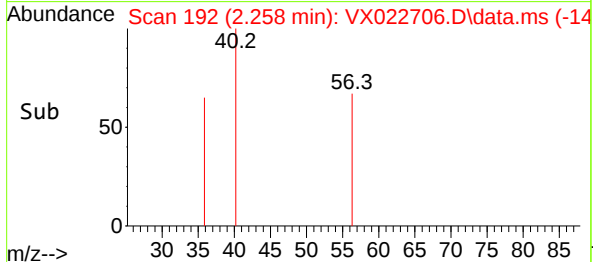

#16
Acetone
Concen: 1.69 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.000 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08

Tgt Ion: 43 Resp: 815
Ion Ratio Lower Upper
43 100
58 24.8 27.8 41.8#




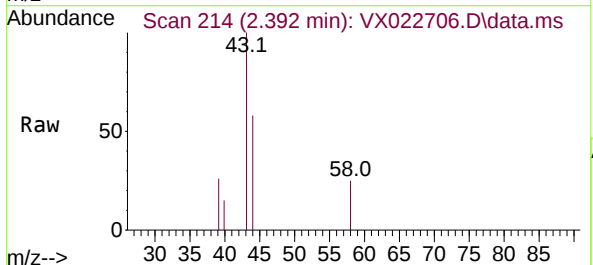


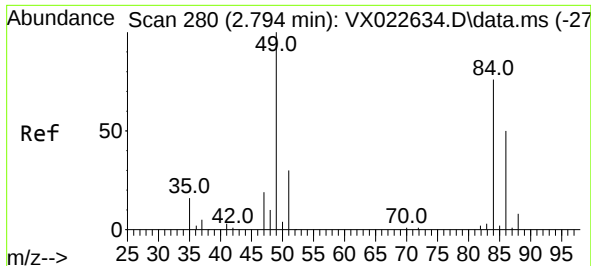

#20
Methylene Chloride
Concen: 0.24 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08




Instrument :
MSVOA_X
ClientSampled :
DUP-1


Tgt Ion:	84	Resp:	483
Ion	Ratio	Lower	Upper
84	100		
49	86.0	88.6	132.8#
51	20.1	27.0	40.6#
86	33.8	50.3	75.5#

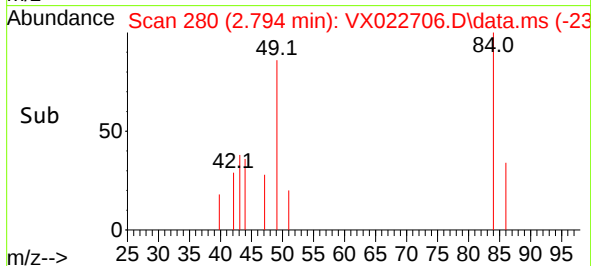

#24
1,1-Dichloroethane
Concen: 19.92 ug/l
RT: 3.617 min Scan# 415
Delta R.T. 0.006 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08

Tgt Ion:	63	Resp:	32210
Ion	Ratio	Lower	Upper
63	100		
98	7.0	3.8	11.2
100	4.7	2.5	7.5

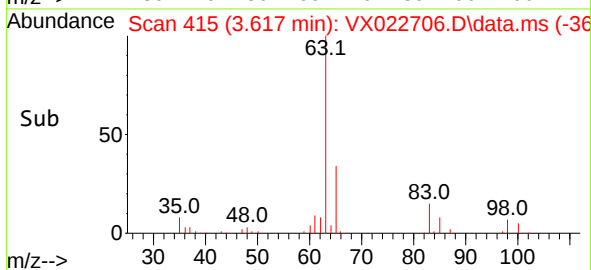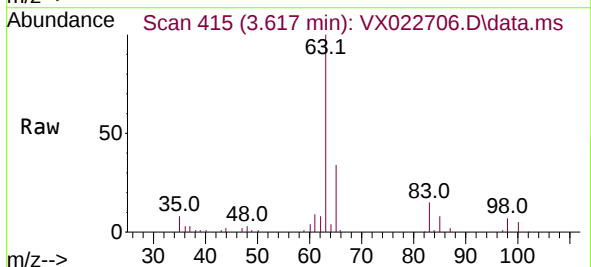



#27

cis-1,2-Dichloroethene

Concen: 5.07 ug/l

RT: 4.501 min Scan# 560

Delta R.T. 0.006 min

Lab File: VX022706.D

Acq: 15 Jun 2021 18:08

Tgt Ion: 96 Resp: 4981





Ion	Ratio	Lower	Upper
96	100		
61	129.7	0.0	285.6
98	65.0	0.0	129.6

Instrument :

MSVOA_X

ClientSampled :

DUP-1

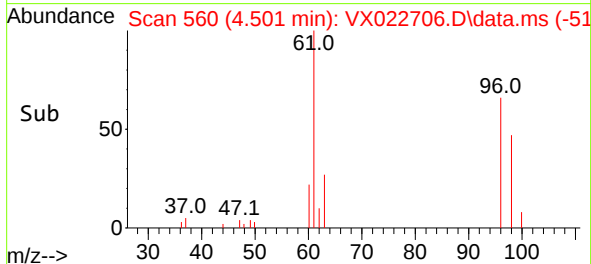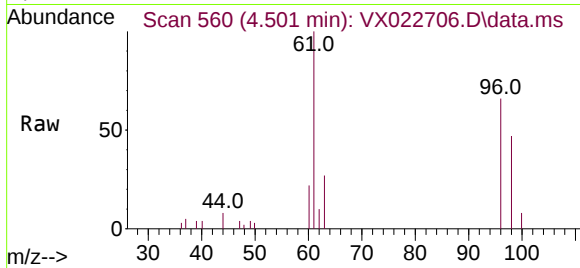

#32

1,1,1-Trichloroethane

Concen: 4.54 ug/l

RT: 5.397 min Scan# 707




Delta R.T. 0.006 min


Lab File: VX022706.D

Acq: 15 Jun 2021 18:08

Tgt Ion: 97 Resp: 5056

Ion	Ratio	Lower	Upper
97	100		
99	65.2	51.5	77.3
61	49.0	34.2	51.4

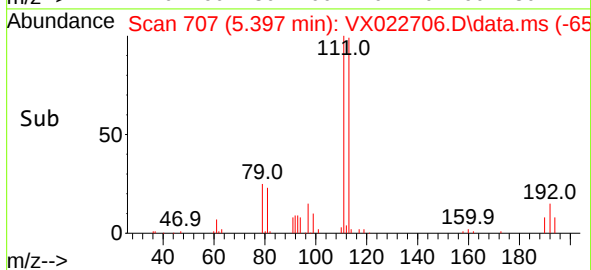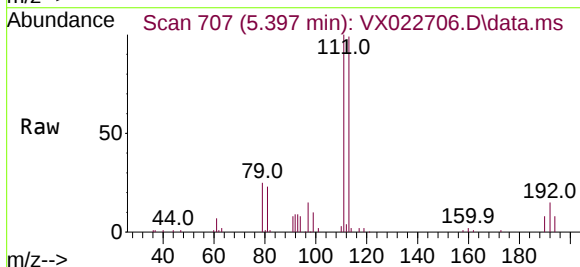

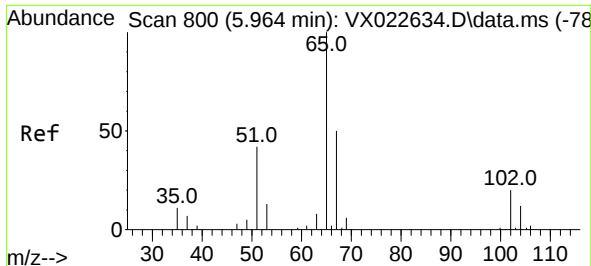

#33

1,2-Dichloroethane-d4

Concen: 46.63 ug/l

RT: 5.964 min Scan# 800

Delta R.T. 0.000 min

Lab File: VX022706.D

Acq: 15 Jun 2021 18:08

Tgt Ion: 65 Resp: 50299

Ion Ratio Lower Upper

65 100





67 50.7 0.0 105.4

Instrument :

MSVOA_X

ClientSampled :

DUP-1

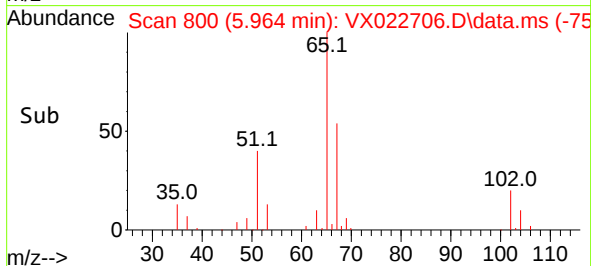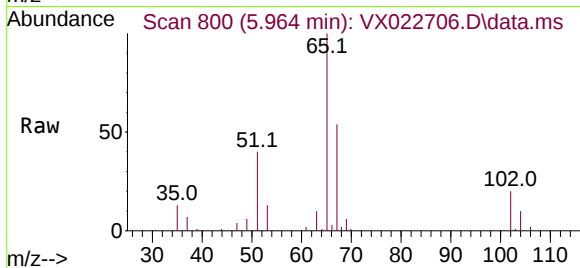

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.000 min

Lab File: VX022706.D

Acq: 15 Jun 2021 18:08




Tgt Ion: 114 Resp: 118798


Ion Ratio Lower Upper

114 100

63 21.3 0.0 40.8

88 17.2 0.0 32.8

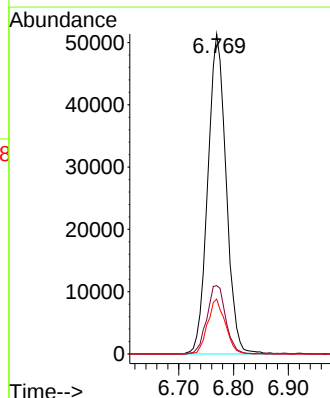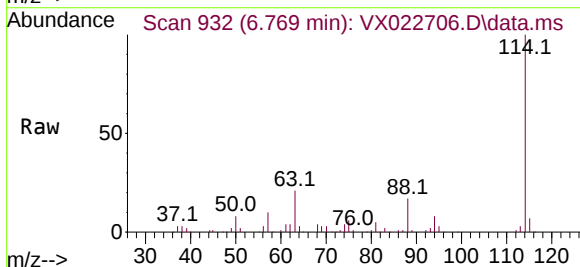

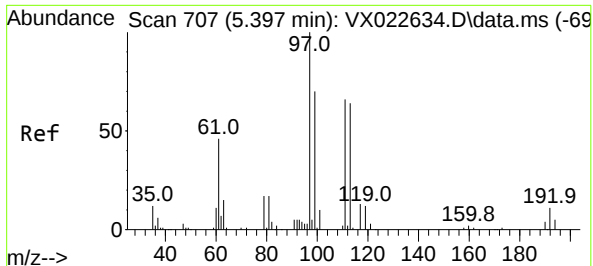

#35

Dibromofluoromethane

Concen: 47.32 ug/l

RT: 5.397 min Scan# 707





Delta R.T. 0.006 min

Lab File: VX022706.D

Acq: 15 Jun 2021 18:08

Tgt Ion:	113	Resp:	35870
Ion	Ratio	Lower	Upper
113	100		
111	103.8	81.9	122.9
192	15.2	16.7	25.1#

Instrument :
MSVOA_X
ClientSampled :
DUP-1

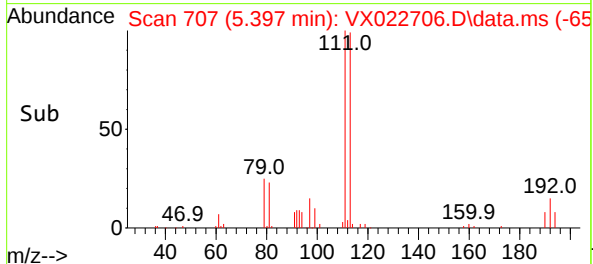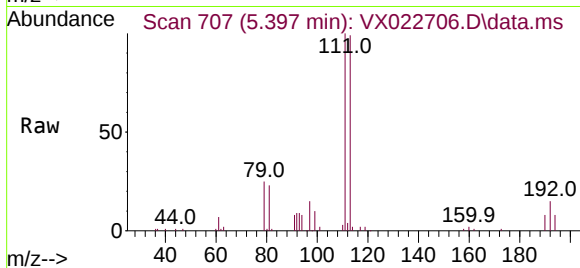

#36

1,1-Dichloropropene

Concen: 4.94 ug/l




RT: 5.562 min Scan# 734


Delta R.T. -0.140 min

Lab File: VX022706.D

Acq: 15 Jun 2021 18:08


Tgt Ion:	75	Resp:	5846
Ion	Ratio	Lower	Upper
75	100		
110	9.8	18.1	54.4#
77	0.0	25.3	37.9#

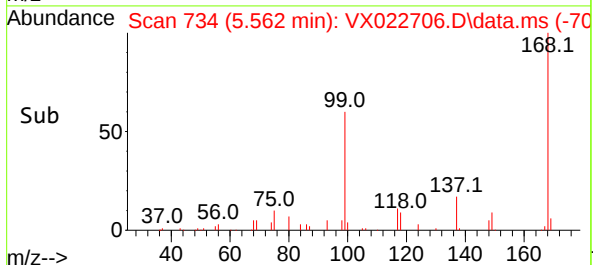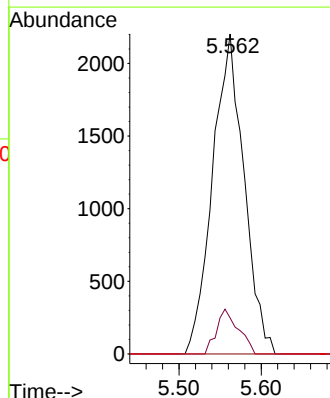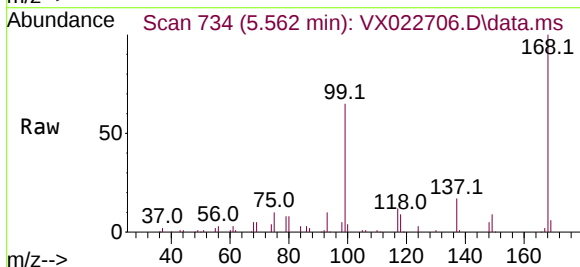



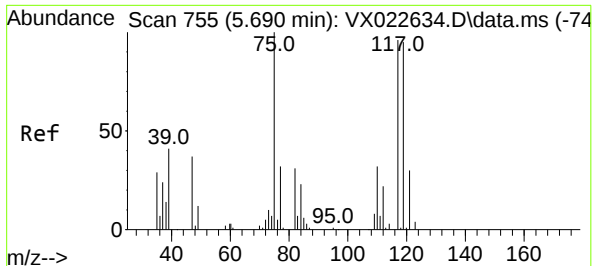


#38
Carbon Tetrachloride
Concen: 6.93 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.116 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08


Instrument :
MSVOA_X
ClientSampled :
DUP-1

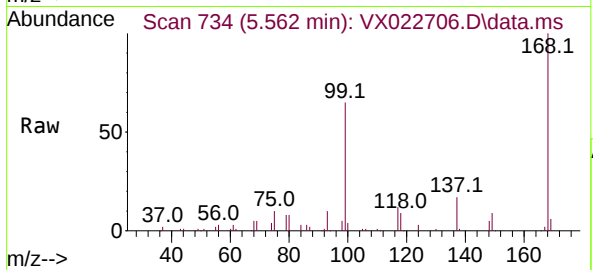



Tgt Ion:117 Resp: 7020
Ion Ratio Lower Upper
117 100
119 2.8 76.2 114.2#
121 0.0 24.8 37.2#

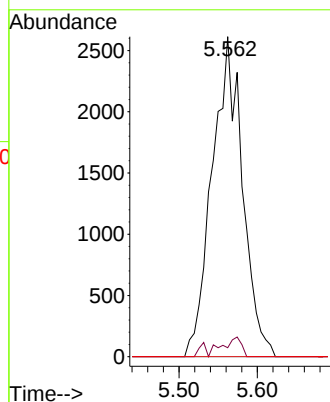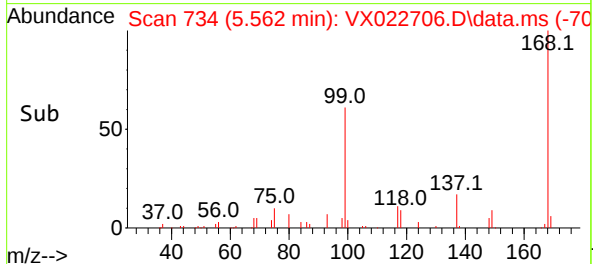


#39
Methylcyclohexane
Concen: 0.69 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. -0.006 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08



Tgt Ion: 83 Resp: 858
Ion Ratio Lower Upper
83 100
55 73.8 58.9 88.3
98 26.8 38.1 57.1#









#40
Benzene
Concen: 0.40 ug/l
RT: 6.044 min Scan# 813
Delta R.T. -0.006 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08




Instrument :
MSVOA_X
ClientSampled :
DUP-1


Tgt Ion: 78 Resp: 1397
Ion Ratio Lower Upper
78 100
77 18.5 18.9 28.3#

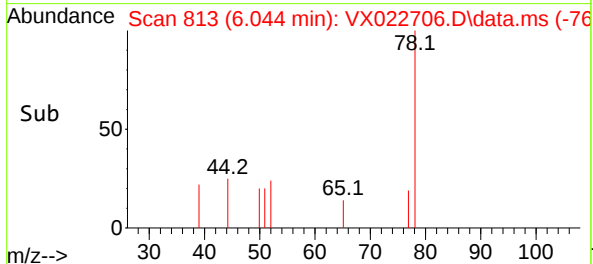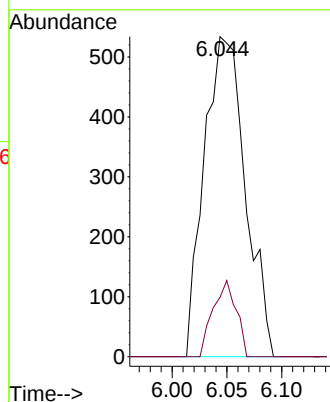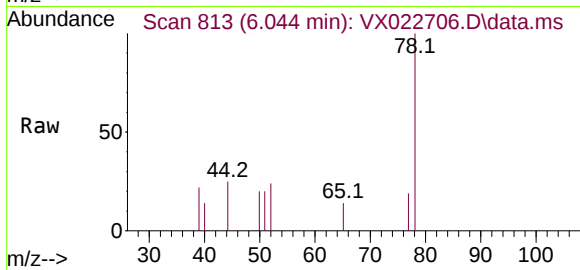

#42
1,2-Dichloroethane
Concen: 2.30 ug/l
RT: 6.099 min Scan# 822
Delta R.T. 0.001 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08

Tgt Ion: 62 Resp: 2977
Ion Ratio Lower Upper
62 100
98 5.7 0.0 20.2



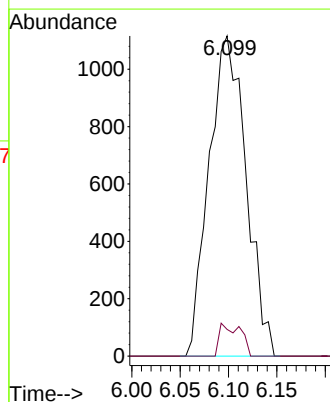
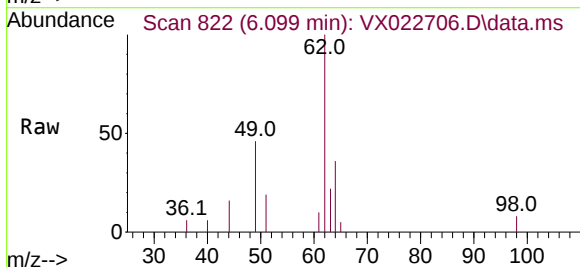




#43
Isopropyl Acetate
Concen: 3.34 ug/l
RT: 6.245 min Scan# 846
Delta R.T. -0.103 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08




Instrument :
MSVOA_X
ClientSampleId :
DUP-1


Tgt Ion: 43 Resp: 7928
Ion Ratio Lower Upper
43 100
61 0.0 18.2 27.4#
87 0.0 12.5 18.7#

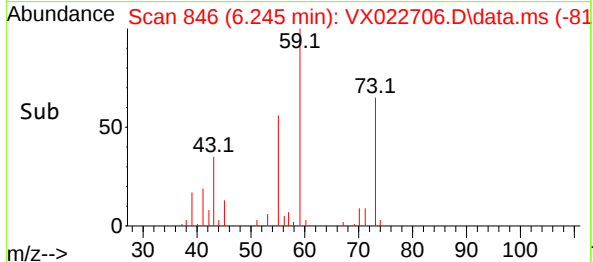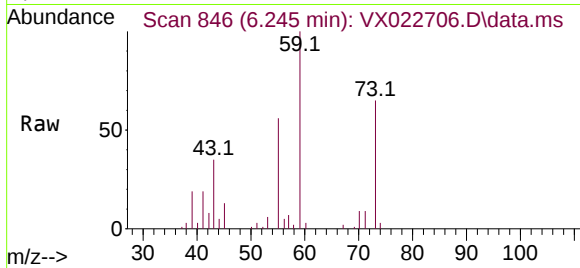

#44
Trichloroethene
Concen: 0.72 ug/l
RT: 7.129 min Scan# 991
Delta R.T. -0.000 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08

Tgt Ion:130 Resp: 596
Ion Ratio Lower Upper
130 100
95 99.7 0.0 198.0




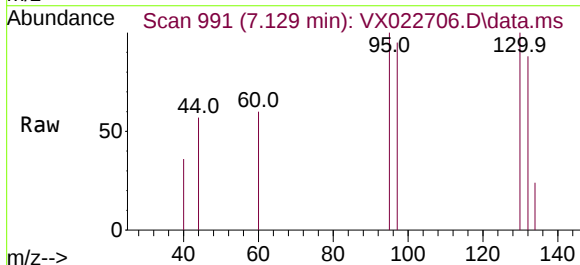


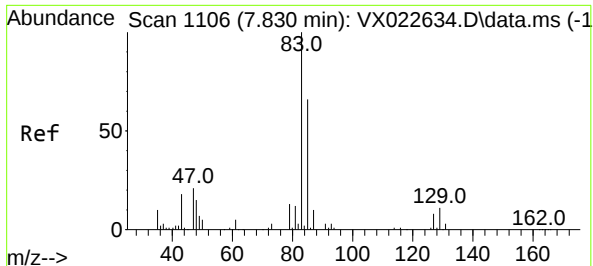

#47
Bromodichloromethane
Concen: 2.77 ug/l
RT: 7.976 min Scan# 1130
Delta R.T. 0.146 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08




Instrument :
MSVOA_X
ClientSampled :
DUP-1


Tgt Ion: 83 Resp: 116
Ion Ratio Lower Upper
83 100
85 71.7 51.4 77.0
127 91.7 6.8 10.2#

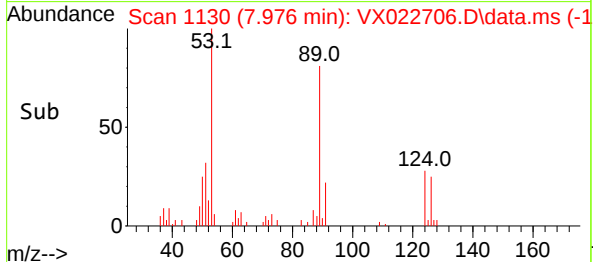

#48
Methyl methacrylate
Concen: 0.38 ug/l
RT: 7.659 min Scan# 1078
Delta R.T. -0.037 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08

Tgt Ion: 41 Resp: 429
Ion Ratio Lower Upper
41 100
69 0.0 76.0 114.0#
39 65.7 44.6 67.0


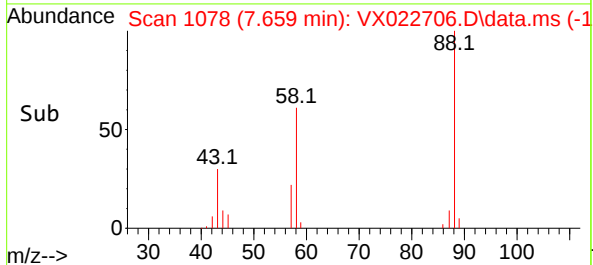






#49
1,4-Dioxane
Concen: 629.52 ug/l
RT: 7.665 min Scan# 1079
Delta R.T. 0.000 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08




Instrument :
MSVOA_X
ClientSampled :
DUP-1


Tgt Ion:	88	Resp:	13666
Ion	Ratio	Lower	Upper
88	100		
43	30.0	23.2	34.8
58	68.6	55.0	82.4

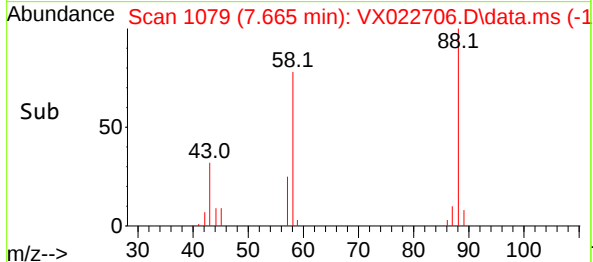

#50
Toluene-d8
Concen: 48.25 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08

Tgt Ion:	98	Resp:	144176
Ion	Ratio	Lower	Upper
98	100		
100	65.6	51.9	77.9




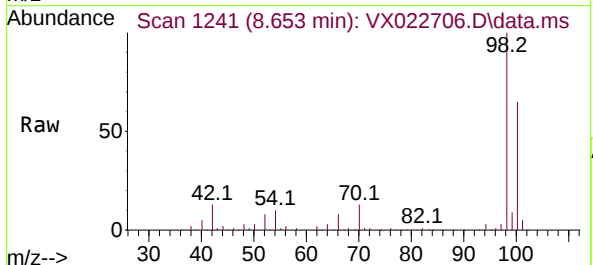




#51
4-Methyl-2-Pentanone
Concen: 0.51 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.073 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08




Instrument :
MSVOA_X
ClientSampled :
DUP-1


Tgt Ion: 43 Resp: 774
Ion Ratio Lower Upper
43 100
58 182.8 35.4 53.0#

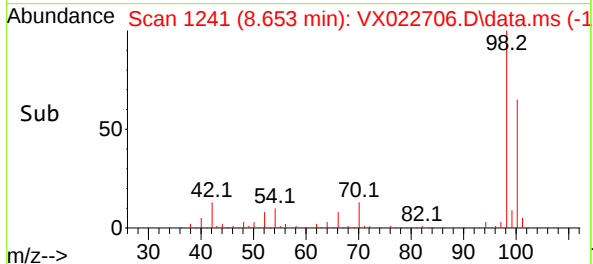

#53
t-1,3-Dichloropropene
Concen: 3.28 ug/l
RT: 8.976 min Scan# 1294
Delta R.T. -0.006 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08

Tgt Ion: 75 Resp: 26
Ion Ratio Lower Upper
75 100
77 0.0 24.9 37.3#



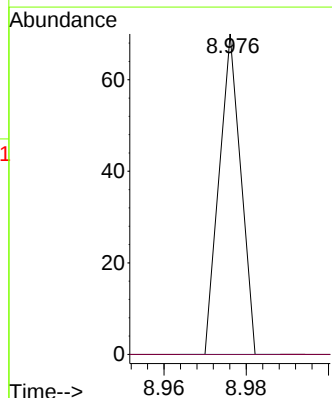



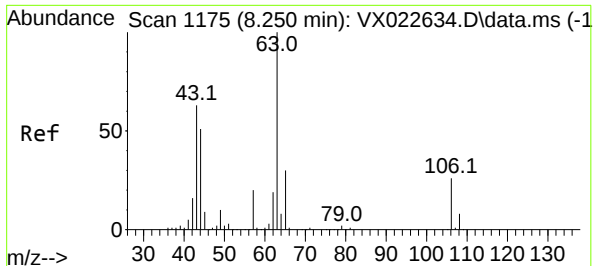

#58
2-Chloroethyl Vinyl ether
Concen: 0.49 ug/l
RT: 7.970 min Scan# 1129
Delta R.T. -0.281 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08




Instrument :
MSVOA_X
ClientSampled :
DUP-1


Tgt Ion: 63 Resp: 399
Ion Ratio Lower Upper
63 100
106 0.0 23.5 35.3#

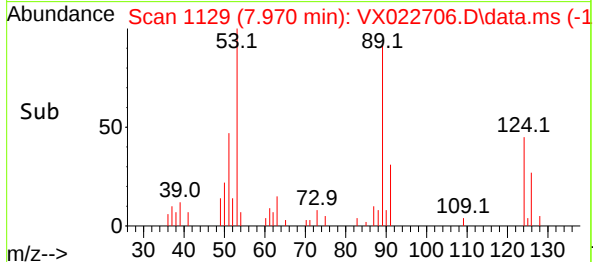

#62
4-Bromofluorobenzene
Concen: 45.38 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08

Tgt Ion: 95 Resp: 51279
Ion Ratio Lower Upper
95 100
174 60.5 0.0 154.6
176 59.0 0.0 155.8




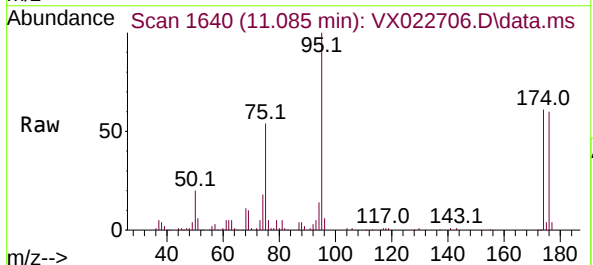




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08




Instrument :
MSVOA_X
ClientSampled :
DUP-1


Tgt Ion:117 Resp: 106372
Ion Ratio Lower Upper
117 100
82 60.5 47.4 71.2
119 31.9 26.6 39.8

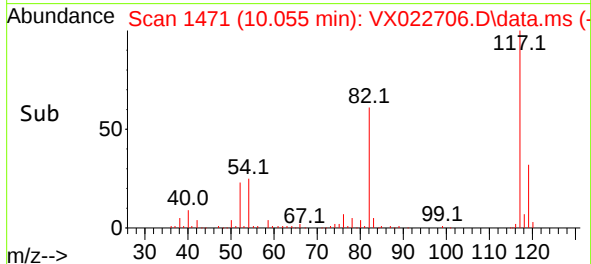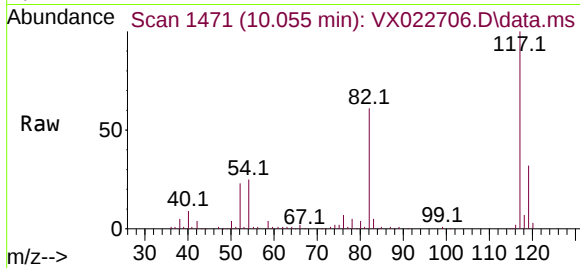

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08

Tgt Ion:152 Resp: 41653
Ion Ratio Lower Upper
152 100
115 67.8 41.1 123.3
150 160.6 0.0 349.0


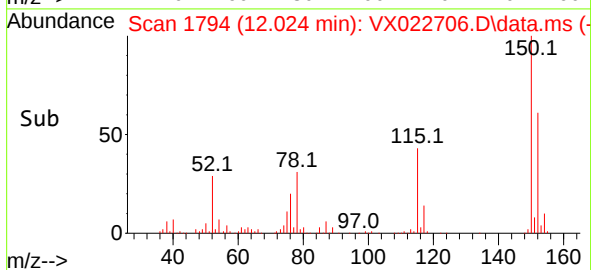

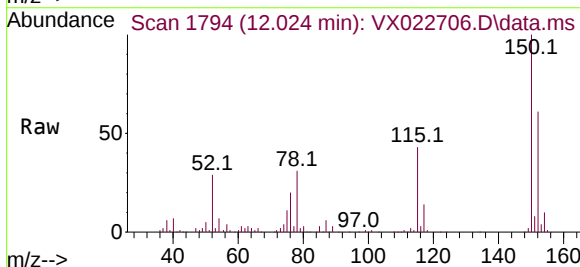


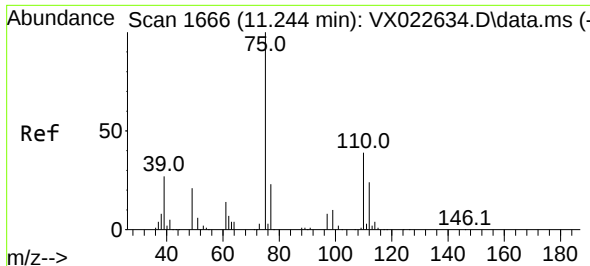

#76
1,2,3-Trichloropropane
Concen: 25.32 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08




Instrument :
MSVOA_X
ClientSampled :
DUP-1


Tgt Ion: 75 Resp: 27964
Ion Ratio Lower Upper
75 100
77 1.4 19.1 57.5#

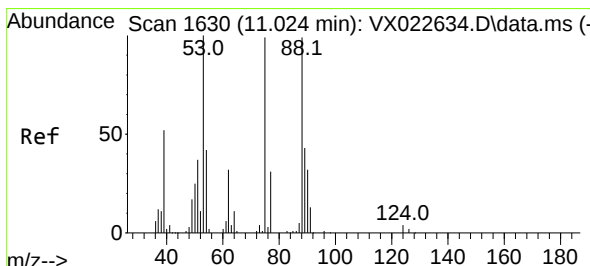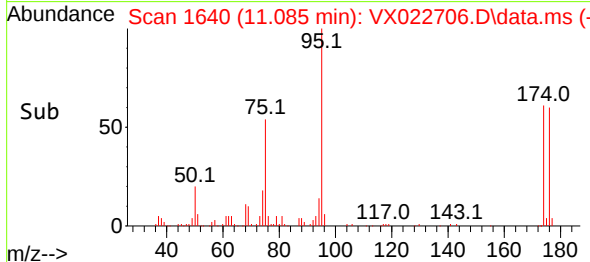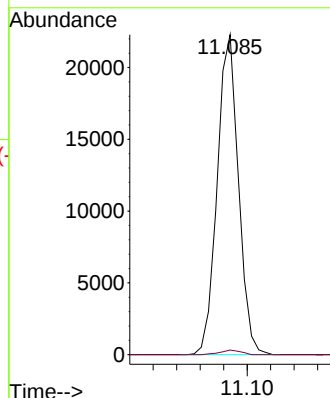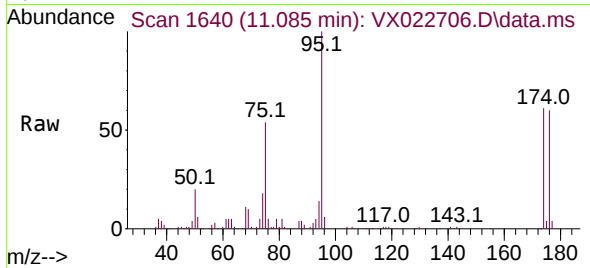

#81
trans-1,4-Dichloro-2-butene
Concen: 63.68 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08

Tgt Ion: 75 Resp: 27964
Ion Ratio Lower Upper
75 100
53 1.0 74.5 111.7#
89 4.9 37.9 56.9#


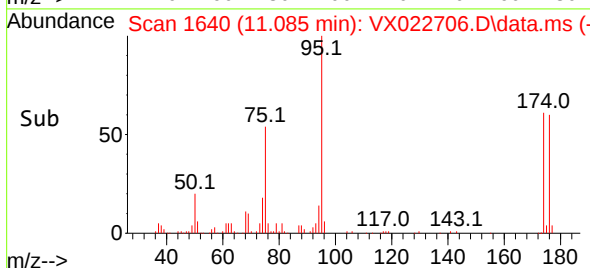
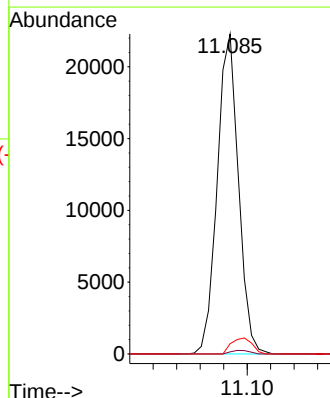
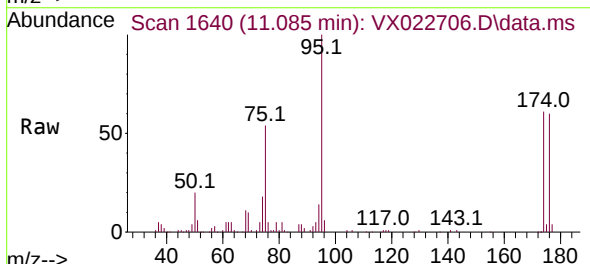




#83
tert-Butylbenzene
Concen: 0.34 ug/l
RT: 11.719 min Scan# 1744
Delta R.T. 0.000 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08




Instrument :
MSVOA_X
ClientSampled :
DUP-1


Tgt Ion:119 Resp: 900
Ion Ratio Lower Upper
119 100
91 44.7 27.9 83.7
134 16.2 11.3 33.9

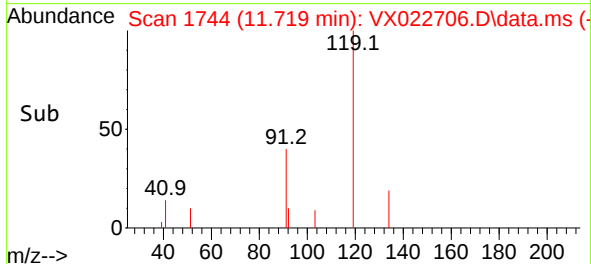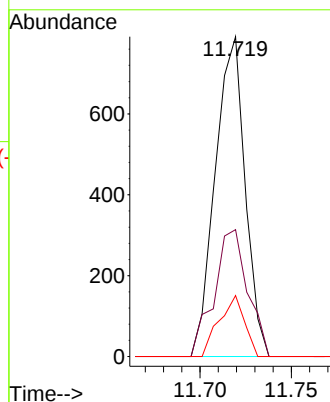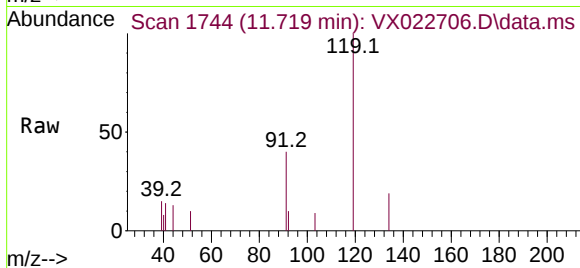

#85
sec-Butylbenzene
Concen: 0.34 ug/l
RT: 11.896 min Scan# 1773
Delta R.T. 0.000 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08

Tgt Ion:105 Resp: 1191
Ion Ratio Lower Upper
105 100
134 16.7 10.0 29.8


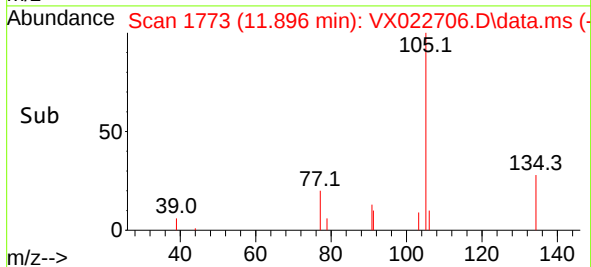
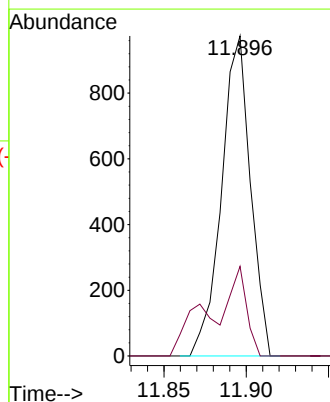
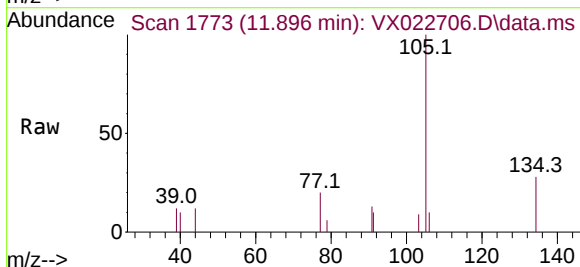




#86
p-Isopropyltoluene
Concen: 0.33 ug/l
RT: 12.250 min Scan# 1831
Delta R.T. 0.238 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08




Instrument :
MSVOA_X
ClientSampled :
DUP-1


Tgt Ion:119 Resp: 939
Ion Ratio Lower Upper
119 100
134 38.3 12.9 38.7
91 34.4 11.7 35.0

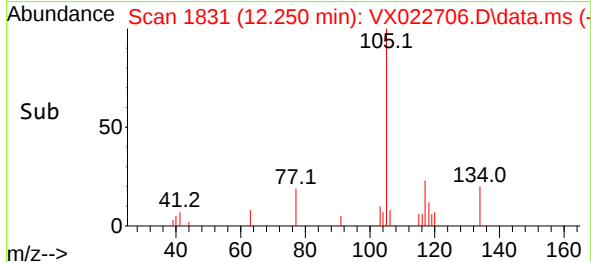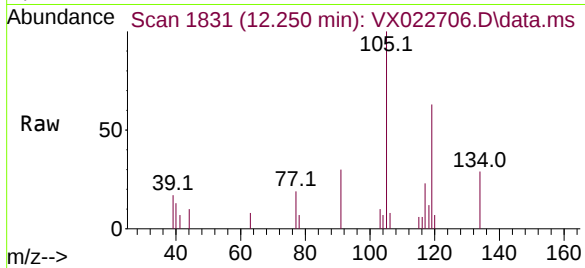

#90
Hexachloroethane
Concen: 6.06 ug/l
RT: 12.701 min Scan# 1905
Delta R.T. 0.159 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08


Tgt Ion:117 Resp: 1236
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#

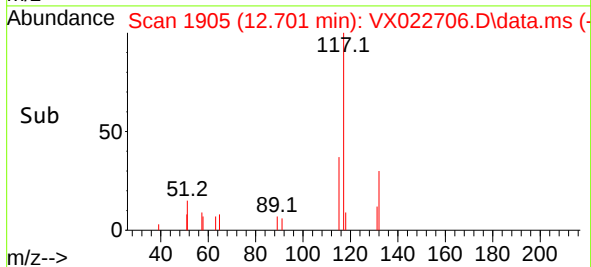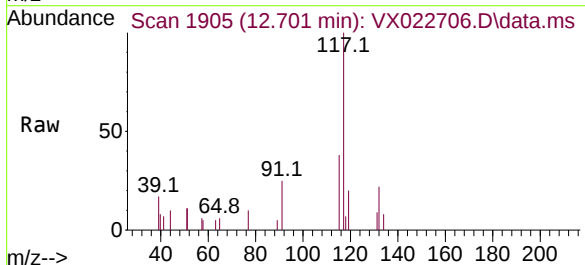



#95
Naphthalene
Concen: 1.53 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX022706.D
Acq: 15 Jun 2021 18:08

Instrument :
MSVOA_X
ClientSampled :
DUP-1

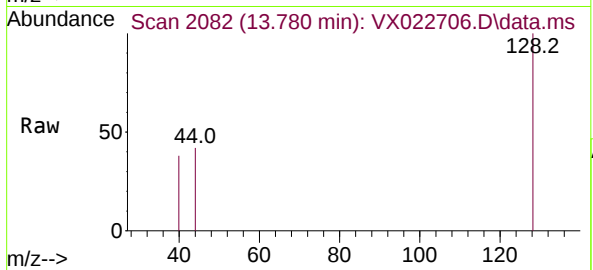

Tgt Ion:	128	Resp:	199
Ion	Ratio	Lower	Upper
128	100		
127	0.0	10.3	15.5#
129	0.0	8.8	13.2#

