

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061521\
 Data File : VX022701.D
 Acq On : 15 Jun 2021 16:00
 Operator : JC/MD
 Sample : VX0615WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0615WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M

Title : SW846 8260

Signal : TIC: VX022701.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.569	75	79	84	rVB4	3375	5280	1.33%	0.263%
2	2.794	272	280	287	rBV4	2329	4813	1.21%	0.239%
3	4.599	566	576	580	rBV2	1574	4498	1.13%	0.224%
4	5.397	694	707	721	rBV2	42377	120772	30.36%	6.010%
5	5.562	721	734	748	rVV2	70767	199031	50.04%	9.904%
6	5.964	790	800	818	rVB	53794	142516	35.83%	7.092%
7	6.769	921	932	942	rBV	124143	289978	72.90%	14.429%
8	8.653	1234	1241	1253	rVB	261238	397775	100.00%	19.793%
9	10.055	1466	1471	1482	rVB	250187	333567	83.86%	16.598%
10	11.085	1634	1640	1650	rVB	177524	231392	58.17%	11.514%
11	12.024	1789	1794	1803	rVB	227541	280005	70.39%	13.933%




Sum of corrected areas: 2009627

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061521\
Data File : VX022701.D
Acq On : 15 Jun 2021 16:00
Operator : JC/MD
Sample : VX0615WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0615WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

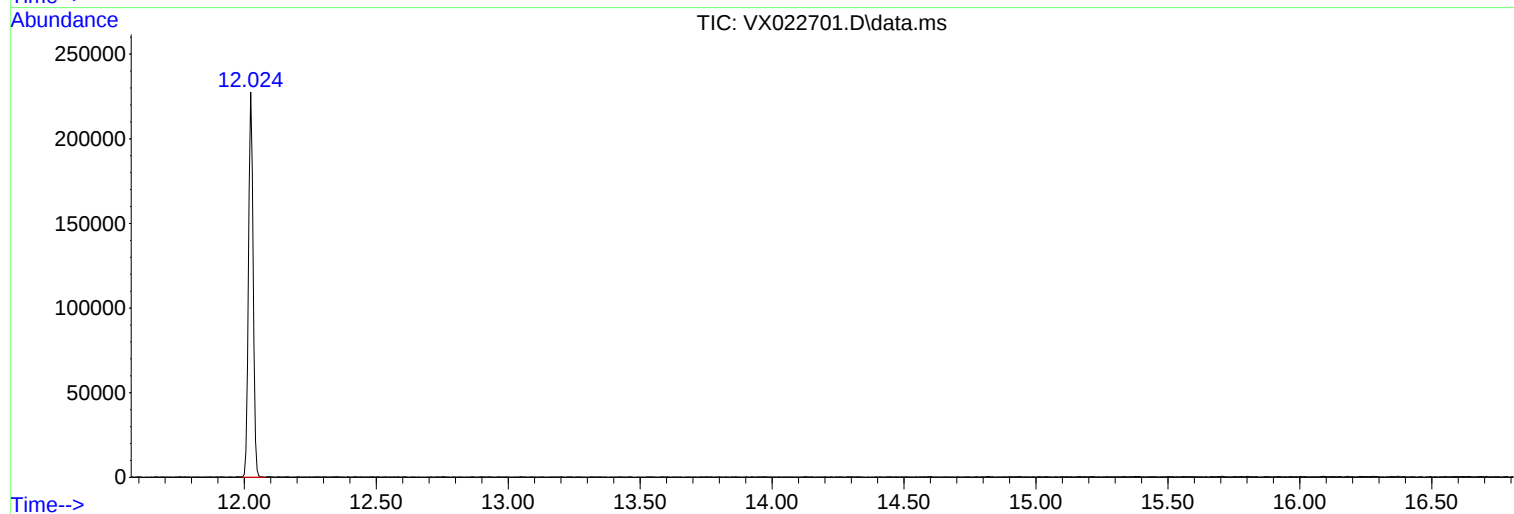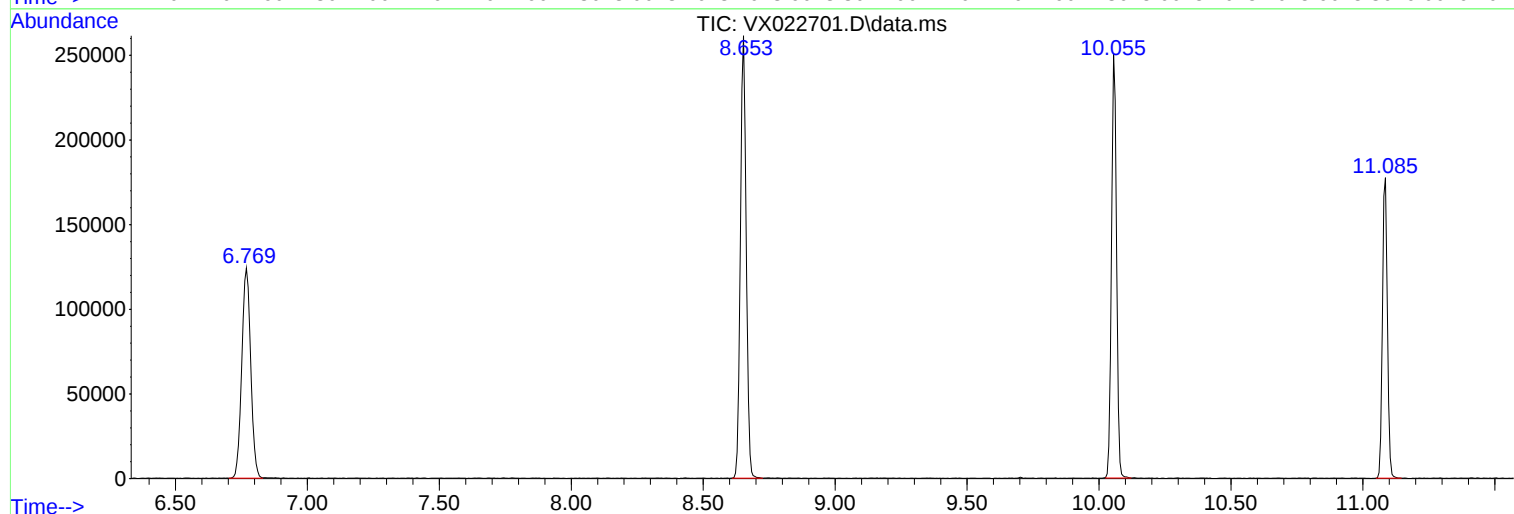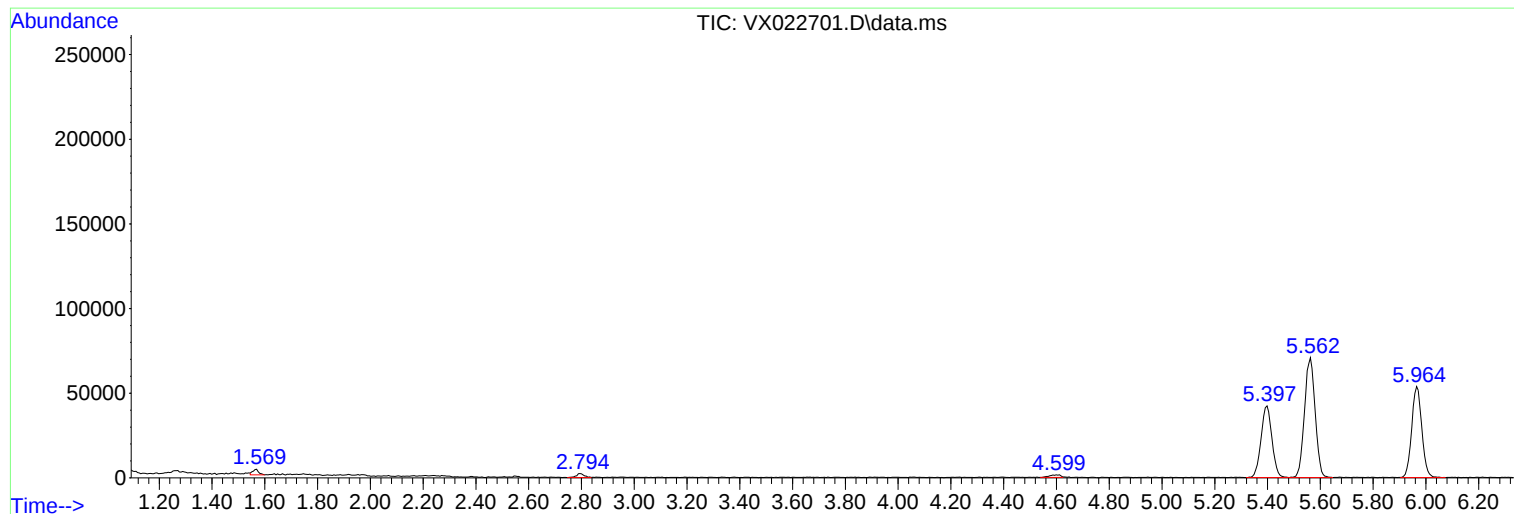

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061521\
Data File : VX022701.D
Acq On : 15 Jun 2021 16:00
Operator : JC/MD
Sample : VX0615WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0615WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061521\
Data File : VX022701.D
Acq On : 15 Jun 2021 16:00
Operator : JC/MD
Sample : VX0615WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0615WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
