

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061521\
 Data File : VX022704.D
 Acq On : 15 Jun 2021 17:21
 Operator : JC/MD
 Sample : M2712-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M

Title : SW846 8260

Signal : TIC: VX022704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.562	73	78	81	rVB3	2805	4390	1.10%	0.206%
2	1.660	89	94	99	rBV3	4466	6149	1.54%	0.288%
3	1.916	133	136	146	rVB3	2274	5918	1.48%	0.277%
4	2.142	168	173	179	rBV2	16178	24933	6.25%	1.167%
5	2.325	197	203	209	rVB	16761	27860	6.98%	1.304%
6	2.550	236	240	248	rVB2	2771	4556	1.14%	0.213%
7	3.617	408	415	425	rVB	6990	15160	3.80%	0.710%
8	4.489	550	558	560	rBV2	2479	4392	1.10%	0.206%
9	5.397	695	707	721	rBV	42386	117868	29.55%	5.518%
10	5.562	723	734	745	rVV	71753	198358	49.73%	9.286%
11	5.964	789	800	811	rBV2	54396	141711	35.53%	6.634%
12	6.769	922	932	945	rBV	121366	287514	72.08%	13.460%
13	7.177	994	999	1005	rVB3	2268	4481	1.12%	0.210%
14	7.976	1121	1130	1136	rBV3	11701	20045	5.03%	0.938%
15	8.653	1234	1241	1251	rBV	266598	398857	100.00%	18.672%
16	9.732	1412	1418	1424	rBV	16093	22851	5.73%	1.070%
17	10.055	1466	1471	1485	rVB	252903	340285	85.32%	15.930%
18	11.085	1634	1640	1648	rBV	185228	234051	58.68%	10.957%
19	12.024	1789	1794	1800	rBV	222138	276696	69.37%	12.953%




Sum of corrected areas: 2136075

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061521\
Data File : VX022704.D
Acq On : 15 Jun 2021 17:21
Operator : JC/MD
Sample : M2712-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

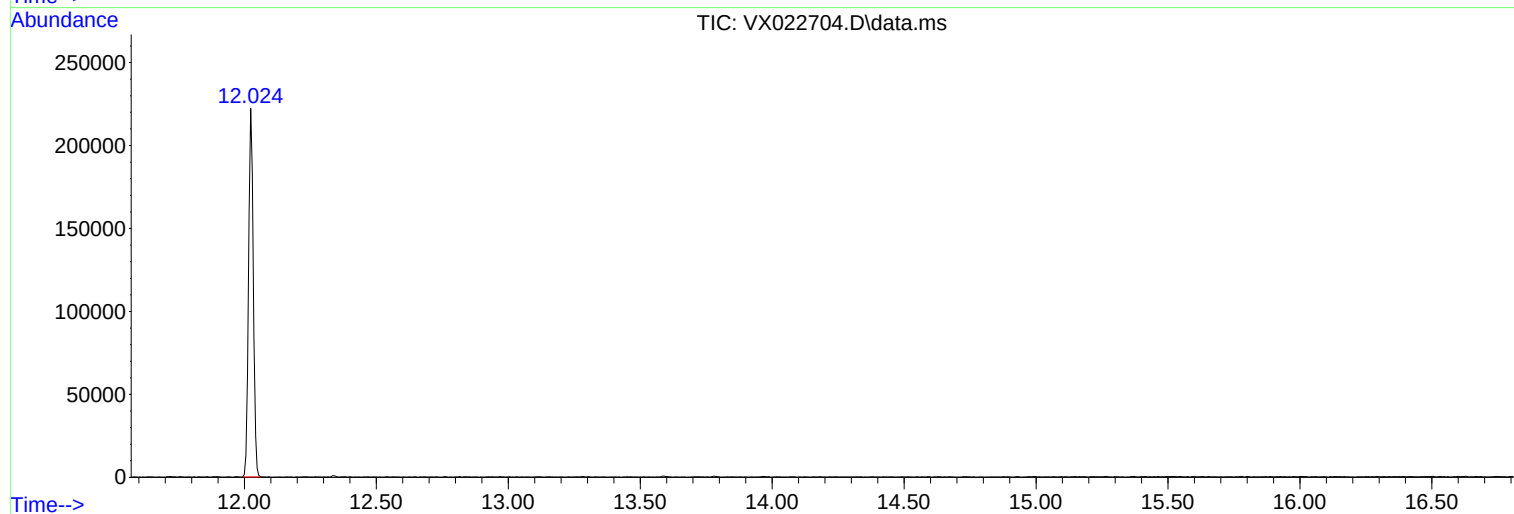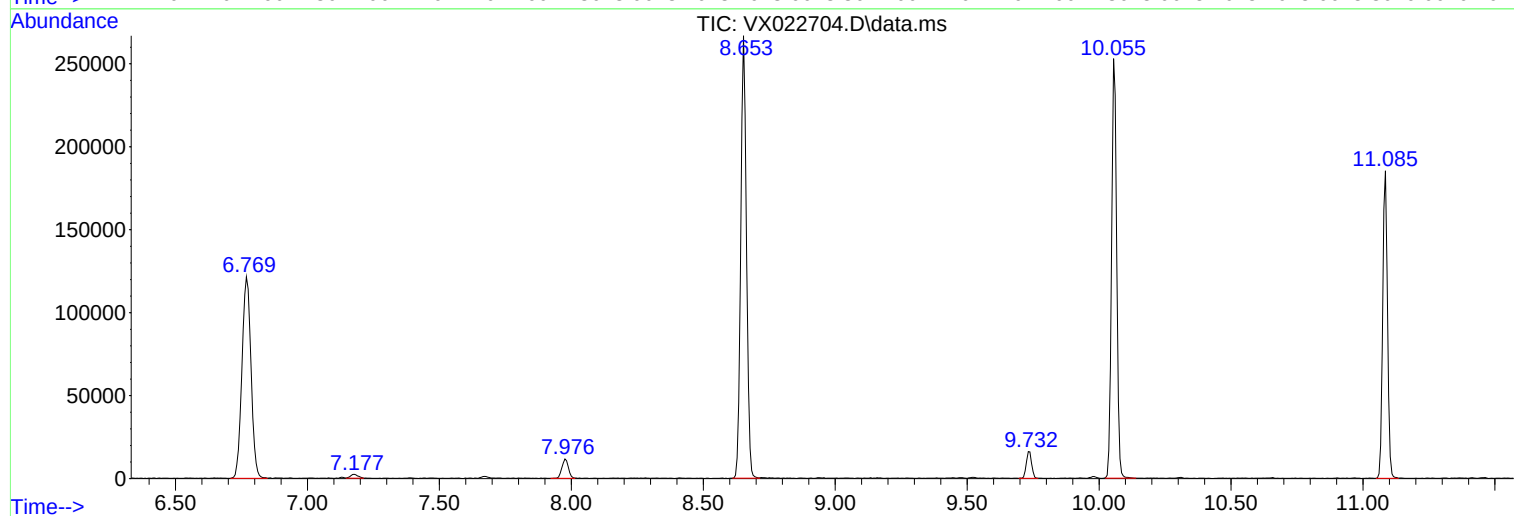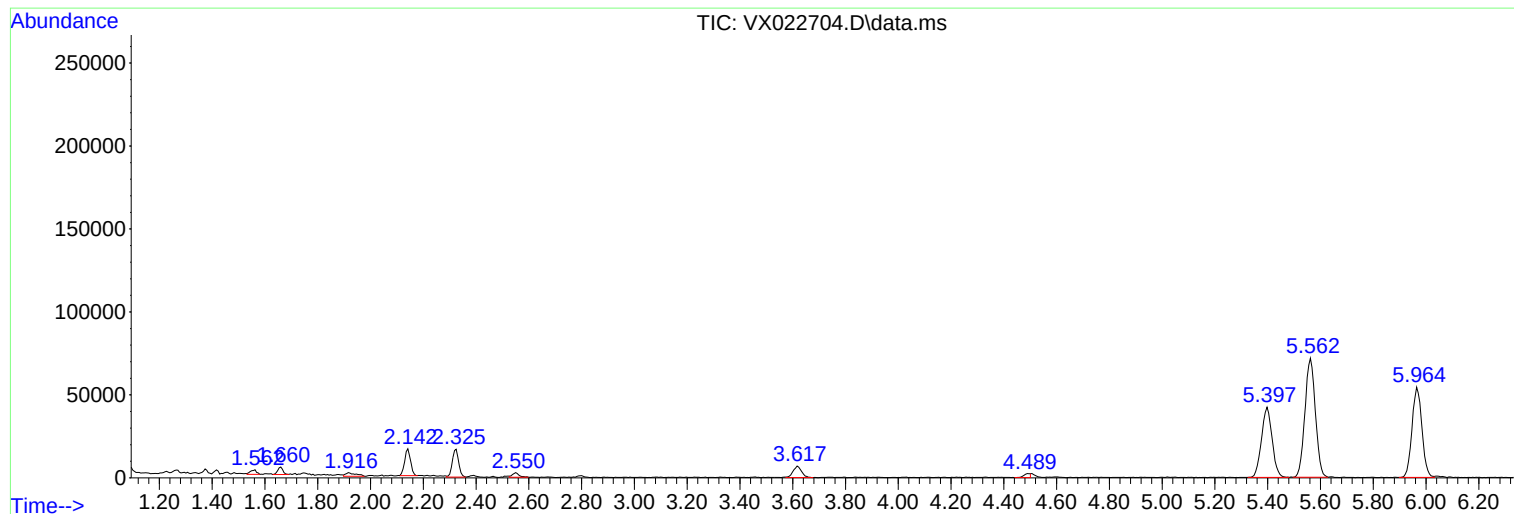

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061521\
Data File : VX022704.D
Acq On : 15 Jun 2021 17:21
Operator : JC/MD
Sample : M2712-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethane, 1,2-dichloro-1,1,2-... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.142	6.28 ug/l	24933	Pentafluorobenzene	5.562

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 1,2-dichloro-1,1,2-trifl...	152	C2HCl2F3	000354-23-4	91
2			Fluorodichloromethane	102	CHCl2F	000075-43-4	17
3			1,4-Pentadiene, 3-methyl-	82	C6H10	001115-08-8	9
4			Cyclopropane, 1,2-dimethyl-3-met...	82	C6H10	062338-02-7	9
5			Benzene, (3-chloro-1-propenyl)-	152	C9H9Cl	002687-12-9	9

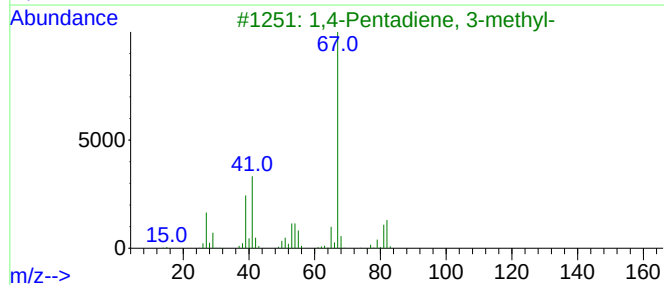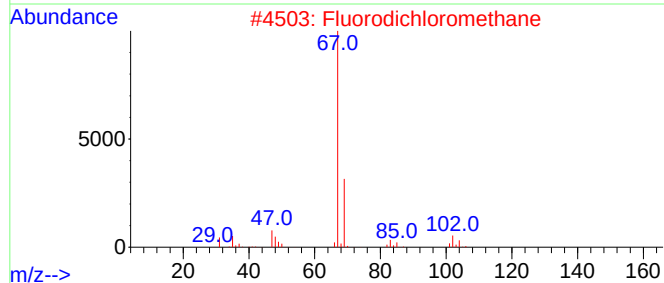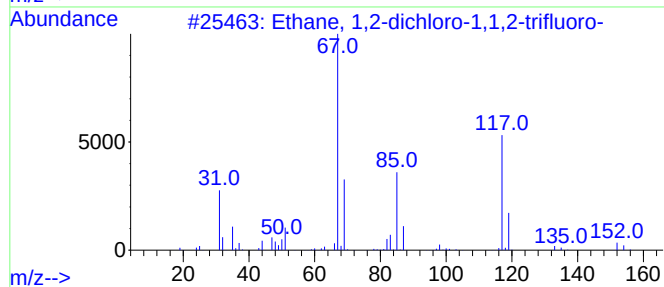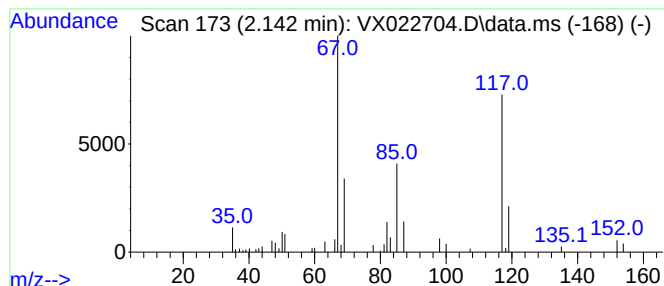

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061521\
Data File : VX022704.D
Acq On : 15 Jun 2021 17:21
Operator : JC/MD
Sample : M2712-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethane, 1,2-dic...	2.142	6.3	ug/l	24933	1	5.562	198358	50.0