

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061522\
 Data File : VX029503.D
 Acq On : 15 Jun 2022 11:02
 Operator : JC/MD
 Sample : VX0615WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0615WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M

Title : SW846 8260

Signal : TIC: VX029503.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.947	293	305	313	rBV	12025	25855	1.95%	0.370%
2	4.574	563	572	582	rBV2	4553	16414	1.24%	0.235%
3	5.385	693	705	719	rBV2	150390	436260	32.98%	6.239%
4	5.550	721	732	751	rVB	288828	824345	62.32%	11.790%
5	5.958	788	799	812	rBV	160100	430598	32.55%	6.158%
6	6.763	920	931	945	rBV	423573	1018002	76.96%	14.560%
7	7.129	982	991	1001	rBV2	8852	20962	1.58%	0.300%
8	8.647	1231	1240	1256	rBV	826195	1322829	100.00%	18.919%
9	10.055	1465	1471	1487	rBV	841133	1118051	84.52%	15.990%
10	11.079	1634	1639	1649	rBV	625315	805759	60.91%	11.524%
11	12.024	1788	1794	1804	rBV	784359	972898	73.55%	13.914%




Sum of corrected areas: 6991973

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061522\
Data File : VX029503.D
Acq On : 15 Jun 2022 11:02
Operator : JC/MD
Sample : VX0615WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0615WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

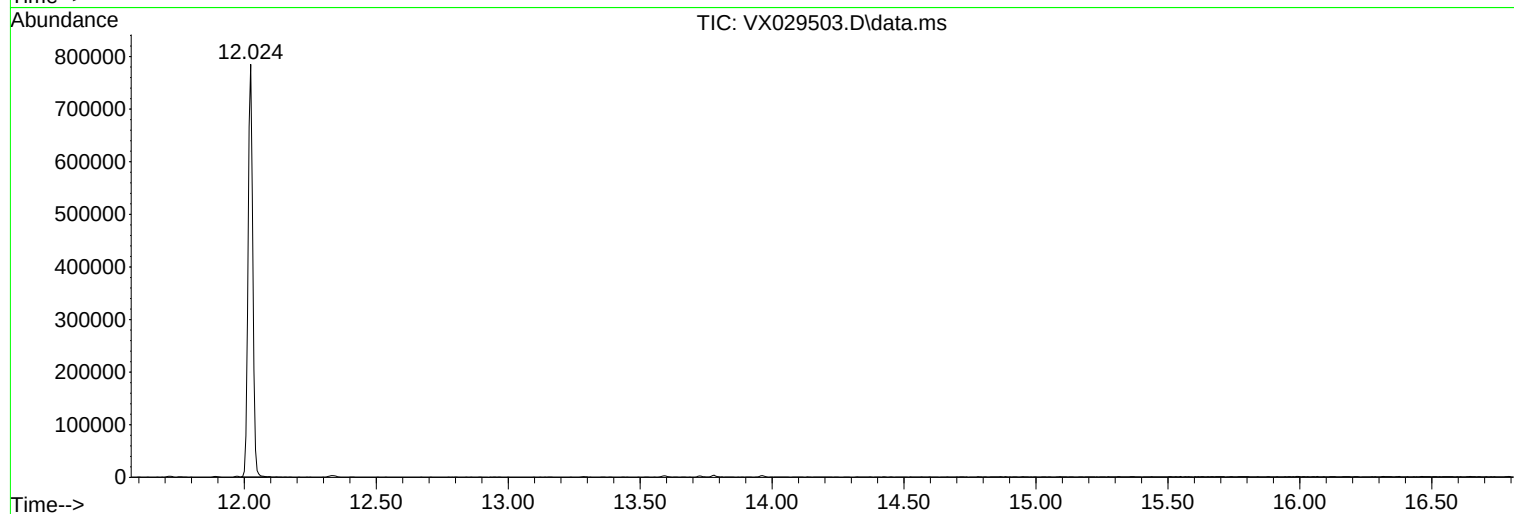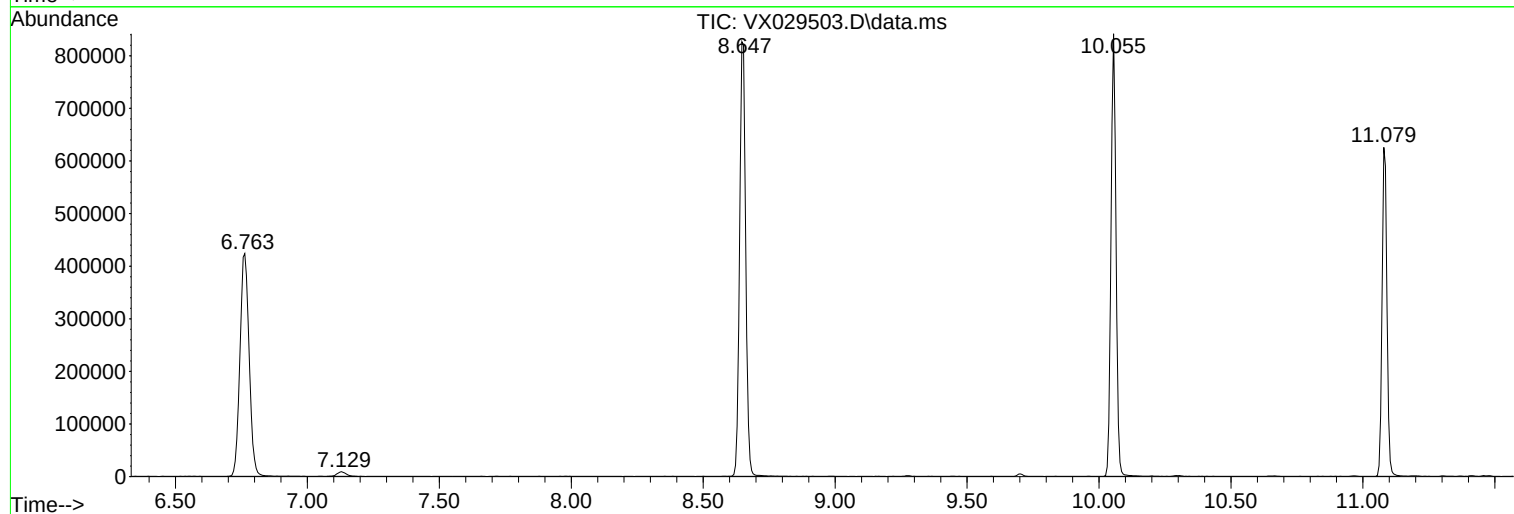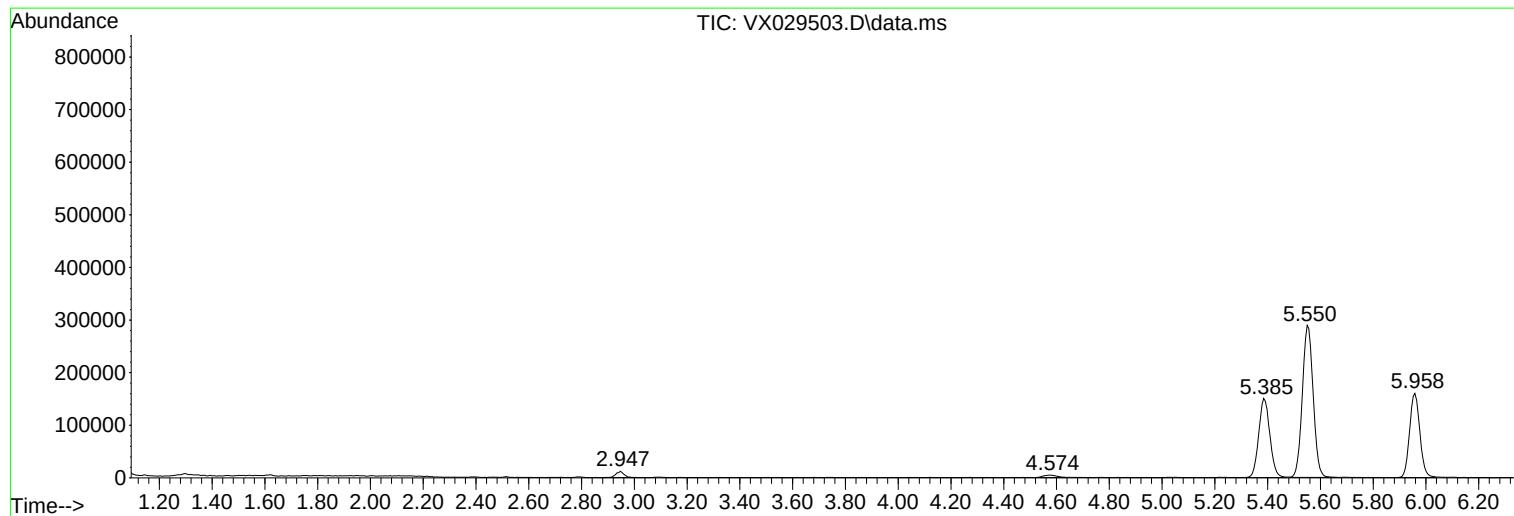

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061522\
Data File : VX029503.D
Acq On : 15 Jun 2022 11:02
Operator : JC/MD
Sample : VX0615WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0615WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061522\
Data File : VX029503.D
Acq On : 15 Jun 2022 11:02
Operator : JC/MD
Sample : VX0615WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0615WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc