


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061523\
Data File : VX036162.D
Acq On : 15 Jun 2023 10:31
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X052323W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue May 23 11:36:37 2023

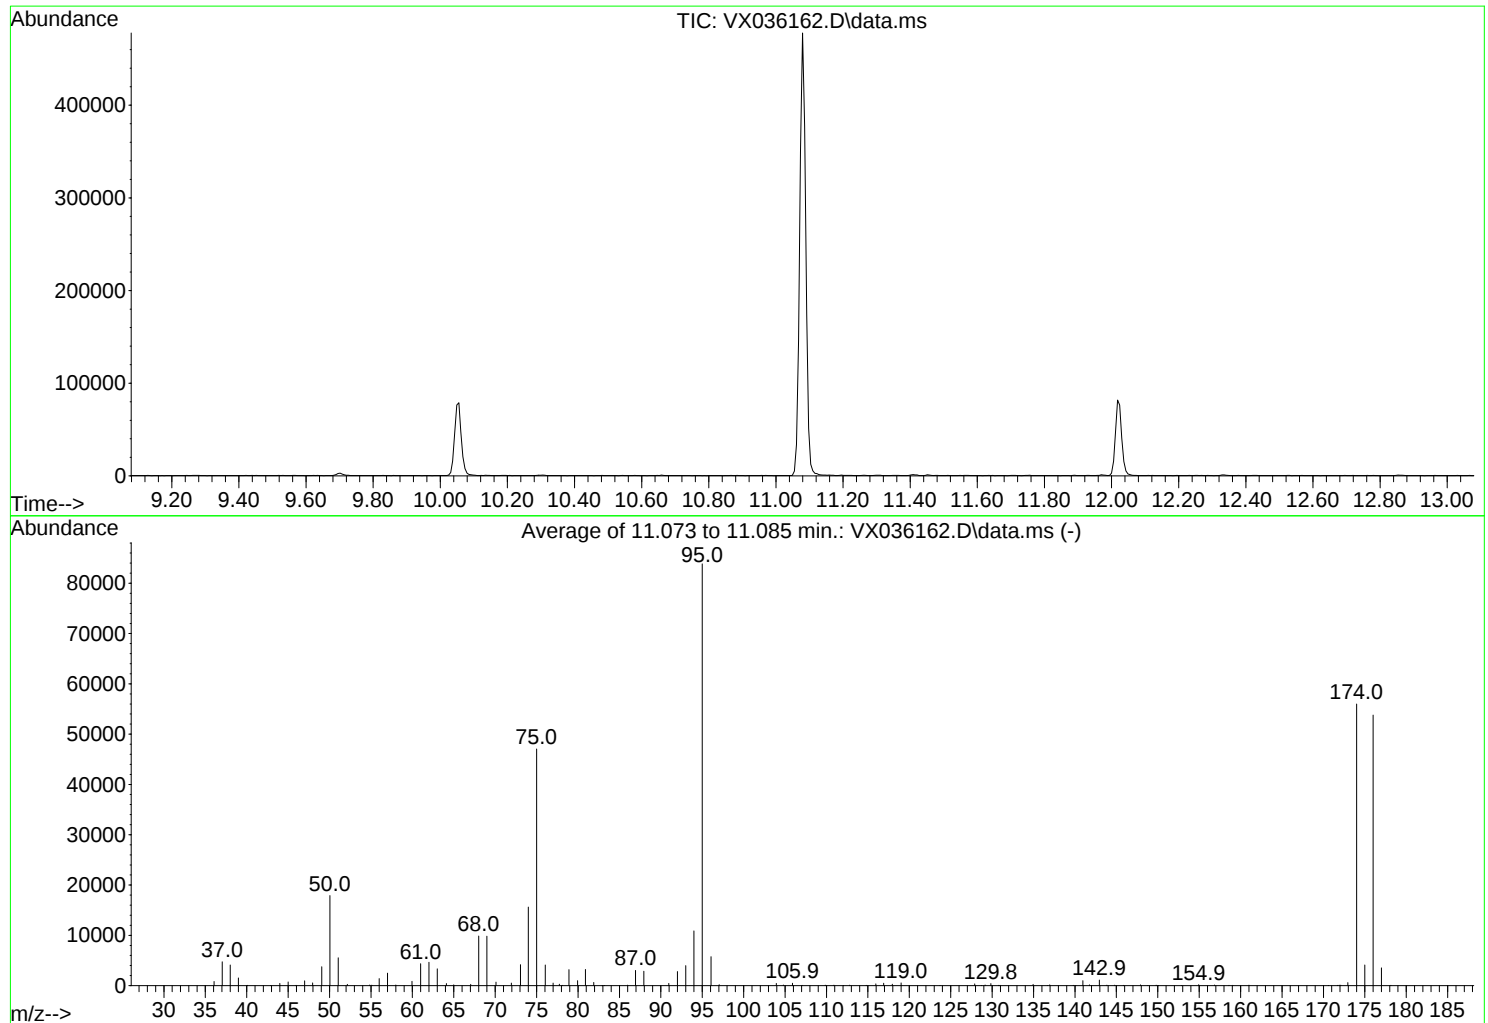

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.4	17908	PASS
75	95	30	60	56.1	47040	PASS
95	95	100	100	100.0	83856	PASS
96	95	5	9	6.9	5774	PASS
173	174	0.00	2	1.1	592	PASS
174	95	50	100	66.8	55987	PASS
175	174	5	9	7.3	4113	PASS
176	174	95	101	96.1	53789	PASS
177	176	5	9	6.6	3546	PASS