

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX061620\
 Data File : VX016784.D
 Acq On : 16 Jun 2020 17:00
 Operator : JC/SP
 Sample : L3005-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 LF017MW001-200611

Quant Time: Jun 17 03:57:29 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061520W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 16 02:02:35 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	226501	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	360285	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	370750	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	190713	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.03	65	131753	51.71	ug/l	0.00
Spiked Amount			Recovery	=	103.42%	
35) Dibromofluoromethane	5.46	113	111416	50.12	ug/l	0.00
Spiked Amount			Recovery	=	100.24%	
50) Toluene-d8	8.70	98	442892	54.03	ug/l	0.00
Spiked Amount			Recovery	=	108.06%	
62) 4-Bromofluorobenzene	11.12	95	179463	57.24	ug/l	0.00
Spiked Amount			Recovery	=	114.48%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
4) Vinyl Chloride	1.39	62	1640	0.622	ug/l	94
8) Diethyl Ether	2.17	74	2722	1.754	ug/l	96
11) Tert butyl alcohol	3.00	59	14814	23.146	ug/l	99
13) Acrolein	2.28	56	484	4.065	ug/l #	76
16) Acetone	2.42	43	14956	12.942	ug/l	98
21) trans-1,2-Dichloroethene	3.14	96	2716	1.142	ug/l	89
25) 2-Butanone	4.65	43	8720	5.007	ug/l #	80
26) 2,2-Dichloropropane	4.64	77	11542	3.064	ug/l #	53
27) cis-1,2-Dichloroethene	4.57	96	3326	1.223	ug/l	81
29) Tetrahydrofuran	5.10	42	5205	4.613	ug/l	96
31) Cyclohexane	5.62	56	3771	1.830	ug/l #	1
36) 1,1-Dichloropropene	5.64	75	15604	4.901	ug/l #	50
37) Ethyl Acetate	4.65	43	8720	2.501	ug/l #	1
38) Carbon Tetrachloride	5.64	117	21600	5.974	ug/l #	17
39) Methylcyclohexane	7.19	83	128	0.987	ug/l #	1
41) Methacrylonitrile	5.09	41	3316	1.784	ug/l #	43
42) 1,2-Dichloroethane	6.17	62	855	0.242	ug/l	94
43) Isopropyl Acetate	6.42	43	2283	0.418	ug/l #	62
44) Trichloroethene	7.19	130	13966	4.658	ug/l	95
49) 1,4-Dioxane	7.71	88	2751	42.919	ug/l #	89
59) 2-Hexanone	9.53	43	13784	5.302	ug/l #	1
65) Chlorobenzene	10.12	112	182567	24.268	ug/l	96
76) 1,2,3-Trichloropropane	11.12	75	85539	21.328	ug/l #	37
81) trans-1,4-Dichloro-2-buten	11.12	75	85539	53.693	ug/l #	13
91) 1,2-Dichlorobenzene	12.37	146	3616	0.605	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX061620\
Data File : VX016784.D
Acq On : 16 Jun 2020 17:00
Operator : JC/SP
Sample : L3005-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LF017MW001-200611

Quant Time: Jun 17 03:57:29 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061520W.M
Quant Title : SW846 8260
QLast Update : Tue Jun 16 02:02:35 2020
Response via : Initial Calibration

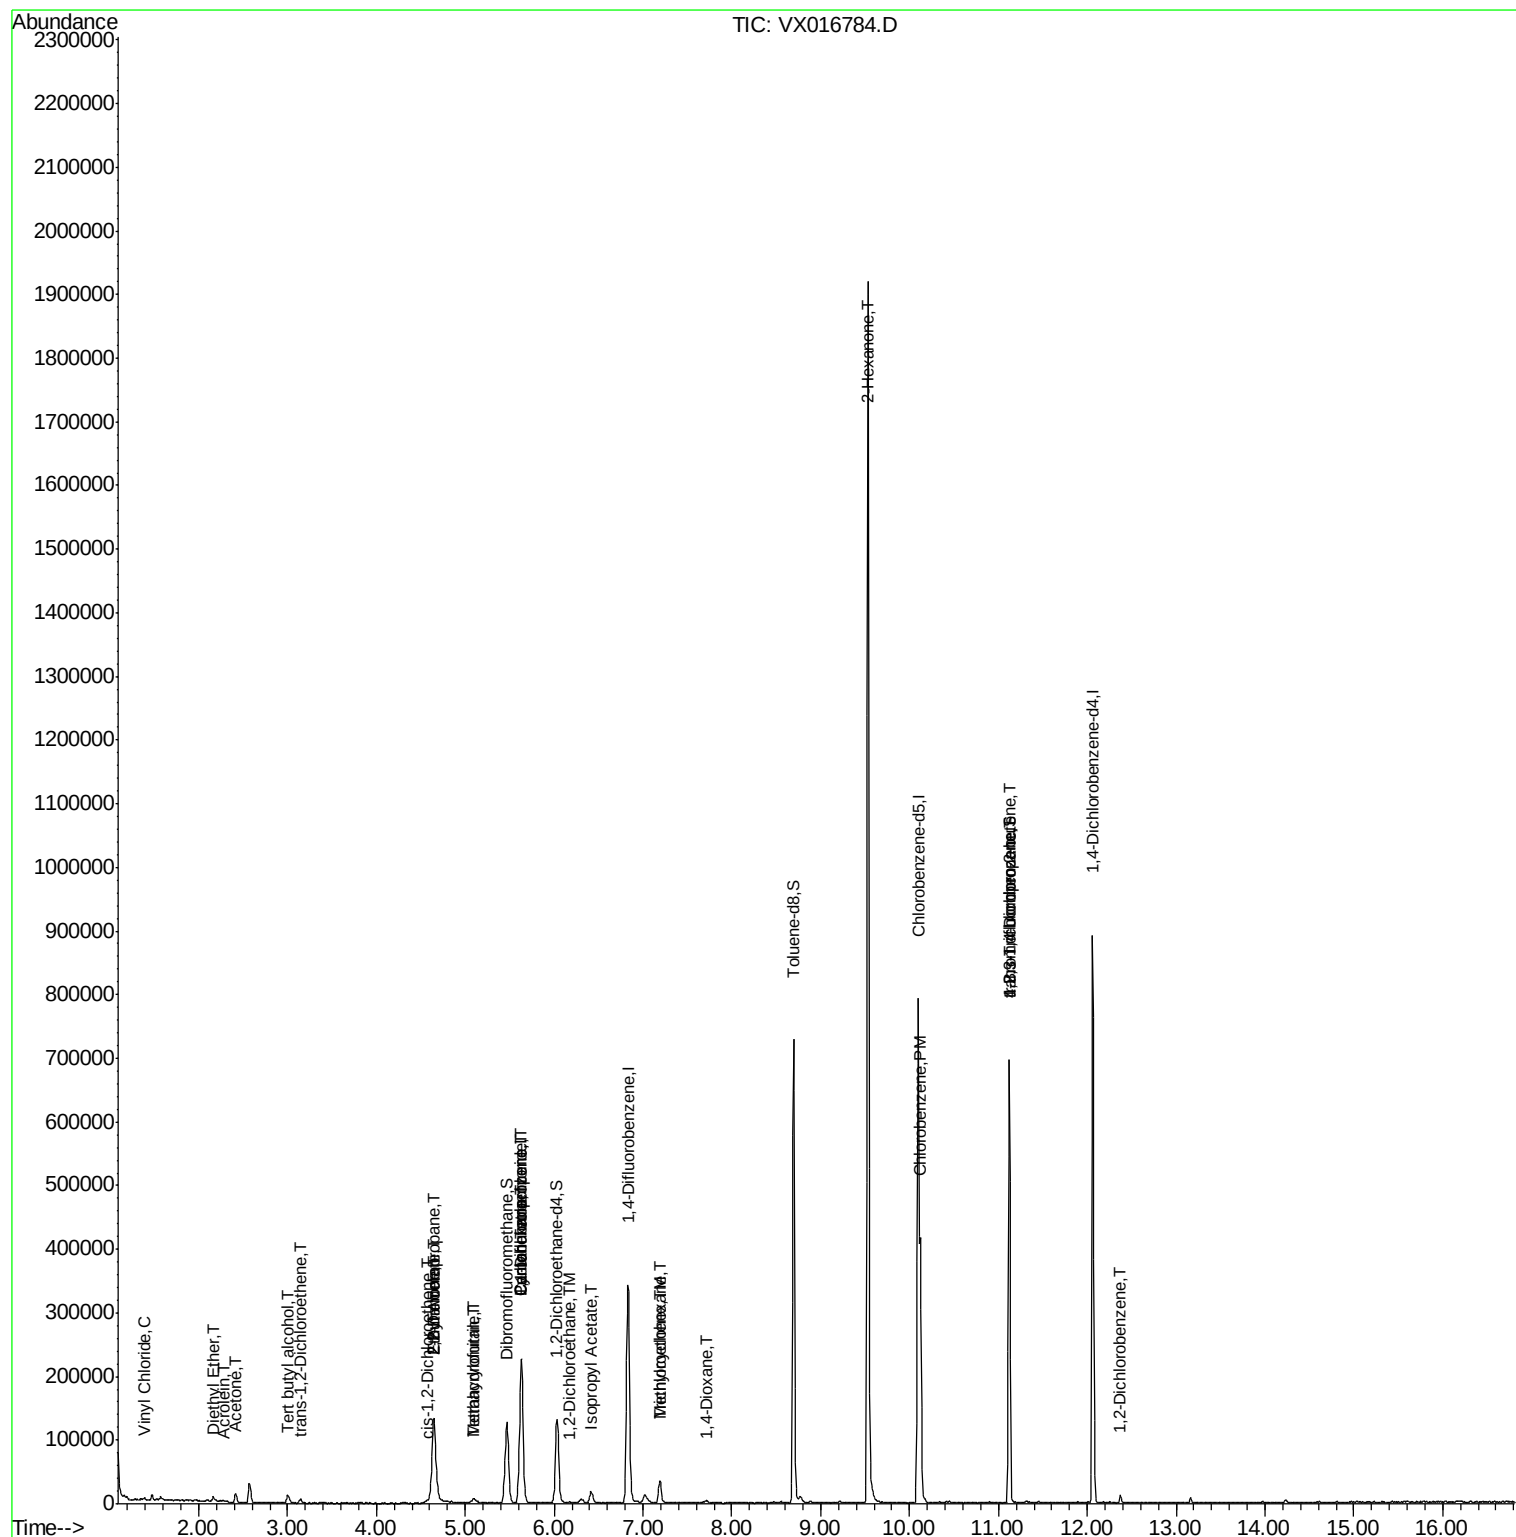



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.00 min

Lab File: VX016784.D

Acq: 16 Jun 2020 17:00

Instrument :

MSVOA_X

ClientSampleId :


LF017MW001-200611

Tot Ion:168 Resp: 226501

Ion Ratio Lower Upper




168 100

99 53.1 43.8 65.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

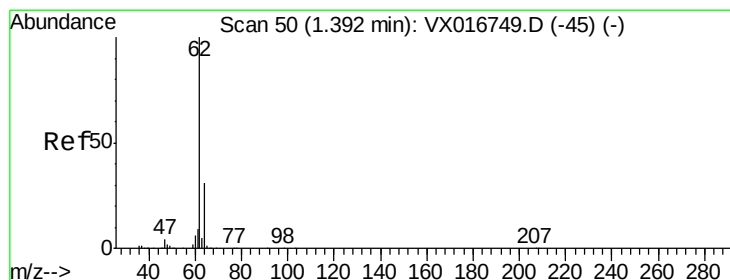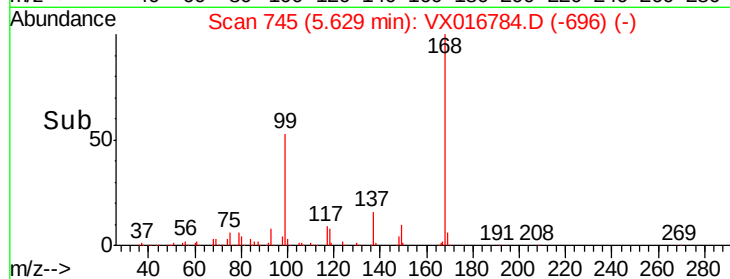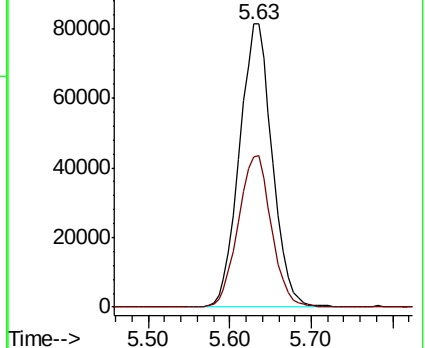

#4

Vinyl Chloride

Concen: 0.622 ug/l

RT: 1.39 min Scan# 50

Delta R.T. -0.00 min

Lab File: VX016784.D


Acq: 16 Jun 2020 17:00

Tgt Ion: 62 Resp: 1640

Ion Ratio Lower Upper



62 100


64 28.0 25.1 37.7



Abundance Ion 61.90 (61.60 to 62.60): VX0

Ion 63.90 (63.60 to 64.60): VX0

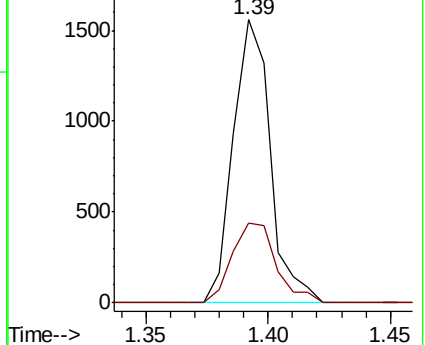



#8

Diethyl Ether

Concen: 1.754 ug/l

RT: 2.17 min Scan# 177

Delta R.T. -0.00 min

Lab File: VX016784.D

Acq: 16 Jun 2020 17:00

Instrument :

MSVOA_X

ClientSampleId :





LF017MW001-200611

Tot Ion: 74 Resp: 2722

Ion Ratio Lower Upper

74 100

45 83.1 43.5 130.7

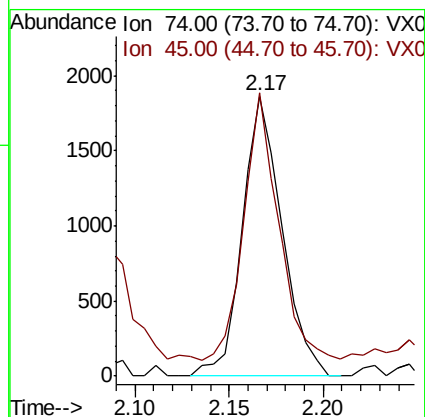

#11

Tert butyl alcohol

Concen: 23.146 ug/l

RT: 3.00 min Scan# 314

Delta R.T. -0.01 min

Lab File: VX016784.D




Acq: 16 Jun 2020 17:00


Tgt Ion: 59 Resp: 14814

Ion Ratio Lower Upper

59 100

57 10.6 8.2 12.2

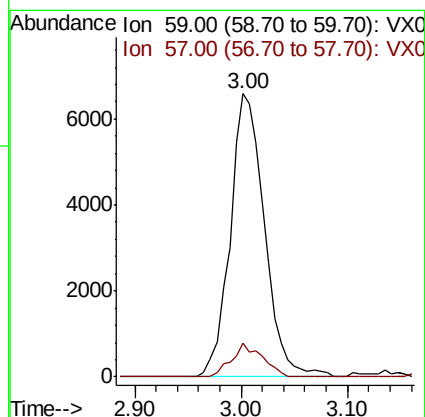



#13

Acrolein

Concen: 4.065 ug/l

RT: 2.28 min Scan# 196

Delta R.T. 0.01 min

Lab File: VX016784.D

Acq: 16 Jun 2020 17:00

Instrument :

MSVOA_X

ClientSampleId :


LF017MW001-200611

Tot Ion: 56 Resp: 484

Ion Ratio Lower Upper




56 100

55 93.0 58.2 87.4#



Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

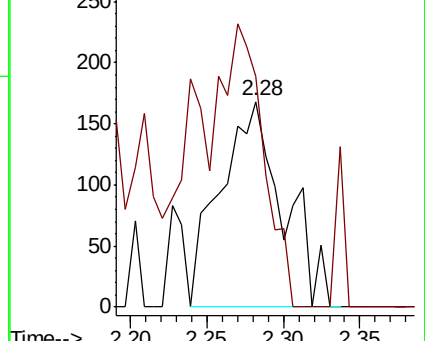

#16

Acetone

Concen: 12.942 ug/l

RT: 2.42 min Scan# 218

Delta R.T. -0.00 min

Lab File: VX016784.D


Acq: 16 Jun 2020 17:00

Tgt Ion: 43 Resp: 14956

Ion Ratio Lower Upper



43 100


58 31.6 26.3 39.5



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

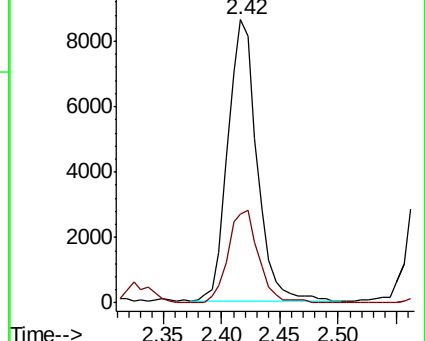



#21

trans-1,2-Dichloroethene

Concen: 1.142 ug/l

RT: 3.14 min Scan# 337

Delta R.T. -0.00 min

Lab File: VX016784.D

Acq: 16 Jun 2020 17:00

Instrument :

MSVOA_X

ClientSampleId :

LF017MW001-200611


Tot Ion: 96 Resp: 2716

Ion Ratio Lower Upper

96 100

61 117.5 105.4 158.2




98 57.5 50.8 76.2



Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

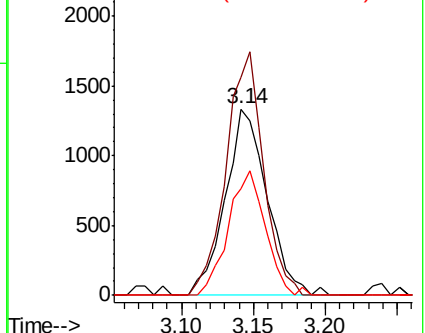

#25

2-Butanone

Concen: 5.007 ug/l

RT: 4.65 min Scan# 584

Delta R.T. 0.01 min

Lab File: VX016784.D


Acq: 16 Jun 2020 17:00

Tgt Ion: 43 Resp: 8720

Ion Ratio Lower Upper



43 100


72 19.4 24.2 36.4#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0




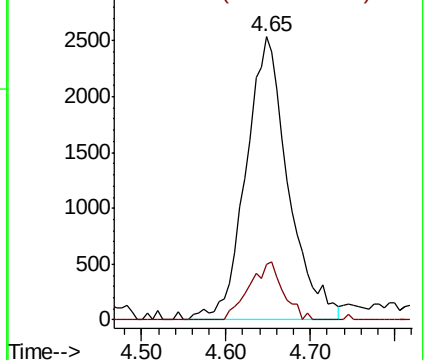




#26
 2,2-Dichloropropane
 Concen: 3.064 ug/l
 RT: 4.64 min Scan# 583
 Delta R.T. 0.09 min
 Lab File: VX016784.D
 Acq: 16 Jun 2020 17:00




Instrument :
 MSVOA_X
 ClientSampleId :
 LF017MW001-200611


Tot Ion: 77 Resp: 11542
 Ion Ratio Lower Upper
 77 100
 97 0.0 11.5 34.4#

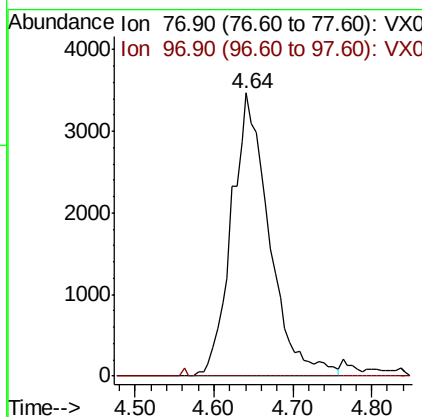

#27
 cis-1,2-Dichloroethene
 Concen: 1.223 ug/l
 RT: 4.57 min Scan# 571
 Delta R.T. -0.00 min
 Lab File: VX016784.D
 Acq: 16 Jun 2020 17:00

Tgt Ion: 96 Resp: 3326
 Ion Ratio Lower Upper
 96 100
 61 110.0 0.0 276.2
 98 56.3 0.0 130.0

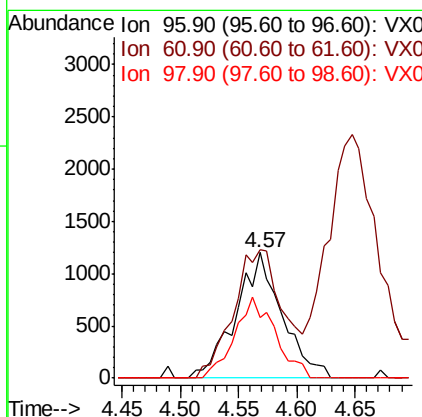



#29

Tetrahydrofuran

Concen: 4.613 ug/l

RT: 5.10 min Scan# 658

Delta R.T. 0.01 min

Lab File: VX016784.D

Acq: 16 Jun 2020 17:00

Instrument :

MSVOA_X

ClientSampleId :

LF017MW001-200611


Tot Ion: 42 Resp: 5205

Ion Ratio Lower Upper

42 100

72 49.1 41.0 61.6




71 50.5 38.2 57.4



Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0

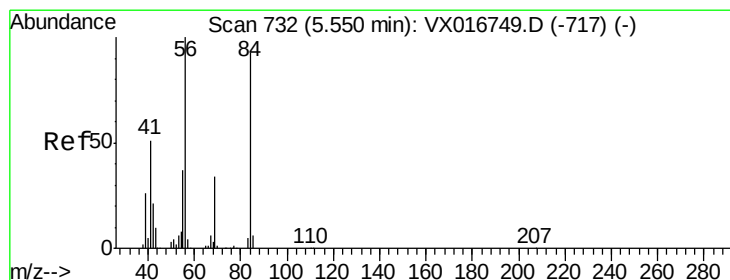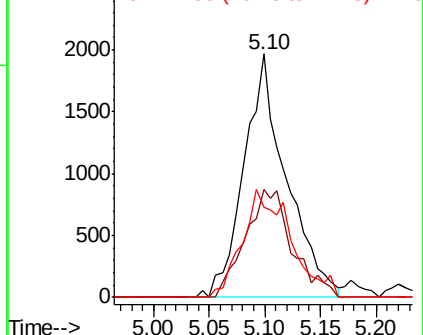

#31

Cyclohexane

Concen: 1.830 ug/l

RT: 5.62 min Scan# 744

Delta R.T. 0.07 min

Lab File: VX016784.D

Acq: 16 Jun 2020 17:00


Tgt Ion: 56 Resp: 3771

Ion Ratio Lower Upper

56 100

69 195.5 27.1 40.7#



84 179.3 74.0 111.0#




Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 84.00 (83.70 to 84.70): VX0

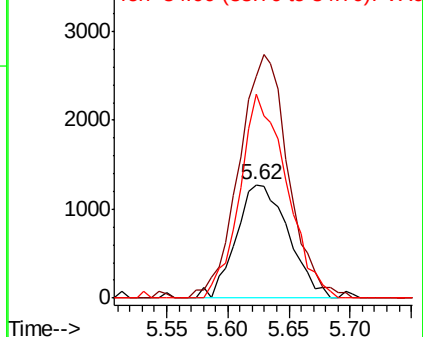



#33

1,2-Dichloroethane-d4

Concen: 51.715 ug/l

RT: 6.03 min Scan# 811

Delta R.T. 0.00 min

Lab File: VX016784.D

Acq: 16 Jun 2020 17:00

Instrument :

MSVOA_X

ClientSampleId :


LF017MW001-200611

Tot Ion: 65 Resp: 131753

Ion Ratio Lower Upper




65 100

67 51.5 0.0 103.0



Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

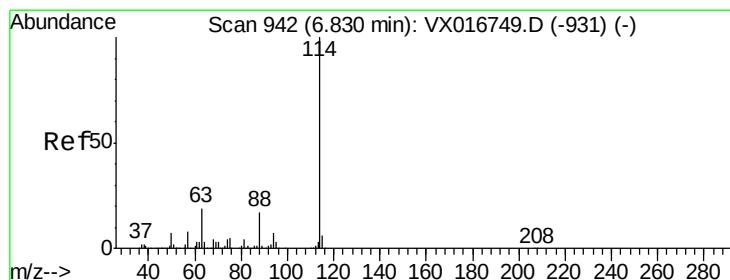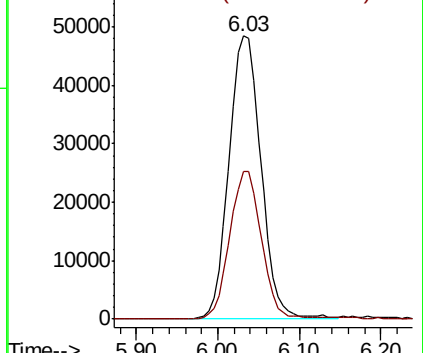

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX016784.D

Acq: 16 Jun 2020 17:00


Tgt Ion: 114 Resp: 360285

Ion Ratio Lower Upper

114 100

63 20.0 0.0 38.8



88 16.5 0.0 33.4




Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

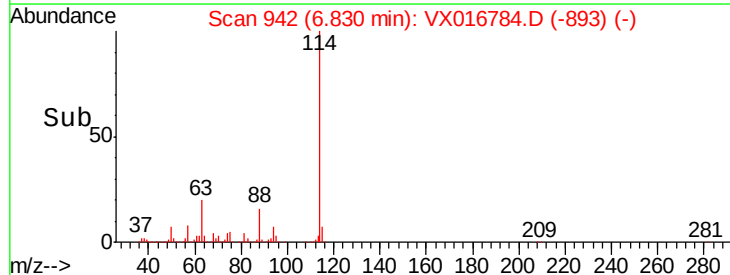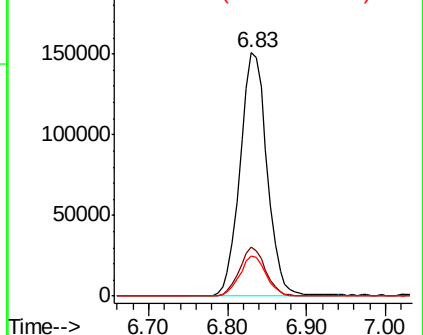

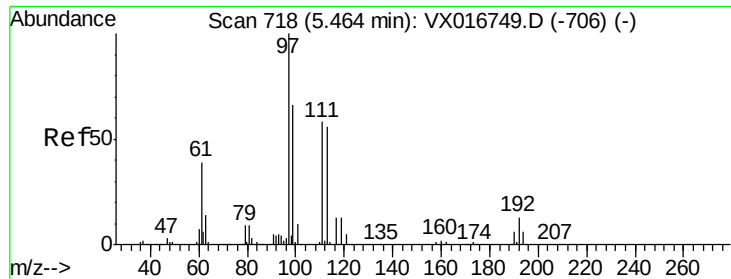

#35

Dibromofluoromethane

Concen: 50.122 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.00 min

Lab File: VX016784.D

Acq: 16 Jun 2020 17:00

Instrument :

MSVOA_X

ClientSampleId :

LF017MW001-200611


Tot Ion:113 Resp: 111416

Ion Ratio Lower Upper

113 100

111 100.5 81.8 122.6




192 23.2 18.2 27.4

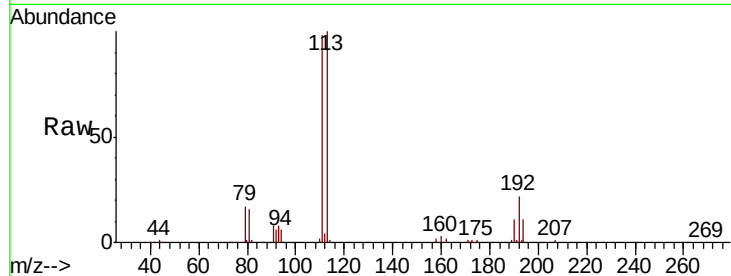

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

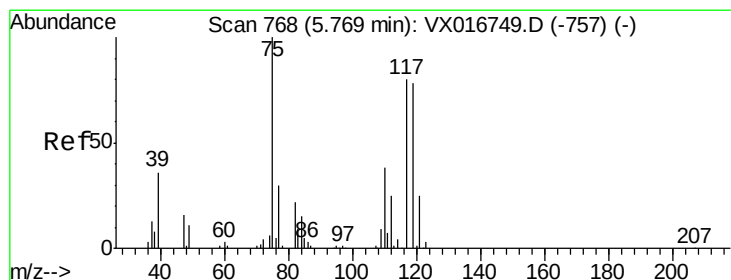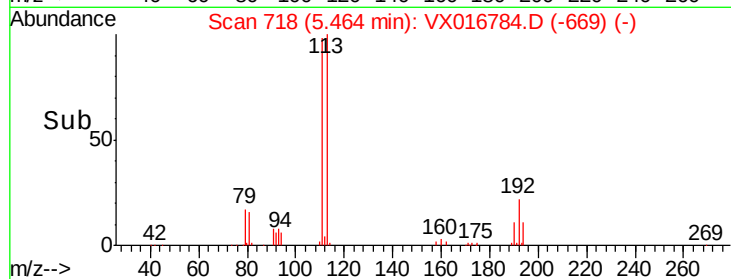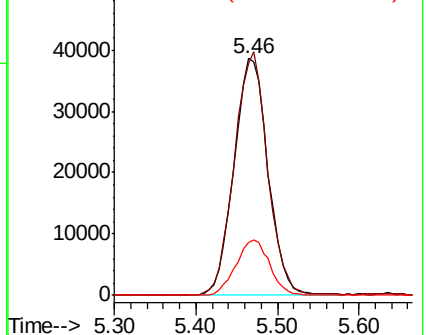

#36

1,1-Dichloropropene

Concen: 4.901 ug/l

RT: 5.64 min Scan# 746

Delta R.T. -0.13 min

Lab File: VX016784.D

Acq: 16 Jun 2020 17:00


Tgt Ion: 75 Resp: 15604

Ion Ratio Lower Upper

75 100

110 10.1 18.4 55.2#



77 0.0 24.7 37.1#

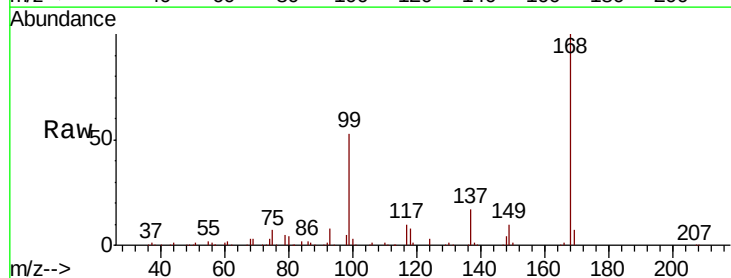


Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

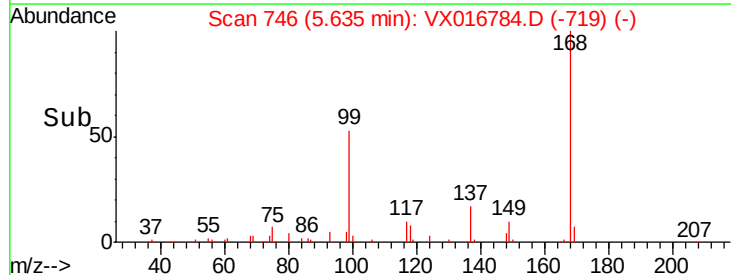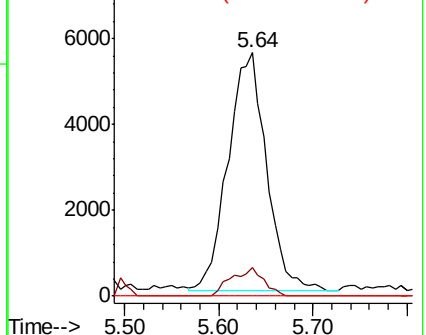



#37

Ethyl Acetate

Concen: 2.501 ug/l

RT: 4.65 min Scan# 584

Delta R.T. -0.15 min

Lab File: VX016784.D

Acq: 16 Jun 2020 17:00

Instrument :

MSVOA_X

ClientSampleId :

LF017MW001-200611


Tot Ion: 43 Resp: 8720

Ion Ratio Lower Upper

43 100

61 86.1 12.4 18.6#




70 3.9 10.8 16.2#

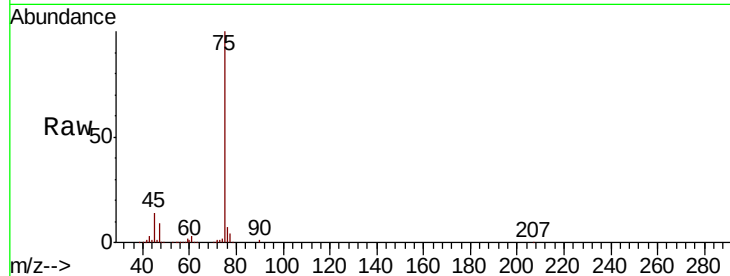

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 70.00 (69.70 to 70.70): VX0

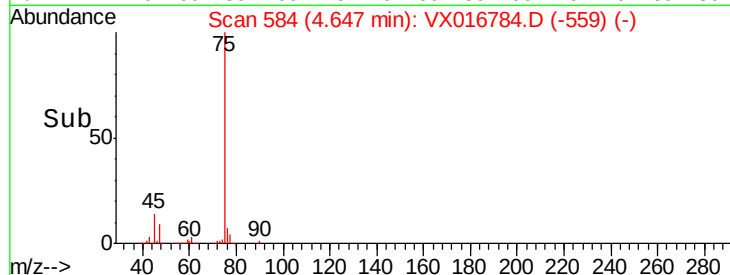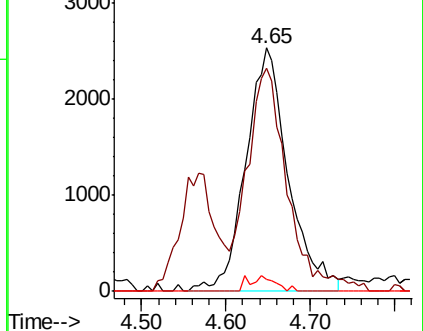

#38

Carbon Tetrachloride

Concen: 5.974 ug/l

RT: 5.64 min Scan# 746

Delta R.T. -0.12 min

Lab File: VX016784.D

Acq: 16 Jun 2020 17:00


Tgt Ion: 117 Resp: 21600

Ion Ratio Lower Upper

117 100

119 5.9 76.7 115.1#



121 0.0 24.7 37.1#

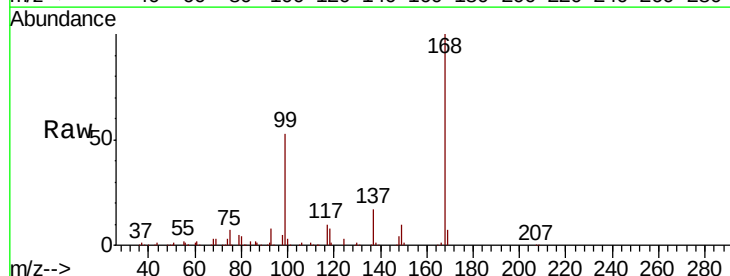


Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V




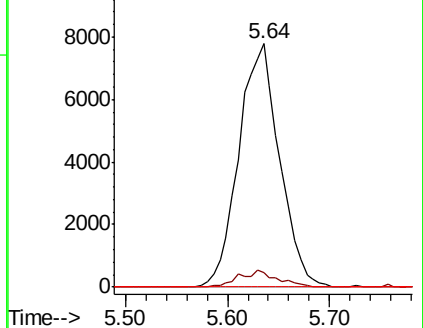




#39
Methylvlcyclohexane
Concen: 0.987 ug/l
RT: 7.19 min Scan# 1001
Delta R.T. -0.25 min
Lab File: VX016784.D
Acq: 16 Jun 2020 17:00




Instrument :
MSVOA_X
ClientSampleId :
LF017MW001-200611


Tot Ion: 83 Resp: 128
Ion Ratio Lower Upper
83 100
55 0.0 57.3 85.9#
98 136.7 40.3 60.5#

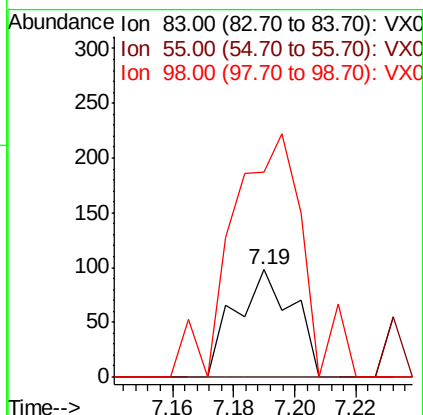

#41
Methacrylonitrile
Concen: 1.784 ug/l
RT: 5.09 min Scan# 657
Delta R.T. 0.09 min
Lab File: VX016784.D
Acq: 16 Jun 2020 17:00

Tgt Ion: 41 Resp: 3316
Ion Ratio Lower Upper
41 100
39 49.8 43.7 65.5
67 0.0 64.6 96.8#
52 0.0 25.6 38.4#

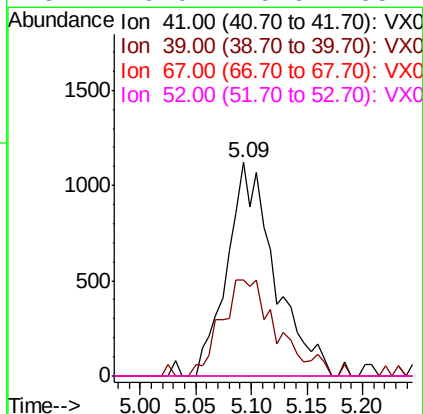



#42

1,2-Dichloroethane

Concen: 0.242 ug/l

RT: 6.17 min Scan# 833

Delta R.T. -0.00 min

Lab File: VX016784.D

Acq: 16 Jun 2020 17:00

Instrument :

MSVOA_X

ClientSampleId :


LF017MW001-200611

Tot Ion: 62 Resp: 855

Ion Ratio Lower Upper

62 100

98 7.8 0.0 20.2



Abundance Ion 61.90 (61.60 to 62.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

6.17

400

300



200

100

0

6.10 6.15 6.20

Time-->



#43

Isopropyl Acetate

Concen: 0.418 ug/l

RT: 6.42 min Scan# 875

Delta R.T. 0.01 min

Lab File: VX016784.D

Acq: 16 Jun 2020 17:00


Tgt Ion: 43 Resp: 2283

Ion Ratio Lower Upper

43 100

61 3.5 17.7 26.5#

87 0.0 12.5 18.7#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

6.42


1000


500

0

6.35 6.40 6.45 6.50

Time-->





#44

Trichloroethene

Concen: 4.658 ug/l

RT: 7.19 min Scan# 1001

Delta R.T. -0.00 min

Lab File: VX016784.D

Acq: 16 Jun 2020 17:00

Instrument :

MSVOA_X

ClientSampleId :


LF017MW001-200611

Tot Ion:130 Resp: 13966

Ion Ratio Lower Upper

130 100

95 96.8 0.0 183.6



Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

7.19



6000

4000

2000

0

Time--> 7.10 7.15 7.20 7.25 7.30



#49

1,4-Dioxane

Concen: 42.919 ug/l

RT: 7.71 min Scan# 1087

Delta R.T. -0.00 min

Lab File: VX016784.D

Acq: 16 Jun 2020 17:00


Tgt Ion: 88 Resp: 2751

Ion Ratio Lower Upper

88 100

43 43.5 22.9 34.3#

58 69.8 53.7 80.5



Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2000


1500


1000

500

0

Time--> 7.65 7.70 7.75 7.80









#50
Toluene-d8
Concen: 54.035 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. -0.00 min
Lab File: VX016784.D
Acq: 16 Jun 2020 17:00




Instrument :
MSVOA_X
ClientSampleId :
LF017MW001-200611


Tot Ion: 98 Resp: 442892
Ion Ratio Lower Upper
98 100
100 66.1 53.9 80.9

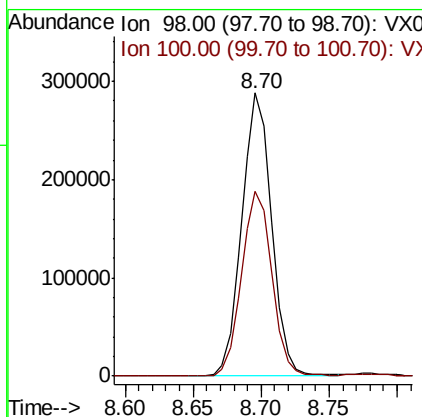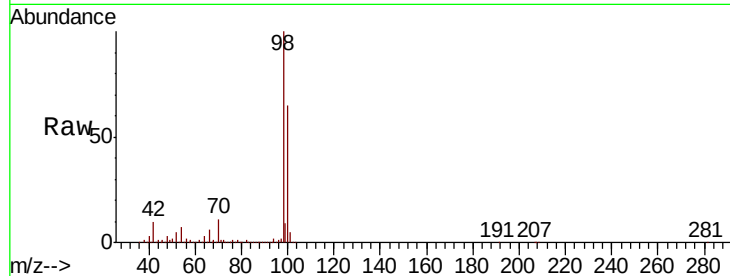

#59
2-Hexanone
Concen: 5.302 ug/l
RT: 9.53 min Scan# 1385
Delta R.T. 0.06 min
Lab File: VX016784.D
Acq: 16 Jun 2020 17:00

Tgt Ion: 43 Resp: 13784
Ion Ratio Lower Upper
43 100
58 567.4 29.9 89.8#

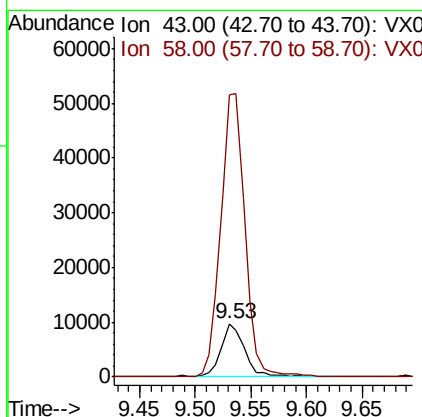



#62

4-Bromofluorobenzene

Concen: 57.243 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX016784.D

Acq: 16 Jun 2020 17:00

Instrument :

MSVOA_X

ClientSampleId :

LF017MW001-200611


Tot Ion: 95 Resp: 179463

Ion Ratio Lower Upper

95 100

174 89.2 0.0 171.0




176 85.0 0.0 166.2

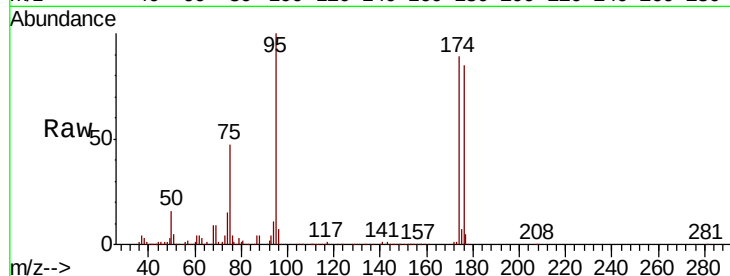

Abundance Ion 94.90 (94.60 to 95.60): VX016784.D (-1597) (-)

Ion 173.80 (173.50 to 174.50): VX016784.D (-1597) (-)

Ion 175.80 (175.50 to 176.50): VX016784.D (-1597) (-)

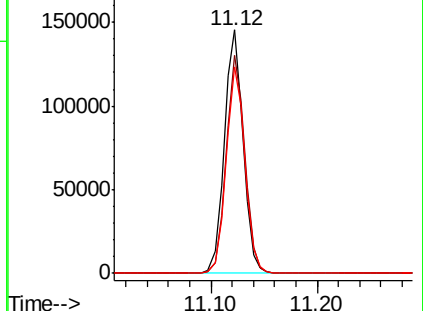

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.10 min Scan# 1478

Delta R.T. -0.00 min

Lab File: VX016784.D

Acq: 16 Jun 2020 17:00


Tgt Ion: 117 Resp: 370750

Ion Ratio Lower Upper

117 100

82 54.0 43.8 65.6



119 32.8 26.2 39.4




Abundance Ion 116.90 (116.60 to 117.60): VX016784.D (-1429) (-)

Ion 82.00 (81.70 to 82.70): VX016784.D (-1429) (-)

Ion 118.90 (118.60 to 119.60): VX016784.D (-1429) (-)



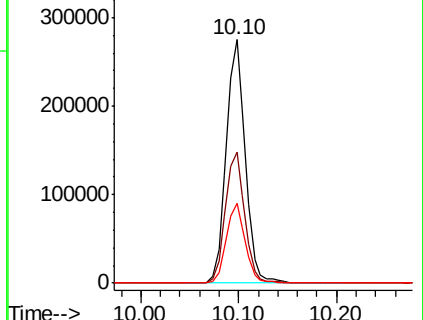





#65
Chlorobenzene
Concen: 24.268 ug/l
RT: 10.12 min Scan# 1482
Delta R.T. -0.00 min
Lab File: VX016784.D
Acq: 16 Jun 2020 17:00




Instrument :
MSVOA_X
ClientSampleId :
LF017MW001-200611


Tot Ion:112 Resp: 182567
Ion Ratio Lower Upper
112 100
114 30.7 26.2 39.4

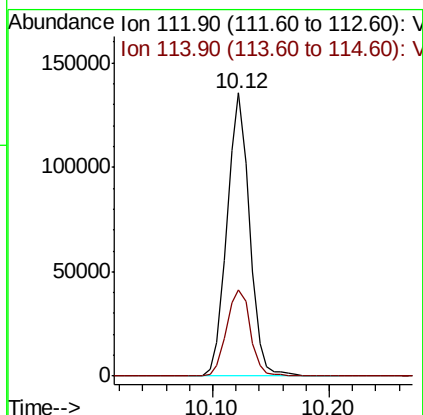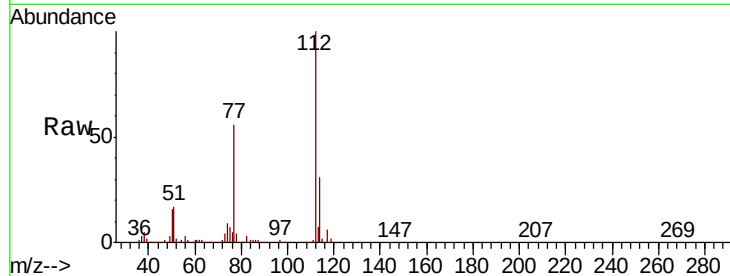

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. -0.00 min
Lab File: VX016784.D
Acq: 16 Jun 2020 17:00

Tgt Ion:152 Resp: 190713
Ion Ratio Lower Upper
152 100
115 57.0 40.3 120.8
150 154.8 0.0 337.4

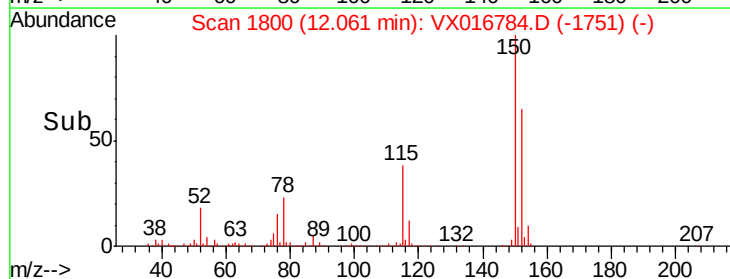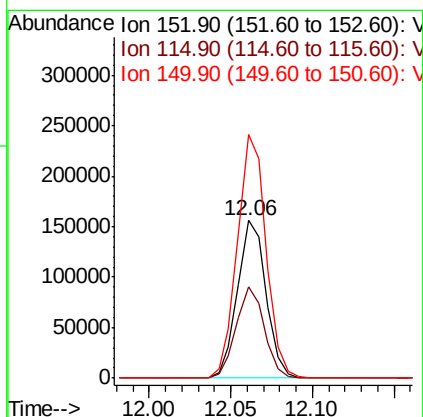

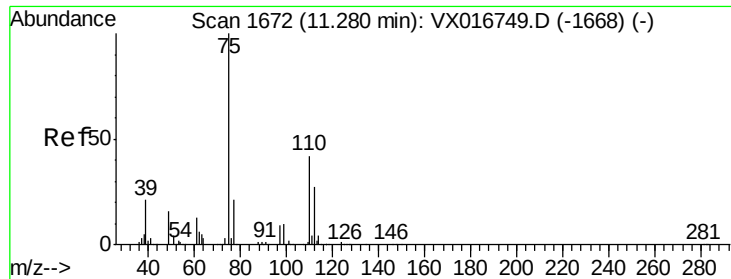

#76

1,2,3-Trichloropropane

Concen: 21.328 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX016784.D

Acq: 16 Jun 2020 17:00

Instrument :

MSVOA_X

ClientSampleId :





LF017MW001-200611

Tot Ion: 75 Resp: 85539

Ion Ratio Lower Upper

75 100

77 1.4 20.3 60.9#

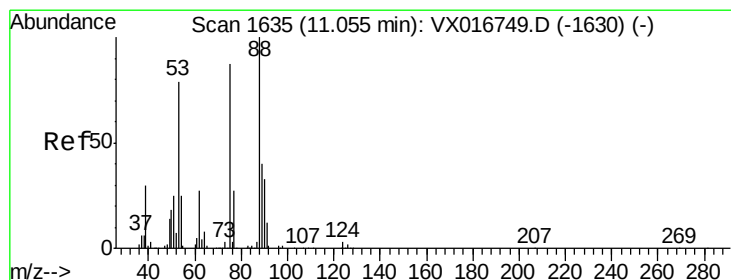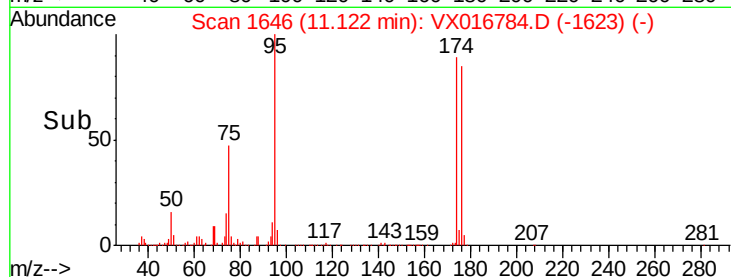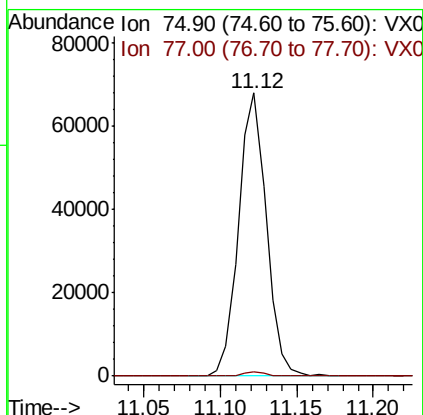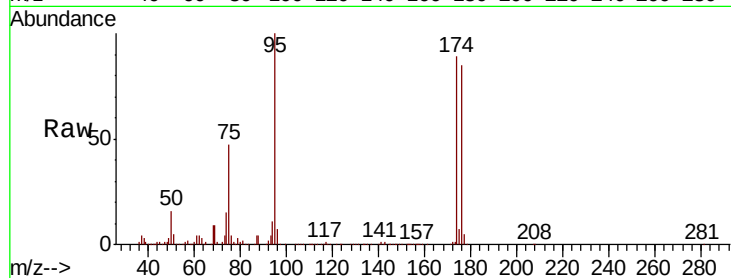

#81

trans-1,4-Dichloro-2-butene

Concen: 53.693 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.07 min

Lab File: VX016784.D

Acq: 16 Jun 2020 17:00




Tgt Ion: 75 Resp: 85539


Ion Ratio Lower Upper

75 100

53 0.1 71.4 107.0#

89 0.1 39.1 58.7#

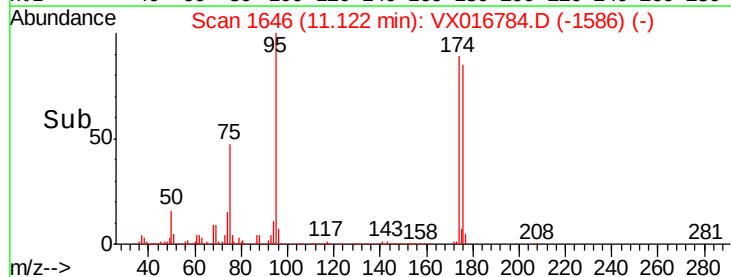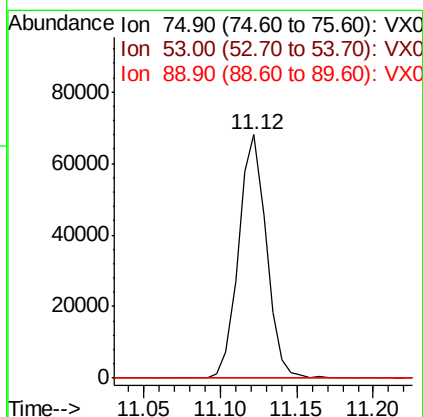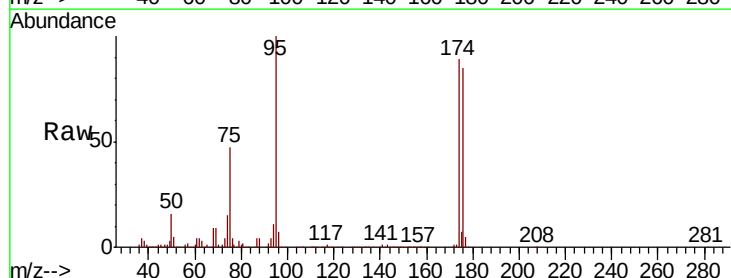

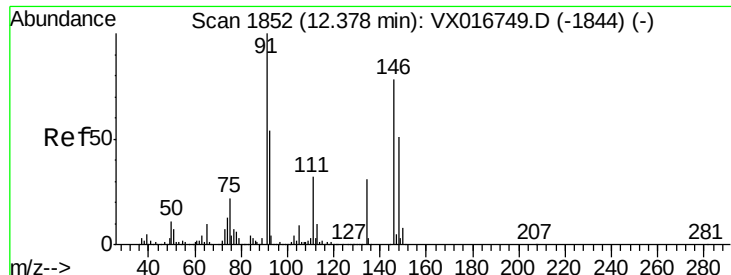

#91
 1,2-Dichlorobenzene
 Concen: 0.605 ug/l
 RT: 12.37 min Scan# 1851
 Delta R.T. -0.01 min
 Lab File: VX016784.D
 Acq: 16 Jun 2020 17:00

Instrument :
 MSVOA_X
 ClientSampleId :
 LF017MW001-200611

Tot Ion	Ratio	Lower	Upper
146	100		
111	41.4	20.8	62.2
148	59.9	32.1	96.5

