

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX061620\
 Data File : VX016777.D
 Acq On : 16 Jun 2020 14:21
 Operator : JC/SP
 Sample : L2993-07RE
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Z1-TB6-200610

Quant Time: Jun 17 04:27:15 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061520W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 16 02:02:35 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	247031	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	392267	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	405085	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	211739	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.03	65	143958	51.81	ug/l	0.00
Spiked Amount						
			Recovery	=	103.62%	
35) Dibromofluoromethane	5.46	113	119329	49.30	ug/l	0.00
Spiked Amount						
			Recovery	=	98.60%	
50) Toluene-d8	8.70	98	486237	54.49	ug/l	0.00
Spiked Amount						
			Recovery	=	108.98%	
62) 4-Bromofluorobenzene	11.12	95	198876	58.26	ug/l	0.00
Spiked Amount						
			Recovery	=	116.52%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX061620\
Data File : VX016777.D
Acq On : 16 Jun 2020 14:21
Operator : JC/SP
Sample : L2993-07RE
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Z1-TB6-200610

Quant Time: Jun 17 04:27:15 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061520W.M
Quant Title : SW846 8260
QLast Update : Tue Jun 16 02:02:35 2020
Response via : Initial Calibration

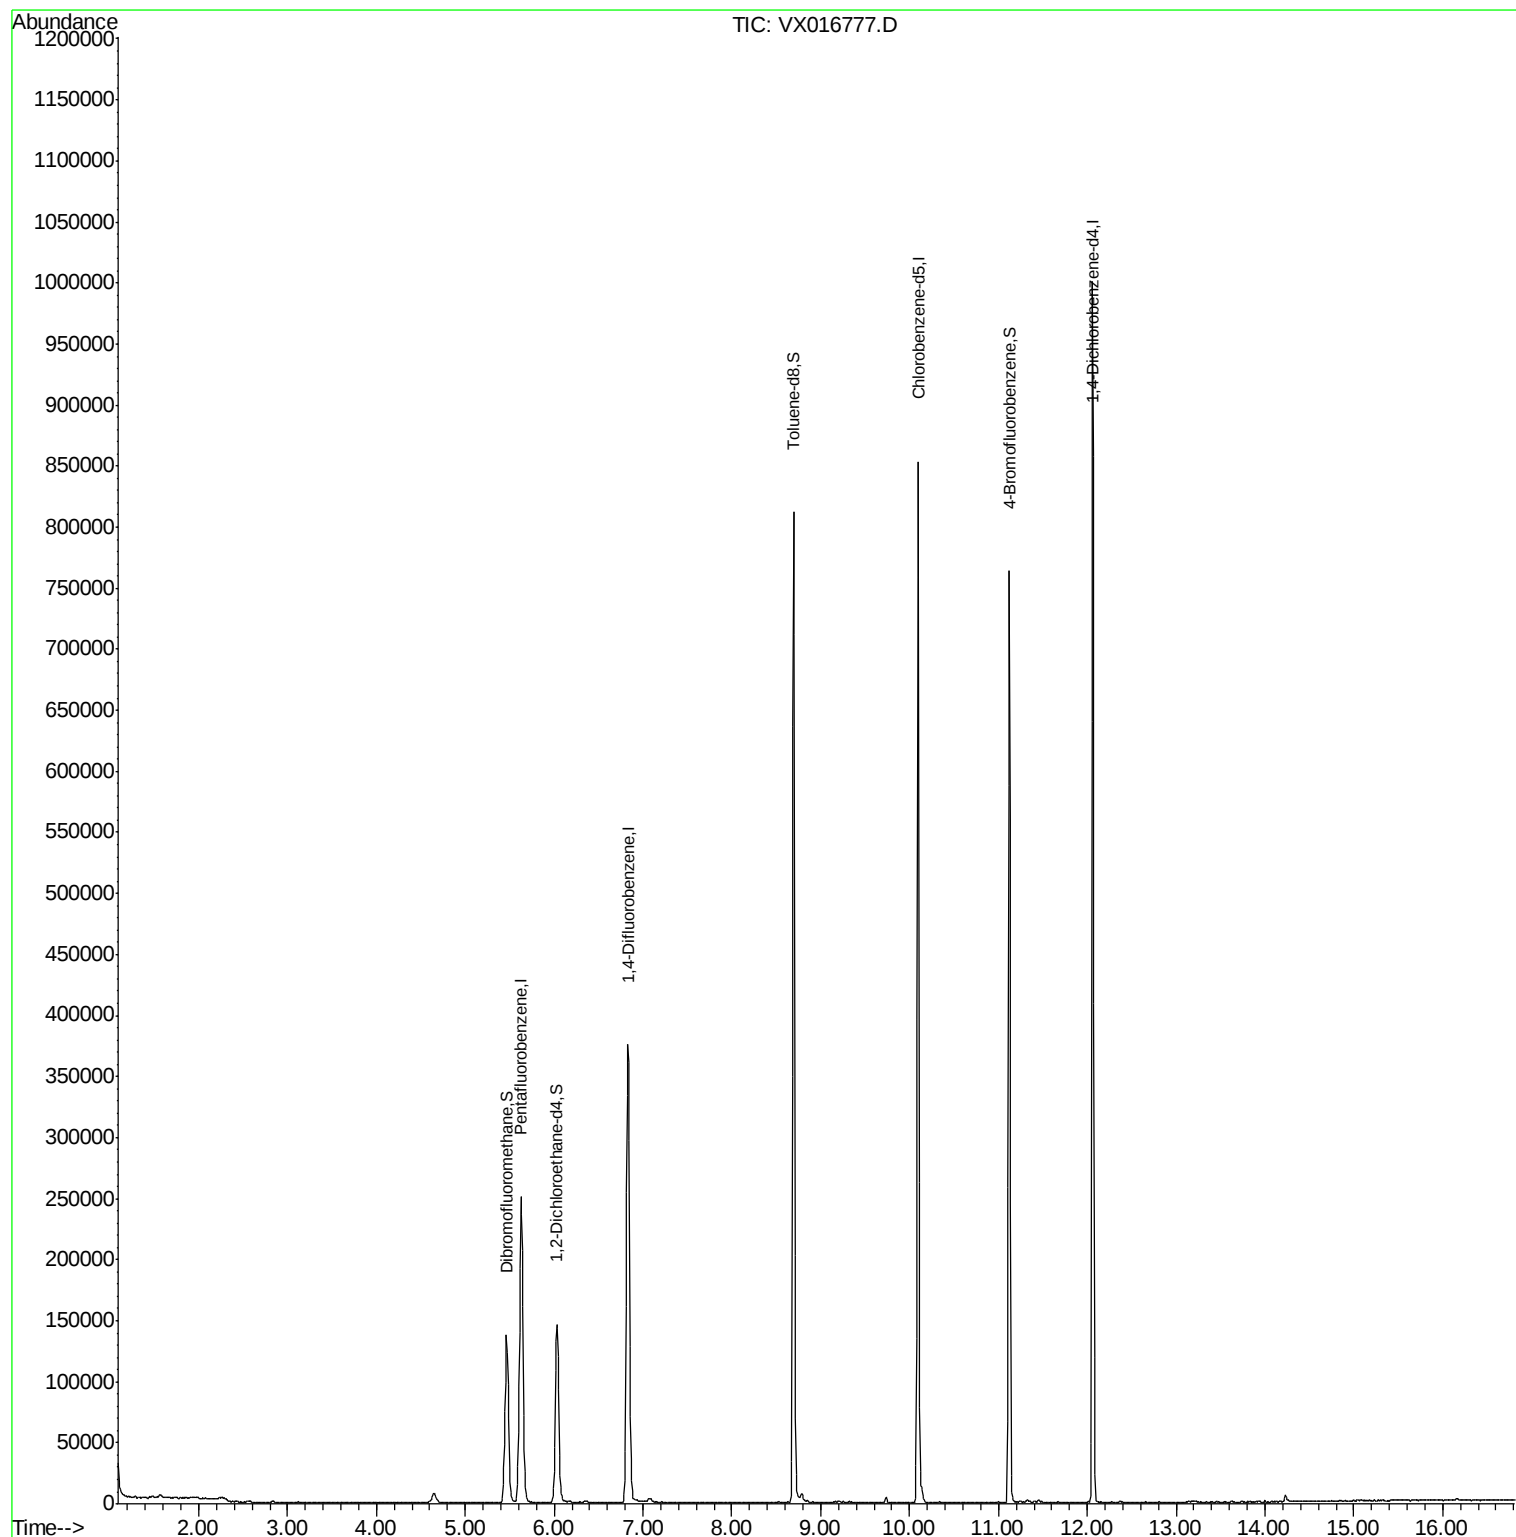

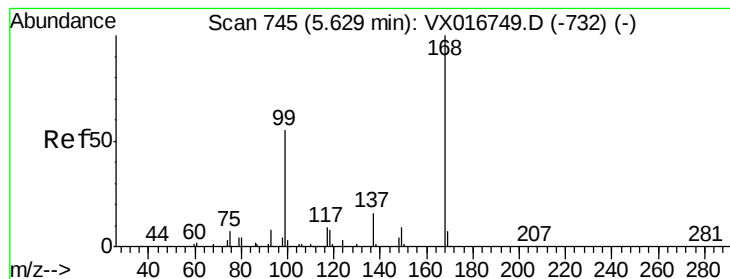

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.00 min

Lab File: VX016777.D

Acq: 16 Jun 2020 14:21

Instrument :

MSVOA_X

ClientSampleId :


Z1-TB6-200610

Tot Ion:168 Resp: 247031

Ion Ratio Lower Upper




168 100

99 55.4 43.8 65.6

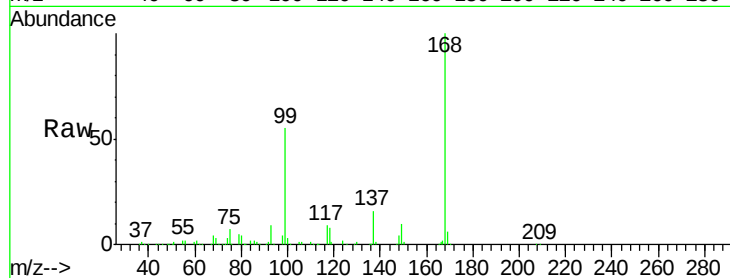

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

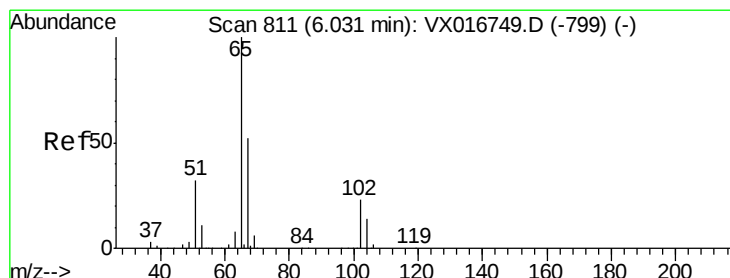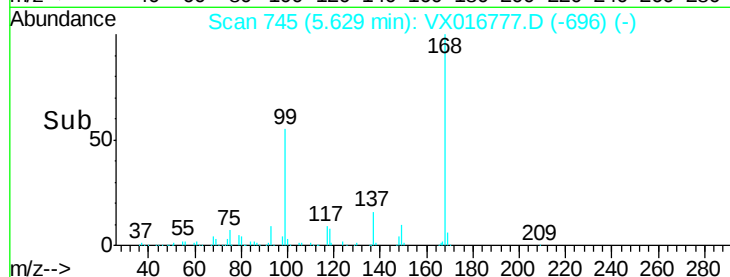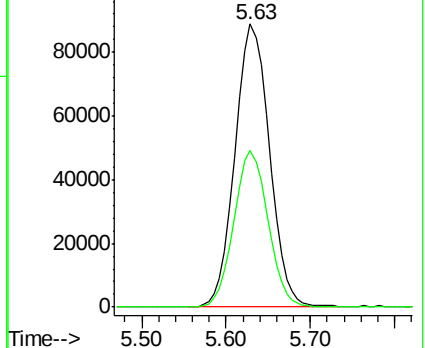

#33

1,2-Dichloroethane-d4

Concen: 51.809 ug/l

RT: 6.03 min Scan# 811

Delta R.T. 0.00 min

Lab File: VX016777.D


Acq: 16 Jun 2020 14:21

Tgt Ion: 65 Resp: 143958

Ion Ratio Lower Upper



65 100


67 51.8 0.0 103.0

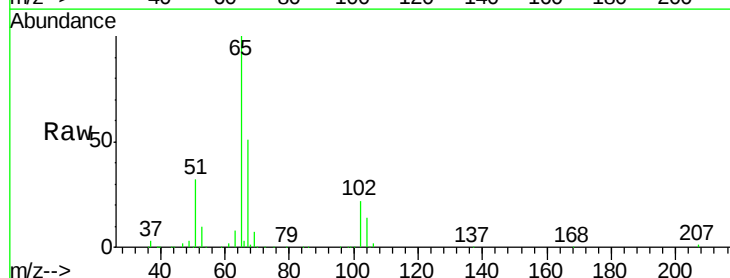

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

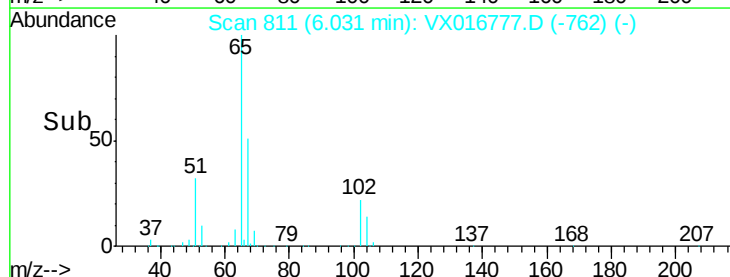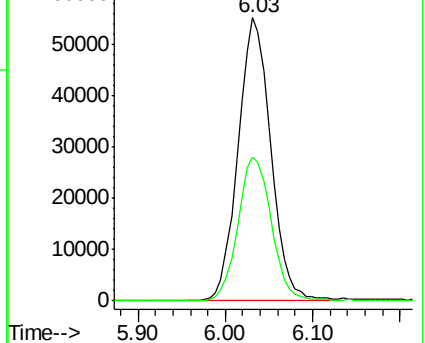

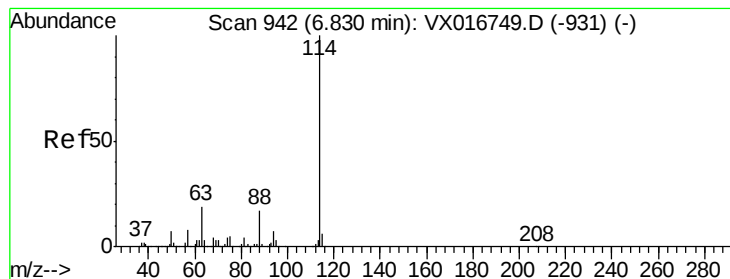

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX016777.D

Acq: 16 Jun 2020 14:21

Instrument :

MSVOA_X

ClientSampleId :

Z1-TB6-200610


Tot Ion:114 Resp: 392267

Ion Ratio Lower Upper

114 100

63 19.1 0.0 38.8




88 16.2 0.0 33.4

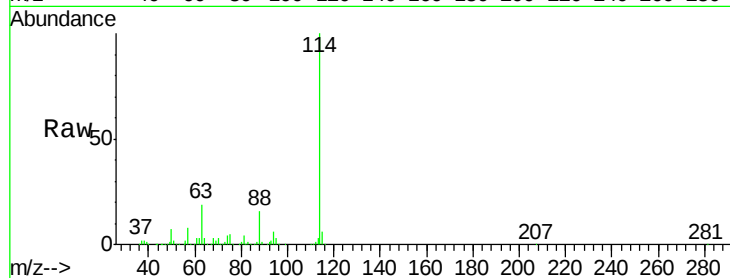

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

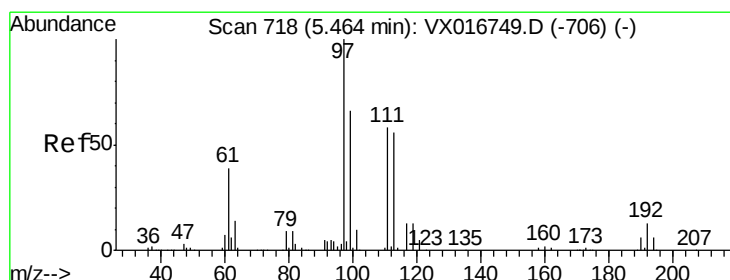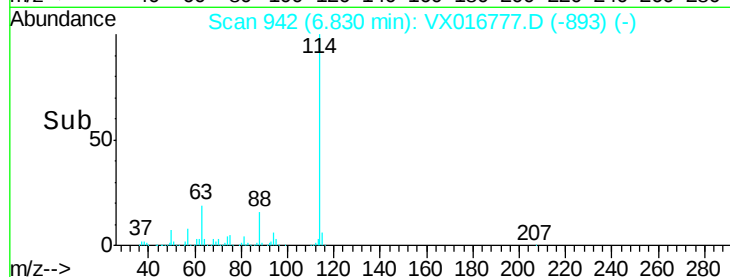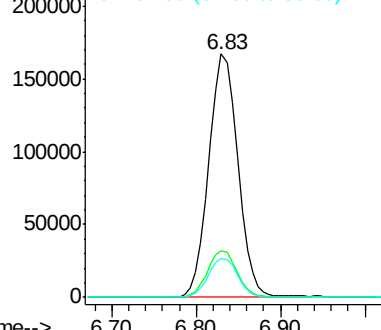

#35

Dibromofluoromethane

Concen: 49.305 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.00 min

Lab File: VX016777.D

Acq: 16 Jun 2020 14:21


Tgt Ion:113 Resp: 119329

Ion Ratio Lower Upper

113 100

111 101.5 81.8 122.6



192 23.0 18.2 27.4

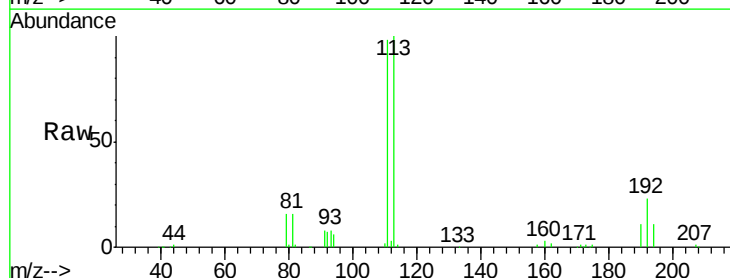


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

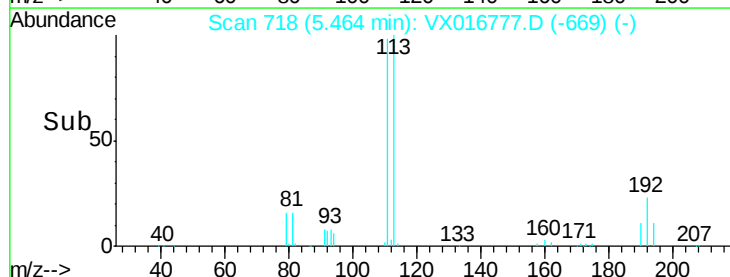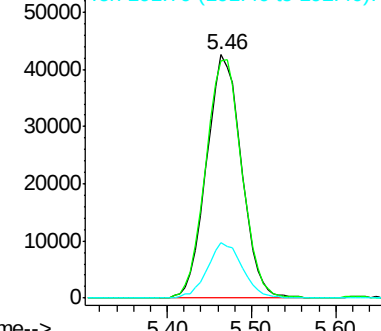

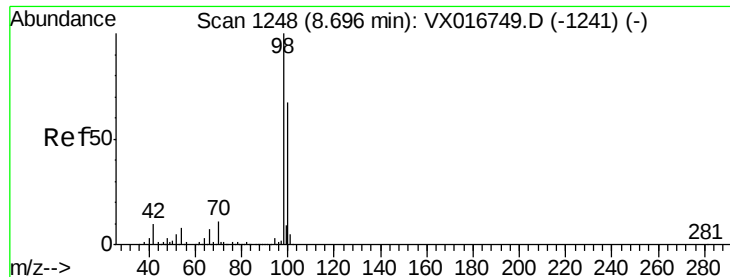

#50

Toluene-d8

Concen: 54.486 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX016777.D

Acq: 16 Jun 2020 14:21

Instrument :

MSVOA_X

ClientSampleId :





Z1-TB6-200610

Tot Ion: 98 Resp: 486237

Ion Ratio Lower Upper

98 100

100 66.3 53.9 80.9

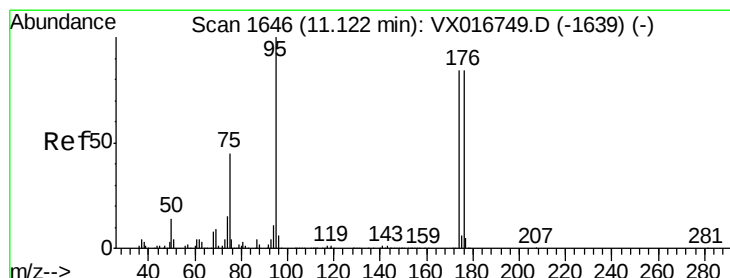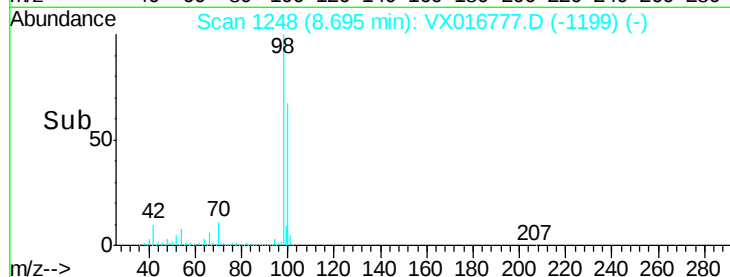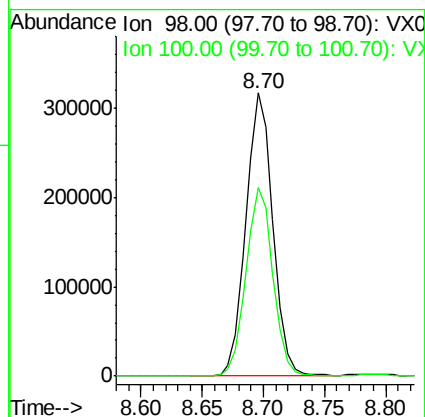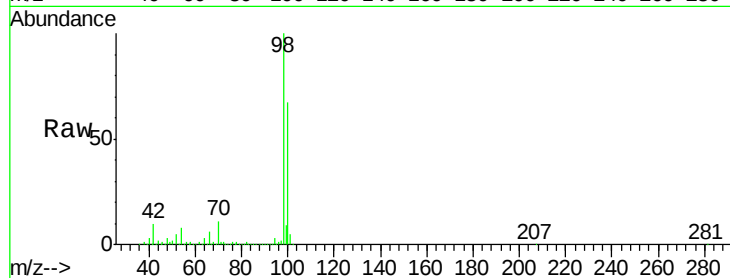

#62

4-Bromofluorobenzene

Concen: 58.263 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX016777.D

Acq: 16 Jun 2020 14:21




Tgt Ion: 95 Resp: 198876


Ion Ratio Lower Upper

95 100

174 86.4 0.0 171.0

176 84.6 0.0 166.2


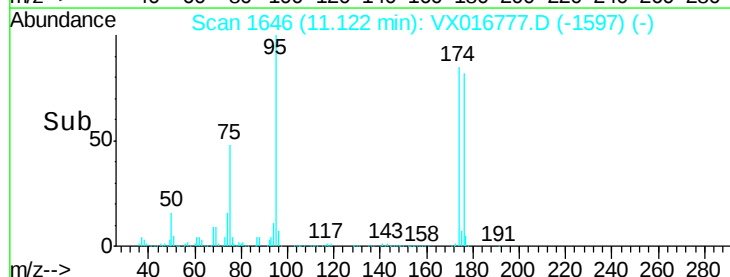
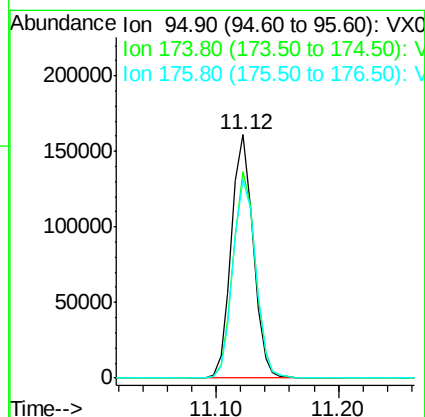
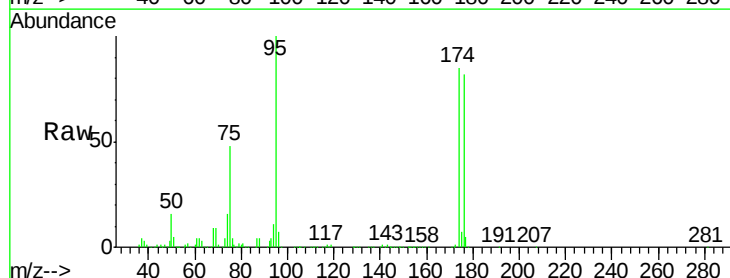


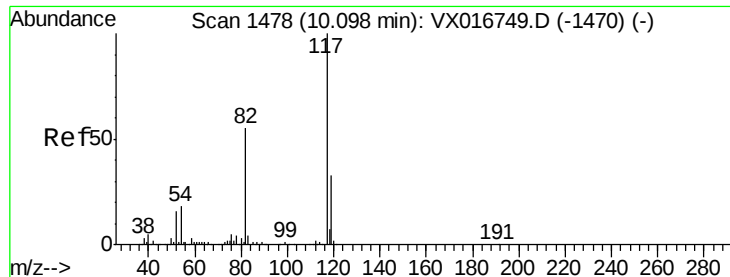

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX016777.D
Acq: 16 Jun 2020 14:21

Instrument :
MSVOA_X
ClientSampleId :
Z1-TB6-200610

Tot Ion:117 Resp: 405085
Ion Ratio Lower Upper
117 100
82 53.9 43.8 65.6
119 32.0 26.2 39.4

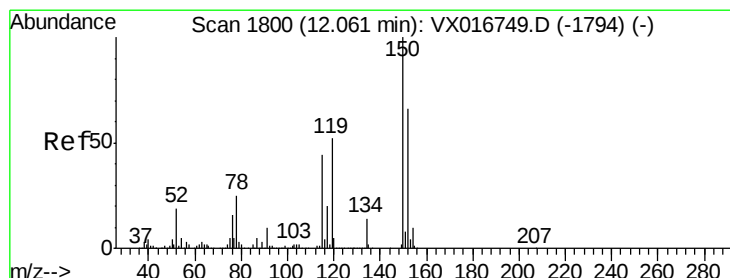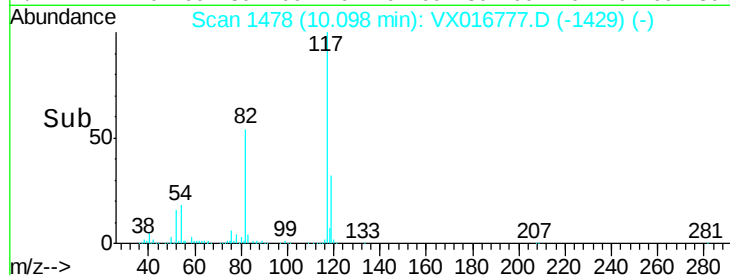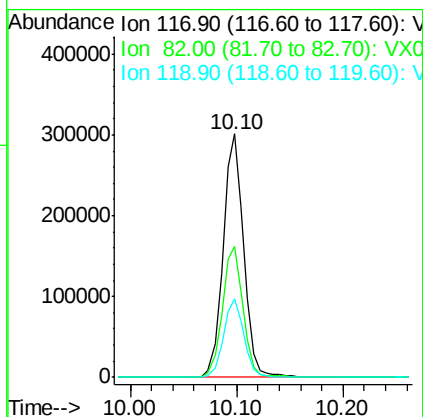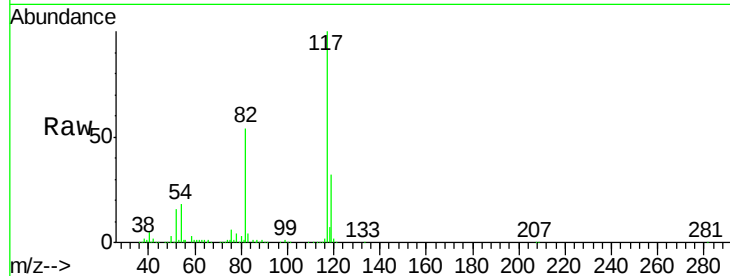

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. -0.00 min
Lab File: VX016777.D
Acq: 16 Jun 2020 14:21

Tgt Ion:152 Resp: 211739
Ion Ratio Lower Upper
152 100
115 57.7 40.3 120.8
150 156.0 0.0 337.4

