


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX061719\
 Data File : VX010314.D
 Acq On : 17 Jun 2019 09:21
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060719W.M
 Title : SW846 8260
 Last Update : Sat Jun 08 02:12:13 2019

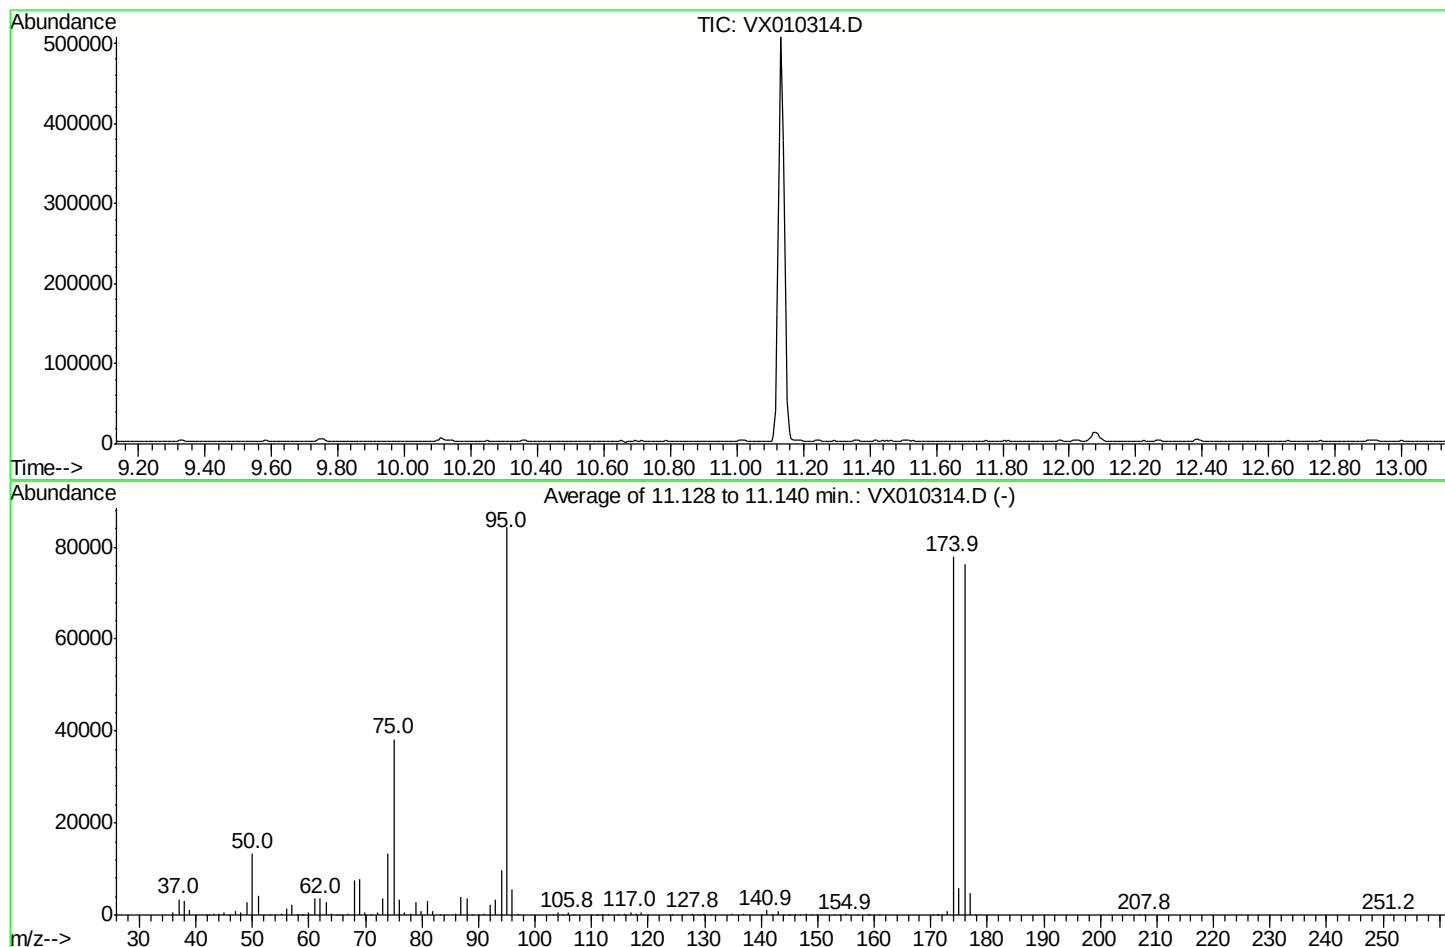

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	13327	PASS
75	95	30	60	45.4	38264	PASS
95	95	100	100	100.0	84288	PASS
96	95	5	9	6.5	5504	PASS
173	174	0.00	2	1.1	889	PASS
174	95	50	100	92.4	77840	PASS
175	174	5	9	7.6	5932	PASS
176	174	95	101	98.0	76314	PASS
177	176	5	9	6.3	4820	PASS