

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX061720\
 Data File : VX016824.D
 Acq On : 17 Jun 2020 18:06
 Operator : JC/SP
 Sample : L3032-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Z1-TB11-200615

Quant Time: Jun 18 01:38:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061520W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 16 02:02:35 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	255052	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	460120	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	410588	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	236967	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.03	65	165672	57.74	ug/l	0.00
Spiked Amount	50.000		Recovery	=	115.48%	
35) Dibromofluoromethane	5.47	113	121589	42.83	ug/l	0.00
Spiked Amount	50.000		Recovery	=	85.66%	
50) Toluene-d8	8.70	98	489158	46.73	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.46%	
62) 4-Bromofluorobenzene	11.12	95	225743	56.38	ug/l	0.00
Spiked Amount	50.000		Recovery	=	112.76%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX061720\
Data File : VX016824.D
Acq On : 17 Jun 2020 18:06
Operator : JC/SP
Sample : L3032-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Z1-TB11-200615

Quant Time: Jun 18 01:38:00 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061520W.M
Quant Title : SW846 8260
QLast Update : Tue Jun 16 02:02:35 2020
Response via : Initial Calibration

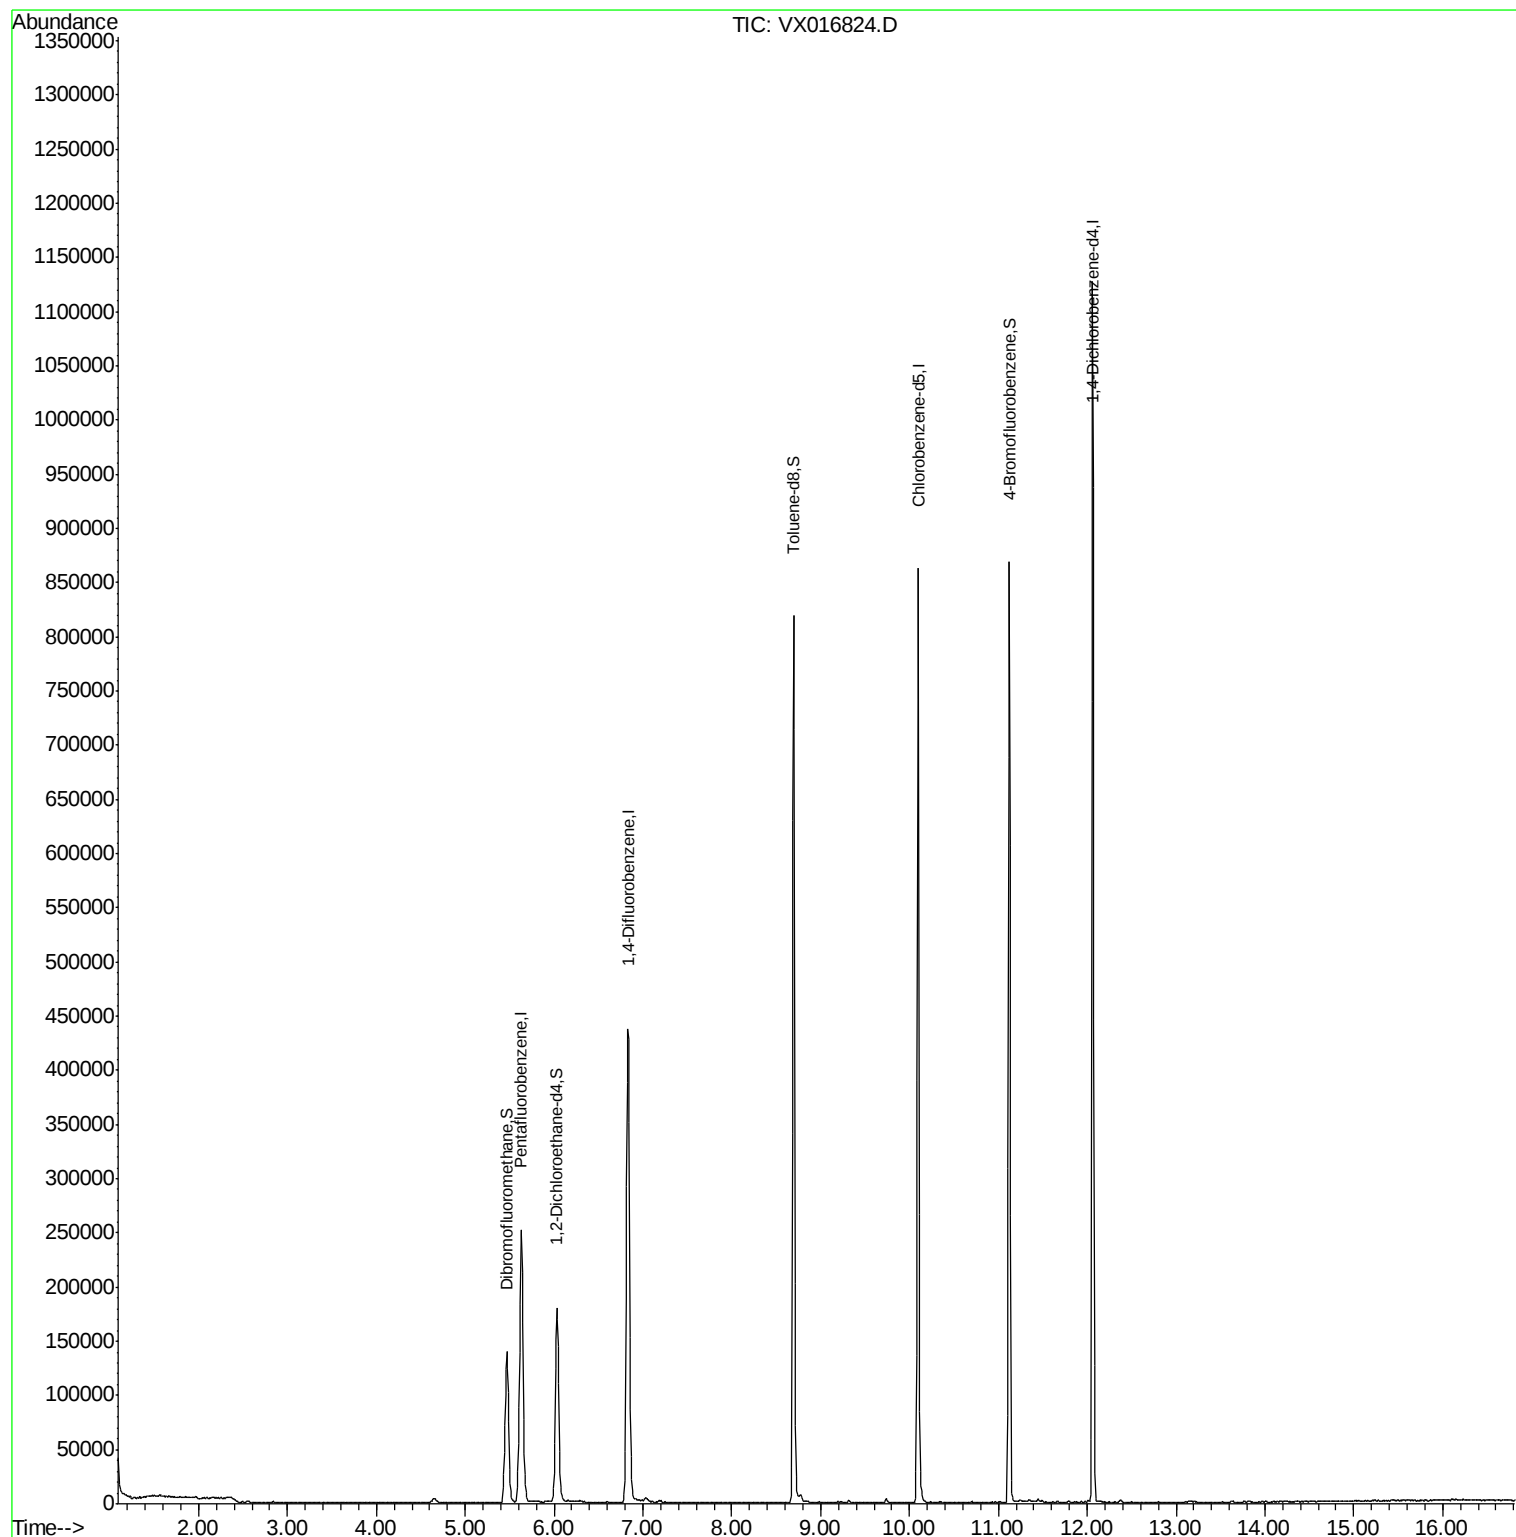

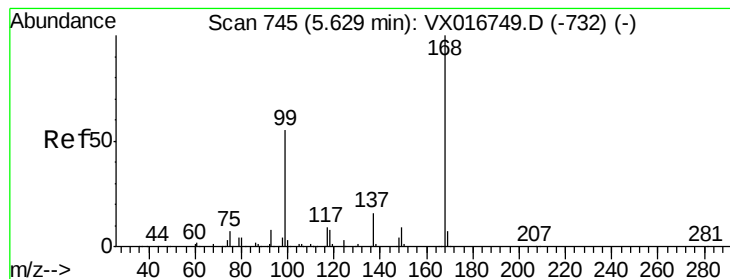

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. 0.00 min

Lab File: VX016824.D

Acq: 17 Jun 2020 18:06

Instrument :

MSVOA_X

ClientSampleId :


Z1-TB11-200615

Tot Ion:168 Resp: 255052

Ion Ratio Lower Upper




168 100

99 55.1 43.8 65.6

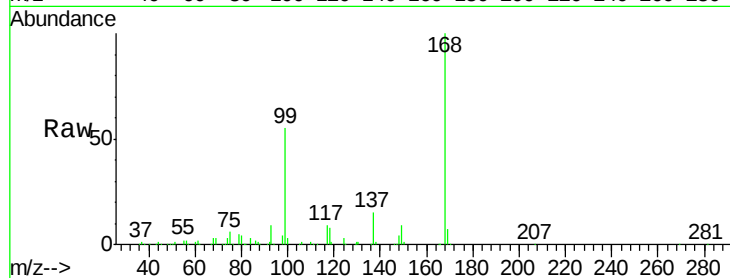

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

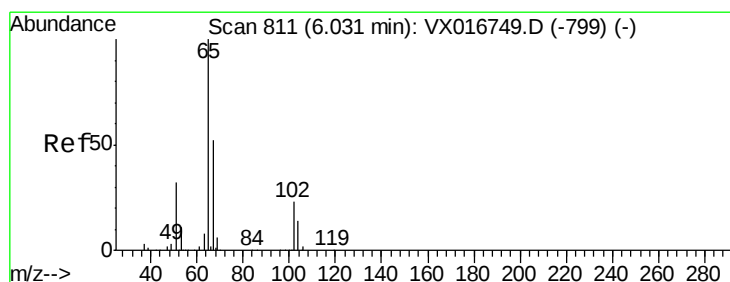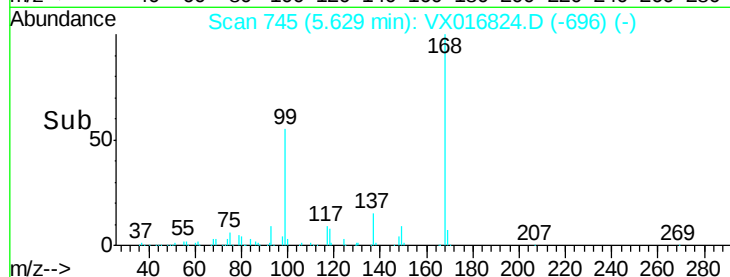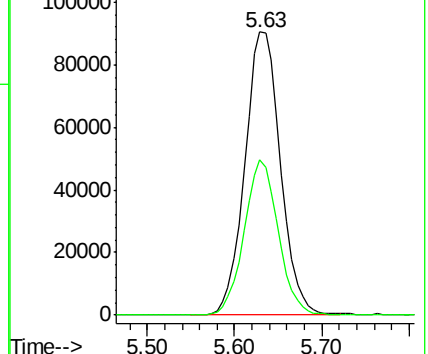

#33

1,2-Dichloroethane-d4

Concen: 57.743 ug/l

RT: 6.03 min Scan# 811

Delta R.T. 0.00 min

Lab File: VX016824.D


Acq: 17 Jun 2020 18:06

Tgt Ion: 65 Resp: 165672

Ion Ratio Lower Upper



65 100


67 52.8 0.0 103.0

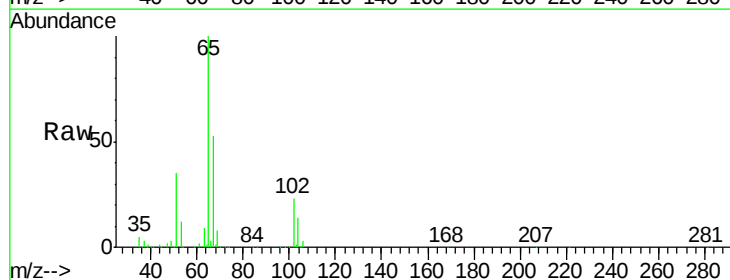

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

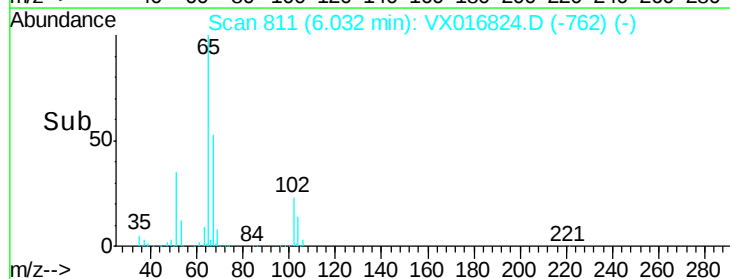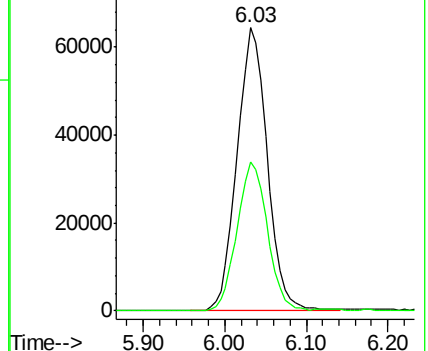

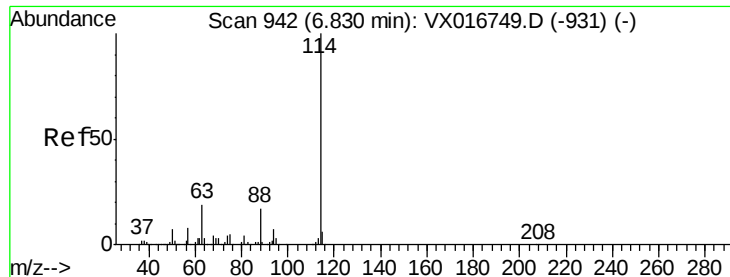

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. 0.00 min

Lab File: VX016824.D

Acq: 17 Jun 2020 18:06

Instrument :

MSVOA_X

ClientSampleId :

Z1-TB11-200615


Tot Ion:114 Resp: 460120

Ion Ratio Lower Upper

114 100

63 19.6 0.0 38.8




88 16.3 0.0 33.4

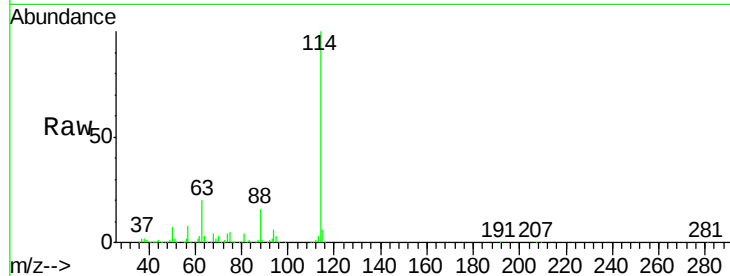

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

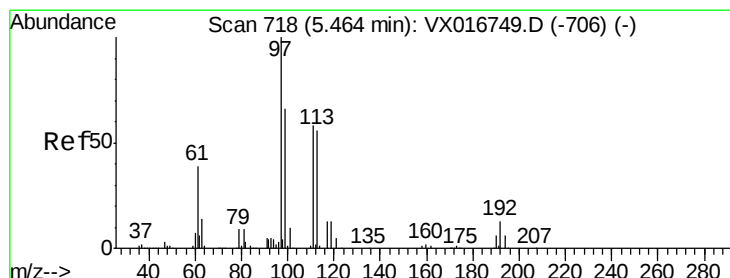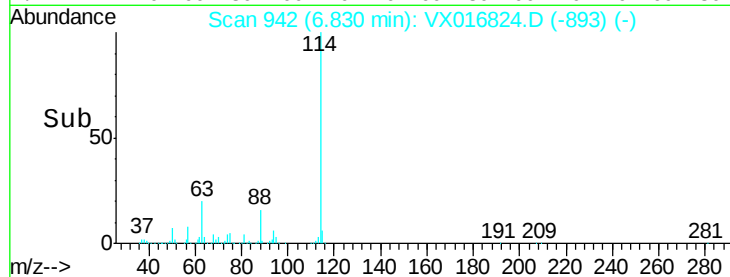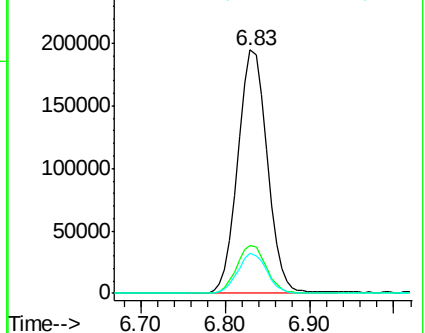

#35

Dibromofluoromethane

Concen: 42.830 ug/l

RT: 5.47 min Scan# 719

Delta R.T. 0.01 min

Lab File: VX016824.D

Acq: 17 Jun 2020 18:06


Tgt Ion:113 Resp: 121589

Ion Ratio Lower Upper

113 100

111 101.5 81.8 122.6



192 23.0 18.2 27.4

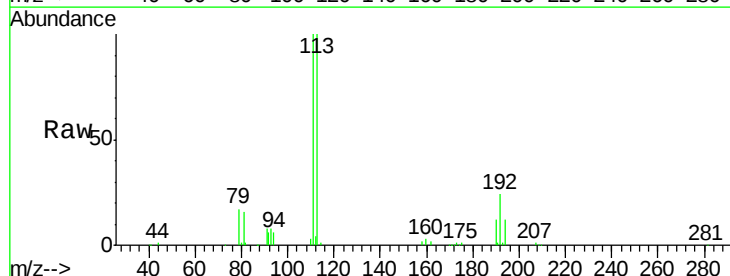


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



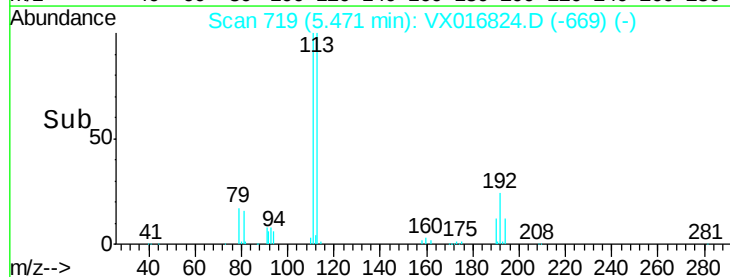
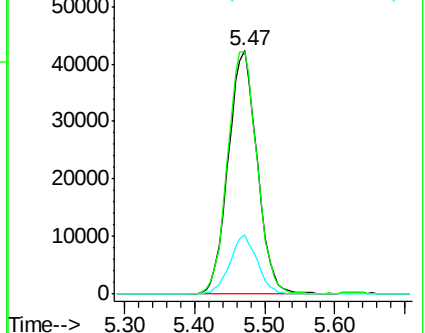


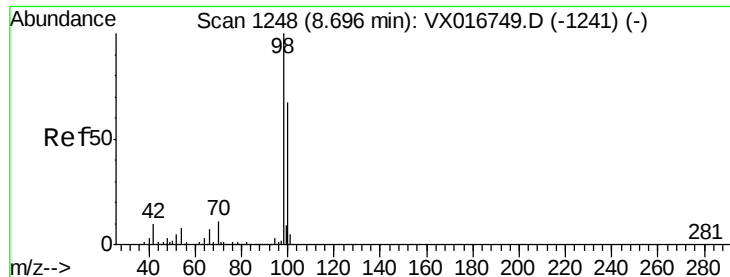

#50
Toluene-d8
Concen: 46.730 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. 0.00 min
Lab File: VX016824.D
Acq: 17 Jun 2020 18:06




Instrument :
MSVOA_X
ClientSampleId :
Z1-TB11-200615


Tot Ion: 98 Resp: 489158
Ion Ratio Lower Upper
98 100
100 66.2 53.9 80.9

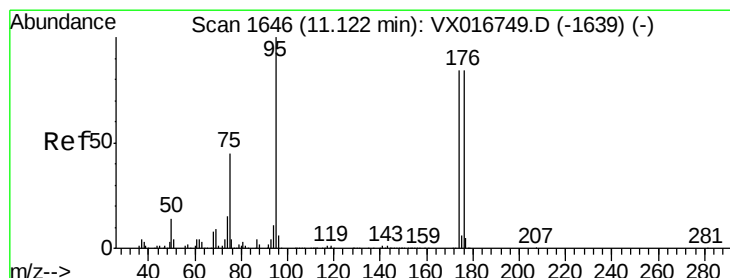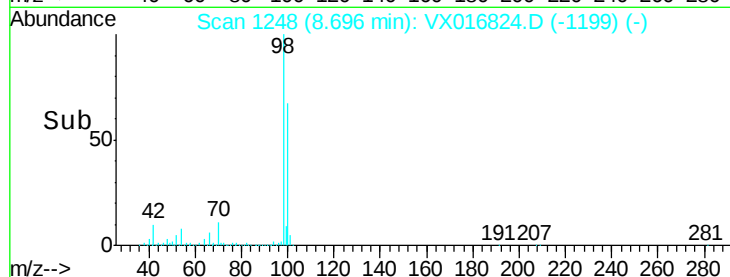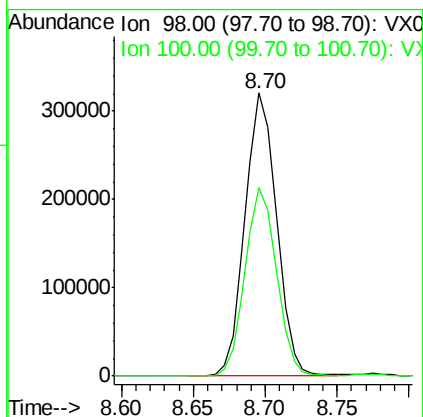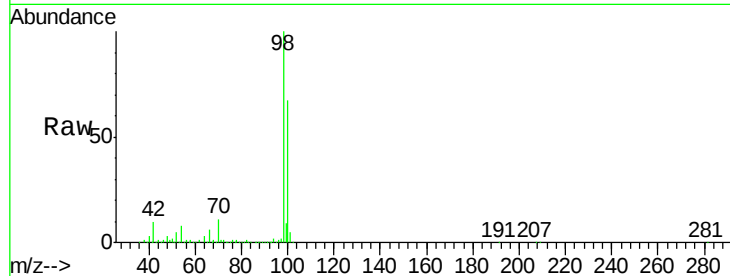

#62
4-Bromofluorobenzene
Concen: 56.381 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. 0.00 min
Lab File: VX016824.D
Acq: 17 Jun 2020 18:06

Tgt Ion: 95 Resp: 225743
Ion Ratio Lower Upper
95 100
174 85.5 0.0 171.0
176 83.4 0.0 166.2


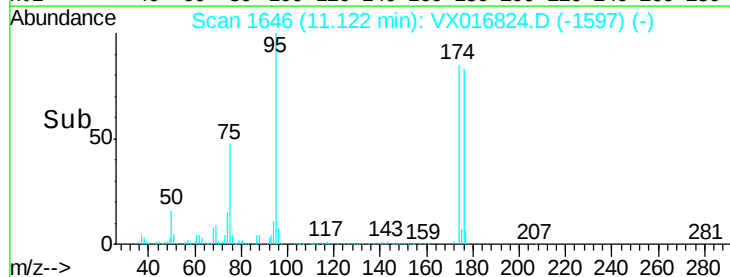
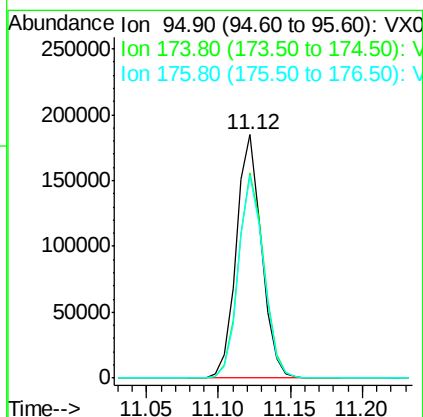
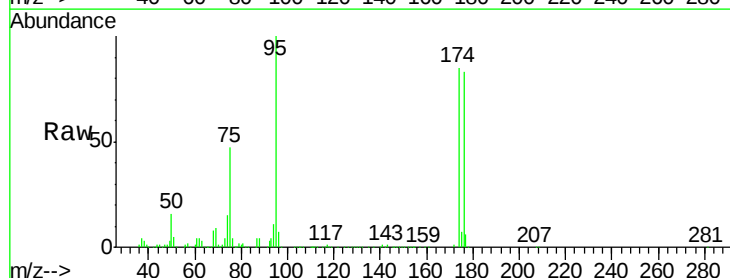


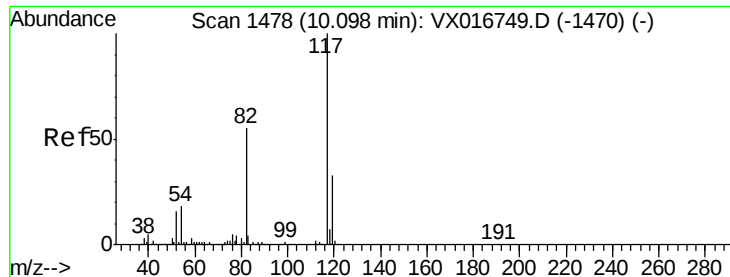

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. 0.00 min
Lab File: VX016824.D
Acq: 17 Jun 2020 18:06

Instrument :
MSVOA_X
ClientSampleId :
Z1-TB11-200615

Tot Ion:117 Resp: 410588
Ion Ratio Lower Upper
117 100
82 53.2 43.8 65.6
119 32.8 26.2 39.4

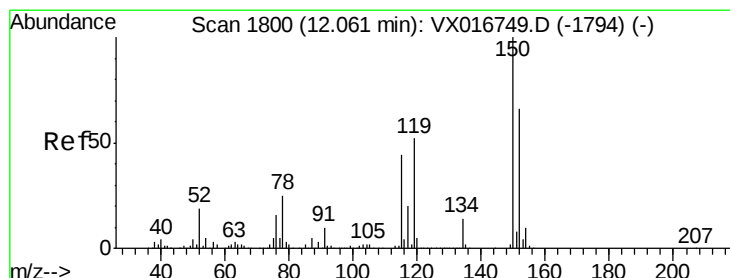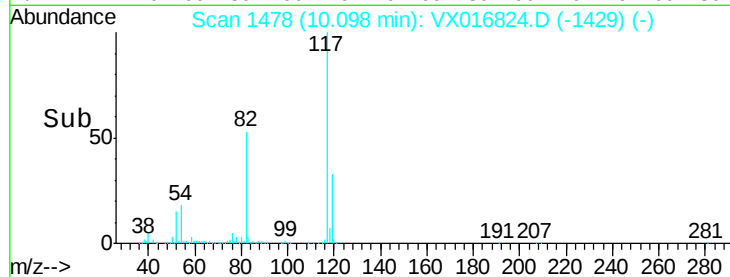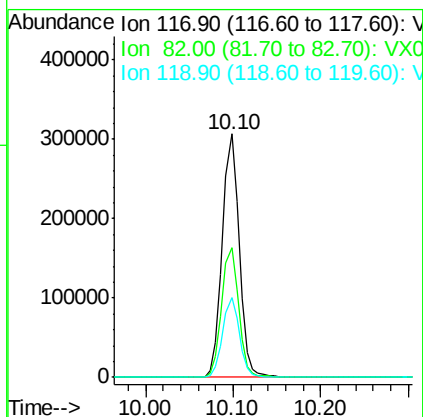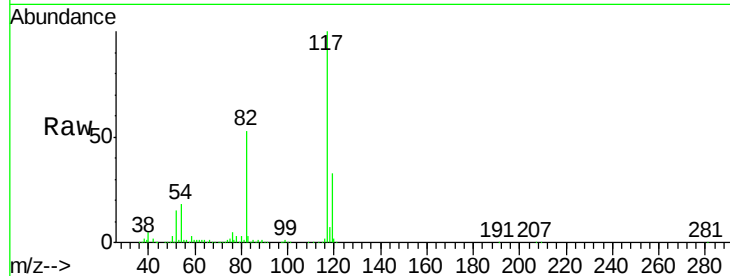

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. 0.00 min
Lab File: VX016824.D
Acq: 17 Jun 2020 18:06

Tgt Ion:152 Resp: 236967
Ion Ratio Lower Upper
152 100
115 58.3 40.3 120.8
150 154.1 0.0 337.4

