

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061721\
 Data File : VX022731.D
 Acq On : 17 Jun 2021 11:32
 Operator : JC/MD
 Sample : M2750-08DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE120D1-20210615DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M

Title : SW846 8260

Signal : TIC: VX022731.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.575	74	80	83	rVB5	3265	7176	1.62%	0.284%
2	2.331	197	204	209	rBV4	3496	6776	1.53%	0.268%
3	5.397	695	707	722	rBV	44351	123346	27.88%	4.880%
4	5.562	722	734	746	rBV2	70633	201092	45.45%	7.955%
5	5.964	790	800	814	rVB2	56399	148358	33.53%	5.869%
6	6.769	923	932	945	rBV	126034	294615	66.59%	11.655%
7	7.129	983	991	1004	rBV	207296	442435	100.00%	17.503%
8	8.653	1235	1241	1249	rBV	269083	412413	93.21%	16.315%
9	10.055	1466	1471	1479	rBV	259754	352058	79.57%	13.927%
10	11.085	1634	1640	1648	rVB	190287	244109	55.17%	9.657%
11	12.024	1789	1794	1801	rVB	243650	295440	66.78%	11.688%




Sum of corrected areas: 2527818

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061721\
Data File : VX022731.D
Acq On : 17 Jun 2021 11:32
Operator : JC/MD
Sample : M2750-08DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D1-20210615DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

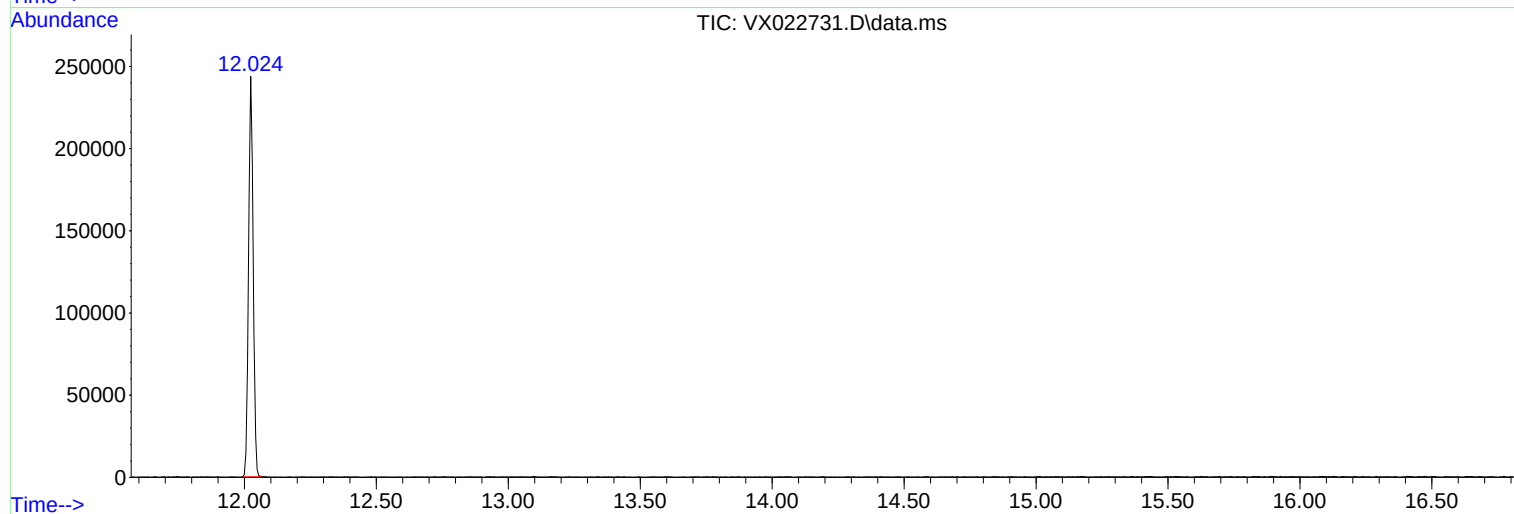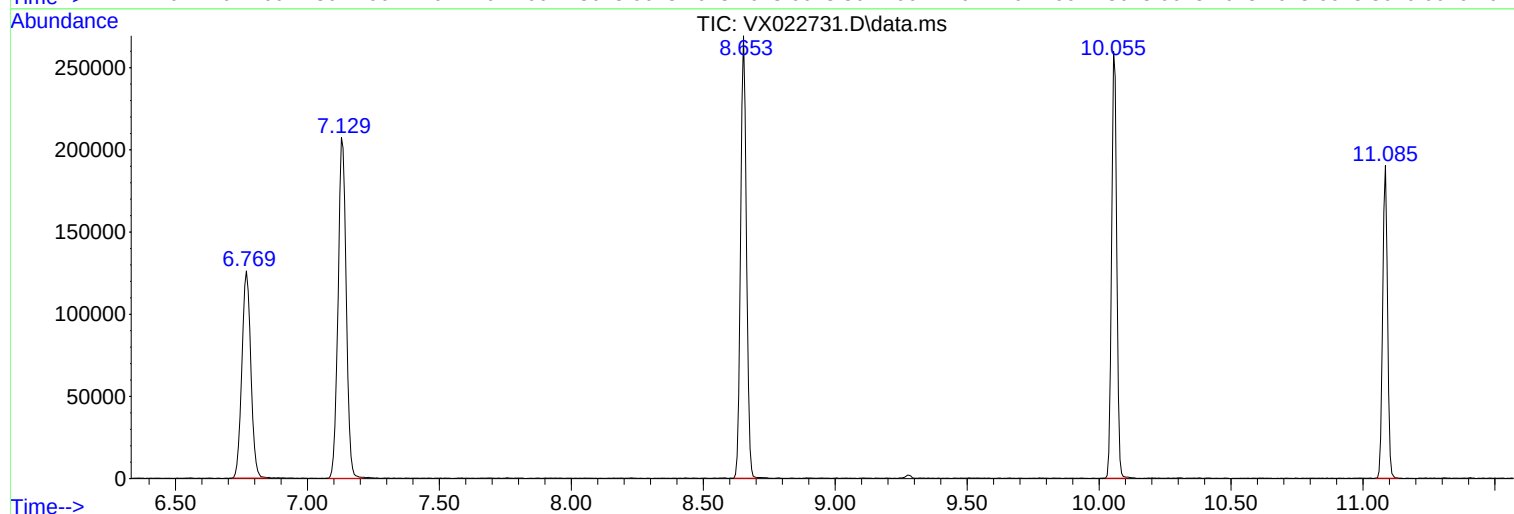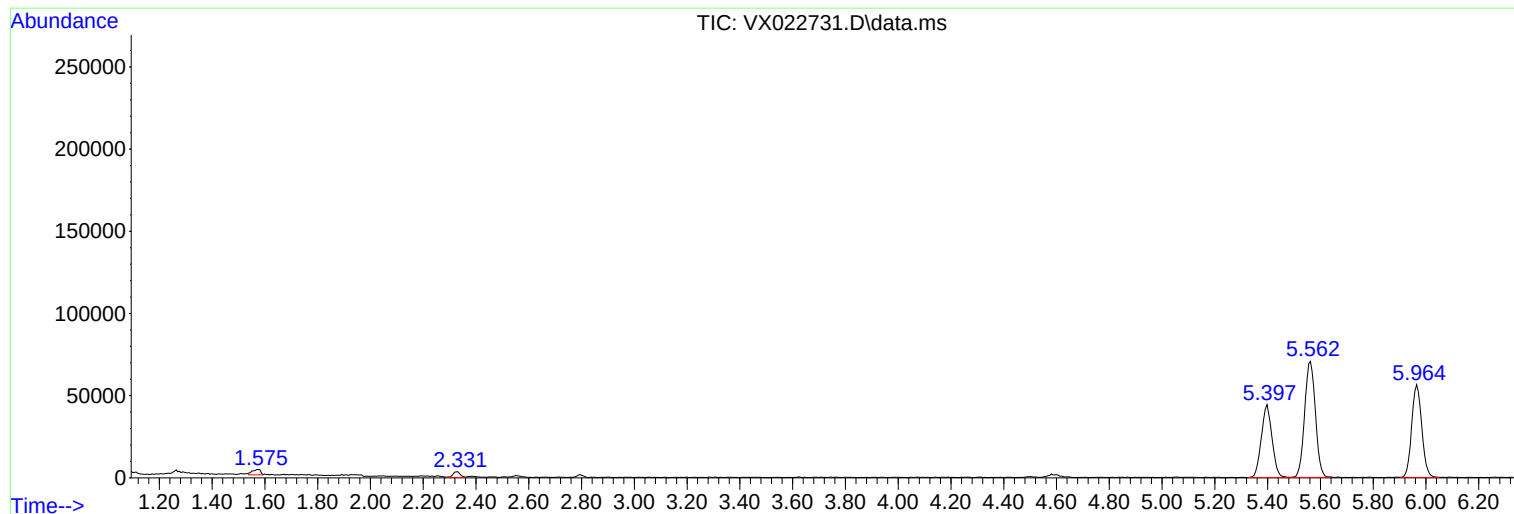

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061721\
Data File : VX022731.D
Acq On : 17 Jun 2021 11:32
Operator : JC/MD
Sample : M2750-08DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D1-20210615DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061721\
Data File : VX022731.D
Acq On : 17 Jun 2021 11:32
Operator : JC/MD
Sample : M2750-08DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D1-20210615DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------