

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061721\
 Data File : VX022735.D
 Acq On : 17 Jun 2021 13:06
 Operator : JC/MD
 Sample : M2750-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE123D1-20210616

Integration Parameters: RTEINT.P

Integrator: RTE

Smoother: ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M

Title : SW846 8260

Signal : TIC: VX022735.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.569	71	79	85	rVB3	2868	5087	1.30%	0.255%
2	2.550	235	240	247	rVB	3461	6699	1.71%	0.336%
3	5.397	694	707	720	rBV	41829	117991	30.08%	5.924%
4	5.562	723	734	750	rVV2	70349	191810	48.90%	9.629%
5	5.964	790	800	812	rBV	53254	138976	35.43%	6.977%
6	6.769	923	932	943	rBV	119796	278841	71.09%	13.999%
7	7.135	985	992	1002	rVB3	20527	43803	11.17%	2.199%
8	8.653	1234	1241	1252	rBV	253830	392242	100.00%	19.692%
9	10.055	1466	1471	1486	rBV	238593	332394	84.74%	16.687%
10	11.085	1635	1640	1650	rVB	181810	224723	57.29%	11.282%
11	12.024	1789	1794	1802	rVB	213512	259342	66.12%	13.020%




Sum of corrected areas: 1991908

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061721\
Data File : VX022735.D
Acq On : 17 Jun 2021 13:06
Operator : JC/MD
Sample : M2750-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE123D1-20210616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

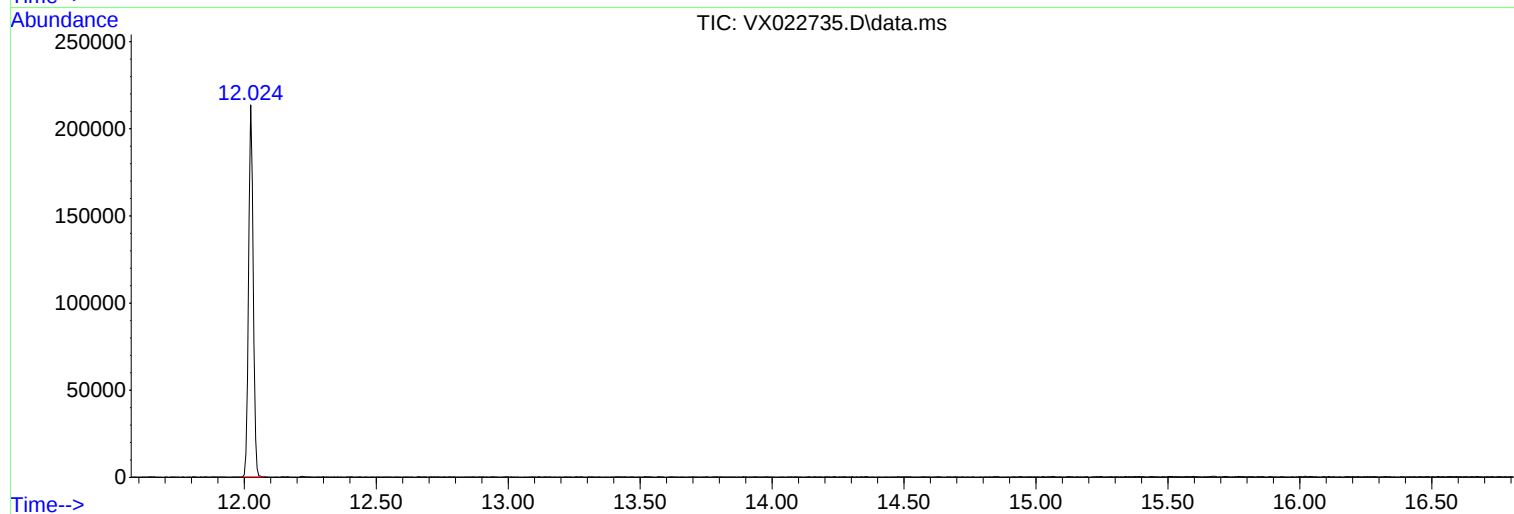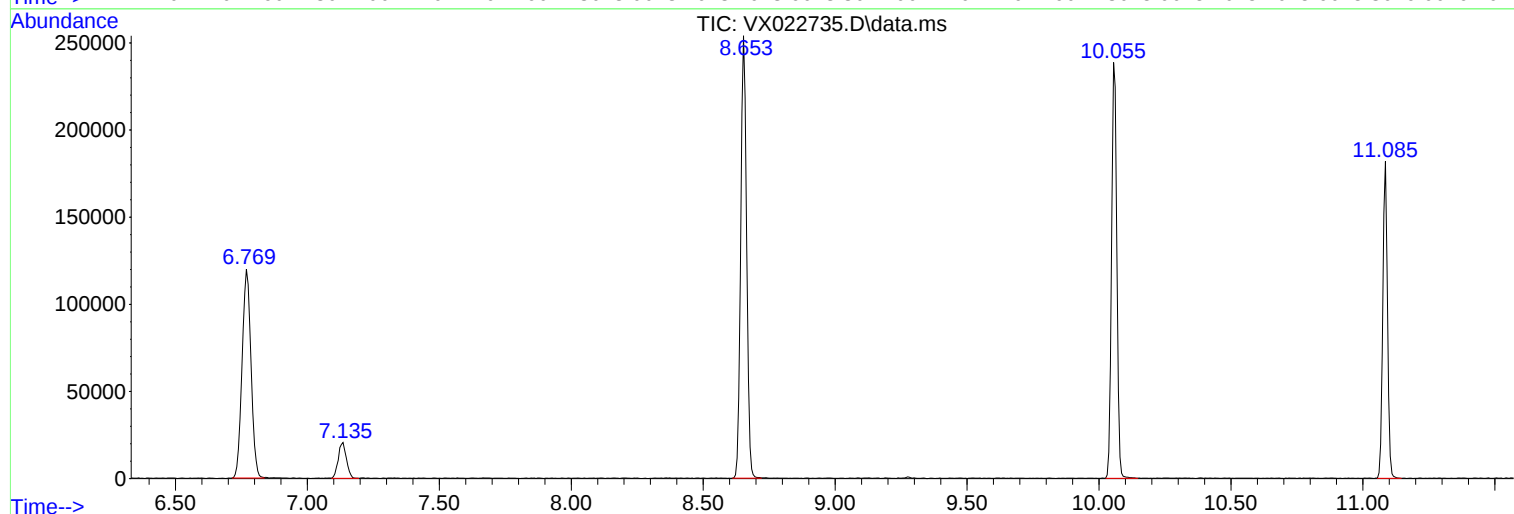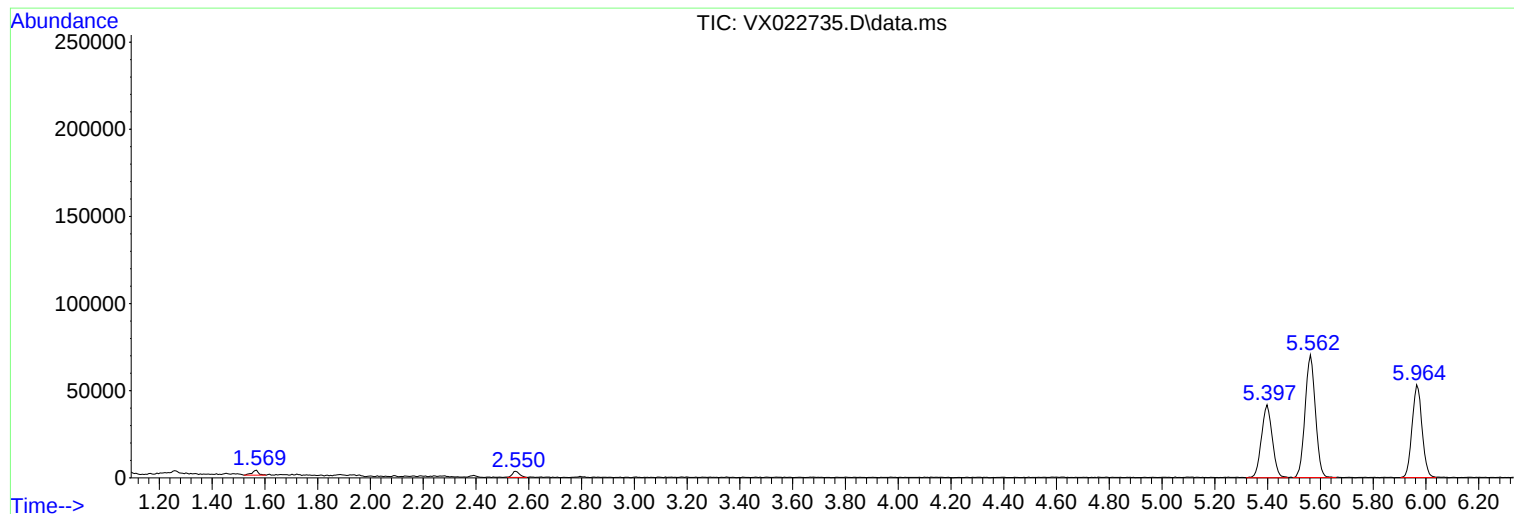

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061721\
Data File : VX022735.D
Acq On : 17 Jun 2021 13:06
Operator : JC/MD
Sample : M2750-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE123D1-20210616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061721\
Data File : VX022735.D
Acq On : 17 Jun 2021 13:06
Operator : JC/MD
Sample : M2750-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE123D1-20210616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
