

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061721\
 Data File : VX022736.D
 Acq On : 17 Jun 2021 13:30
 Operator : JC/MD
 Sample : M2750-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE123D2-20210616

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M

Title : SW846 8260

Signal : TIC: VX022736.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.550	233	240	246	rBV	4625	7096	1.85%	0.367%
2	5.397	696	707	717	rBV	41279	114058	29.67%	5.902%
3	5.562	723	734	747	rVB2	67265	187408	48.75%	9.697%
4	5.964	790	800	811	rBV2	54117	137585	35.79%	7.119%
5	6.769	920	932	943	rBV	120021	279286	72.65%	14.451%
6	7.129	985	991	1000	rBV3	7386	14892	3.87%	0.771%
7	8.653	1234	1241	1249	rBV	253985	384440	100.00%	19.892%
8	9.275	1338	1343	1349	rBV2	10041	14302	3.72%	0.740%
9	10.055	1465	1471	1482	rBV	236452	322676	83.93%	16.696%
10	11.085	1634	1640	1651	rBV	172135	218987	56.96%	11.331%
11	12.024	1789	1794	1801	rBV	211417	251884	65.52%	13.033%




Sum of corrected areas: 1932614

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061721\
Data File : VX022736.D
Acq On : 17 Jun 2021 13:30
Operator : JC/MD
Sample : M2750-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE123D2-20210616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

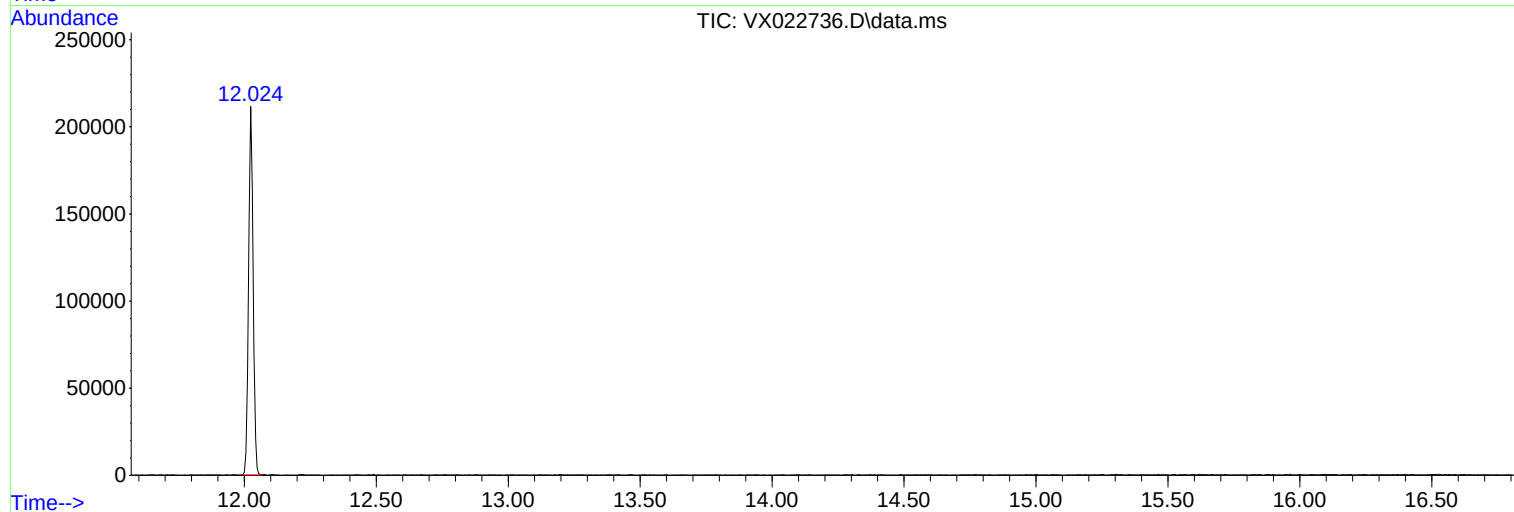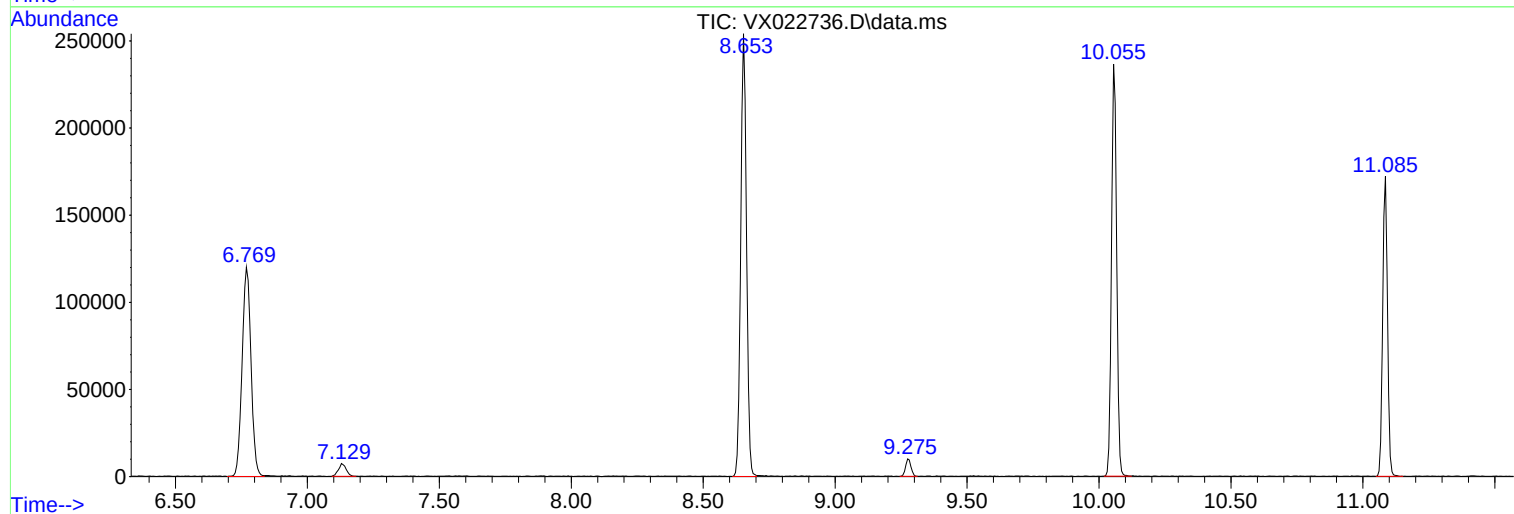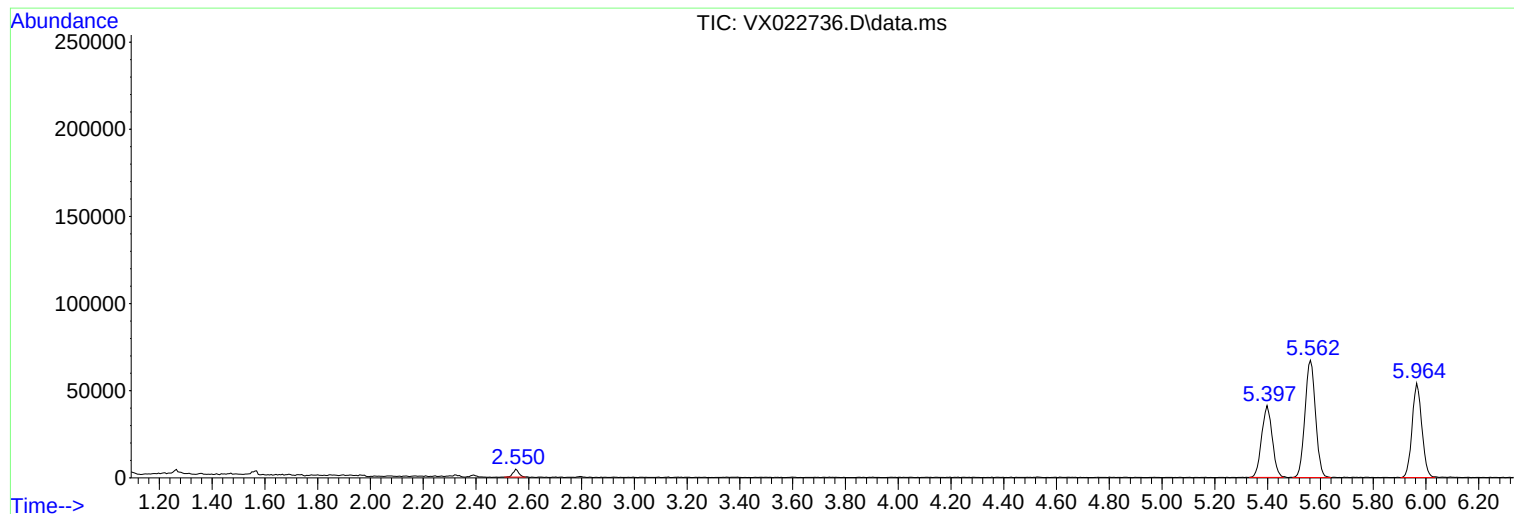

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061721\
Data File : VX022736.D
Acq On : 17 Jun 2021 13:30
Operator : JC/MD
Sample : M2750-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE123D2-20210616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061721\
Data File : VX022736.D
Acq On : 17 Jun 2021 13:30
Operator : JC/MD
Sample : M2750-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE123D2-20210616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
