

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061721\
 Data File : VX022746.D
 Acq On : 17 Jun 2021 17:26
 Operator : JC/MD
 Sample : M2750-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE125D3-20210615

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M

Title : SW846 8260

Signal : TIC: VX022746.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.331	197	204	218	rVB	162292	299190	25.22%	8.838%
2	5.397	692	707	718	rBV2	39274	111845	9.43%	3.304%
3	5.562	722	734	746	rBV	64904	181260	15.28%	5.355%
4	5.964	791	800	815	rBV	53319	135212	11.40%	3.994%
5	6.769	922	932	944	rBV	113205	266905	22.50%	7.885%
6	7.135	982	992	1009	rBV	545211	1186246	100.00%	35.043%
7	8.653	1234	1241	1254	rBV	242915	374262	31.55%	11.056%
8	9.275	1338	1343	1350	rVB	34126	50783	4.28%	1.500%
9	10.055	1466	1471	1481	rBV	233154	312935	26.38%	9.245%
10	11.085	1635	1640	1649	rBV	173091	214781	18.11%	6.345%
11	12.024	1789	1794	1802	rVB	209727	251674	21.22%	7.435%




Sum of corrected areas: 3385093

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061721\
Data File : VX022746.D
Acq On : 17 Jun 2021 17:26
Operator : JC/MD
Sample : M2750-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D3-20210615

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

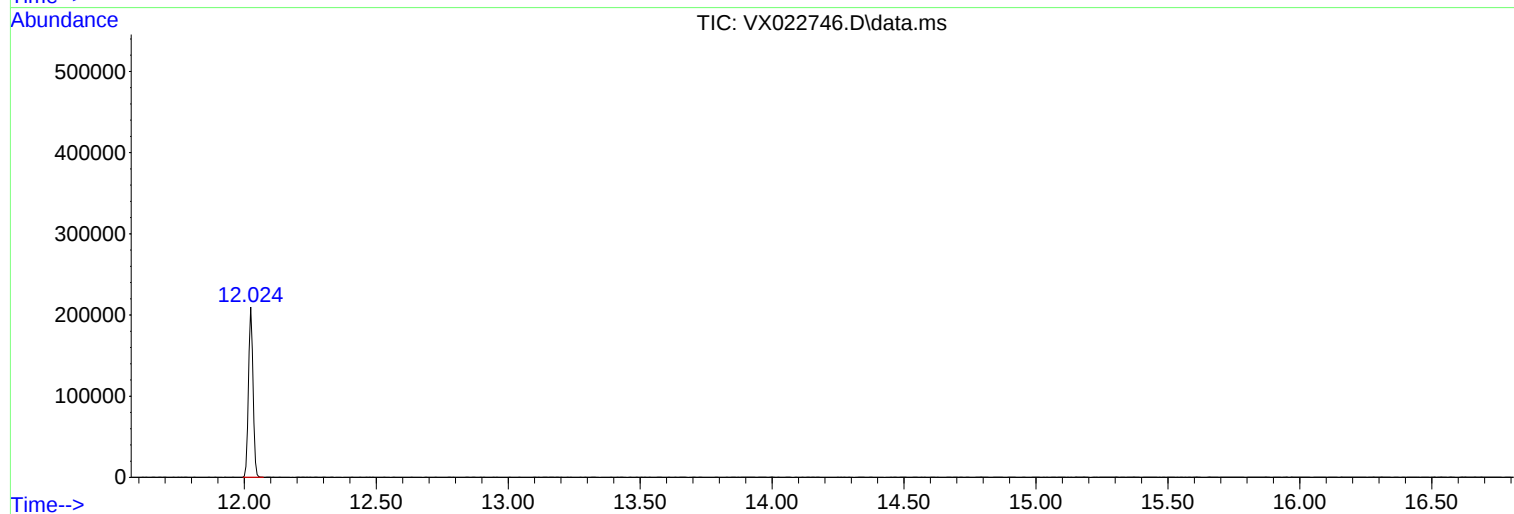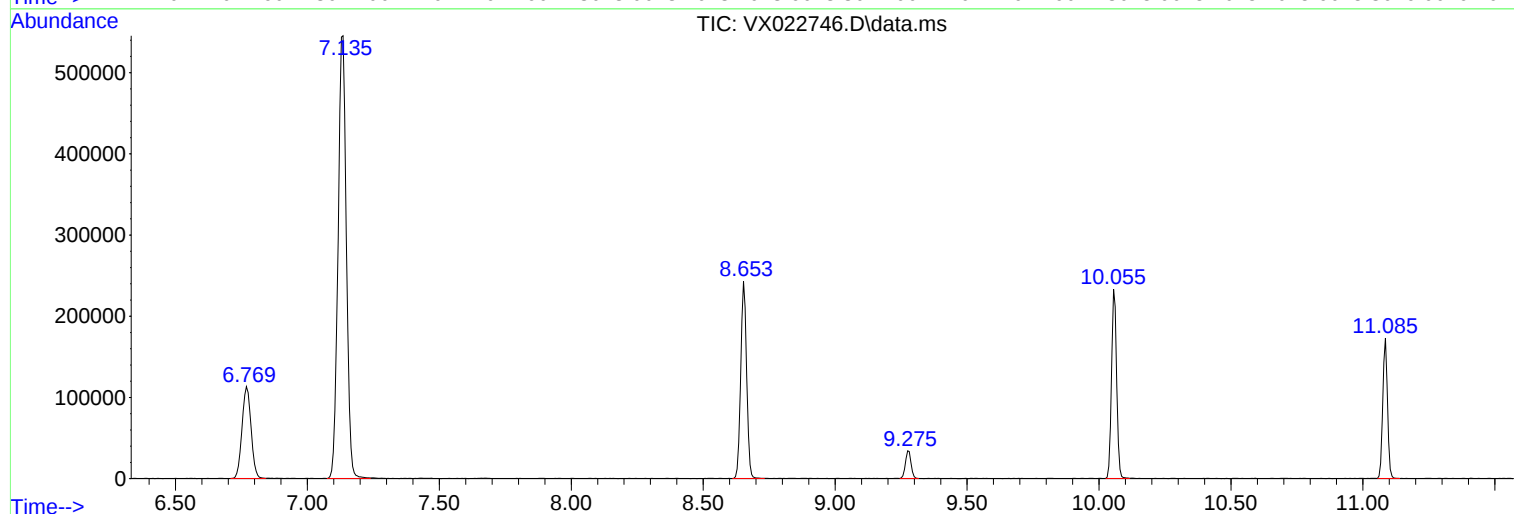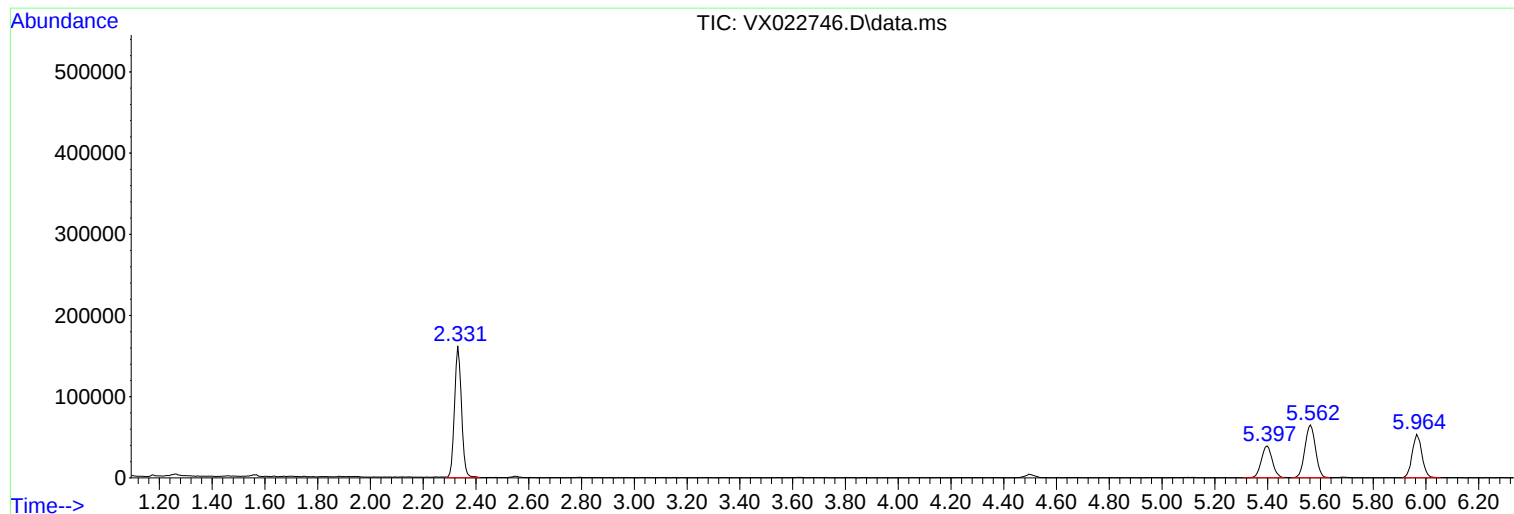

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061721\
Data File : VX022746.D
Acq On : 17 Jun 2021 17:26
Operator : JC/MD
Sample : M2750-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D3-20210615

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061721\
Data File : VX022746.D
Acq On : 17 Jun 2021 17:26
Operator : JC/MD
Sample : M2750-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D3-20210615

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------