

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061724\
 Data File : VX041908.D
 Acq On : 17 Jun 2024 14:41
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Jun 18 02:08:13 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X061424W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Sat Jun 15 04:02:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	4.898	128	29336	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	6.763	114	146035	30.000	ug/l	0.00
57) Chlorobenzene-d5	10.055	117	132491	30.000	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	5.952	65	59689	29.557	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	98.533%
60) 4-Bromofluorobenzene	11.079	95	56022	27.316	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	91.067%
63) Toluene-d8	8.647	98	166631	29.396	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	98.000%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061724\
Data File : VX041908.D
Acq On : 17 Jun 2024 14:41
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Jun 18 02:08:13 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X061424W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Sat Jun 15 04:02:59 2024
Response via : Initial Calibration




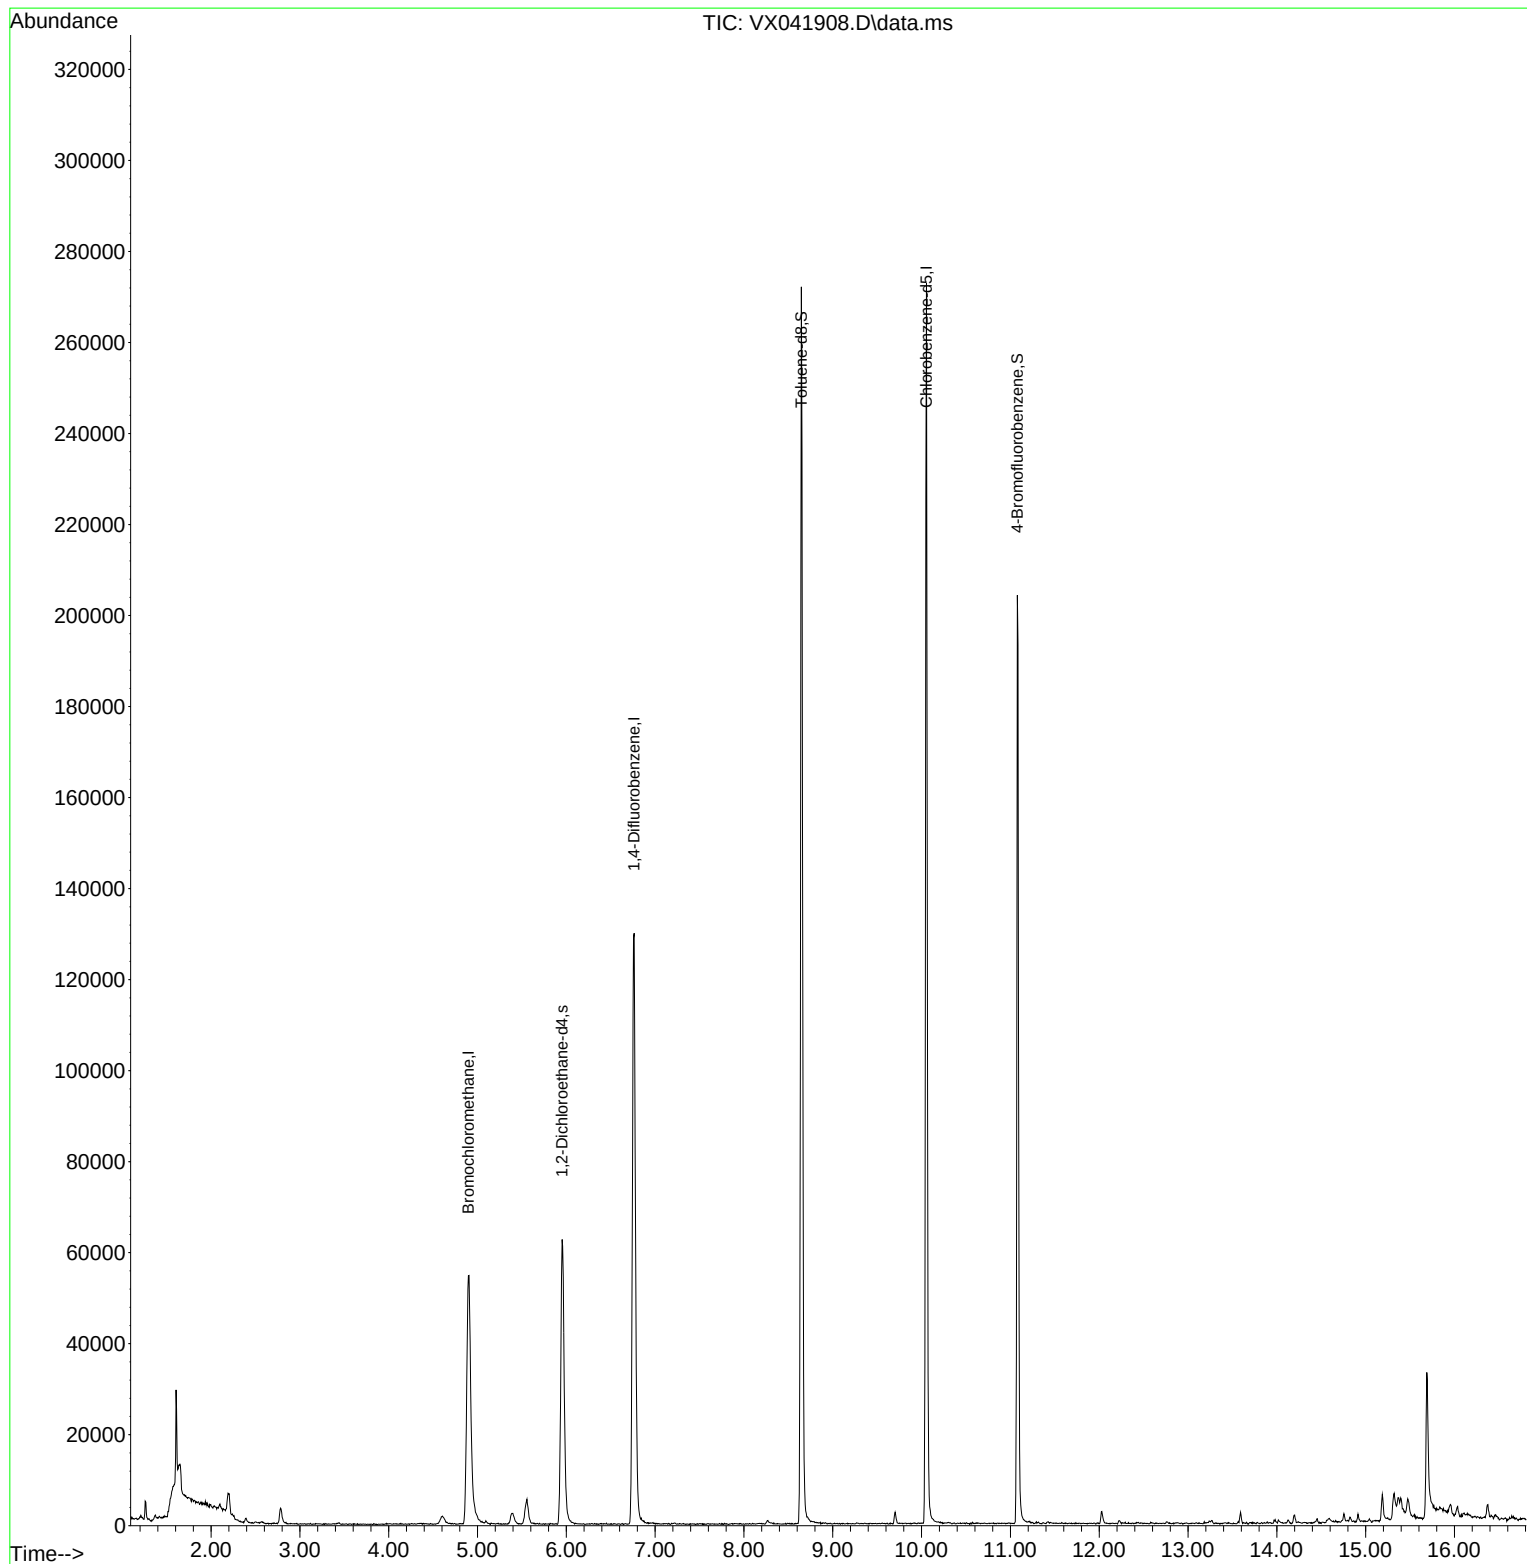


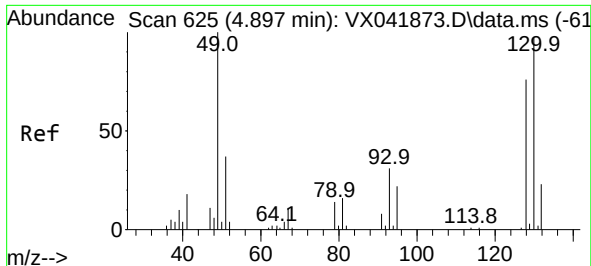

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 4.898 min Scan# 61
Delta R.T. 0.001 min
Lab File: VX041908.D
Acq: 17 Jun 2024 14:41




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:128 Resp: 29336
Ion Ratio Lower Upper
128 100
49 135.1 0.0 338.5
130 127.9 0.0 324.5

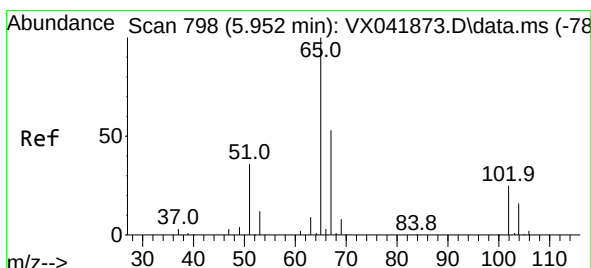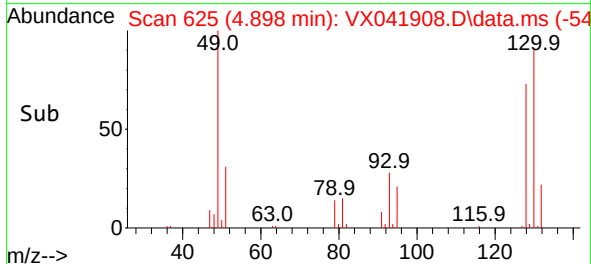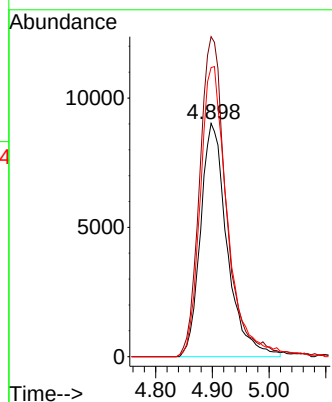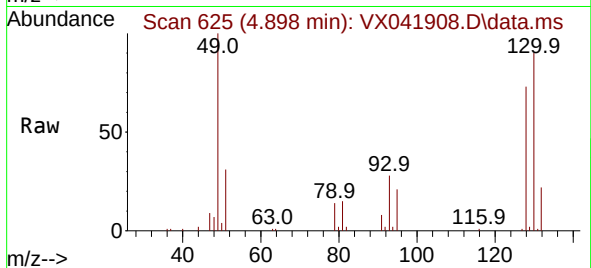

#27
1,2-Dichloroethane-d4
Concen: 29.557 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX041908.D
Acq: 17 Jun 2024 14:41

Tgt Ion: 65 Resp: 59689
Ion Ratio Lower Upper
65 100
67 53.2 43.4 65.0


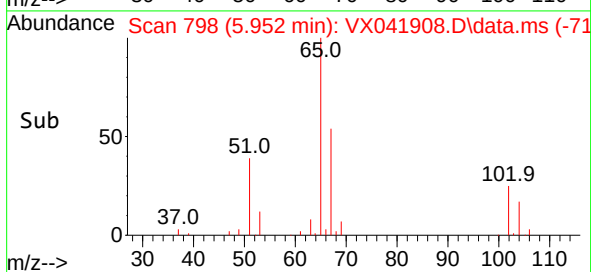
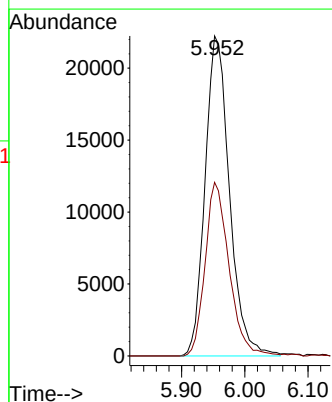
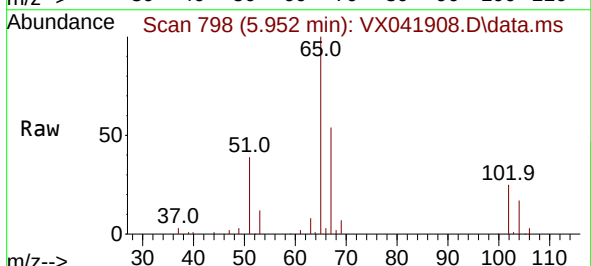


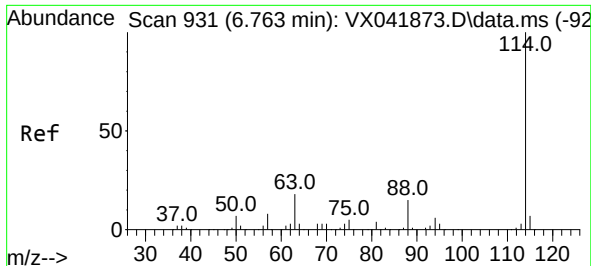

#28
1,4-Difluorobenzene
Concen: 30.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX041908.D
Acq: 17 Jun 2024 14:41




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:114 Resp: 146035
Ion Ratio Lower Upper
114 100
63 18.2 14.6 21.8
88 15.0 11.8 17.8

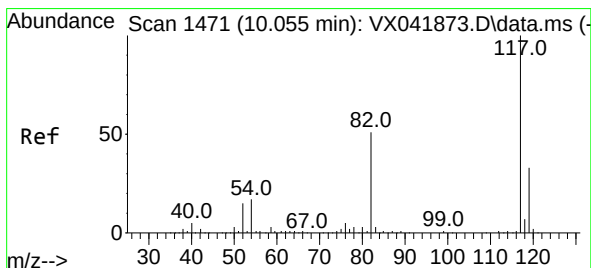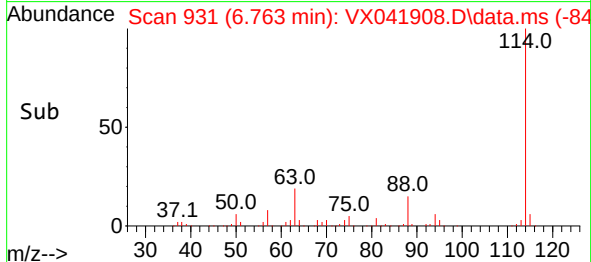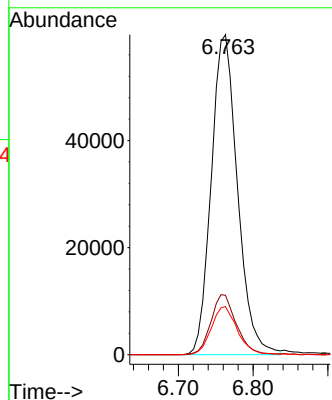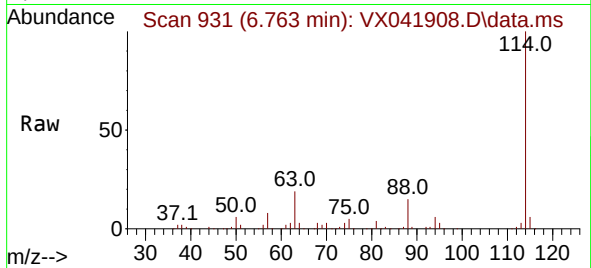

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX041908.D
Acq: 17 Jun 2024 14:41

Tgt Ion:117 Resp: 132491
Ion Ratio Lower Upper
117 100
82 51.4 41.1 61.7
119 32.1 26.1 39.1


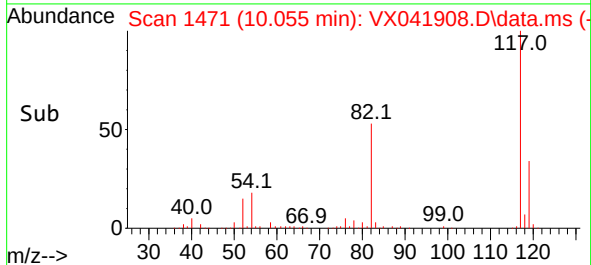
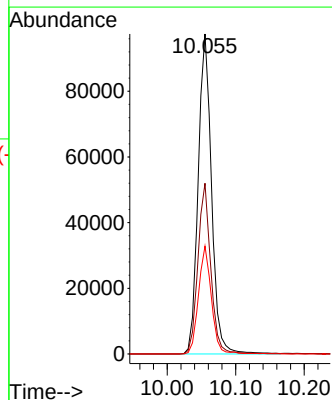
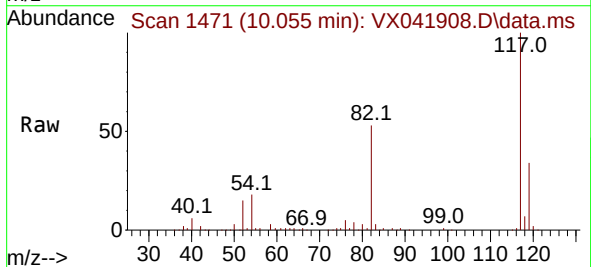


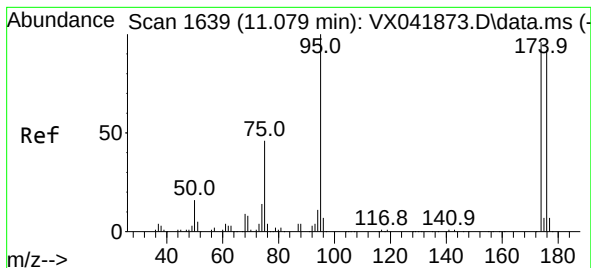

#60
4-Bromofluorobenzene
Concen: 27.316 ug/l
RT: 11.079 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX041908.D
Acq: 17 Jun 2024 14:41

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion: 95 Resp: 56022
Ion Ratio Lower Upper
95 100
174 97.4 78.9 118.3
176 94.3 77.1 115.7

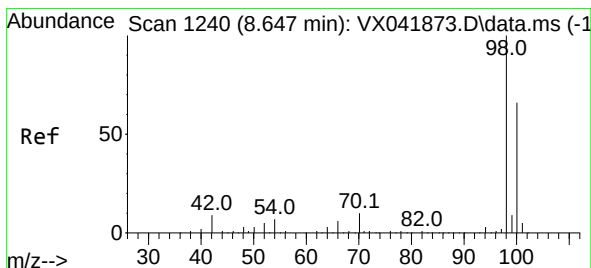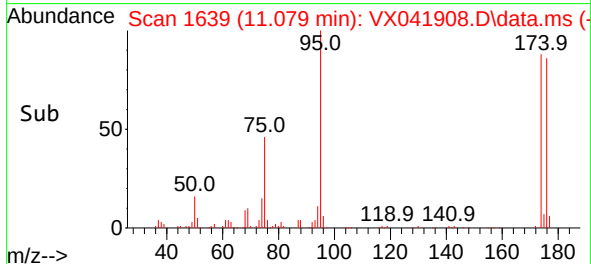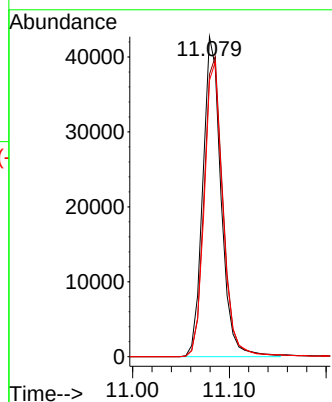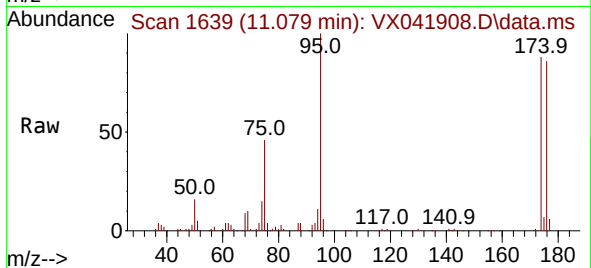

#63
Toluene-d8
Concen: 29.396 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX041908.D
Acq: 17 Jun 2024 14:41

Tgt Ion: 98 Resp: 166631
Ion Ratio Lower Upper
98 100
100 67.0 52.7 79.1

