

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061725\
 Data File : VX046723.D
 Acq On : 17 Jun 2025 15:23
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
 Title : SW846 8260

Signal : TIC: VX046723.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.532	231	237	244	rVB	3911	6903	1.15%	0.213%
2	5.397	695	707	724	rBV3	62089	198139	32.95%	6.115%
3	5.562	724	734	756	rVB	113893	351793	58.50%	10.858%
4	5.964	791	800	821	rBV	69902	200112	33.28%	6.176%
5	6.769	920	932	950	rBV	172947	444837	73.98%	13.730%
6	8.647	1234	1240	1260	rBV	356460	601309	100.00%	18.559%
7	10.055	1465	1471	1486	rBV	350670	506936	84.31%	15.646%
8	10.305	1507	1512	1526	rVB	3765	6710	1.12%	0.207%
9	11.079	1634	1639	1654	rBV	288298	374232	62.24%	11.550%
10	11.457	1696	1701	1710	rVB2	6564	9872	1.64%	0.305%
11	11.890	1766	1772	1778	rBV	5825	7102	1.18%	0.219%
12	11.969	1781	1785	1788	rBV	5700	6689	1.11%	0.206%
13	12.018	1788	1793	1807	rVB	362102	463516	77.08%	14.306%
14	12.335	1837	1845	1852	rBV	11643	15807	2.63%	0.488%
15	13.280	1997	2000	2006	rBV	4628	6535	1.09%	0.202%
16	13.591	2046	2051	2057	rBV4	8691	11512	1.91%	0.355%
17	13.719	2069	2072	2076	rVB3	7106	8924	1.48%	0.275%
18	13.774	2076	2081	2093	rBV	5320	8841	1.47%	0.273%
19	13.963	2108	2112	2117	rBV	7022	10225	1.70%	0.316%




Sum of corrected areas: 3239994

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061725\
Data File : VX046723.D
Acq On : 17 Jun 2025 15:23
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

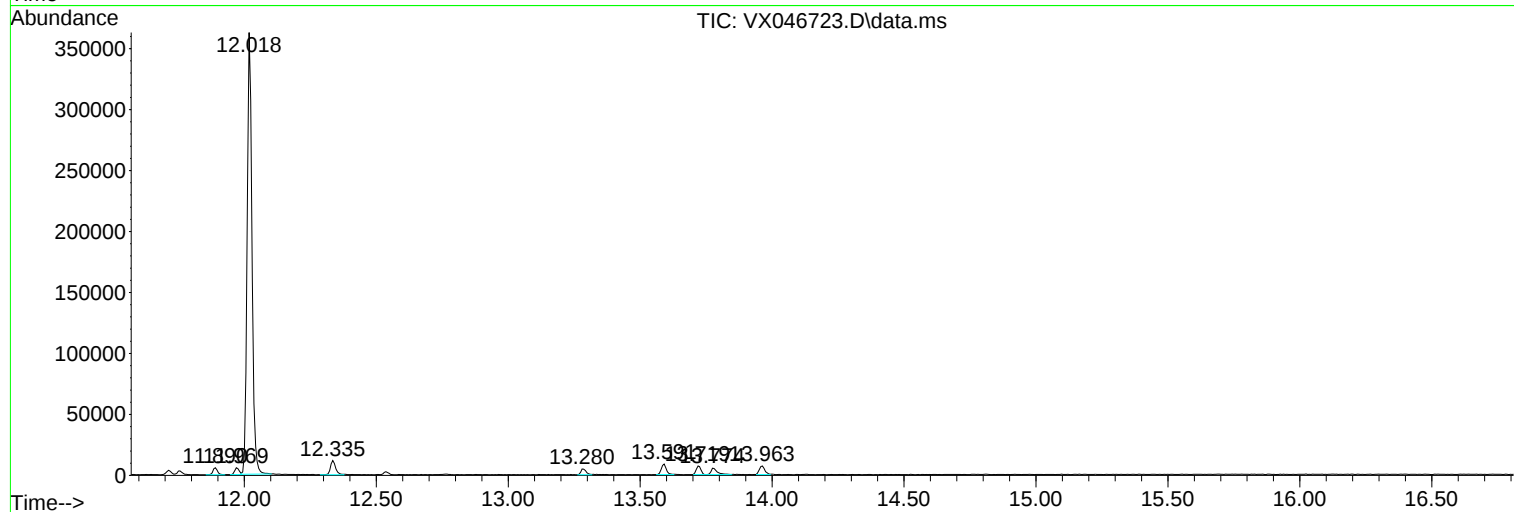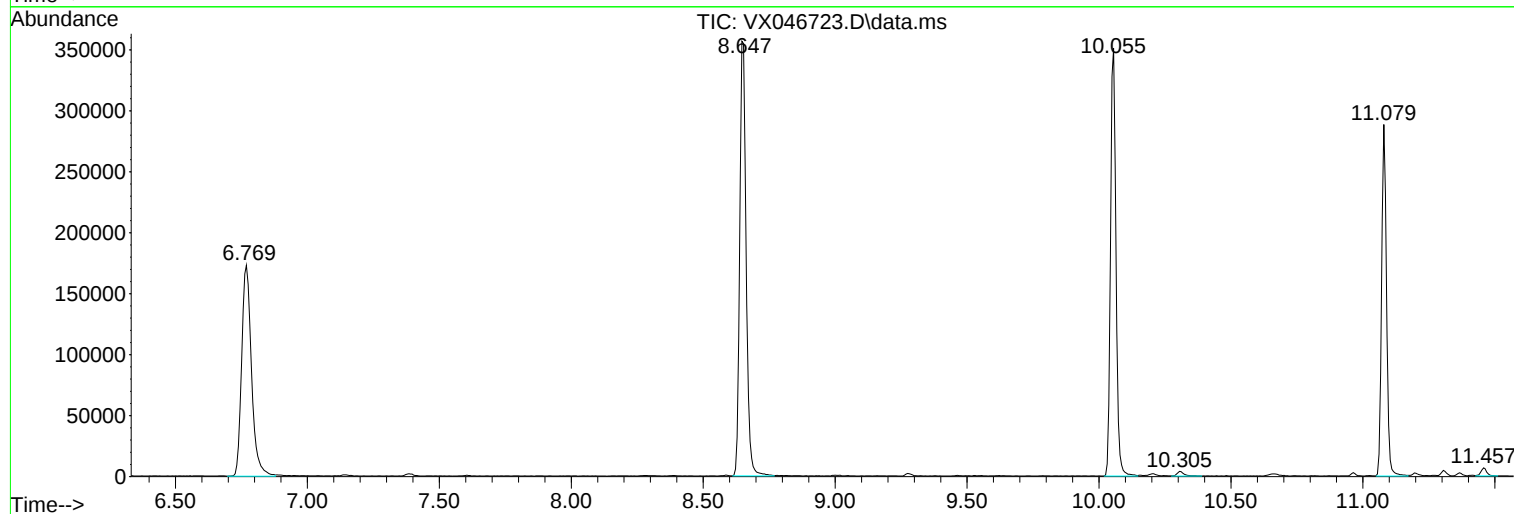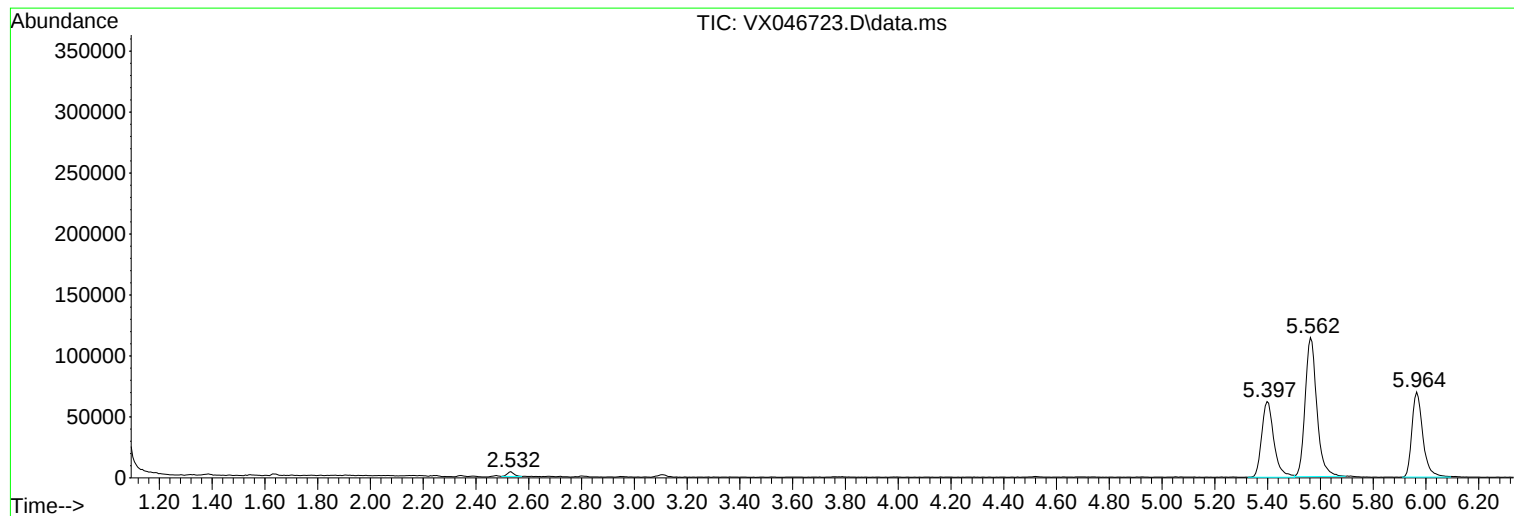

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061725\
Data File : VX046723.D
Acq On : 17 Jun 2025 15:23
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061725\
Data File : VX046723.D
Acq On : 17 Jun 2025 15:23
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc