

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX061819\  
Data File : VX010335.D  
Acq On : 18 Jun 2019 12:06  
Operator : JC/SP  
Sample : K3427-01  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TB-01-190617

## Integration Parameters: RTEINT.P

Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X060719W.M  
Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 4.690       | 570           | 580         | 591          | rBV2     | 7271           | 25746         | 1.88%           | 0.356%        |
| 2         | 5.501       | 702           | 713         | 725          | rBV      | 162363         | 467235        | 34.10%          | 6.458%        |
| 3         | 5.659       | 728           | 739         | 752          | rVB      | 289954         | 807186        | 58.91%          | 11.156%       |
| 4         | 6.062       | 794           | 805         | 817          | rBV      | 156876         | 404773        | 29.54%          | 5.595%        |
| 5         | 6.860       | 924           | 936         | 951          | rBV      | 416175         | 989266        | 72.20%          | 13.673%       |
| 6         | 8.714       | 1231          | 1240        | 1251         | rBV      | 874812         | 1370161       | 100.00%         | 18.938%       |
| 7         | 9.750       | 1403          | 1410        | 1415         | rBV      | 9788           | 14751         | 1.08%           | 0.204%        |
| 8         | 10.110      | 1462          | 1469        | 1479         | rBV      | 850577         | 1157420       | 84.47%          | 15.997%       |
| 9         | 11.134      | 1631          | 1637        | 1654         | rBV      | 719390         | 918072        | 67.00%          | 12.689%       |
| 10        | 12.073      | 1786          | 1791        | 1801         | rVB      | 822190         | 1080550       | 78.86%          | 14.935%       |


Sum of corrected areas: 7235160

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX061819\  
Data File : VX010335.D  
Acq On : 18 Jun 2019 12:06  
Operator : JC/SP  
Sample : K3427-01  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TB-01-190617

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X060719W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

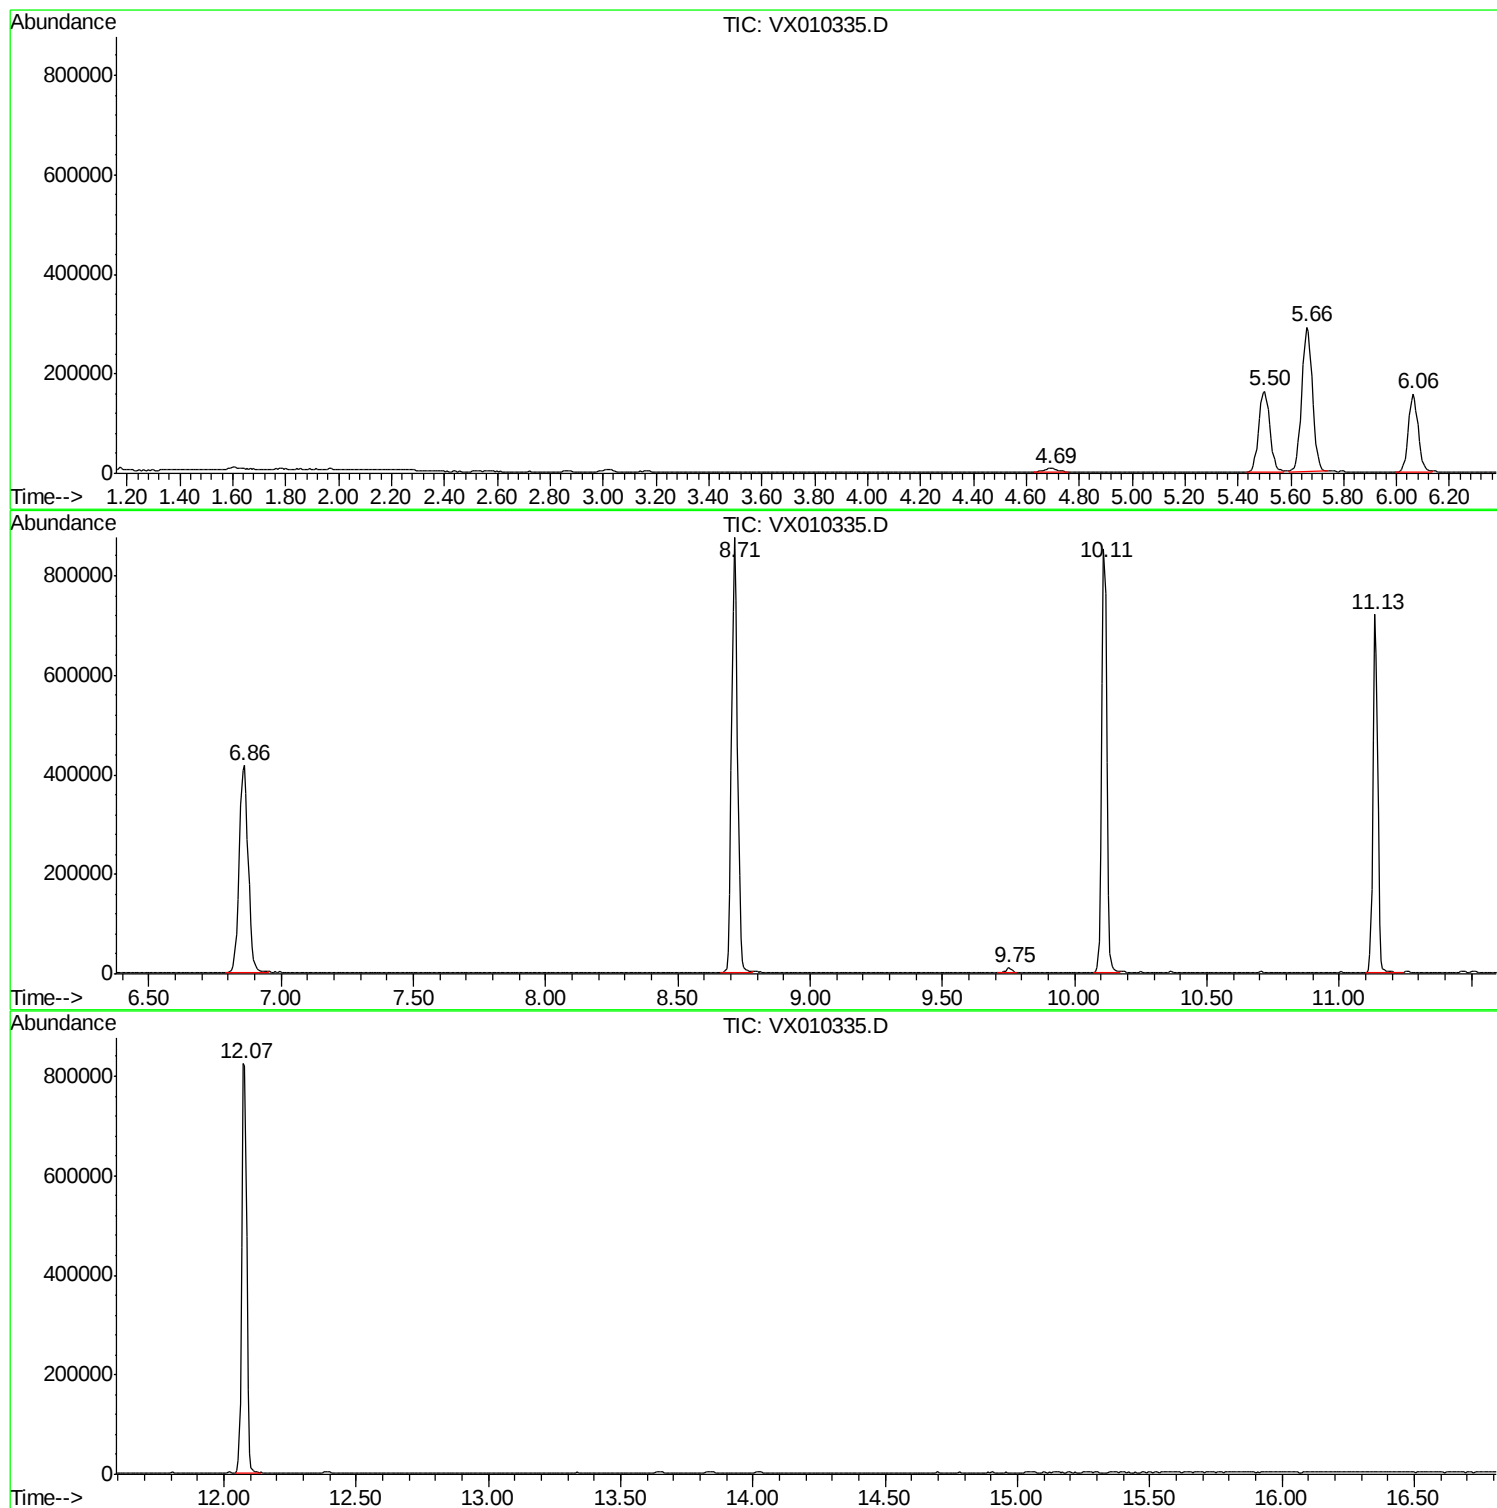

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX061819\  
Data File : VX010335.D  
Acq On : 18 Jun 2019 12:06  
Operator : JC/SP  
Sample : K3427-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TB-01-190617

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X060719W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX061819\  
Data File : VX010335.D  
Acq On : 18 Jun 2019 12:06  
Operator : JC/SP  
Sample : K3427-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TB-01-190617

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X060719W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |