


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX061820\
Data File : VX016846.D
Acq On : 18 Jun 2020 17:51
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061820W.M
Title : SW846 8260
Last Update : Fri Jun 19 12:07:48 2020

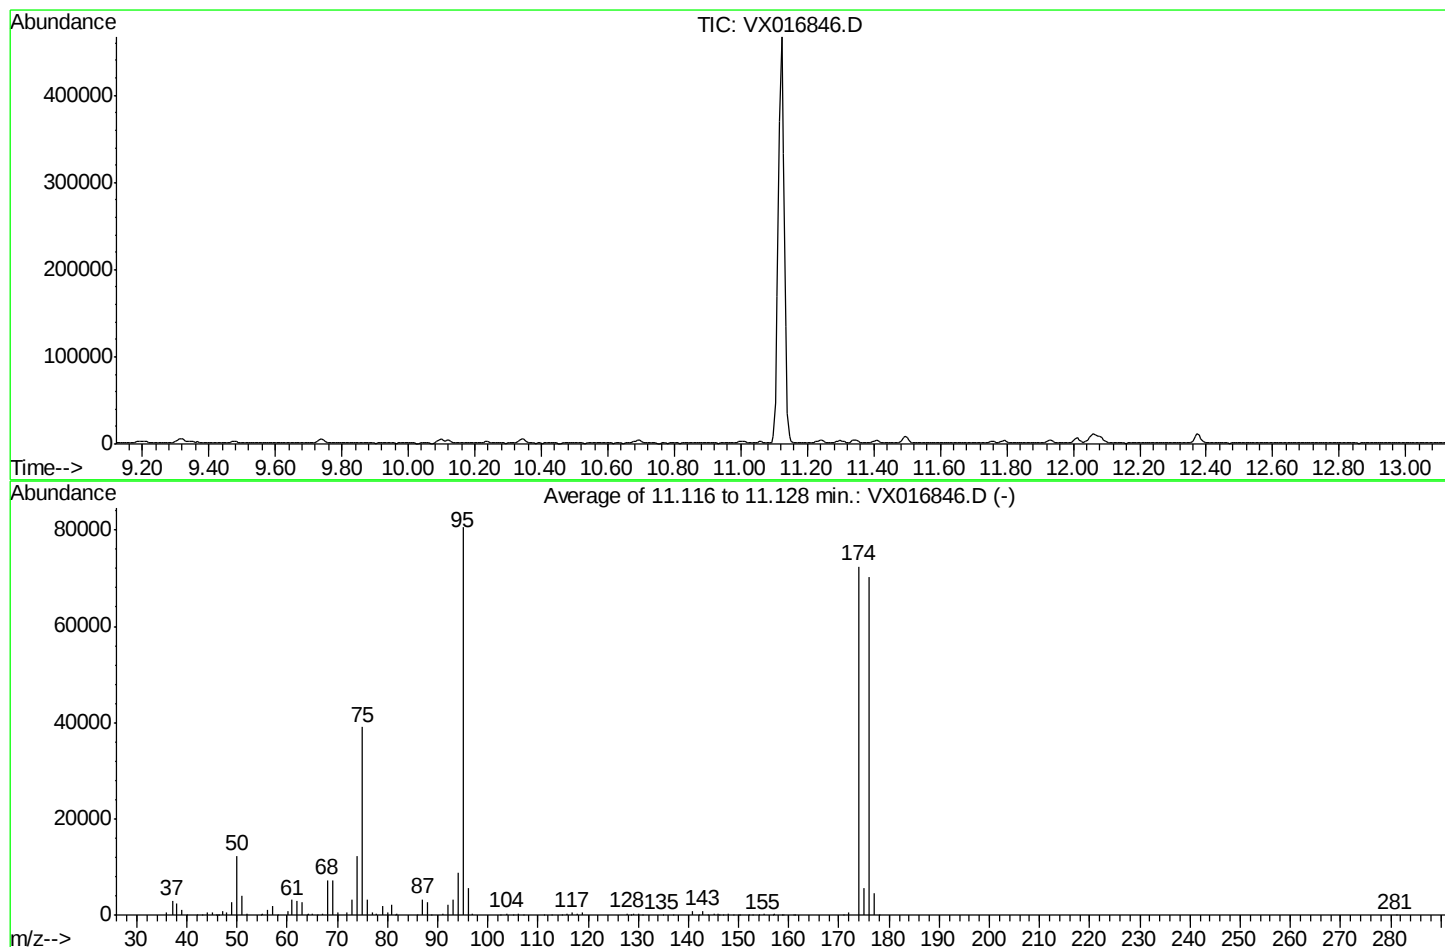

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	12273	PASS
75	95	30	60	48.5	39075	PASS
95	95	100	100	100.0	80581	PASS
96	95	5	9	6.9	5546	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	89.9	72464	PASS
175	174	5	9	7.7	5571	PASS
176	174	95	101	97.1	70378	PASS
177	176	5	9	6.5	4548	PASS