

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061821\
 Data File : VX022770.D
 Acq On : 18 Jun 2021 16:35
 Operator : JC/MD
 Sample : M2753-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FB01-20210616

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M

Title : SW846 8260

Signal : TIC: VX022770.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	26	30	37	rVB3	9194	10526	2.67%	0.562%
2	1.556	71	77	83	rVB3	2620	4387	1.11%	0.234%
3	2.550	235	240	245	rVB	4791	8216	2.09%	0.439%
4	4.580	564	573	584	rBV2	3183	11118	2.82%	0.594%
5	5.397	695	707	722	rBV2	41013	119800	30.42%	6.399%
6	5.568	722	735	745	rVV	63448	179245	45.51%	9.574%
7	5.964	789	800	812	rBV2	54605	143655	36.47%	7.673%
8	6.769	923	932	944	rBV	111440	261033	66.28%	13.943%
9	8.653	1234	1241	1249	rBV	254341	393858	100.00%	21.037%
10	10.055	1466	1471	1484	rVB	217119	300164	76.21%	16.033%
11	11.085	1634	1640	1648	rVB	169450	216961	55.09%	11.589%
12	12.024	1789	1794	1800	rBV	181309	223231	56.68%	11.923%




Sum of corrected areas: 1872194

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061821\
Data File : VX022770.D
Acq On : 18 Jun 2021 16:35
Operator : JC/MD
Sample : M2753-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB01-20210616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

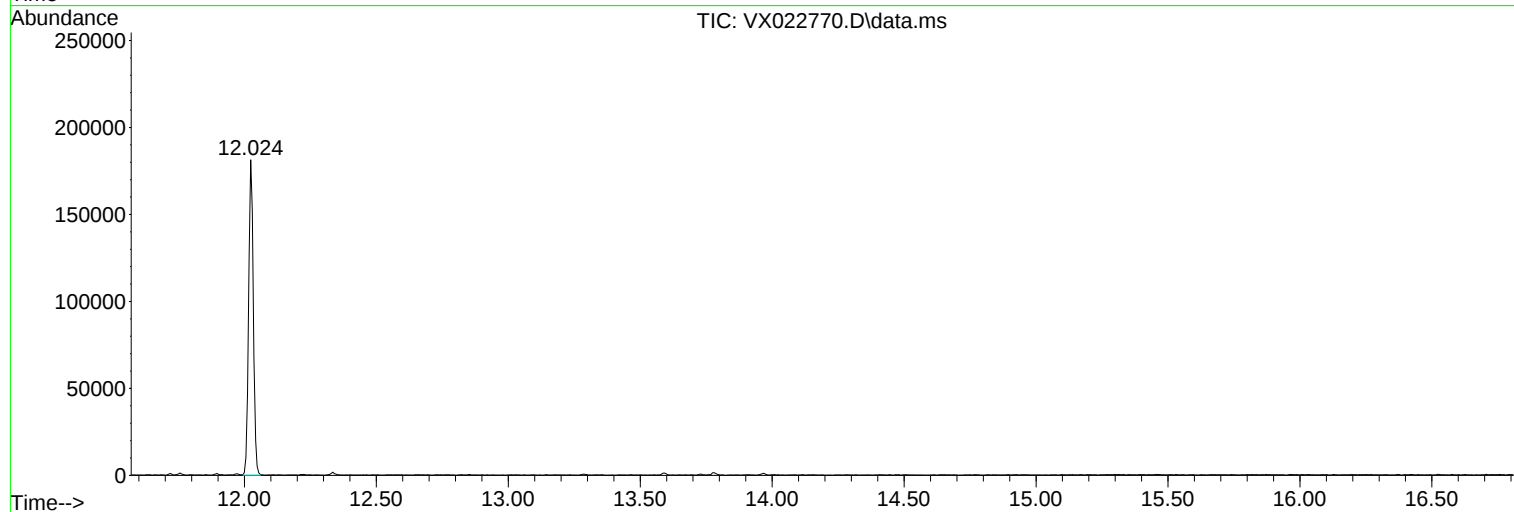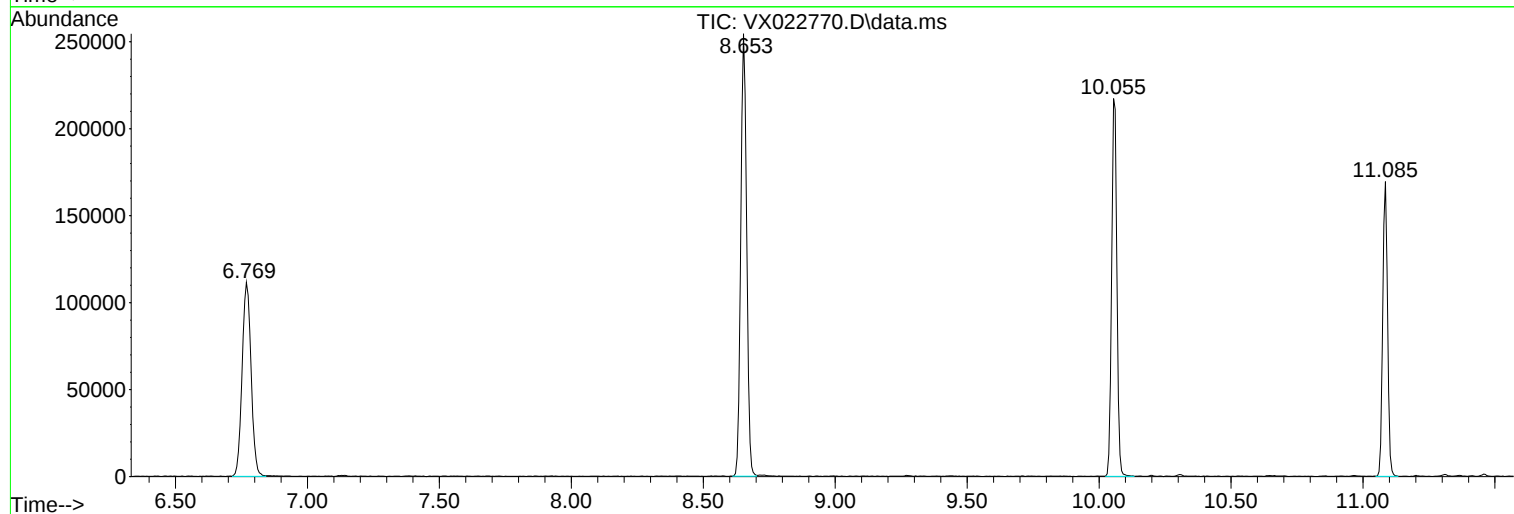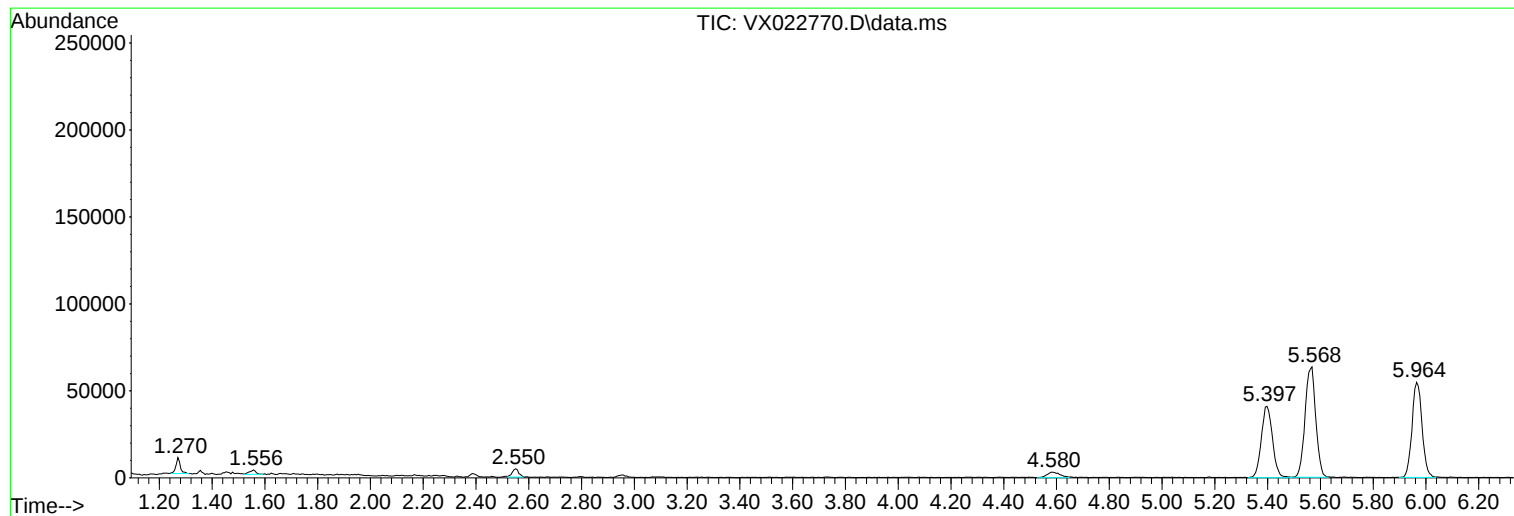

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061821\
Data File : VX022770.D
Acq On : 18 Jun 2021 16:35
Operator : JC/MD
Sample : M2753-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB01-20210616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061821\
Data File : VX022770.D
Acq On : 18 Jun 2021 16:35
Operator : JC/MD
Sample : M2753-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB01-20210616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
