

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061824\
 Data File : VX041931.D
 Acq On : 18 Jun 2024 18:22
 Operator : JC/MD
 Sample : P2927-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1


Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-189-GW-498-500

Quant Time: Jun 19 08:49:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 19 07:57:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	132041	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	204686	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	207742	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	104564	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	67435	44.289	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	88.580%
35) Dibromofluoromethane	5.391	113	63940	44.025	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	88.060%
50) Toluene-d8	8.653	98	244506	47.922	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	95.840%
62) 4-Bromofluorobenzene	11.079	95	93226	49.567	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.140%
Target Compounds						
						Qvalue
2) Dichlorodifluoromethane	1.166	85	2704	2.688	ug/l	93
3) Chloromethane	1.307	50	401	0.318	ug/l	95
5) Bromomethane	1.605	94	363	0.581	ug/l	# 44
6) Chloroethane	1.666	64	303	Below Cal	#	43
9) 1,1,2-Trichlorotrifluo...	2.319	101	18647	16.333	ug/l	86
11) Tert butyl alcohol	3.001	59	443	1.533	ug/l	# 78
12) 1,1-Dichloroethene	2.306	96	3499	3.072	ug/l	83
13) Acrolein	2.239	56	84	0.259	ug/l	# 14
16) Acetone	2.392	43	4970	7.434	ug/l	99
17) Carbon Disulfide	2.501	76	8717	3.754	ug/l	98
20) Methylene Chloride	2.782	84	705	0.482	ug/l	94
24) 1,1-Dichloroethane	3.605	63	1273	0.595	ug/l	# 83
25) 2-Butanone	4.611	43	909	0.874	ug/l	# 89
27) cis-1,2-Dichloroethene	4.489	96	5387	3.721	ug/l	78
28) Bromochloromethane	5.086	49	604	0.660	ug/l	# 16
29) Tetrahydrofuran	5.050	42	215	0.320	ug/l	# 34
30) Chloroform	5.105	83	9263	4.159	ug/l	96
31) Cyclohexane	5.544	56	1829	1.027	ug/l	# 1
32) 1,1,1-Trichloroethane	5.379	97	851	0.457	ug/l	# 44
36) 1,1-Dichloropropene	5.550	75	7888	5.115	ug/l	# 51
37) Ethyl Acetate	4.611	43	909	0.452	ug/l	# 69
38) Carbon Tetrachloride	5.672	117	2815	1.652	ug/l	86
39) Methylcyclohexane	7.129	83	5683	2.914	ug/l	# 1
42) 1,2-Dichloroethane	6.098	62	648	0.387	ug/l	# 77
44) Trichloroethene	7.129	130	567167	406.787	ug/l	87
49) 1,4-Dioxane	7.689	88	299	27.457	ug/l	# 65
51) 4-Methyl-2-Pentanone	8.647	43	969	0.456	ug/l	# 1
55) 1,1,2-Trichloroethane	9.159	97	1791	1.298	ug/l	96
76) 1,2,3-Trichloropropane	11.079	75	42689	22.489	ug/l	# 39
81) trans-1,4-Dichloro-2-b...	11.079	75	42689	63.865	ug/l	# 5
95) Naphthalene	13.786	128	407	0.801	ug/l	# 69

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.556 min Scan# 71

Delta R.T. 0.006 min

Lab File: VX041931.D

Acq: 18 Jun 2024 18:22

Instrument :

MSVOA_X

ClientSampleId :





BP-VPB-189-GW-498-500

Tgt Ion:168 Resp: 132041

Ion Ratio Lower Upper

168 100

99 46.3 56.6 85.0#

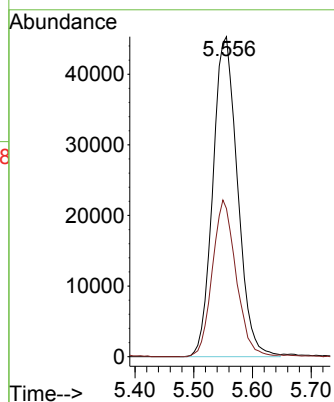

#2

Dichlorodifluoromethane

Concen: 2.688 ug/l

RT: 1.166 min Scan# 13

Delta R.T. -0.000 min

Lab File: VX041931.D




Acq: 18 Jun 2024 18:22


Tgt Ion: 85 Resp: 2704

Ion Ratio Lower Upper

85 100

87 37.6 16.7 50.1


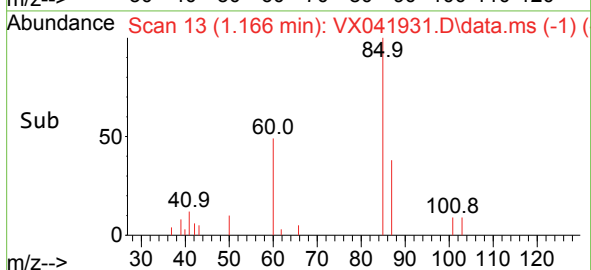
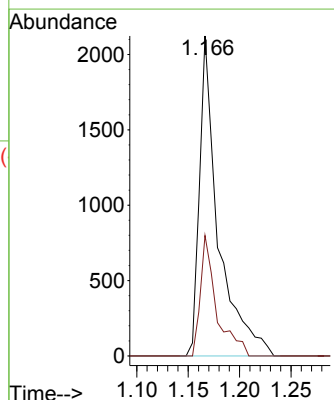



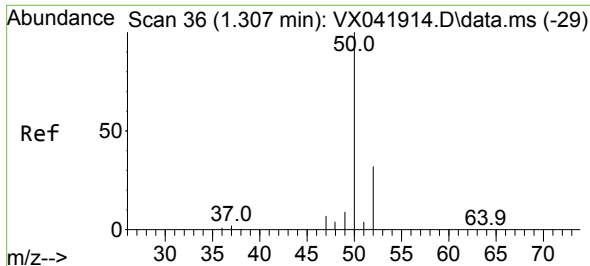

#3
Chloromethane
Concen: 0.318 ug/l
RT: 1.307 min Scan# 30
Delta R.T. -0.000 min
Lab File: VX041931.D
Acq: 18 Jun 2024 18:22




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-189-GW-498-500


Tgt Ion: 50 Resp: 401
Ion Ratio Lower Upper
50 100
52 28.9 25.5 38.3

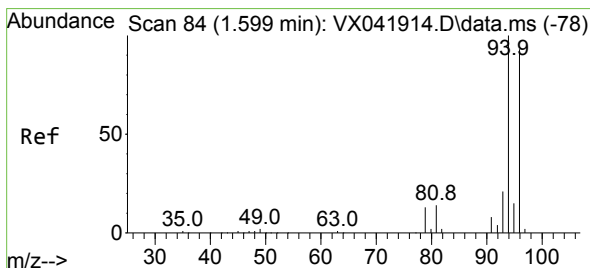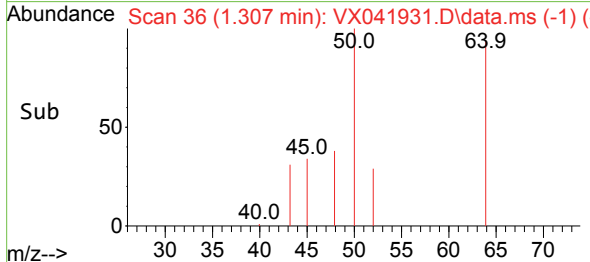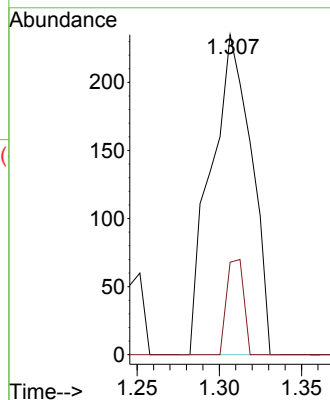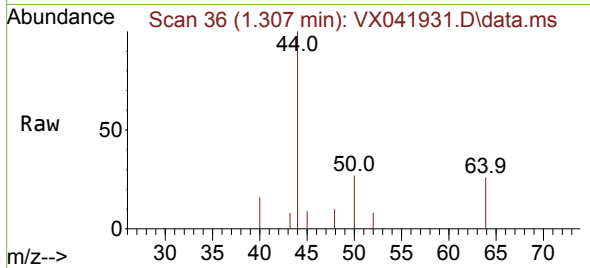

#5
Bromomethane
Concen: 0.581 ug/l
RT: 1.605 min Scan# 85
Delta R.T. 0.006 min
Lab File: VX041931.D
Acq: 18 Jun 2024 18:22

Tgt Ion: 94 Resp: 363
Ion Ratio Lower Upper
94 100
96 39.4 74.6 111.8#


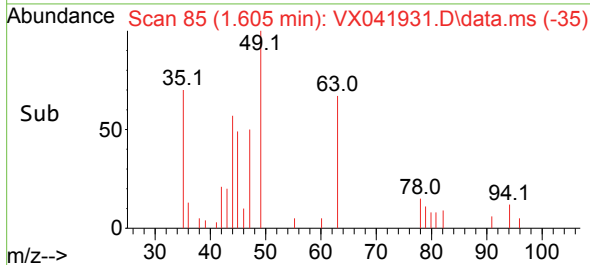
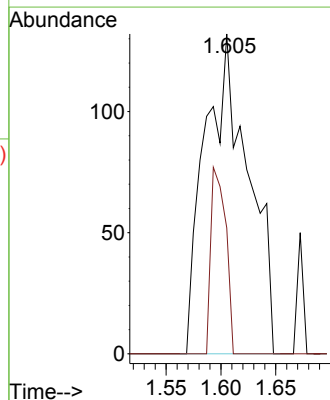
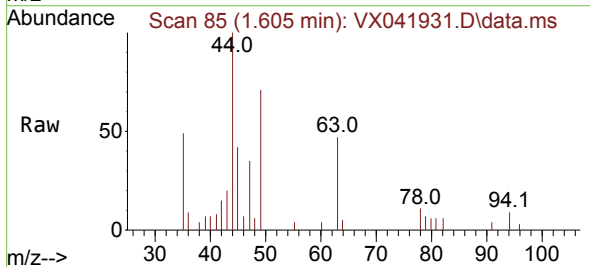


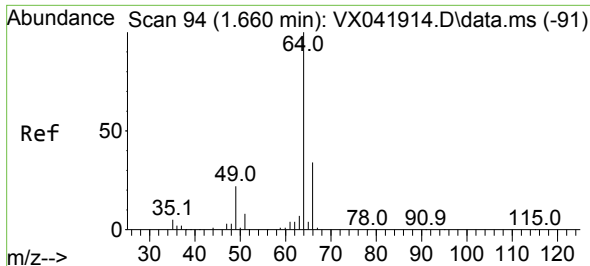

#6
Chloroethane
Concen: Below Cal
RT: 1.666 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX041931.D
Acq: 18 Jun 2024 18:22




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-189-GW-498-500


Tgt Ion: 64 Resp: 303
Ion Ratio Lower Upper
64 100
66 0.0 25.1 37.7#

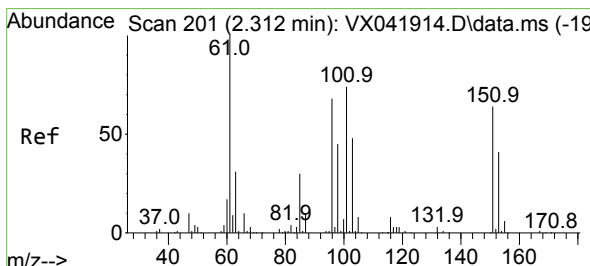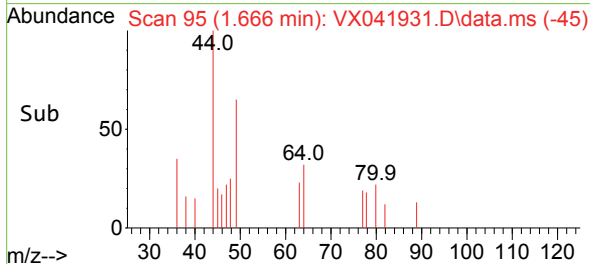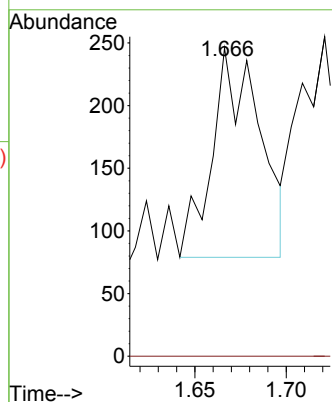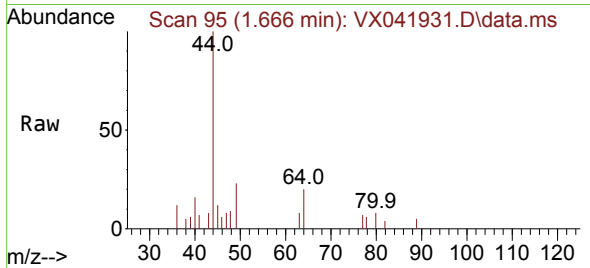

#9
1,1,2-Trichlorotrifluoroethane
Concen: 16.333 ug/l
RT: 2.319 min Scan# 202
Delta R.T. 0.006 min
Lab File: VX041931.D
Acq: 18 Jun 2024 18:22

Tgt Ion: 101 Resp: 18647
Ion Ratio Lower Upper
101 100
85 40.2 37.0 55.6
151 87.7 58.6 87.8

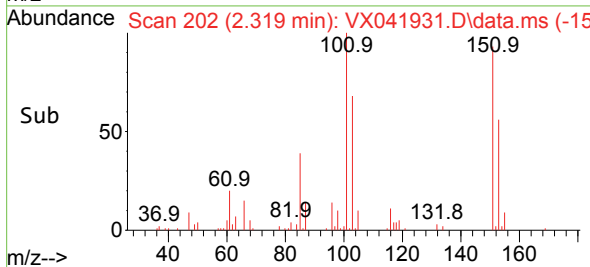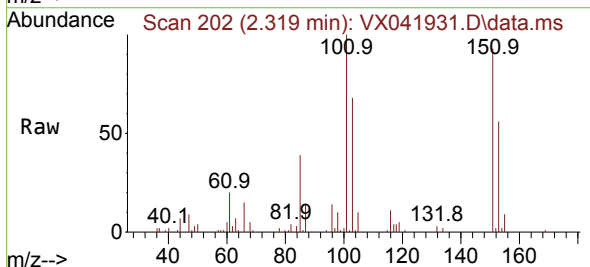



#11

Tert butyl alcohol

Concen: 1.533 ug/l

RT: 3.001 min Scan# 31

Delta R.T. -0.006 min

Lab File: VX041931.D

Acq: 18 Jun 2024 18:22

Instrument :

MSVOA_X

ClientSampleId :





BP-VPB-189-GW-498-500

Tgt Ion: 59 Resp: 443

Ion Ratio Lower Upper

59 100

57 0.0 6.0 9.0#

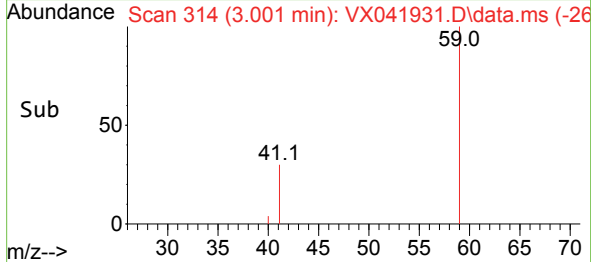

#12

1,1-Dichloroethene

Concen: 3.072 ug/l

RT: 2.306 min Scan# 200

Delta R.T. -0.000 min

Lab File: VX041931.D

Acq: 18 Jun 2024 18:22




Tgt Ion: 96 Resp: 3499


Ion Ratio Lower Upper

96 100

61 151.8 144.6 216.8

98 70.2 50.4 75.6

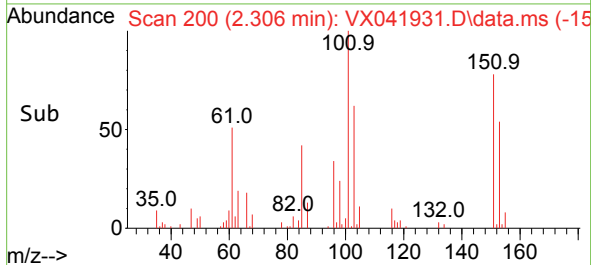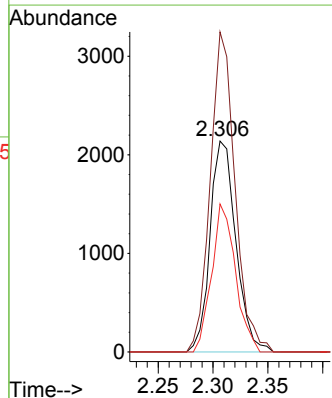



#13

Acrolein

Concen: 0.259 ug/l

RT: 2.239 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX041931.D

Acq: 18 Jun 2024 18:22

Instrument :

MSVOA_X

ClientSampleId :





BP-VPB-189-GW-498-500

Tgt Ion: 56 Resp: 84

Ion Ratio Lower Upper

56 100

55 0.0 57.1 85.7#

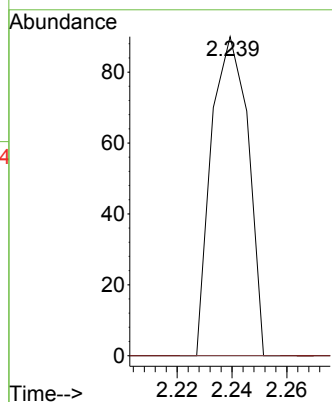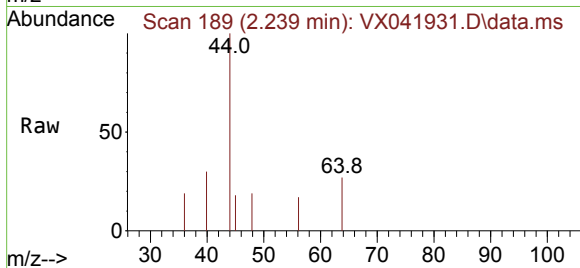

#16

Acetone

Concen: 7.434 ug/l

RT: 2.392 min Scan# 214

Delta R.T. -0.006 min

Lab File: VX041931.D




Acq: 18 Jun 2024 18:22


Tgt Ion: 43 Resp: 4970

Ion Ratio Lower Upper

43 100

58 27.8 21.9 32.9

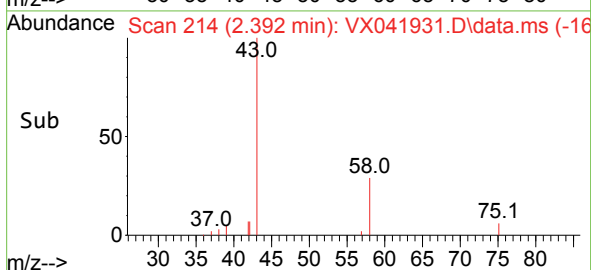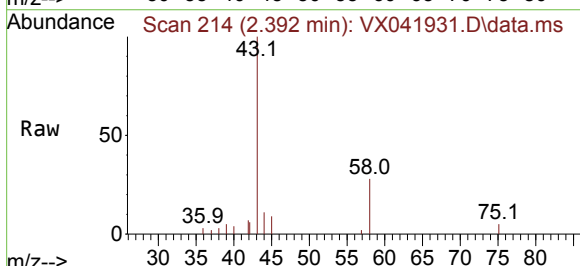



#17

Carbon Disulfide

Concen: 3.754 ug/l

RT: 2.501 min Scan# 21

Delta R.T. -0.000 min

Lab File: VX041931.D


Acq: 18 Jun 2024 18:22

Instrument :

MSVOA_X

ClientSampleId :

BP-VPB-189-GW-498-500






Tgt Ion: 76 Resp: 8717

Ion Ratio Lower Upper

76 100

78 9.4 7.0 10.6

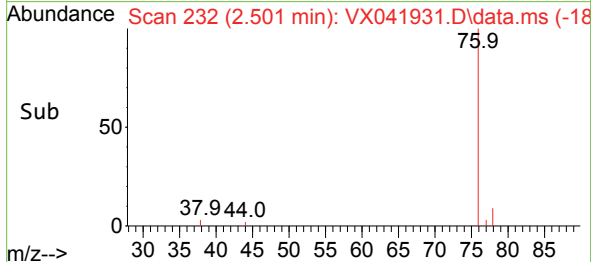

#20

Methylene Chloride

Concen: 0.482 ug/l

RT: 2.782 min Scan# 278

Delta R.T. -0.000 min

Lab File: VX041931.D

Acq: 18 Jun 2024 18:22

Tgt Ion: 84 Resp: 705




Ion Ratio Lower Upper


84 100

49 119.3 103.6 155.4

51 38.9 33.8 50.6

86 61.4 49.4 74.0




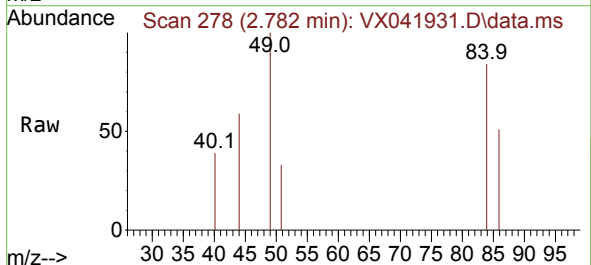




#24
1,1-Dichloroethane
Concen: 0.595 ug/l
RT: 3.605 min Scan# 41
Delta R.T. -0.000 min
Lab File: VX041931.D
Acq: 18 Jun 2024 18:22




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-189-GW-498-500


Tgt Ion: 63 Resp: 1273
Ion Ratio Lower Upper
63 100
98 0.0 3.3 9.8#
100 0.0 2.1 6.5#

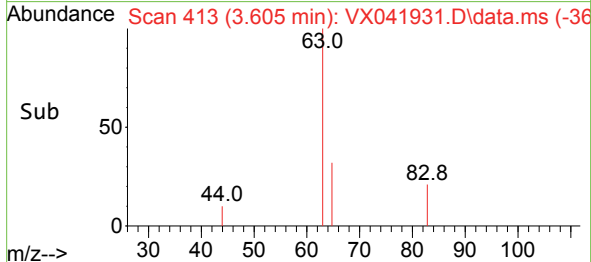

#25
2-Butanone
Concen: 0.874 ug/l
RT: 4.611 min Scan# 578
Delta R.T. 0.037 min
Lab File: VX041931.D
Acq: 18 Jun 2024 18:22

Tgt Ion: 43 Resp: 909
Ion Ratio Lower Upper
43 100
72 18.7 19.4 29.2#

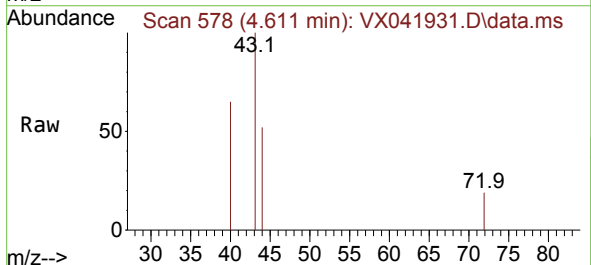



#27

cis-1,2-Dichloroethene

Concen: 3.721 ug/l

RT: 4.489 min Scan# 51

Delta R.T. -0.000 min

Lab File: VX041931.D

Acq: 18 Jun 2024 18:22

Instrument :

MSVOA_X

ClientSampleId :

BP-VPB-189-GW-498-500





Tgt Ion: 96 Resp: 5387

Ion Ratio Lower Upper

96 100

61 117.9 0.0 312.2

98 68.3 0.0 129.0

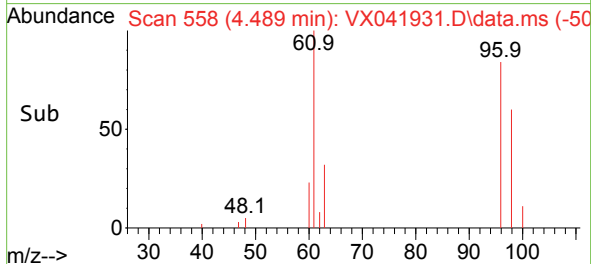

#28

Bromochloromethane

Concen: 0.660 ug/l

RT: 5.086 min Scan# 656

Delta R.T. 0.183 min

Lab File: VX041931.D

Acq: 18 Jun 2024 18:22




Tgt Ion: 49 Resp: 604


Ion Ratio Lower Upper

49 100

129 0.0 0.0 3.8

130 0.0 57.5 86.3#

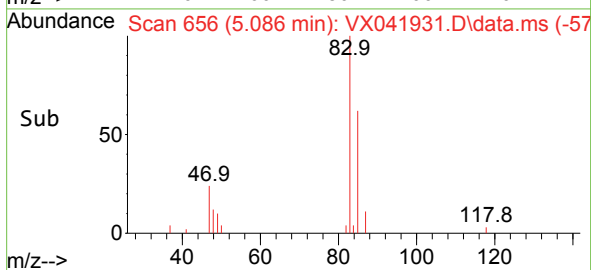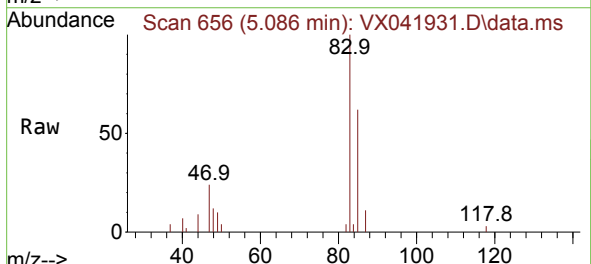



#29

Tetrahydrofuran

Concen: 0.320 ug/l

RT: 5.050 min Scan# 61

Delta R.T. 0.030 min

Lab File: VX041931.D

Acq: 18 Jun 2024 18:22

Instrument :

MSVOA_X

ClientSampleId :

BP-VPB-189-GW-498-500





Tgt Ion: 42 Resp: 215

Ion Ratio Lower Upper

42 100

72 0.0 34.2 51.4#

71 0.0 32.2 48.2#

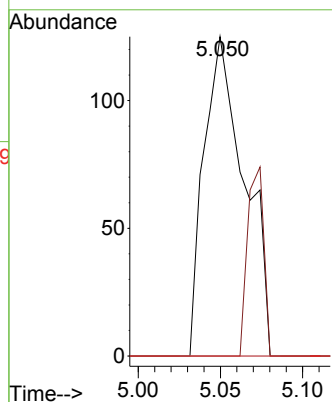

#30

Chloroform

Concen: 4.159 ug/l

RT: 5.105 min Scan# 659

Delta R.T. 0.006 min

Lab File: VX041931.D




Acq: 18 Jun 2024 18:22


Tgt Ion: 83 Resp: 9263

Ion Ratio Lower Upper

83 100


85 66.1 50.3 75.5

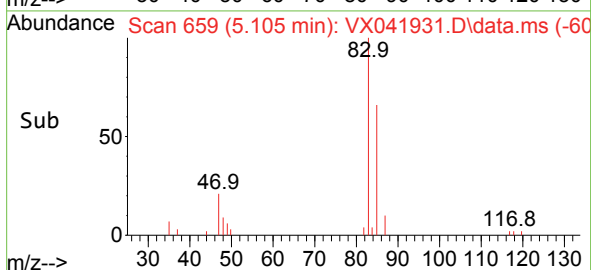

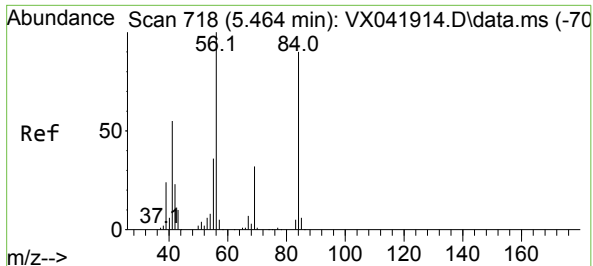




#31
Cyclohexane
Concen: 1.027 ug/l
RT: 5.544 min Scan# 718
Delta R.T. 0.079 min
Lab File: VX041931.D
Acq: 18 Jun 2024 18:22

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-189-GW-498-500

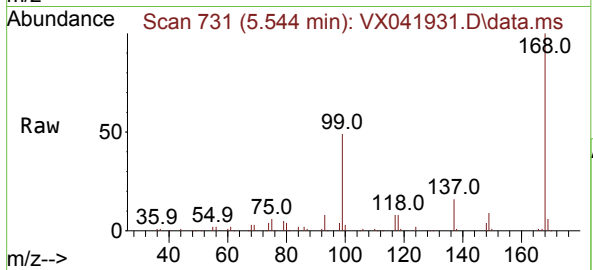


Tgt Ion: 56 Resp: 1829

Ion	Ratio	Lower	Upper
56	100		
69	192.4	23.4	35.2#
84	140.8	65.9	98.9#

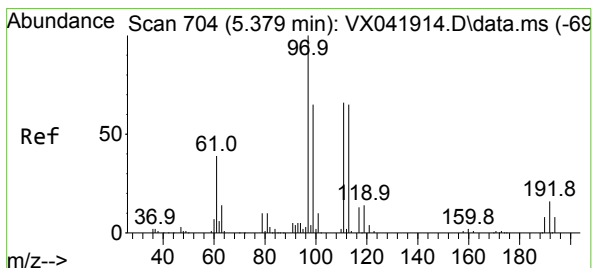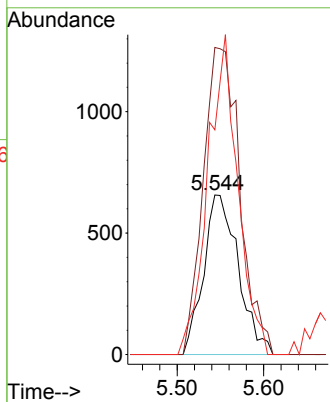
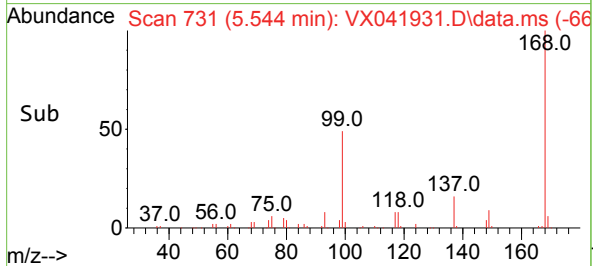



#32
1,1,1-Trichloroethane
Concen: 0.457 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.000 min
Lab File: VX041931.D
Acq: 18 Jun 2024 18:22

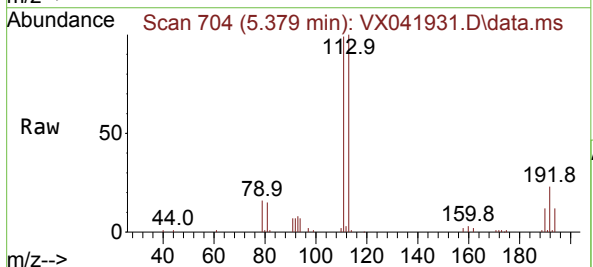

Tgt Ion: 97 Resp: 851

Ion	Ratio	Lower	Upper
97	100		
99	0.0	51.1	76.7#
61	31.7	36.4	54.6#

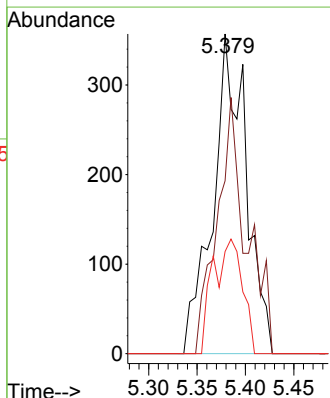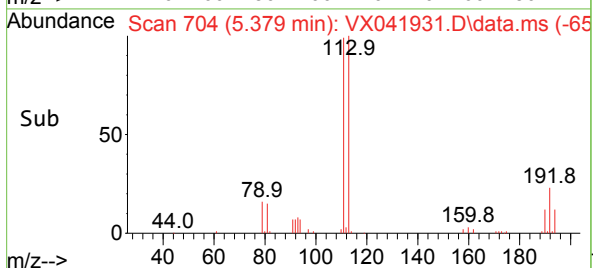



#33

1,2-Dichloroethane-d4

Concen: 44.289 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.000 min

Lab File: VX041931.D

Acq: 18 Jun 2024 18:22

Instrument :

MSVOA_X

ClientSampleId :





BP-VPB-189-GW-498-500

Tgt Ion: 65 Resp: 67435

Ion Ratio Lower Upper

65 100

67 53.4 0.0 100.2

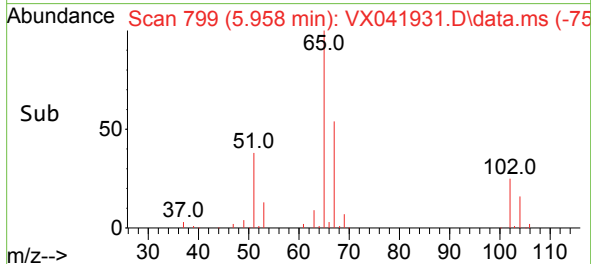

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX041931.D

Acq: 18 Jun 2024 18:22




Tgt Ion: 114 Resp: 204686


Ion Ratio Lower Upper

114 100

63 18.9 0.0 45.0

88 15.4 0.0 36.6





#35

Dibromofluoromethane

Concen: 44.025 ug/l

RT: 5.391 min Scan# 706

Delta R.T. -0.000 min

Lab File: VX041931.D


Acq: 18 Jun 2024 18:22

Instrument :




MSVOA_X

ClientSampleId :

BP-VPB-189-GW-498-500



Tgt Ion:	113	Resp:	63940
Ion	Ratio	Lower	Upper
113	100		
111	102.2	82.9	124.3
192	25.5	13.3	19.9#

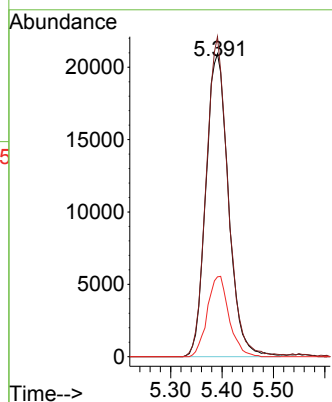

#36

1,1-Dichloropropene

Concen: 5.115 ug/l




RT: 5.550 min Scan# 732


Delta R.T. -0.140 min

Lab File: VX041931.D

Acq: 18 Jun 2024 18:22

Tgt Ion:	75	Resp:	7888
Ion	Ratio	Lower	Upper
75	100		
110	9.8	17.0	50.9#
77	0.0	24.7	37.1#

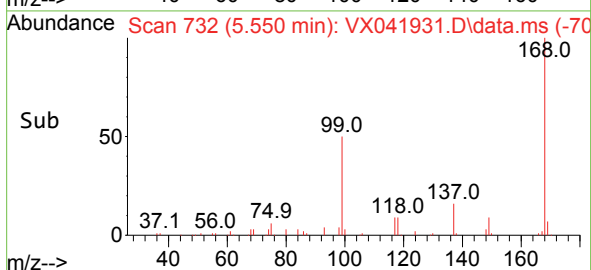



#37

Ethyl Acetate

Concen: 0.452 ug/l

RT: 4.611 min Scan# 51

Delta R.T. -0.116 min

Lab File: VX041931.D

Acq: 18 Jun 2024 18:22





Instrument :

MSVOA_X

ClientSampleId :

BP-VPB-189-GW-498-500

Tgt Ion: 43	Resp:	909
Ion	Ratio	Lower Upper
43	100	
61	0.0	10.6 16.0#
70	0.0	8.3 12.5#

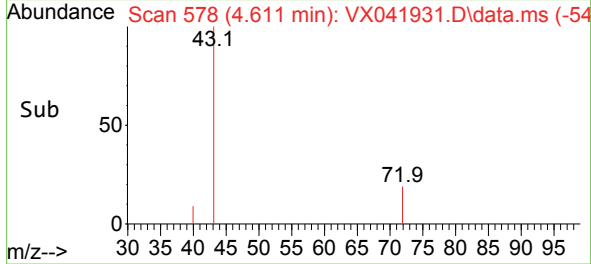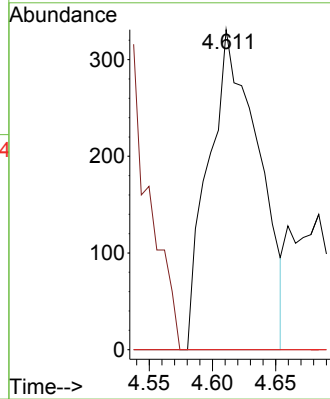

#38

Carbon Tetrachloride

Concen: 1.652 ug/l




RT: 5.672 min Scan# 752


Delta R.T. -0.006 min

Lab File: VX041931.D

Acq: 18 Jun 2024 18:22


Tgt Ion: 117	Resp:	2815
Ion	Ratio	Lower Upper
117	100	
119	81.6	78.2 117.2
121	33.5	24.4 36.6

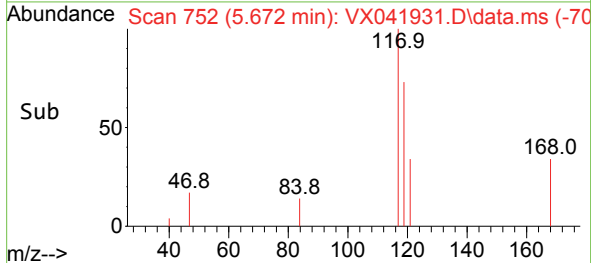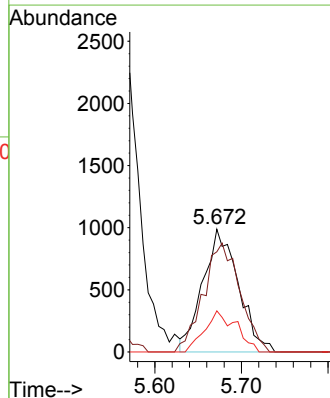






#39
Methylcyclohexane
Concen: 2.914 ug/l
RT: 7.129 min Scan# 91
Delta R.T. -0.250 min
Lab File: VX041931.D
Acq: 18 Jun 2024 18:22

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-189-GW-498-500







Tgt Ion: 83 Resp: 5683
Ion Ratio Lower Upper
83 100
55 0.0 64.6 97.0#
98 221.8 36.7 55.1#

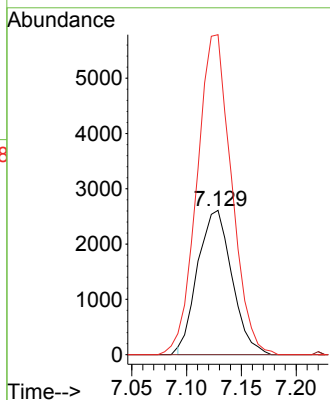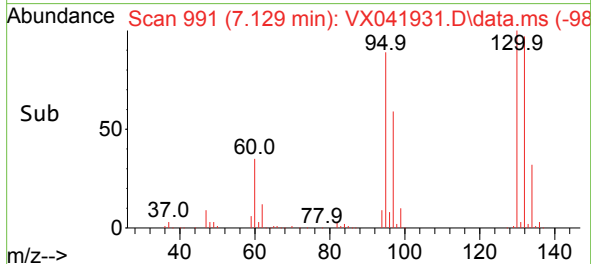

#42
1,2-Dichloroethane
Concen: 0.387 ug/l
RT: 6.098 min Scan# 822
Delta R.T. 0.012 min
Lab File: VX041931.D
Acq: 18 Jun 2024 18:22

Tgt Ion: 62 Resp: 648
Ion Ratio Lower Upper
62 100
98 0.0 0.0 16.0


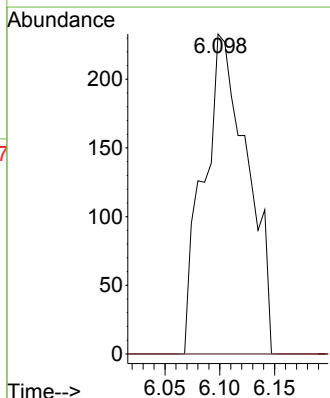
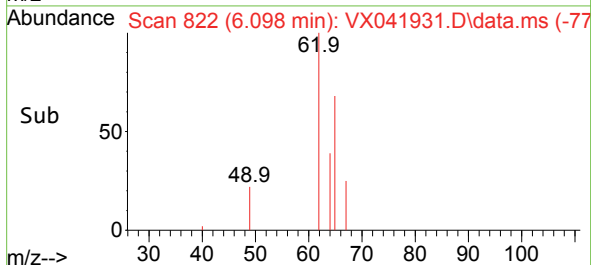



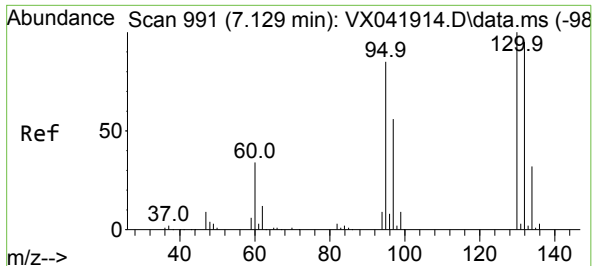

#44
Trichloroethene
Concen: 406.787 ug/l
RT: 7.129 min Scan# 991
Delta R.T. -0.000 min
Lab File: VX041931.D
Acq: 18 Jun 2024 18:22




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-189-GW-498-500


Tgt Ion:130 Resp: 567167
Ion Ratio Lower Upper
130 100
95 89.2 0.0 204.4

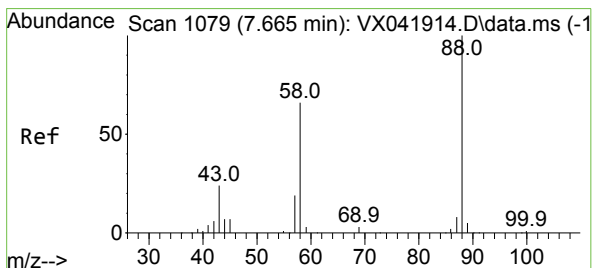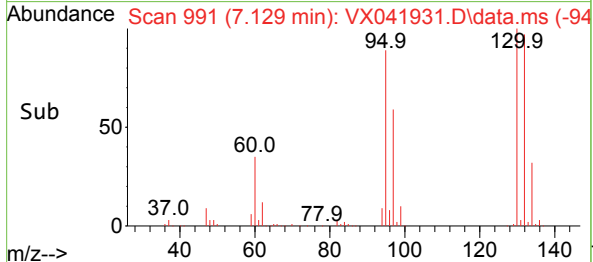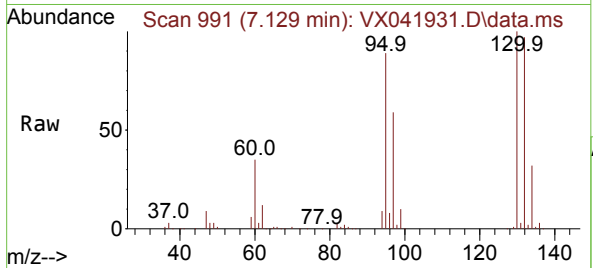

#49
1,4-Dioxane
Concen: 27.457 ug/l
RT: 7.689 min Scan# 1083
Delta R.T. 0.024 min
Lab File: VX041931.D
Acq: 18 Jun 2024 18:22

Tgt Ion: 88 Resp: 299
Ion Ratio Lower Upper
88 100
43 70.2 0.0 0.0#
58 104.7 60.1 90.1#


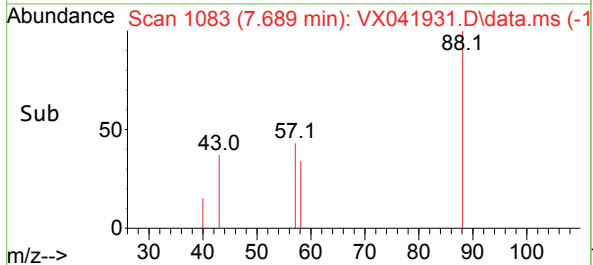

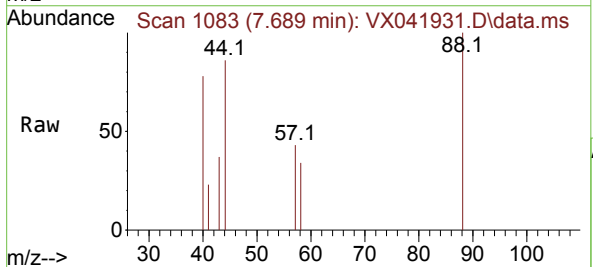




#50
Toluene-d8
Concen: 47.922 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX041931.D
Acq: 18 Jun 2024 18:22




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-189-GW-498-500


Tgt Ion: 98 Resp: 244506
Ion Ratio Lower Upper
98 100
100 66.8 53.1 79.7

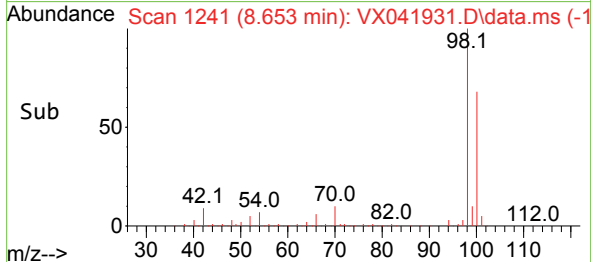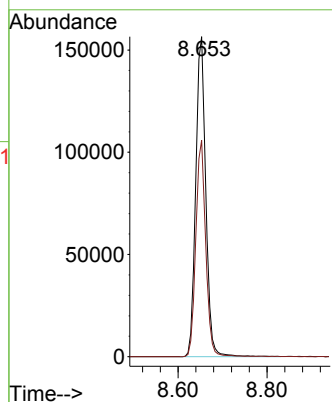

#51
4-Methyl-2-Pentanone
Concen: 0.456 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.067 min
Lab File: VX041931.D
Acq: 18 Jun 2024 18:22

Tgt Ion: 43 Resp: 969
Ion Ratio Lower Upper
43 100
58 185.7 30.4 45.6#



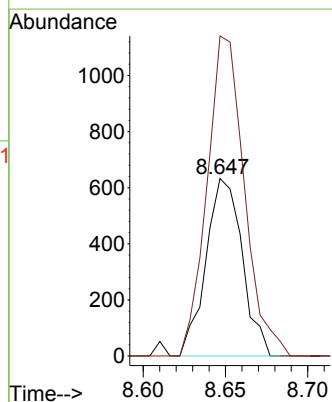
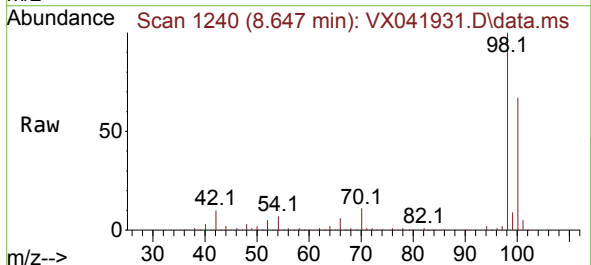




#55
 1,1,2-Trichloroethane
 Concen: 1.298 ug/l
 RT: 9.159 min Scan# 1323
 Delta R.T. 0.006 min
 Lab File: VX041931.D
 Acq: 18 Jun 2024 18:22




Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-189-GW-498-500


Tgt Ion:	97	Resp:	1791
Ion	Ratio	Lower	Upper
97	100		
83	77.7	65.8	98.8
85	48.4	41.6	62.4
99	59.1	47.8	71.8

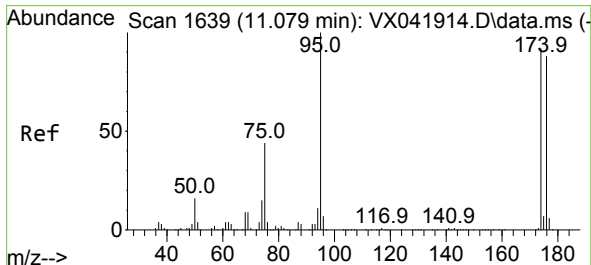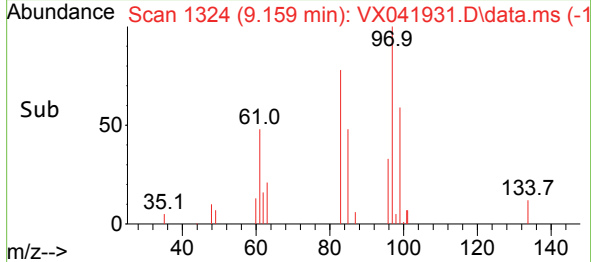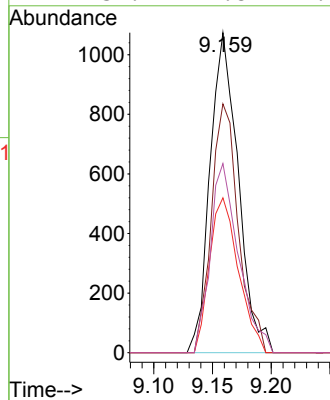

#62
 4-Bromofluorobenzene
 Concen: 49.567 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. -0.000 min
 Lab File: VX041931.D
 Acq: 18 Jun 2024 18:22

Tgt Ion:	95	Resp:	93226
Ion	Ratio	Lower	Upper
95	100		
174	97.2	0.0	135.6
176	94.0	0.0	131.0



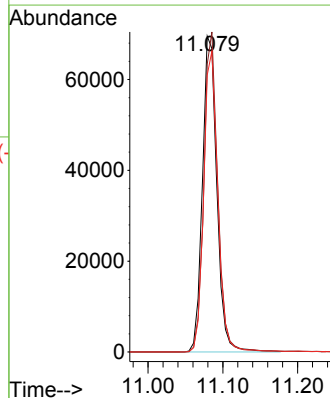
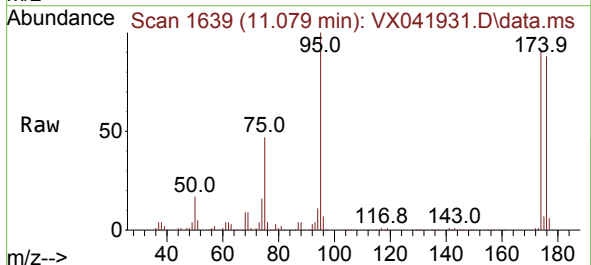




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX041931.D
Acq: 18 Jun 2024 18:22




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-189-GW-498-500


Tgt Ion:117 Resp: 207742
Ion Ratio Lower Upper
117 100
82 50.3 46.2 69.4
119 32.3 25.5 38.3

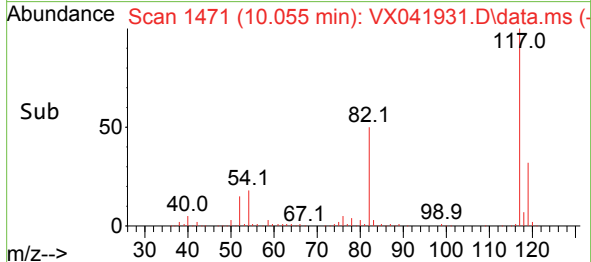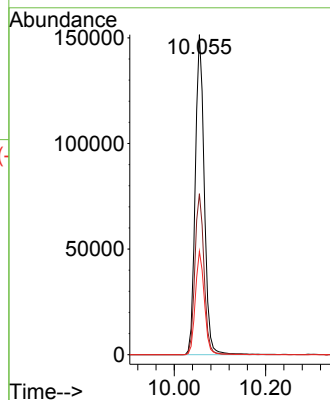

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX041931.D
Acq: 18 Jun 2024 18:22

Tgt Ion:152 Resp: 104564
Ion Ratio Lower Upper
152 100
115 53.4 43.3 129.9
150 158.0 0.0 345.0



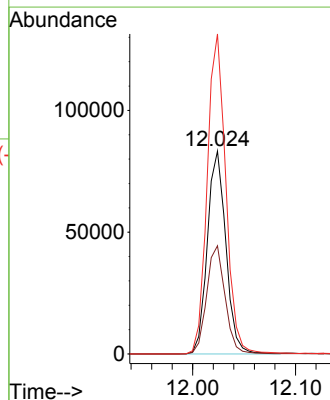
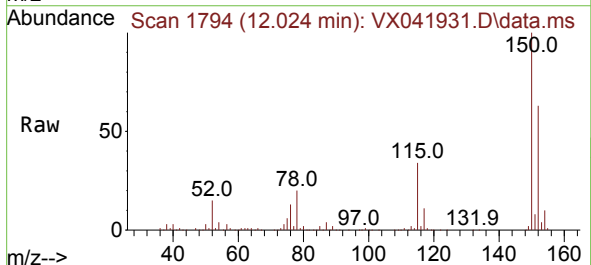




#76
1,2,3-Trichloropropane
Concen: 22.489 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX041931.D
Acq: 18 Jun 2024 18:22




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-189-GW-498-500


Tgt Ion: 75 Resp: 42689
Ion Ratio Lower Upper
75 100
77 1.3 19.1 57.5#

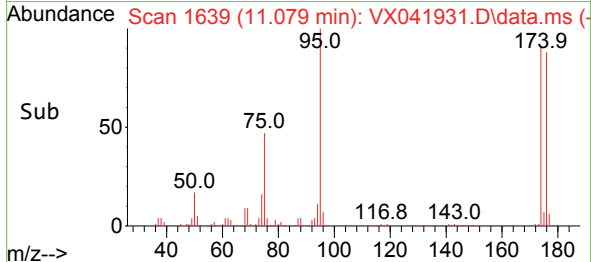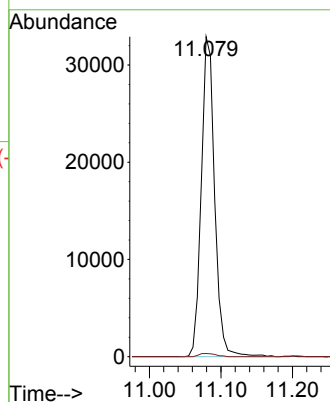

#81
trans-1,4-Dichloro-2-butene
Concen: 63.865 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX041931.D
Acq: 18 Jun 2024 18:22


Tgt Ion: 75 Resp: 42689
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#

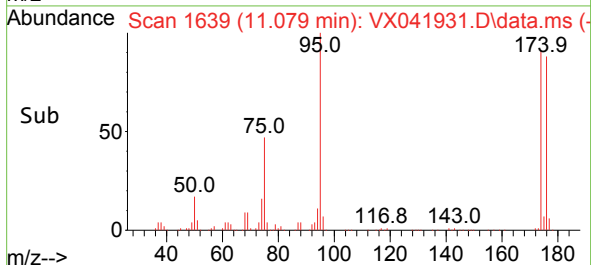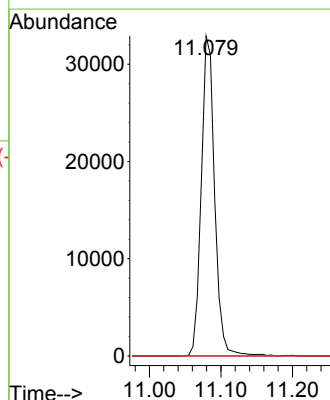



#95
Naphthalene
Concen: 0.801 ug/l
RT: 13.786 min Scan# 2083
Delta R.T. 0.012 min
Lab File: VX041931.D
Acq: 18 Jun 2024 18:22

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-189-GW-498-500



Tgt Ion:128 Resp: 407
Ion Ratio Lower Upper
128 100
127 0.0 10.3 15.5#
129 0.0 8.8 13.2#

