

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061824\
 Data File : VX041929.D
 Acq On : 18 Jun 2024 17:35
 Operator : JC/MD
 Sample : P2927-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-189-DUP-20240614

Quant Time: Jun 19 08:48:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 19 07:57:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	137354	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	212041	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	212571	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	105913	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	68829	43.456	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	86.920%
35) Dibromofluoromethane	5.385	113	65836	43.758	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	87.520%
50) Toluene-d8	8.647	98	250148	47.327	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	94.660%
62) 4-Bromofluorobenzene	11.079	95	94128	48.311	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	96.620%
Target Compounds						
16) Acetone	2.392	43	2895	4.163	ug/l	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061824\
Data File : VX041929.D
Acq On : 18 Jun 2024 17:35
Operator : JC/MD
Sample : P2927-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-189-DUP-20240614

Quant Time: Jun 19 08:48:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 19 07:57:22 2024
Response via : Initial Calibration




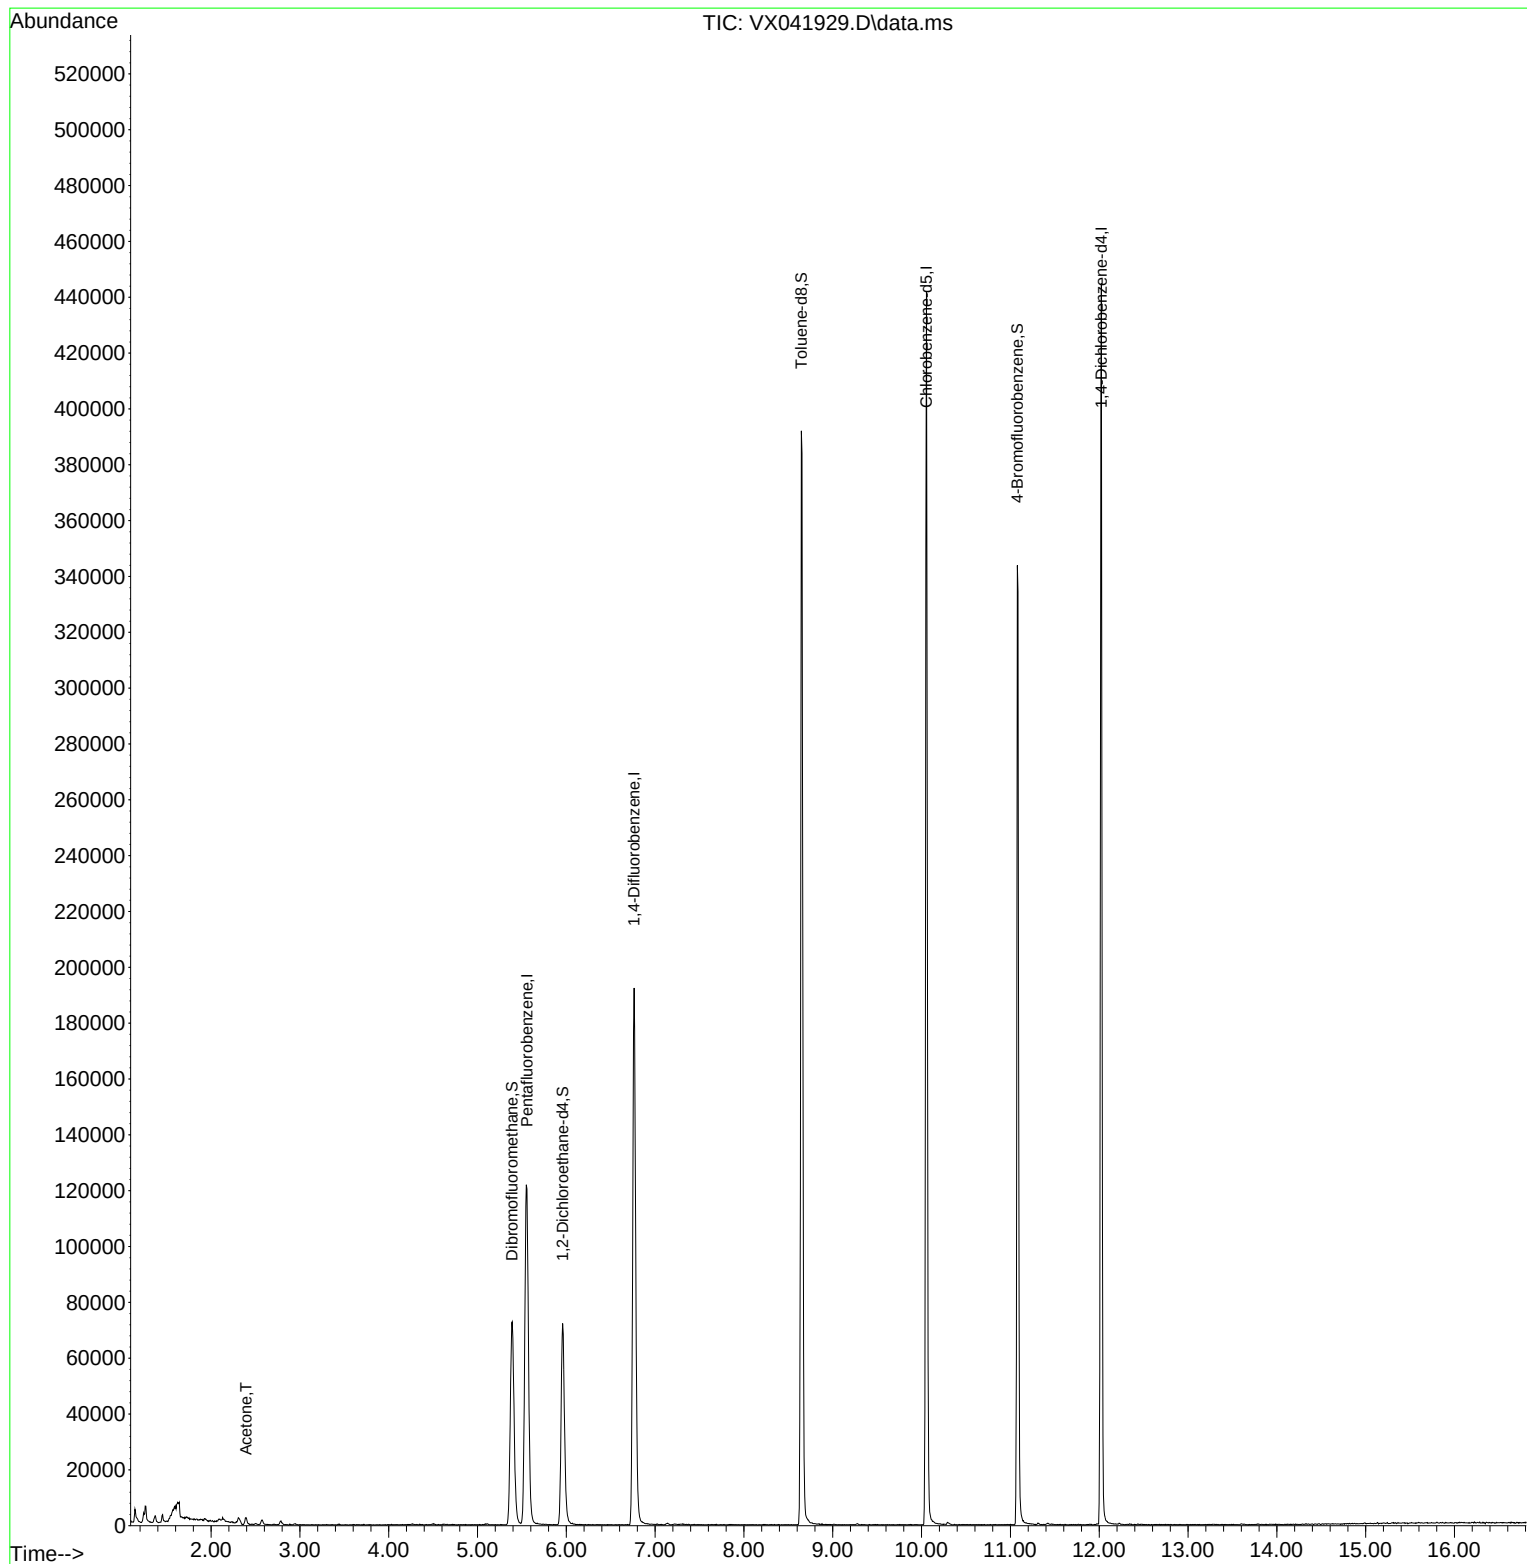


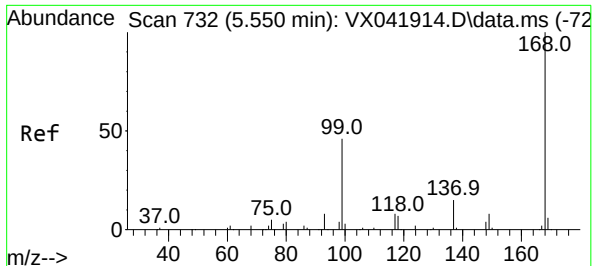

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX041929.D
Acq: 18 Jun 2024 17:35




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-189-DUP-20240614


Tgt Ion:168 Resp: 137354
Ion Ratio Lower Upper
168 100
99 43.6 56.6 85.0#

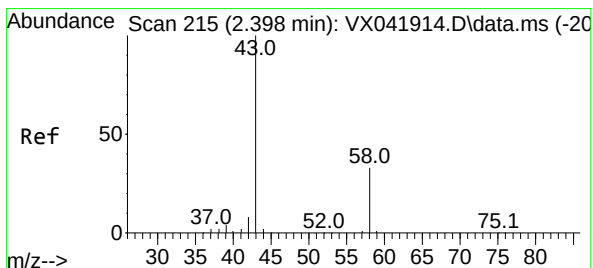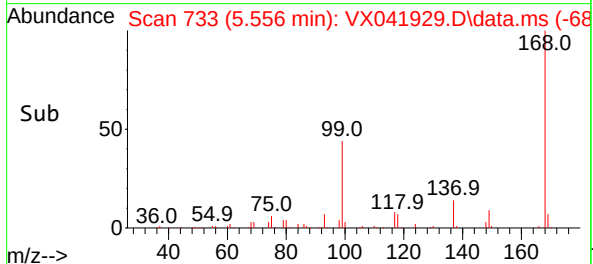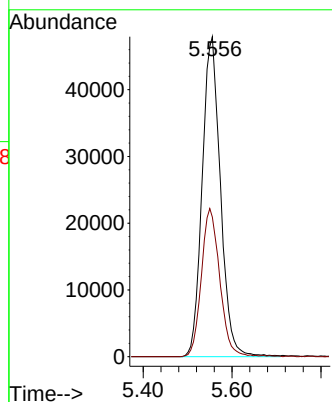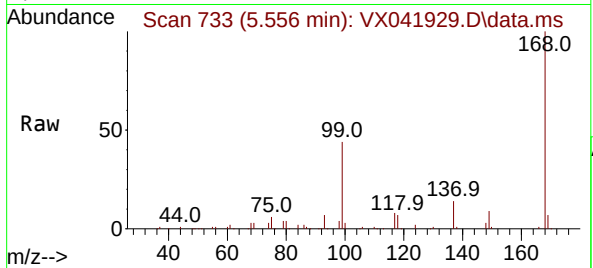

#16
Acetone
Concen: 4.163 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.006 min
Lab File: VX041929.D
Acq: 18 Jun 2024 17:35

Tgt Ion: 43 Resp: 2895
Ion Ratio Lower Upper
43 100
58 32.0 21.9 32.9

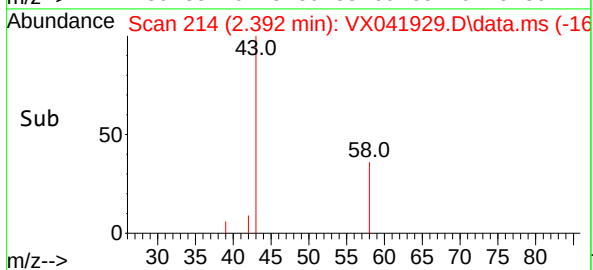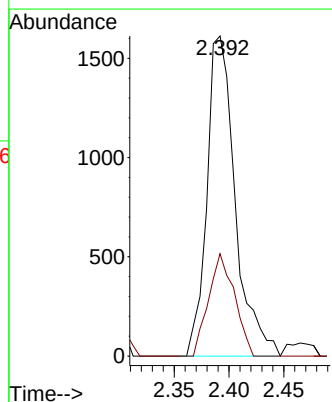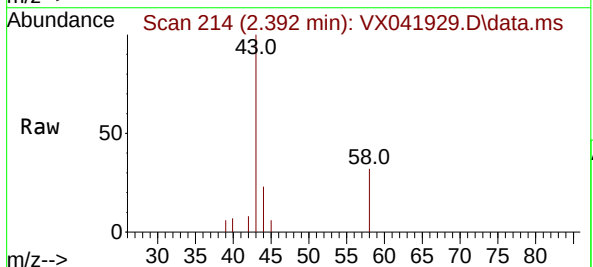

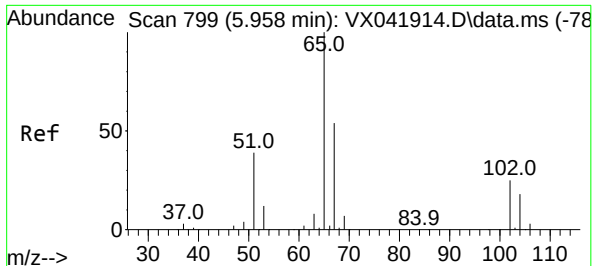

#33

1,2-Dichloroethane-d4

Concen: 43.456 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX041929.D

Acq: 18 Jun 2024 17:35

Instrument :

MSVOA_X

ClientSampleId :





BP-VPB-189-DUP-20240614

Tgt Ion: 65 Resp: 68829

Ion Ratio Lower Upper

65 100

67 53.3 0.0 100.2

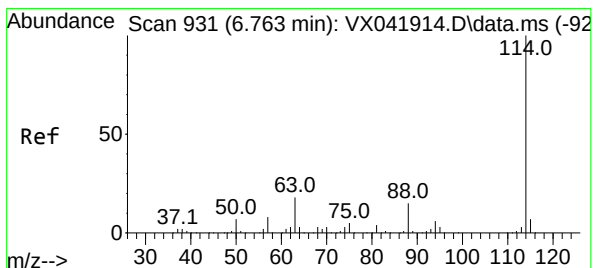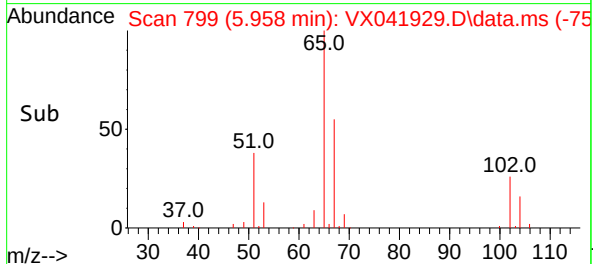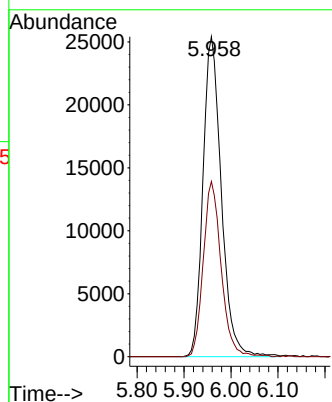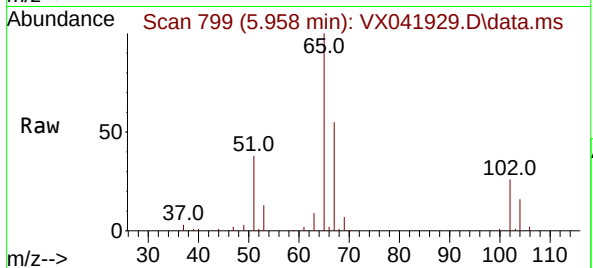

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.000 min

Lab File: VX041929.D

Acq: 18 Jun 2024 17:35




Tgt Ion: 114 Resp: 212041


Ion Ratio Lower Upper

114 100

63 17.9 0.0 45.0

88 15.5 0.0 36.6


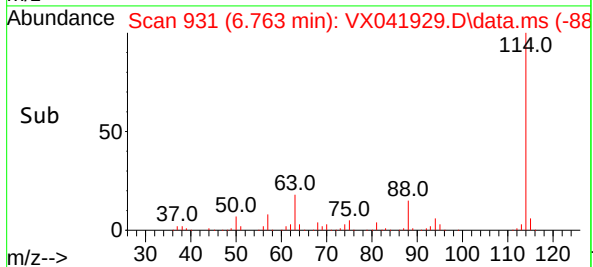
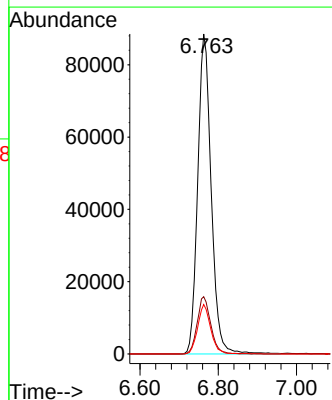
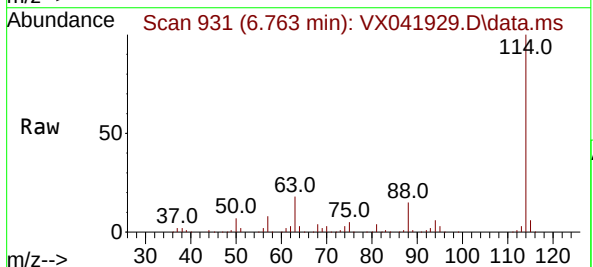


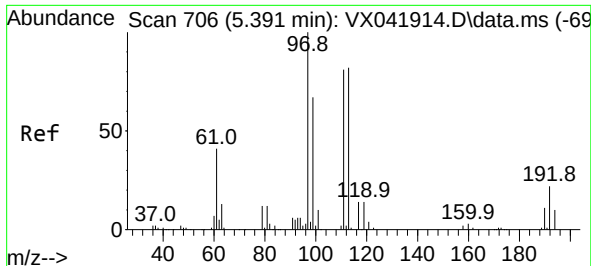

#35
Dibromofluoromethane
Concen: 43.758 ug/l
RT: 5.385 min Scan# 706
Delta R.T. -0.006 min
Lab File: VX041929.D
Acq: 18 Jun 2024 17:35




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-189-DUP-20240614


Tgt Ion:113 Resp: 65836
Ion Ratio Lower Upper
113 100
111 101.7 82.9 124.3
192 25.0 13.3 19.9#

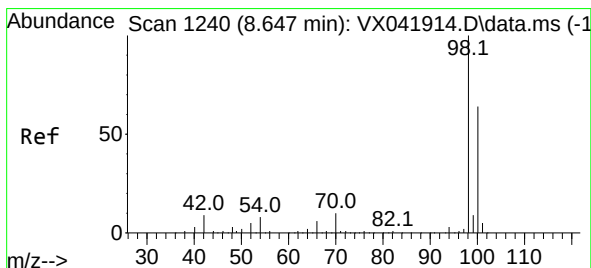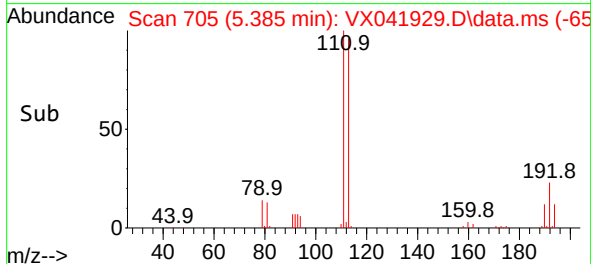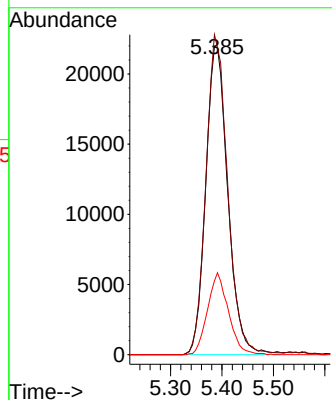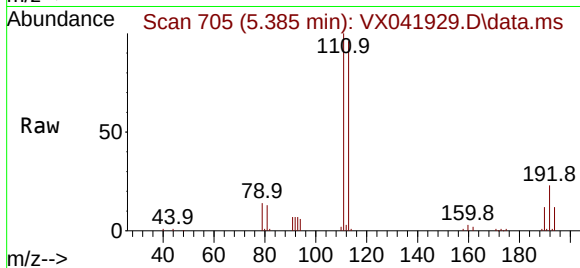

#50
Toluene-d8
Concen: 47.327 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX041929.D
Acq: 18 Jun 2024 17:35

Tgt Ion: 98 Resp: 250148
Ion Ratio Lower Upper
98 100
100 67.1 53.1 79.7


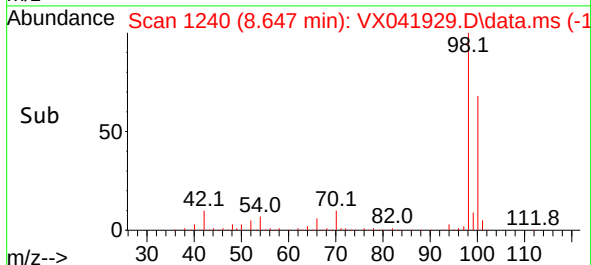
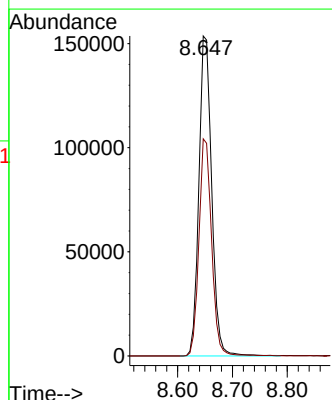
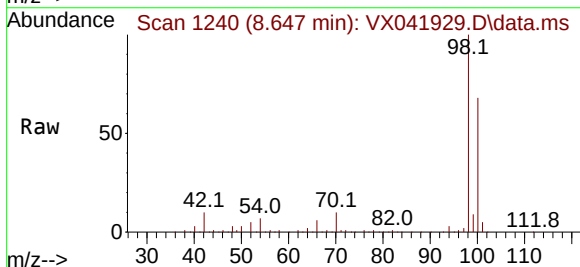


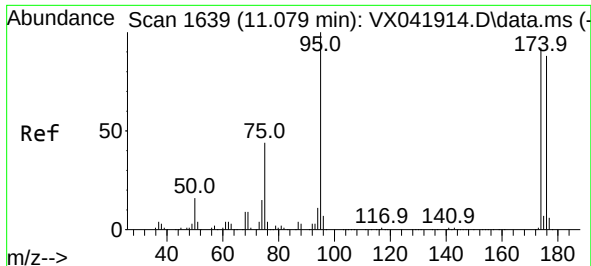

#62
4-Bromofluorobenzene
Concen: 48.311 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX041929.D
Acq: 18 Jun 2024 17:35




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-189-DUP-20240614


Tgt Ion: 95 Resp: 94128
Ion Ratio Lower Upper
95 100
174 98.3 0.0 135.6
176 96.4 0.0 131.0

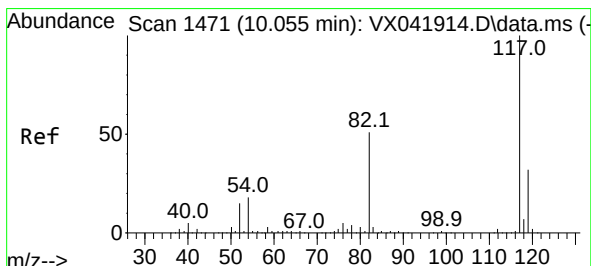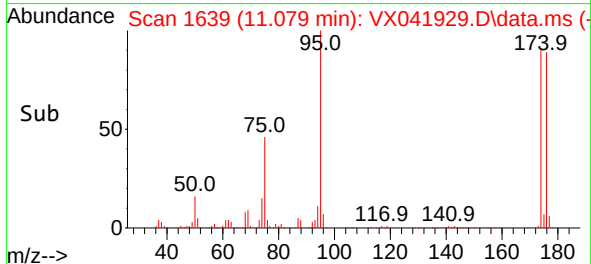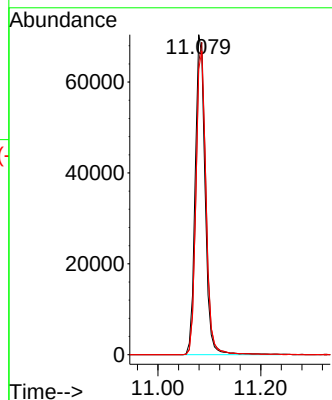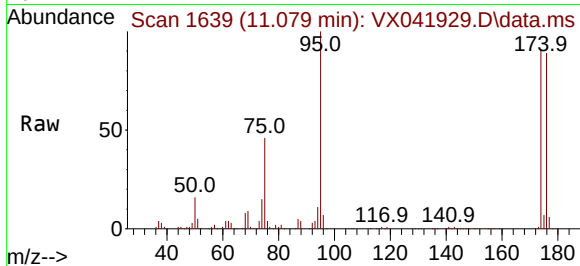

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX041929.D
Acq: 18 Jun 2024 17:35

Tgt Ion: 117 Resp: 212571
Ion Ratio Lower Upper
117 100
82 49.9 46.2 69.4
119 31.3 25.5 38.3

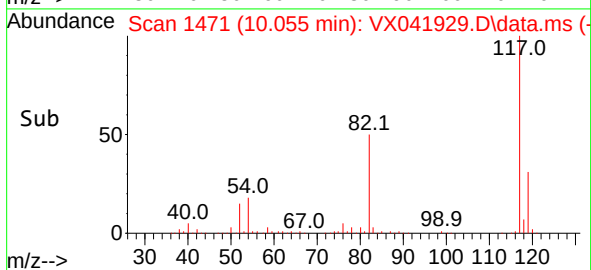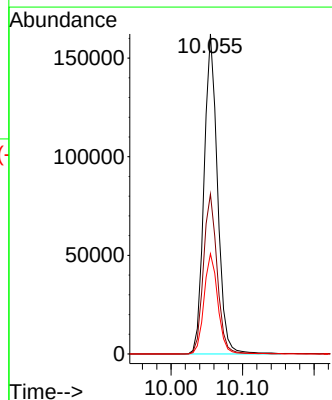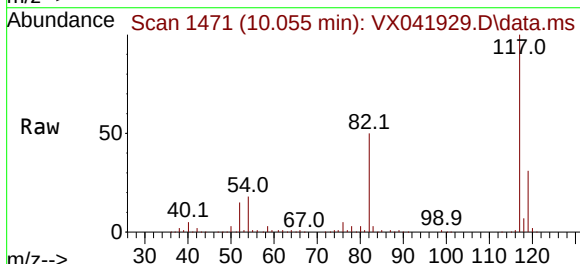

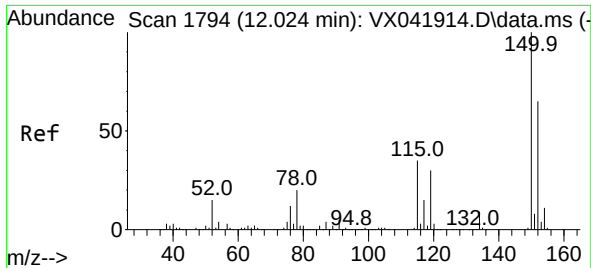

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX041929.D


Acq: 18 Jun 2024 17:35

Instrument :

MSVOA_X

ClientSampleId :

BP-VPB-189-DUP-20240614

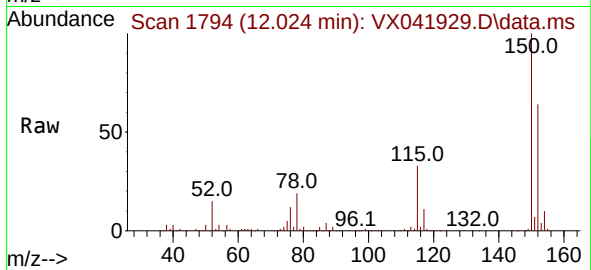

Tgt Ion:152 Resp: 105913

Ion Ratio Lower Upper

152 100

115 53.3 43.3 129.9

150 154.9 0.0 345.0

