

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061825\
 Data File : VX046751.D
 Acq On : 18 Jun 2025 18:16
 Operator : JC/MD
 Sample : Q2344-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-4

Quant Time: Jun 19 01:28:34 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 18 03:09:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	192926	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	318077	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	278709	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	130790	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	124150	46.524	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	93.040%
35) Dibromofluoromethane	5.397	113	102626	48.765	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.540%
50) Toluene-d8	8.647	98	374699	49.557	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	99.120%
62) 4-Bromofluorobenzene	11.079	95	135286	48.000	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	96.000%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061825\
Data File : VX046751.D
Acq On : 18 Jun 2025 18:16
Operator : JC/MD
Sample : Q2344-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-4

Quant Time: Jun 19 01:28:34 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 18 03:09:16 2025
Response via : Initial Calibration




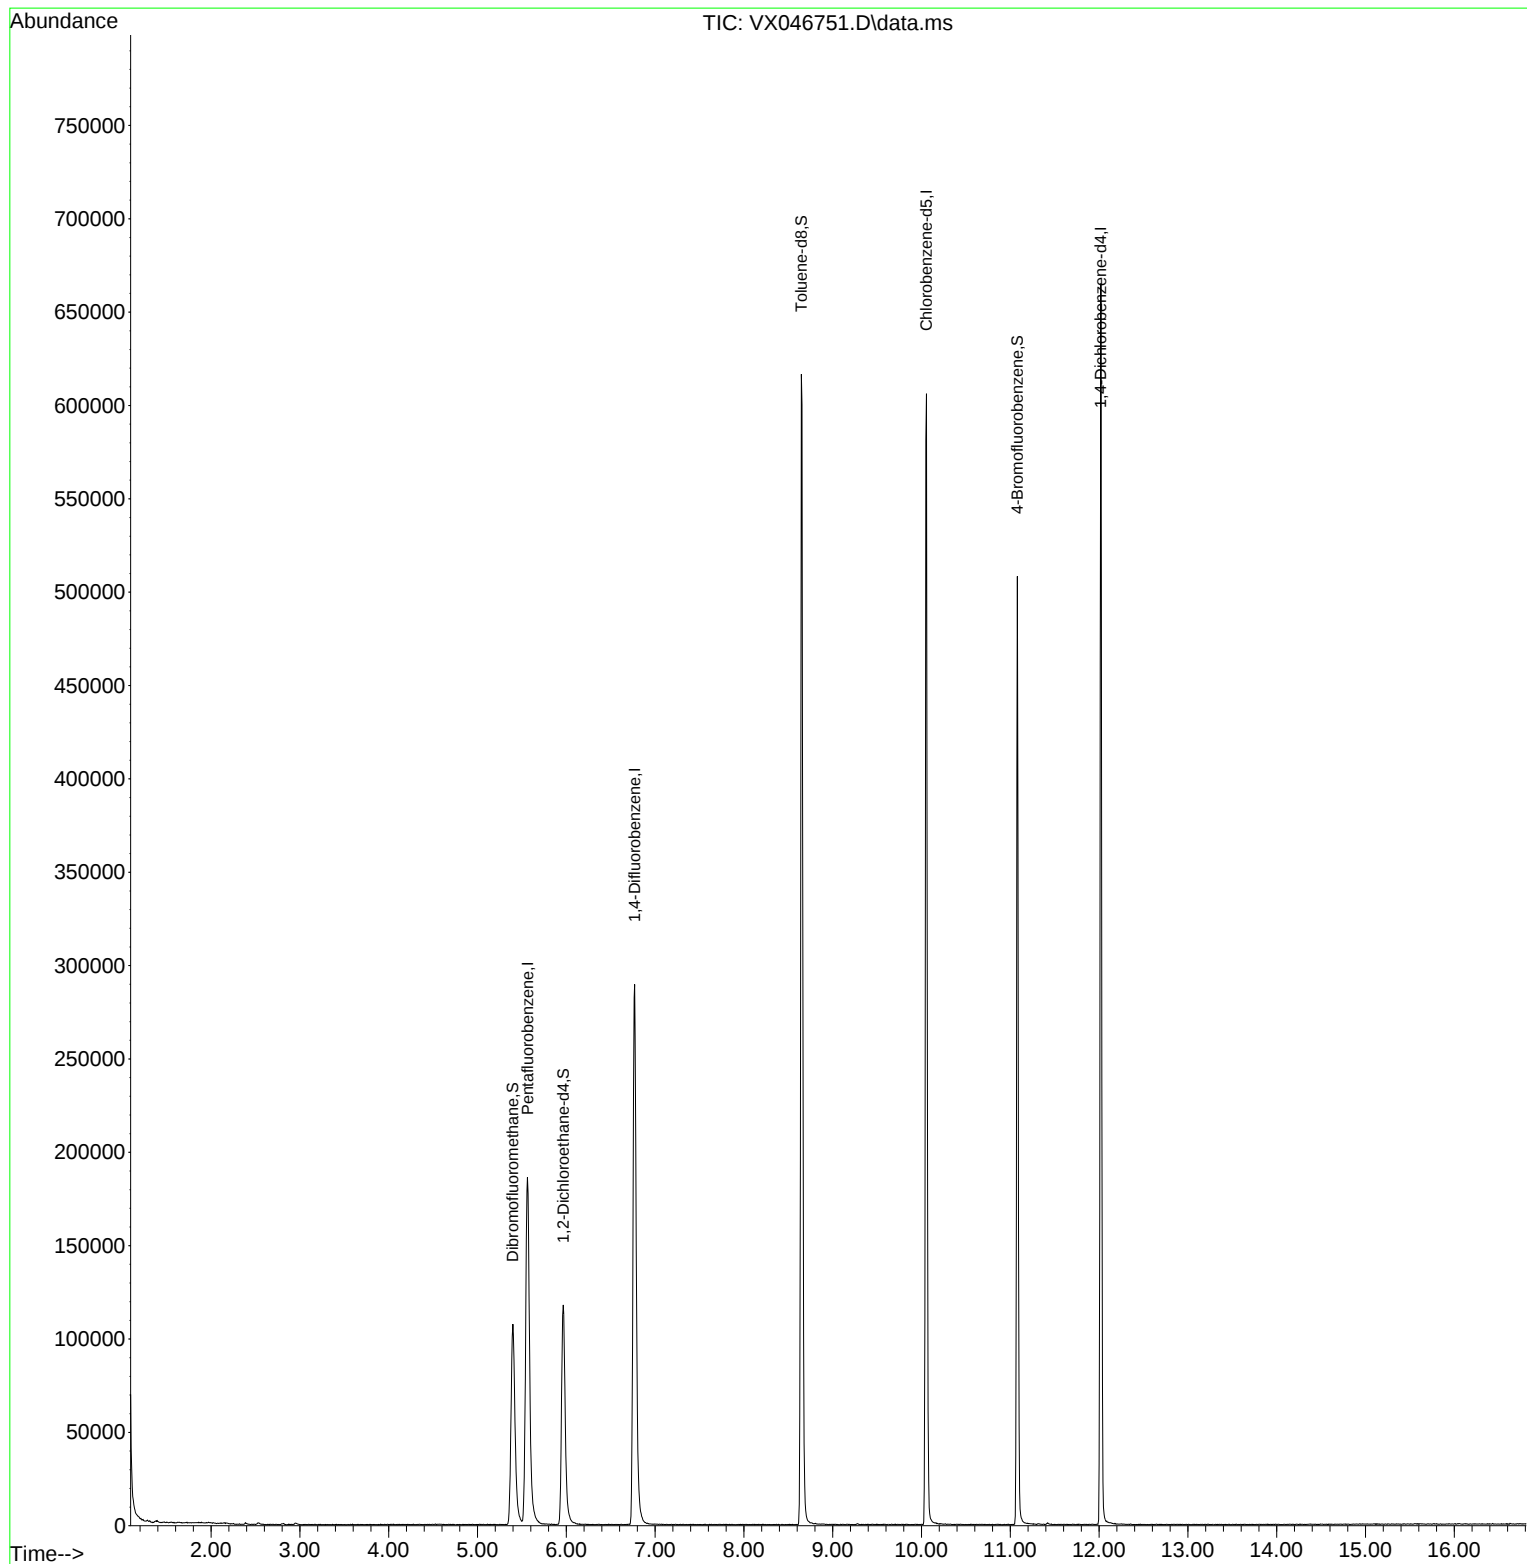


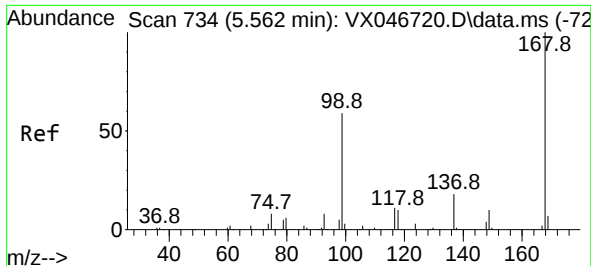

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.000 min
Lab File: VX046751.D
Acq: 18 Jun 2025 18:16




Instrument :
MSVOA_X
ClientSampleId :
MW-4


Tgt Ion:168 Resp: 192926
Ion Ratio Lower Upper
168 100
99 60.3 48.5 72.7

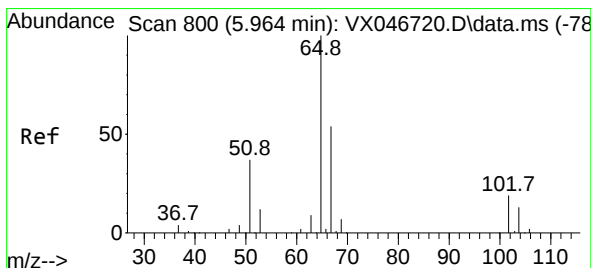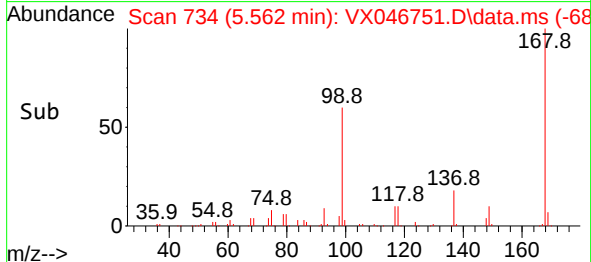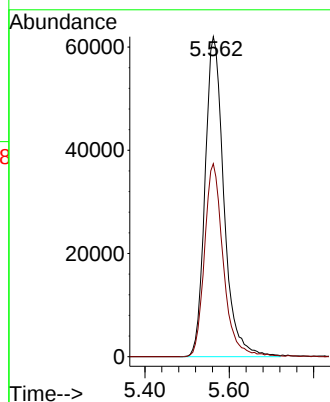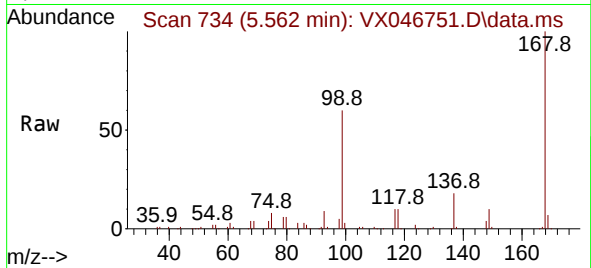

#33
1,2-Dichloroethane-d4
Concen: 46.524 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX046751.D
Acq: 18 Jun 2025 18:16

Tgt Ion: 65 Resp: 124150
Ion Ratio Lower Upper
65 100
67 52.8 0.0 105.4


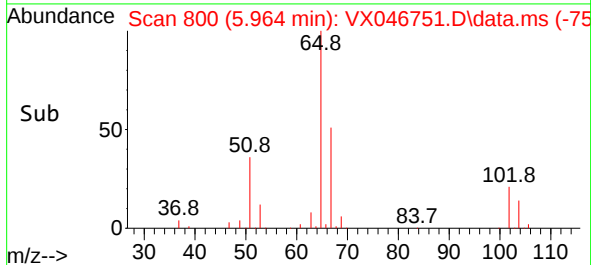
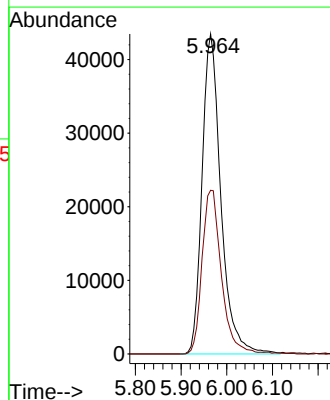
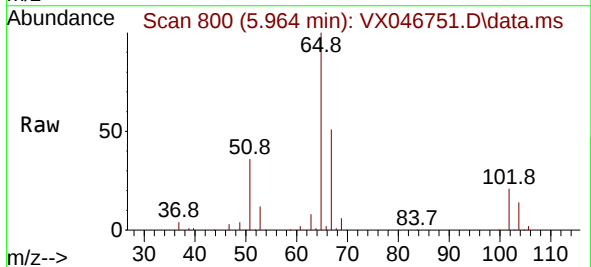


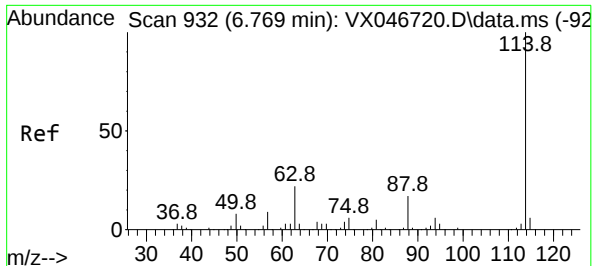

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX046751.D
Acq: 18 Jun 2025 18:16




Instrument :
MSVOA_X
ClientSampleId :
MW-4


Tgt Ion:114 Resp: 318077
Ion Ratio Lower Upper
114 100
63 20.9 0.0 44.2
88 16.6 0.0 33.2

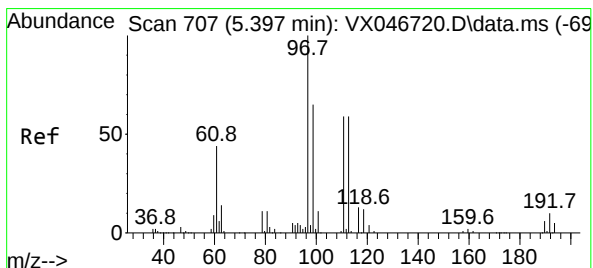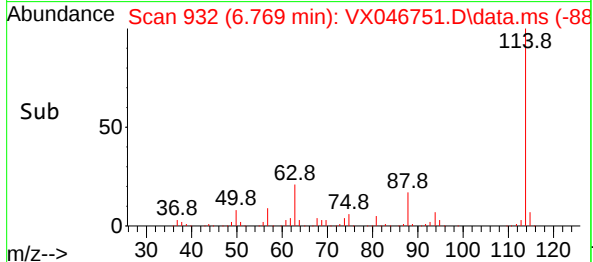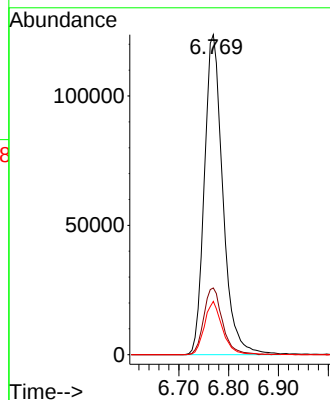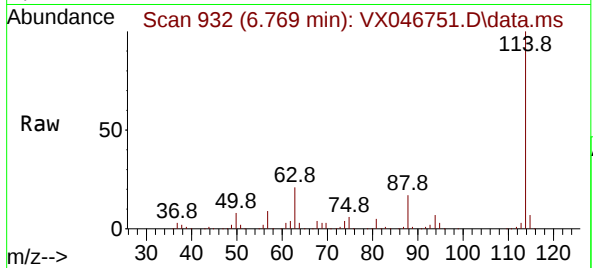

#35
Dibromofluoromethane
Concen: 48.765 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX046751.D
Acq: 18 Jun 2025 18:16

Tgt Ion:113 Resp: 102626
Ion Ratio Lower Upper
113 100
111 103.7 82.0 123.0
192 19.3 15.3 22.9


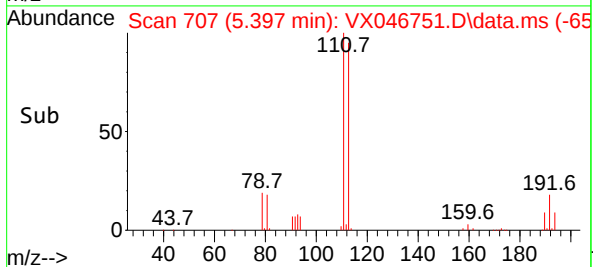
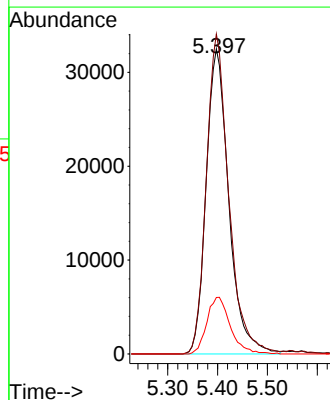
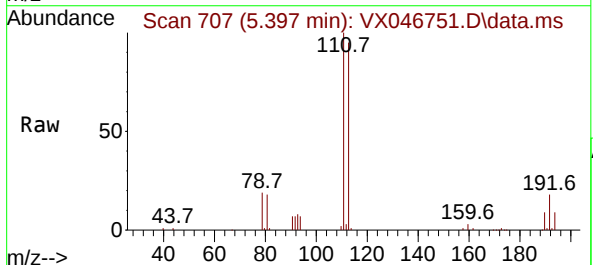


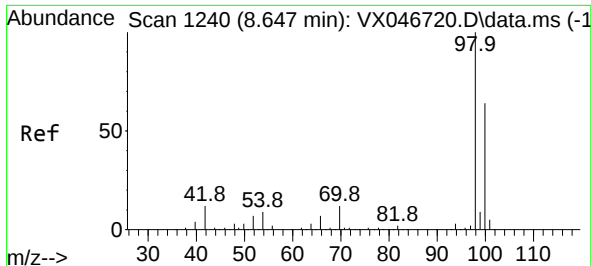

#50
Toluene-d8
Concen: 49.557 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX046751.D
Acq: 18 Jun 2025 18:16




Instrument :
MSVOA_X
ClientSampleId :
MW-4


Tgt Ion: 98 Resp: 374699
Ion Ratio Lower Upper
98 100
100 66.9 53.0 79.4

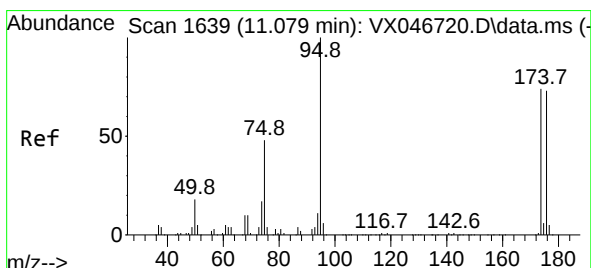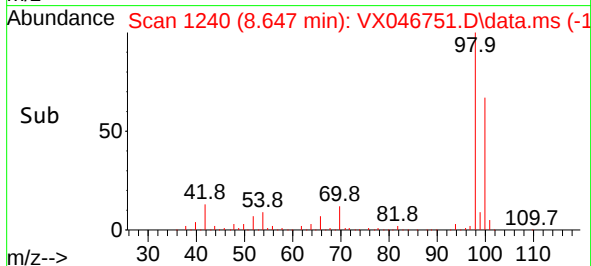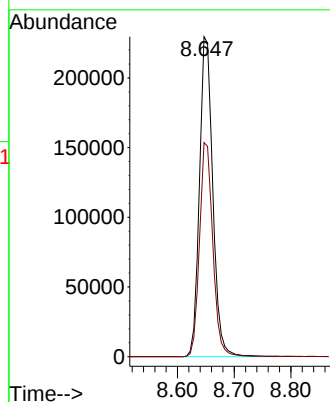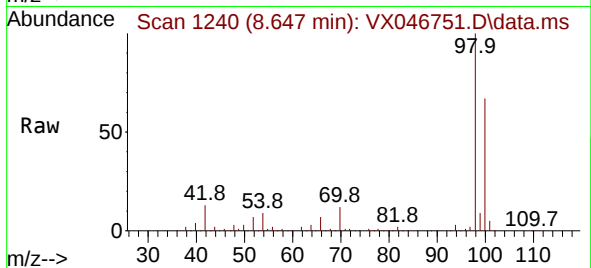

#62
4-Bromofluorobenzene
Concen: 48.000 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX046751.D
Acq: 18 Jun 2025 18:16

Tgt Ion: 95 Resp: 135286
Ion Ratio Lower Upper
95 100
174 75.6 0.0 150.4
176 71.6 0.0 145.0


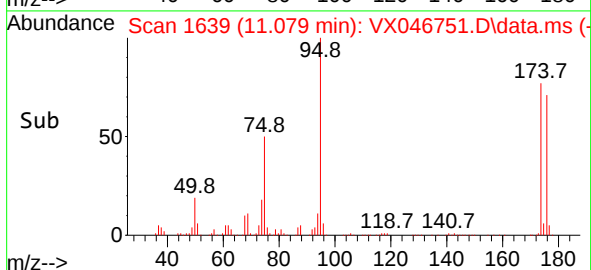
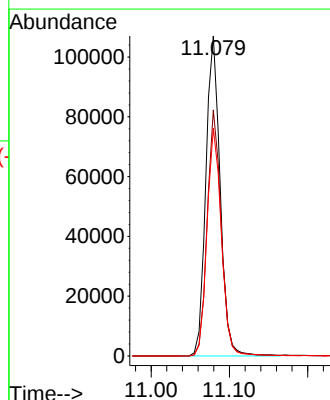
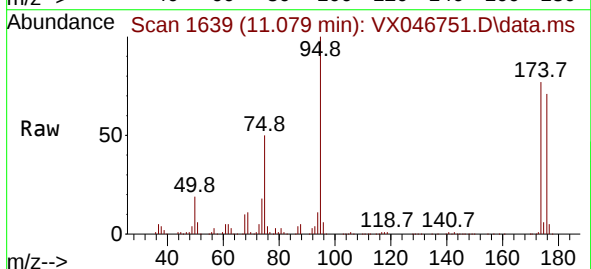


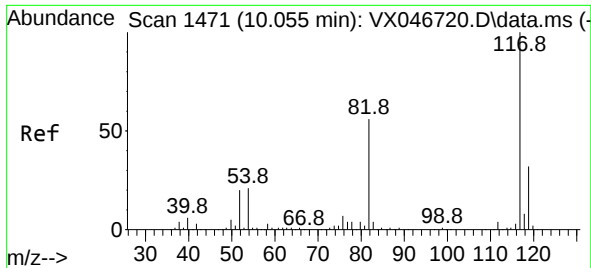

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX046751.D
Acq: 18 Jun 2025 18:16

Instrument :
MSVOA_X
ClientSampleId :
MW-4

Tgt Ion:117 Resp: 278709
Ion Ratio Lower Upper
117 100
82 55.2 44.6 66.8
119 31.9 25.8 38.8

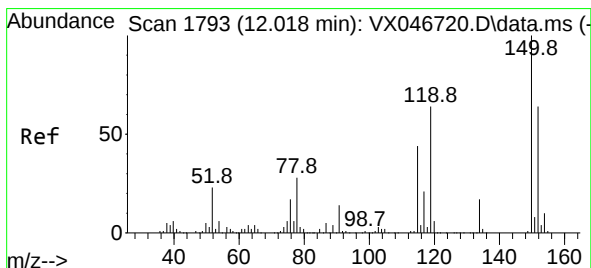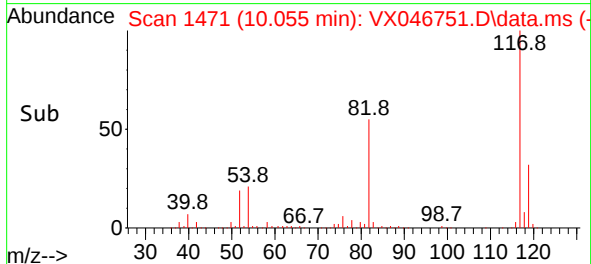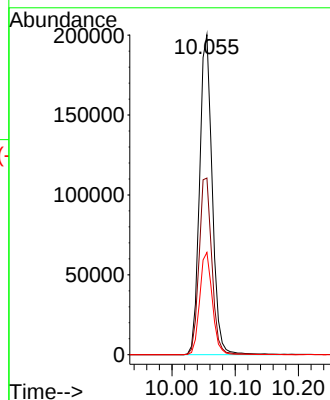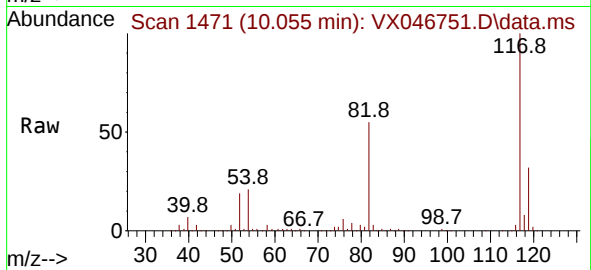

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX046751.D
Acq: 18 Jun 2025 18:16

Tgt Ion:152 Resp: 130790
Ion Ratio Lower Upper
152 100
115 61.2 43.2 129.6
150 160.8 0.0 346.8

