


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX061919\
Data File : VX010342.D
Acq On : 19 Jun 2019 11:43
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Title : SW846 8260
Last Update : Thu Jun 20 03:31:56 2019

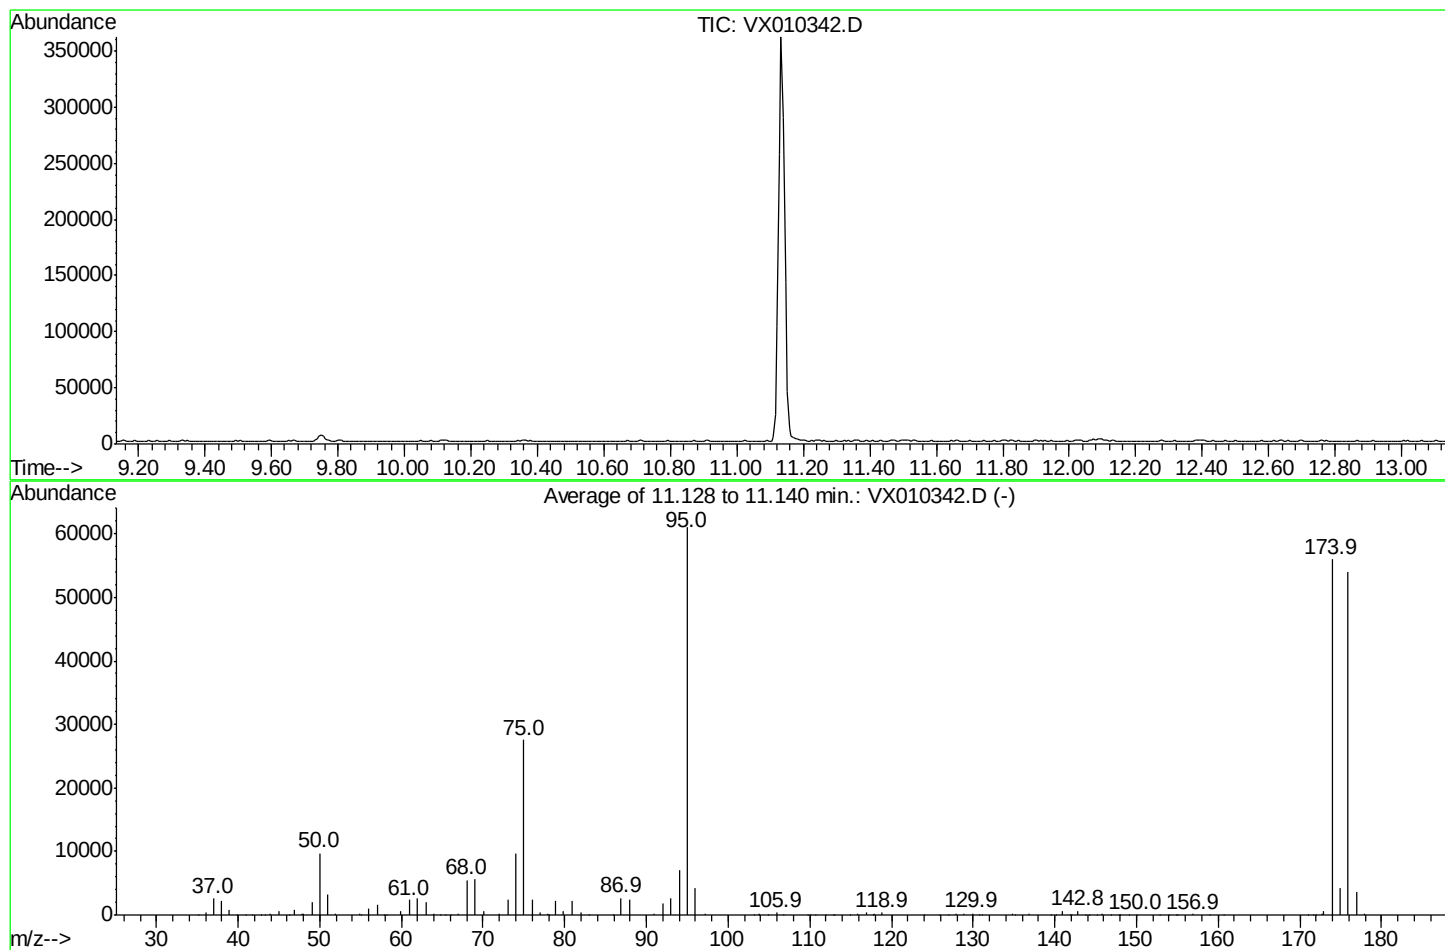

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	9745	PASS
75	95	30	60	45.2	27565	PASS
95	95	100	100	100.0	61021	PASS
96	95	5	9	7.0	4275	PASS
173	174	0.00	2	1.1	640	PASS
174	95	50	100	91.7	55976	PASS
175	174	5	9	7.4	4158	PASS
176	174	95	101	96.5	54042	PASS
177	176	5	9	6.6	3542	PASS