

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX061920\
 Data File : VX016903.D
 Acq On : 20 Jun 2020 03:14
 Operator : JC/SP
 Sample : L3063-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TW-1

Quant Time: Jun 22 01:50:18 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061820W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 19 12:07:48 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.64	168	279850	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	492125	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	456481	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	266052	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.03	65	148241	44.04	ug/l	0.00
Spiked Amount			Recovery	=	88.08%	
35) Dibromofluoromethane	5.47	113	137107	43.55	ug/l	0.00
Spiked Amount			Recovery	=	87.10%	
50) Toluene-d8	8.70	98	560675	44.51	ug/l	0.00
Spiked Amount			Recovery	=	89.02%	
62) 4-Bromofluorobenzene	11.12	95	231538	47.98	ug/l	0.00
Spiked Amount			Recovery	=	95.96%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.31	50	994	0.285	ug/l #	87
5) Bromomethane	1.64	94	601	0.254	ug/l #	79
6) Chloroethane	1.53	64	391583	161.994	ug/l #	52
10) Methyl Iodide	2.50	142	1143	0.411	ug/l #	87
11) Tert butyl alcohol	3.01	59	1202	2.113	ug/l #	72
13) Acrolein	2.25	56	2393	6.937	ug/l #	1
14) Allyl chloride	2.82	41	174220	44.042	ug/l #	60
15) Acrylonitrile	3.15	53	23456	17.990	ug/l #	41
16) Acetone	2.37	43	204562	167.426	ug/l #	50
17) Carbon Disulfide	2.56	76	21945	2.839	ug/l	100
18) Methyl Acetate	2.82	43	478215	153.920	ug/l #	48
19) Methyl tert-butyl Ether	3.17	73	4252	0.499	ug/l #	1
20) Methylene Chloride	2.82	84	1570	0.536	ug/l #	1
21) trans-1,2-Dichloroethene	3.14	96	570	0.202	ug/l #	45
23) Vinyl Acetate	3.79	43	4661	0.746	ug/l #	77
25) 2-Butanone	4.64	43	17871	10.628	ug/l	99
29) Tetrahydrofuran	5.03	42	2637	2.490	ug/l #	28
30) Chloroform	5.25	83	95923	19.192	ug/l #	26
31) Cyclohexane	5.57	56	184356	44.294	ug/l #	55
37) Ethyl Acetate	4.86	43	3366	0.838	ug/l #	27
38) Carbon Tetrachloride	5.63	117	26042	5.108	ug/l #	16
39) Methylcyclohexane	7.44	83	363729	68.843	ug/l	97
40) Benzene	6.12	78	5701	0.418	ug/l	100
41) Methacrylonitrile	5.03	41	20367	9.344	ug/l #	52
43) Isopropyl Acetate	6.43	43	26551	3.787	ug/l #	59
45) 1,2-Dichloropropane	7.44	63	4722	1.378	ug/l #	1
46) Dibromomethane	7.62	93	2111	0.908	ug/l #	1
47) Bromodichloromethane	7.93	83	57239	11.578	ug/l #	26
48) Methyl methacrylate	7.76	41	20822	6.307	ug/l #	87
51) 4-Methyl-2-Pentanone	8.62	43	10747	2.549	ug/l	100
52) Toluene	8.77	92	14832	1.640	ug/l	98
55) 1,1,2-Trichloroethane	9.15	97	63558	18.611	ug/l #	20
56) Ethyl methacrylate	9.17	69	26530	5.366	ug/l #	27
58) 2-Chloroethyl Vinyl ether	8.24	63	1886	0.820	ug/l #	42

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX061920\
 Data File : VX016903.D
 Acq On : 20 Jun 2020 03:14
 Operator : JC/SP
 Sample : L3063-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 36 Sample Multiplier: 1


Instrument :
 MSVOA_X
 ClientSampleId :
 TW-1

Quant Time: Jun 22 01:50:18 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061820W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 19 12:07:48 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)

59) 2-Hexanone	9.48	43	11915	3.902	ug/l	94
67) Ethyl Benzene	10.24	91	1279924	82.066	ug/l	99
68) m/p-Xylenes	10.34	106	1056514	174.084	ug/l	99
69) o-Xylene	10.68	106	48383	8.622	ug/l	98
70) Styrene	10.68	104	3439	0.361	ug/l #	1
73) Isopropylbenzene	11.00	105	1270785	74.185	ug/l	100
74) N-amyl acetate	10.89	43	1224	0.205	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	11.26	83	1234	0.255	ug/l #	55
76) 1,2,3-Trichloropropane	11.34	75	9300	1.914	ug/l #	1
78) n-propylbenzene	11.34	91	1537918	80.446	ug/l	100
79) 2-Chlorotoluene	11.42	91	305575	26.125	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.49	105	1523549	103.084	ug/l	99
81) trans-1,4-Dichloro-2-buten	11.00	75	13737	6.923	ug/l #	50
82) 4-Chlorotoluene	11.49	91	156157	11.128	ug/l #	46
83) tert-Butylbenzene	11.79	119	531650	36.356	ug/l #	62
84) 1,2,4-Trimethylbenzene	11.79	105	4143017	272.126	ug/l	97
85) sec-Butylbenzene	11.93	105	537770	31.664	ug/l	91
86) p-Isopropyltoluene	12.05	119	149876	9.632	ug/l	99
87) 1,3-Dichlorobenzene	12.01	146	1833	0.215	ug/l #	84
88) 1,4-Dichlorobenzene	12.01	146	1833	0.212	ug/l	93
89) n-Butylbenzene	12.37	91	1415463	106.077	ug/l #	28
90) Hexachloroethane	12.57	117	160768	57.355	ug/l #	5
92) 1,2-Dibromo-3-Chloropropan	13.00	75	12916	11.262	ug/l #	1
93) 1,2,4-Trichlorobenzene	13.63	180	3187	0.576	ug/l #	1
94) Hexachlorobutadiene	13.77	225	1890	0.757	ug/l	93
95) Naphthalene	13.82	128	290735	17.898	ug/l	98
96) 1,2,3-Trichlorobenzene	14.00	180	2626	0.476	ug/l #	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.64 min Scan# 746

Delta R.T. 0.01 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampleId :


TW-1

Tot Ion:168 Resp: 279850

Ion Ratio Lower Upper

168 100

99 50.6 42.2 63.2



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.64

100000

80000



60000

40000

20000

0

Time-->



#3

Chloromethane

Concen: 0.285 ug/l

RT: 1.31 min Scan# 37

Delta R.T. 0.00 min

Lab File: VX016903.D


Acq: 20 Jun 2020 03:14

Tgt Ion: 50 Resp: 994

Ion Ratio Lower Upper

50 100

52 25.3 26.1 39.1#



Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

1.31

800


600


400

200

0

Time-->





#5

Bromomethane

Concen: 0.254 ug/l

RT: 1.64 min Scan# 91

Delta R.T. 0.02 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampleId :





TW-1

Tot Ion: 94 Resp: 601

Ion Ratio Lower Upper

94 100

96 72.4 74.4 111.6#

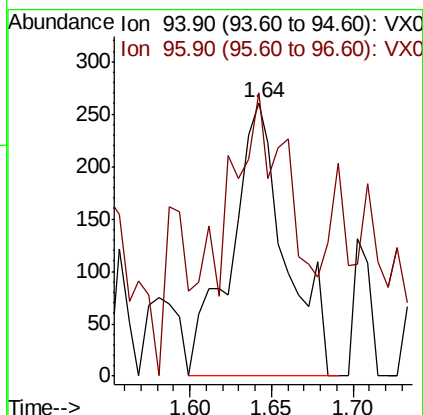

#6

Chloroethane

Concen: 161.994 ug/l

RT: 1.53 min Scan# 73

Delta R.T. -0.18 min

Lab File: VX016903.D




Acq: 20 Jun 2020 03:14


Tgt Ion: 64 Resp: 391583

Ion Ratio Lower Upper

64 100

66 5.4 25.7 38.5#









#10
Methvl Iodide
Concen: 0.411 ug/l
RT: 2.50 min Scan# 231
Delta R.T. 0.01 min
Lab File: VX016903.D
Acq: 20 Jun 2020 03:14




Instrument :
MSVOA_X
ClientSampled :
TW-1


Tot Ion:142 Resp: 1143
Ion Ratio Lower Upper
142 100
127 35.8 35.1 52.7
141 9.3 11.6 17.4#

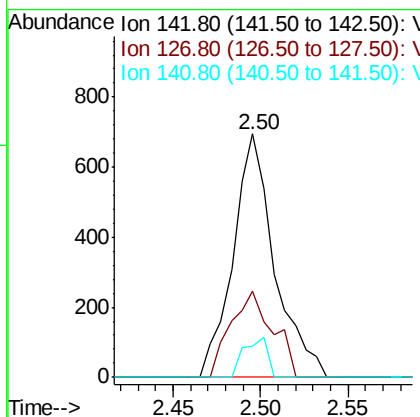

#11
Tert butyl alcohol
Concen: 2.113 ug/l
RT: 3.01 min Scan# 316
Delta R.T. 0.01 min
Lab File: VX016903.D
Acq: 20 Jun 2020 03:14

Tgt Ion: 59 Resp: 1202
Ion Ratio Lower Upper
59 100
57 0.0 8.4 12.6#

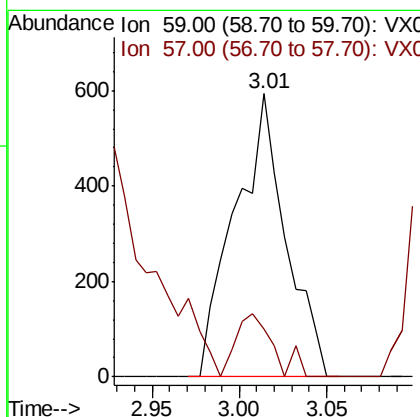



#13

Acrolein

Concen: 6.937 ug/l

RT: 2.25 min Scan# 191

Delta R.T. -0.02 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampled :





TW-1

Tot Ion: 56 Resp: 2393

Ion Ratio Lower Upper

56 100

55 1783.4 55.7 83.5#

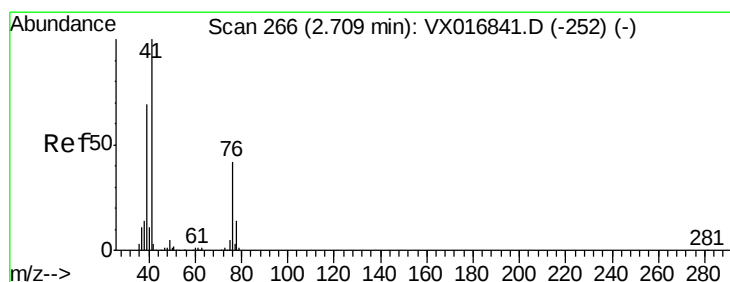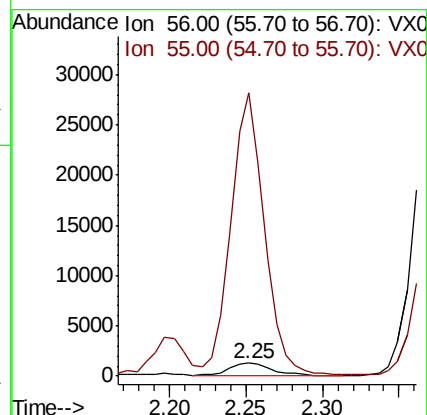

#14

Allyl chloride

Concen: 44.042 ug/l

RT: 2.82 min Scan# 285

Delta R.T. 0.12 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14




Tgt Ion: 41 Resp: 174220


Ion Ratio Lower Upper

41 100

39 43.3 50.7 76.1#

76 0.0 30.9 46.3#

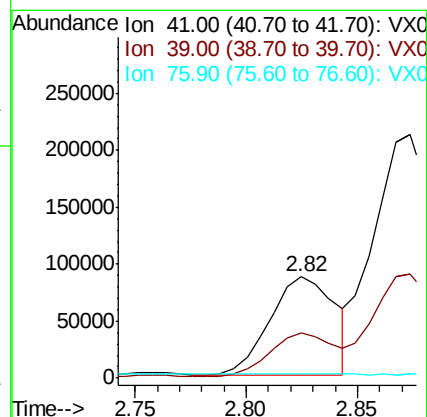



#15

Acrylonitrile

Concen: 17.990 ug/l

RT: 3.15 min Scan# 339

Delta R.T. 0.04 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampleId :

TW-1


Tot Ion: 53 Resp: 23456

Ion Ratio Lower Upper

53 100

52 21.0 66.2 99.2#




51 57.9 28.7 43.1#



Abundance Ion 53.00 (52.70 to 53.70): VX0

Ion 52.00 (51.70 to 52.70): VX0

Ion 51.00 (50.70 to 51.70): VX0

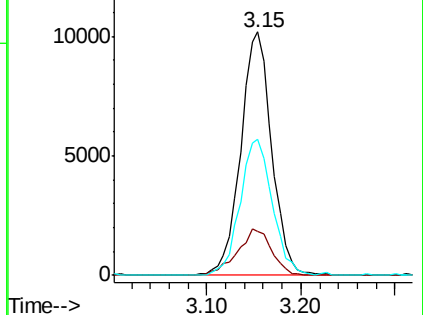

#16

Acetone

Concen: 167.426 ug/l

RT: 2.37 min Scan# 211

Delta R.T. -0.04 min

Lab File: VX016903.D


Acq: 20 Jun 2020 03:14

Tgt Ion: 43 Resp: 204562

Ion Ratio Lower Upper



43 100


58 5.0 26.6 39.8#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

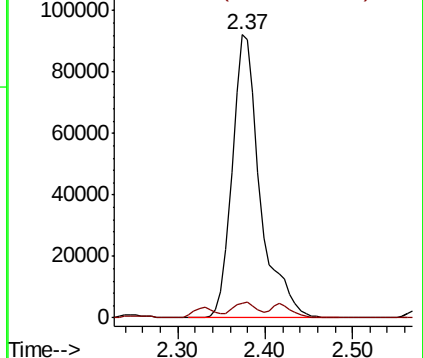



#17

Carbon Disulfide

Concen: 2.839 ug/l

RT: 2.56 min Scan# 241

Delta R.T. 0.01 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampleId :


TW-1

Tot Ion: 76 Resp: 21945

Ion Ratio Lower Upper

76 100

78 9.2 7.5 11.3



Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

12000

10000

8000

6000



4000

2000

0

2.50 2.55 2.60

Time-->



#18

Methyl Acetate

Concen: 153.920 ug/l

RT: 2.82 min Scan# 285

Delta R.T. 0.08 min

Lab File: VX016903.D


Acq: 20 Jun 2020 03:14

Tgt Ion: 43 Resp: 478215

Ion Ratio Lower Upper

43 100

74 0.0 21.8 32.8#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 74.00 (73.70 to 74.70): VX0

600000

500000

400000

300000


200000


100000

0

2.75 2.80 2.85

Time-->









#19

Methyl tert-butyl Ether
 Concen: 0.499 ug/l
 RT: 3.17 min Scan# 341
 Delta R.T. 0.00 min
 Lab File: VX016903.D
 Acq: 20 Jun 2020 03:14

Instrument :
 MSVOA_X
 ClientSampleId :
 TW-1




Tot Ion: 73 Resp: 4252
 Ion Ratio Lower Upper
 73 100
 57 13205.4 16.9 25.3#

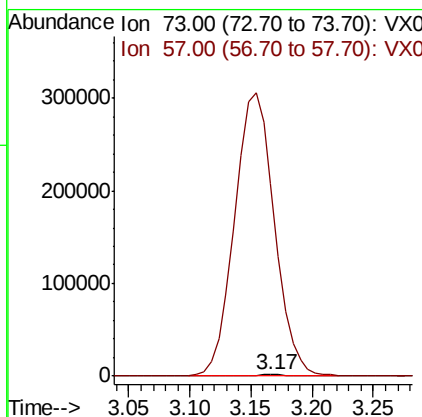


#20

Methylene Chloride
 Concen: 0.536 ug/l
 RT: 2.82 min Scan# 285
 Delta R.T. -0.01 min
 Lab File: VX016903.D
 Acq: 20 Jun 2020 03:14

Tgt Ion: 84 Resp: 1570
 Ion Ratio Lower Upper
 84 100
 49 68.6 86.6 129.8#
 51 480.1 27.1 40.7#
 86 2198.1 53.1 79.7#

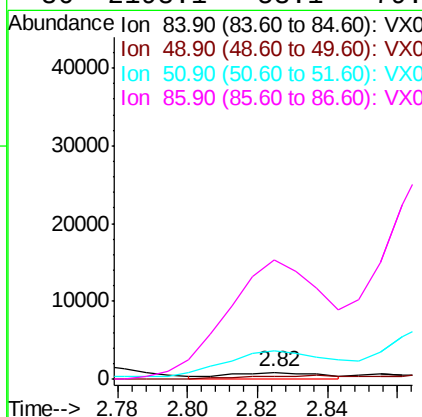



#21

trans-1,2-Dichloroethene

Concen: 0.202 ug/l

RT: 3.14 min Scan# 337

Delta R.T. 0.00 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampleId :

TW-1


Tot Ion: 96 Resp: 570

Ion Ratio Lower Upper

96 100

61 220.3 105.4 158.0#




98 73.8 51.3 76.9



Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

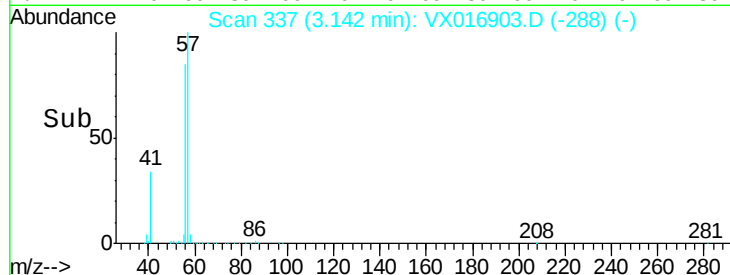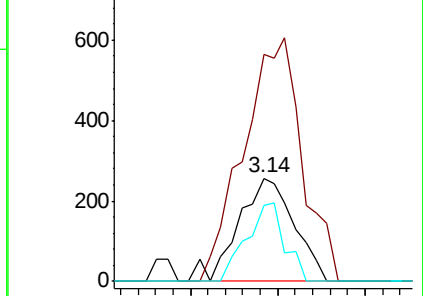

#23

Vinyl Acetate

Concen: 0.746 ug/l

RT: 3.79 min Scan# 444

Delta R.T. 0.01 min

Lab File: VX016903.D


Acq: 20 Jun 2020 03:14

Tgt Ion: 43 Resp: 4661

Ion Ratio Lower Upper



43 100


86 3.3 9.9 14.9#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 86.00 (85.70 to 86.70): VX0

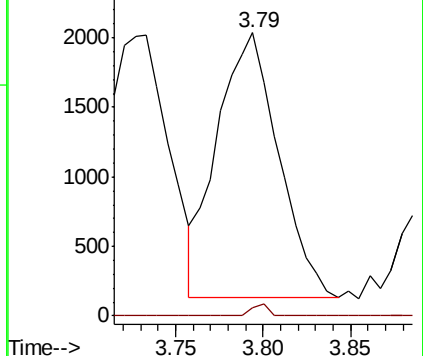



#25

2-Butanone

Concen: 10.628 ug/l

RT: 4.64 min Scan# 582

Delta R.T. 0.01 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampleId :





TW-1

Tot Ion: 43 Resp: 17871

Ion Ratio Lower Upper

43 100

72 29.0 23.5 35.3

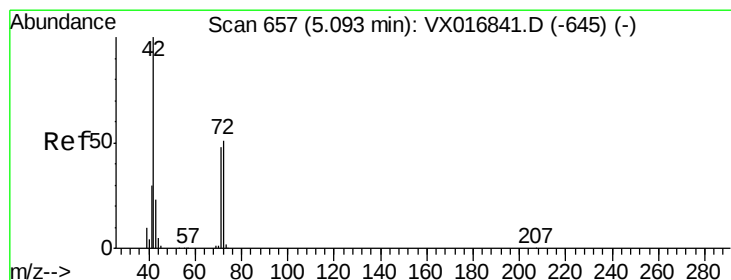

#29

Tetrahydrofuran

Concen: 2.490 ug/l

RT: 5.03 min Scan# 646

Delta R.T. -0.07 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14




Tgt Ion: 42 Resp: 2637


Ion Ratio Lower Upper

42 100

72 0.0 41.1 61.7#

71 0.0 38.4 57.6#



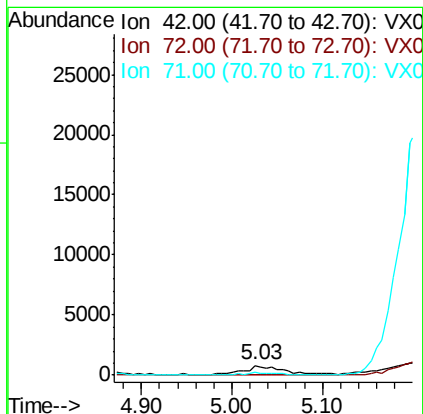





#30
Chloroform
Concen: 19.192 ug/l
RT: 5.25 min Scan# 682
Delta R.T. 0.07 min
Lab File: VX016903.D
Acq: 20 Jun 2020 03:14




Instrument :
MSVOA_X
ClientSampleId :
TW-1


Tot Ion: 83 Resp: 95923
Ion Ratio Lower Upper
83 100
85 7.5 53.4 80.0#

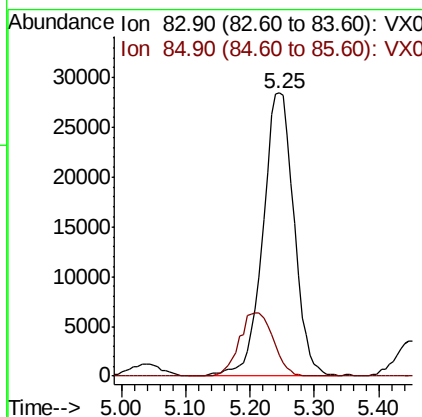

#31
Cyclohexane
Concen: 44.294 ug/l
RT: 5.57 min Scan# 736
Delta R.T. 0.02 min
Lab File: VX016903.D
Acq: 20 Jun 2020 03:14

Tgt Ion: 56 Resp: 184356
Ion Ratio Lower Upper
56 100
69 0.0 26.1 39.1#
84 53.3 73.0 109.6#

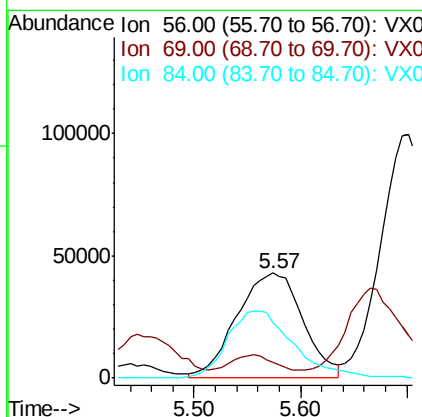



#33

1,2-Dichloroethane-d4

Concen: 44.045 ug/l

RT: 6.03 min Scan# 811

Delta R.T. 0.00 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampleId :





TW-1

Tot Ion: 65 Resp: 148241

Ion Ratio Lower Upper

65 100

67 52.2 0.0 102.6



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. 0.00 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14




Tgt Ion: 114 Resp: 492125


Ion Ratio Lower Upper

114 100

63 20.4 0.0 37.0

88 15.9 0.0 32.0





#35

Dibromofluoromethane

Concen: 43.552 ug/l

RT: 5.47 min Scan# 719

Delta R.T. 0.01 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampleId :

TW-1


Tot Ion:113 Resp: 137107

Ion Ratio Lower Upper

113 100

111 104.0 81.0 121.4




192 22.8 18.5 27.7



Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

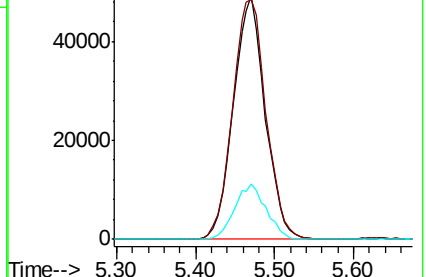

#37

Ethyl Acetate

Concen: 0.838 ug/l

RT: 4.86 min Scan# 619

Delta R.T. 0.07 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14


Tgt Ion: 43 Resp: 3366

Ion Ratio Lower Upper

43 100

61 0.0 12.2 18.2#



70 58.9 10.5 15.7#




Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 70.00 (69.70 to 70.70): VX0

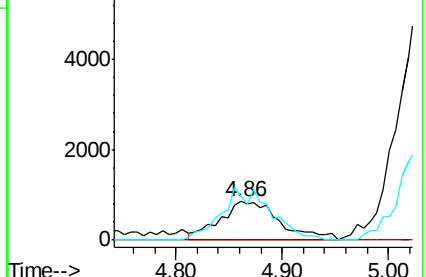



#38

Carbon Tetrachloride

Concen: 5.108 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.13 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampled :

TW-1


Tot Ion:117 Resp: 26042

Ion Ratio Lower Upper

117 100

119 5.1 77.4 116.2#




121 0.0 24.7 37.1#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

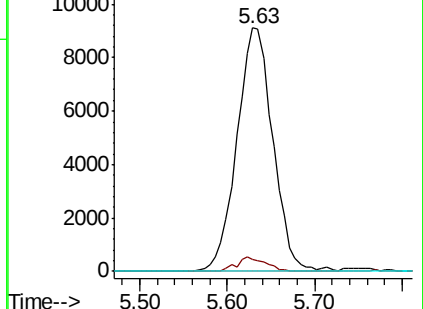

#39

Methylcyclohexane

Concen: 68.843 ug/l

RT: 7.44 min Scan# 1042

Delta R.T. 0.00 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14


Tgt Ion: 83 Resp: 363729

Ion Ratio Lower Upper

83 100

55 81.0 61.7 92.5



98 48.1 39.0 58.6




Abundance Ion 83.00 (82.70 to 83.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 98.00 (97.70 to 98.70): VX0

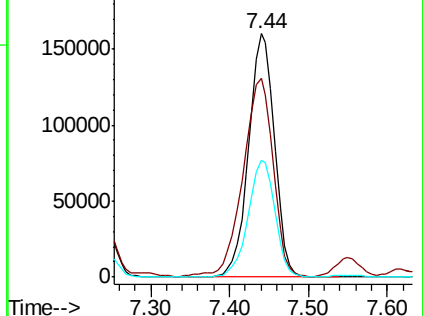



#40

Benzene

Concen: 0.418 ug/l

RT: 6.12 min Scan# 825

Delta R.T. 0.00 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampleId :





TW-1

Tot Ion: 78 Resp: 5701

Ion Ratio Lower Upper

78 100

77 23.4 18.6 27.8

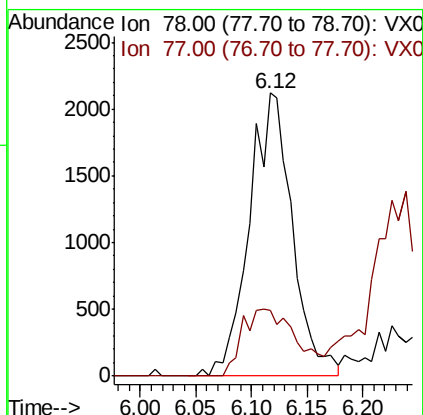

#41

Methacrylonitrile

Concen: 9.344 ug/l

RT: 5.03 min Scan# 647

Delta R.T. 0.02 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Tgt Ion: 41 Resp: 20367




Ion Ratio Lower Upper


41 100

39 51.4 42.6 64.0

67 12.8 64.2 96.2#

52 2.3 25.6 38.4#

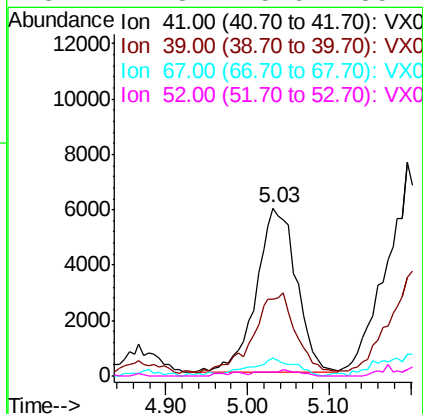



#43

Isopropyl Acetate

Concen: 3.787 ug/l

RT: 6.43 min Scan# 877

Delta R.T. 0.02 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampled :

TW-1





Tot Ion: 43 Resp: 26551

Ion Ratio Lower Upper

43 100

61 1.5 17.9 26.9#

87 0.0 12.4 18.6#

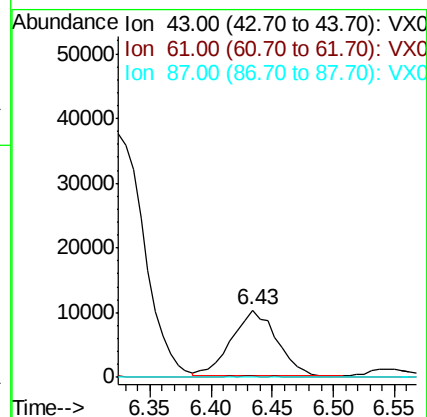

#45

1,2-Dichloropropane

Concen: 1.378 ug/l

RT: 7.44 min Scan# 1042

Delta R.T. -0.05 min

Lab File: VX016903.D




Acq: 20 Jun 2020 03:14


Tgt Ion: 63 Resp: 4722

Ion Ratio Lower Upper

63 100

65 200.4 25.8 38.8#

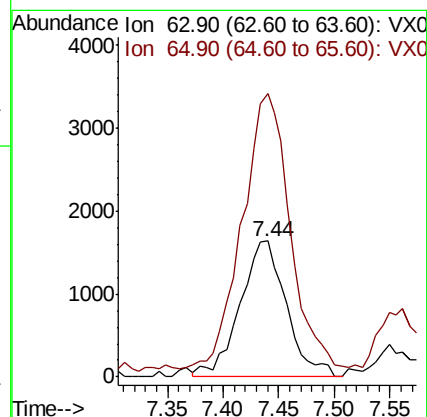



#46

Dibromomethane

Concen: 0.908 ug/l

RT: 7.62 min Scan# 1071

Delta R.T. -0.02 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampleId :

TW-1





Tot Ion: 93 Resp: 2111

Ion Ratio Lower Upper

93 100

95 1063.9 65.7 98.5#

174 5.3 92.8 139.2#



#47

Bromodichloromethane

Concen: 11.578 ug/l

RT: 7.93 min Scan# 1122

Delta R.T. 0.05 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14




Tgt Ion: 83 Resp: 57239


Ion Ratio Lower Upper

83 100

85 0.5 50.9 76.3#

127 0.0 7.4 11.0#









#48
Methvl methacrylate
Concen: 6.307 ug/l
RT: 7.76 min Scan# 1095
Delta R.T. 0.02 min
Lab File: VX016903.D
Acq: 20 Jun 2020 03:14




Instrument :
MSVOA_X
ClientSampled :
TW-1


Tot Ion: 41 Resp: 20822
Ion Ratio Lower Upper
41 100
69 84.6 73.3 109.9
39 37.6 42.4 63.6#

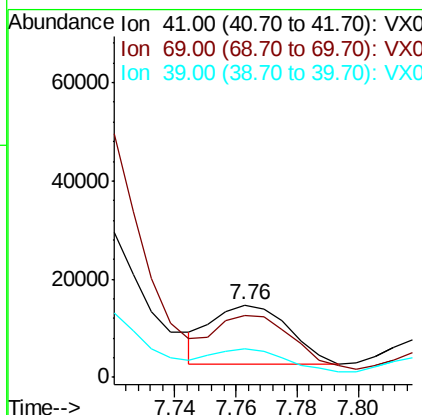

#50
Toluene-d8
Concen: 44.515 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. 0.00 min
Lab File: VX016903.D
Acq: 20 Jun 2020 03:14

Tgt Ion: 98 Resp: 560675
Ion Ratio Lower Upper
98 100
100 63.9 54.0 81.0

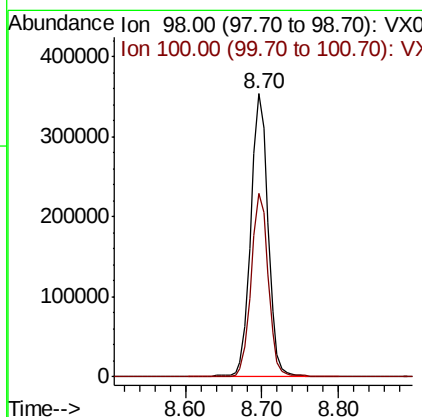

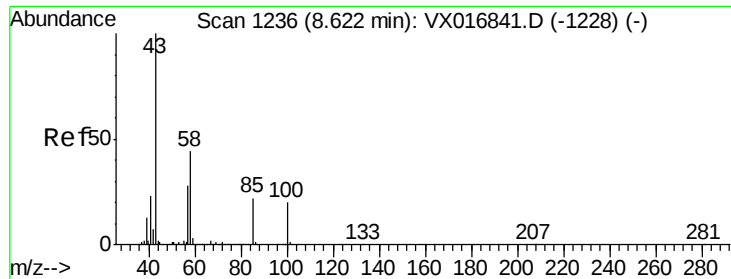

#51

4-Methyl-2-Pentanone

Concen: 2.549 ug/l

RT: 8.62 min Scan# 1236

Delta R.T. 0.00 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampled :


TW-1

Tot Ion: 43 Resp: 10747

Ion Ratio Lower Upper




43 100

58 43.2 34.3 51.5

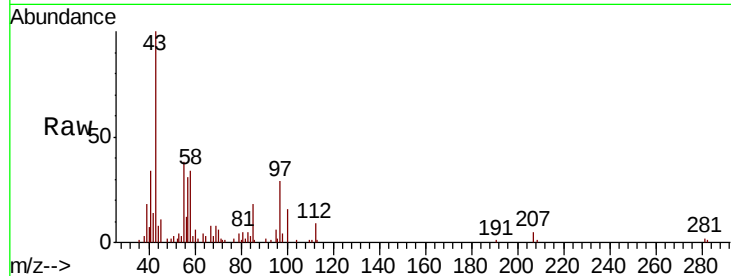

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

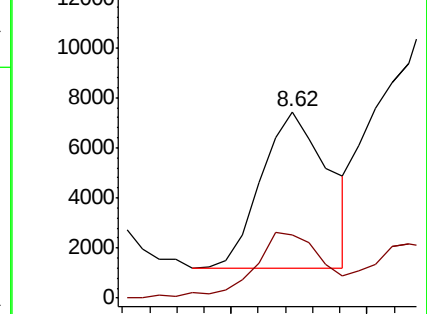

#52

Toluene

Concen: 1.640 ug/l

RT: 8.77 min Scan# 1260

Delta R.T. 0.01 min

Lab File: VX016903.D


Acq: 20 Jun 2020 03:14

Tgt Ion: 92 Resp: 14832

Ion Ratio Lower Upper



92 100


91 165.0 134.2 201.2



Abundance Ion 92.00 (91.70 to 92.70): VX0

Ion 91.00 (90.70 to 91.70): VX0



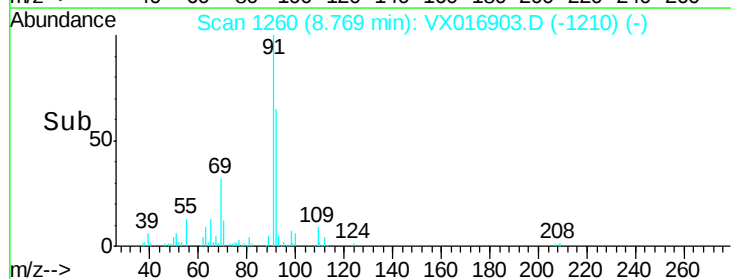
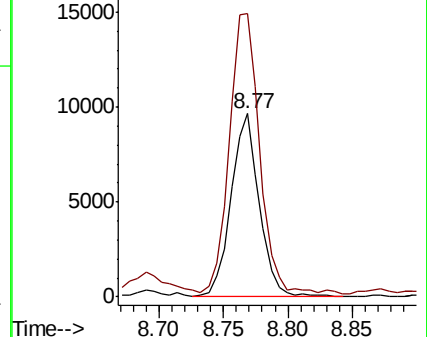




#55
 1,1,2-Trichloroethane
 Concen: 18.611 ug/l
 RT: 9.15 min Scan# 1322
 Delta R.T. -0.05 min
 Lab File: VX016903.D
 Acq: 20 Jun 2020 03:14




Instrument :
 MSVOA_X
 ClientSampled :
 TW-1


Tot Ion: 97 Resp: 63558
 Ion Ratio Lower Upper
 97 100
 83 7.1 65.5 98.3#
 85 0.7 42.6 63.8#
 99 0.3 49.4 74.0#

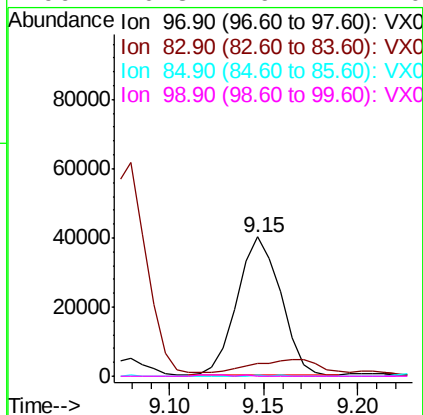

#56
 Ethyl methacrylate
 Concen: 5.366 ug/l
 RT: 9.17 min Scan# 1326
 Delta R.T. 0.01 min
 Lab File: VX016903.D
 Acq: 20 Jun 2020 03:14

Tgt Ion: 69 Resp: 26530
 Ion Ratio Lower Upper
 69 100
 41 121.4 47.9 71.9#
 39 0.0 24.2 36.4#


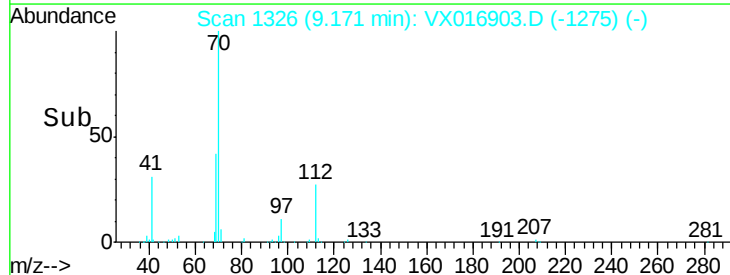






#58
2-Chloroethyl Vinyl ether
Concen: 0.820 ug/l
RT: 8.24 min Scan# 1174
Delta R.T. -0.05 min
Lab File: VX016903.D
Acq: 20 Jun 2020 03:14




Instrument :
MSVOA_X
ClientSampled :
TW-1


Tot Ion: 63 Resp: 1886
Ion Ratio Lower Upper
63 100
106 0.0 25.8 38.6#

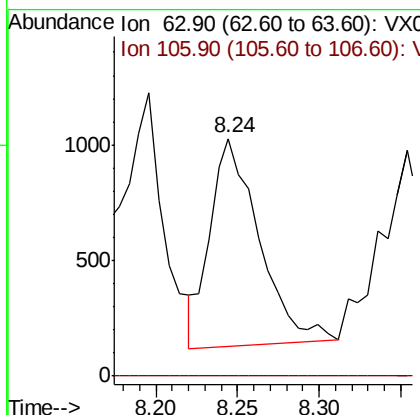

#59
2-Hexanone
Concen: 3.902 ug/l
RT: 9.48 min Scan# 1376
Delta R.T. 0.01 min
Lab File: VX016903.D
Acq: 20 Jun 2020 03:14

Tgt Ion: 43 Resp: 11915
Ion Ratio Lower Upper
43 100
58 64.0 29.8 89.4

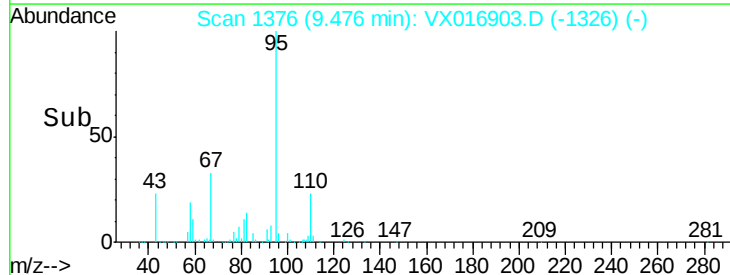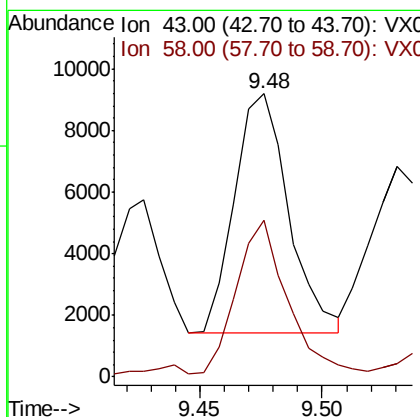



#62

4-Bromofluorobenzene

Concen: 47.980 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.00 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampleId :

TW-1


Tot Ion: 95 Resp: 231538

Ion Ratio Lower Upper

95 100

174 82.3 0.0 174.2




176 80.2 0.0 170.0



Abundance Ion 94.90 (94.60 to 95.60): VX016903.D (-1597) (-)

Ion 173.80 (173.50 to 174.50): VX016903.D (-1597) (-)

Ion 175.80 (175.50 to 176.50): VX016903.D (-1597) (-)

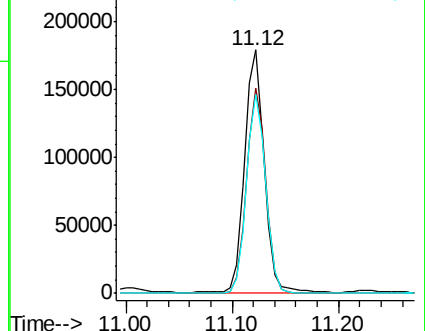

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.10 min Scan# 1478

Delta R.T. 0.00 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14


Tgt Ion: 117 Resp: 456481

Ion Ratio Lower Upper

117 100

82 52.7 43.4 65.0



119 31.1 25.7 38.5




Abundance Ion 116.90 (116.60 to 117.60): VX016903.D (-1429) (-)

Ion 82.00 (81.70 to 82.70): VX016903.D (-1429) (-)

Ion 118.90 (118.60 to 119.60): VX016903.D (-1429) (-)

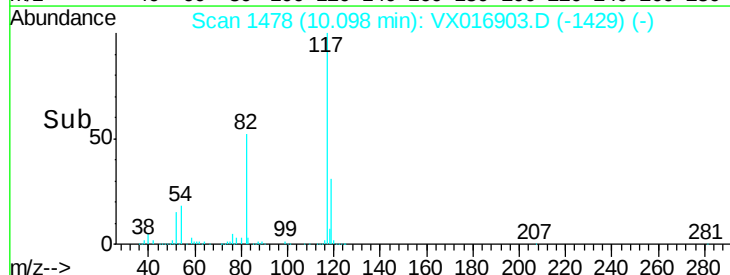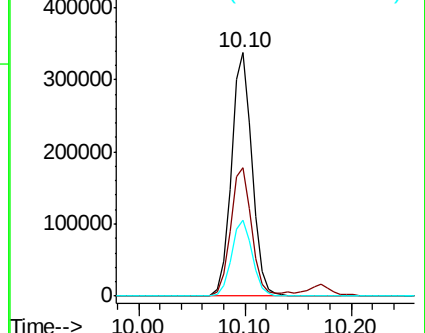



#67

Ethyl Benzene

Concen: 82.066 ug/l

RT: 10.24 min Scan# 1501

Delta R.T. 0.00 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampled :


TW-1

Tot Ion: 91 Resp: 1279924

Ion Ratio Lower Upper




91 100

106 32.0 25.1 37.7



Abundance Ion 91.00 (90.70 to 91.70): VX016841.D (-1493) (-)

Ion 106.00 (105.70 to 106.70): VX016841.D (-1493) (-)

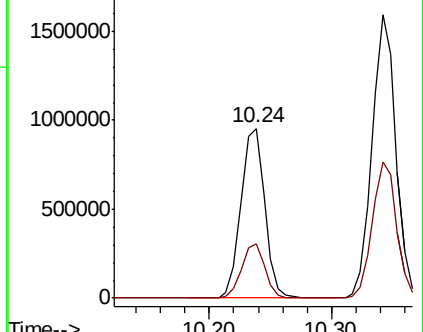

#68

m/p-Xylenes

Concen: 174.084 ug/l

RT: 10.34 min Scan# 1518

Delta R.T. 0.00 min

Lab File: VX016903.D


Acq: 20 Jun 2020 03:14

Tgt Ion: 106 Resp: 1056514

Ion Ratio Lower Upper



106 100


91 202.9 161.5 242.3



Abundance Ion 106.00 (105.70 to 106.70): VX016841.D (-1511) (-)

Ion 91.00 (90.70 to 91.70): VX016841.D (-1511) (-)




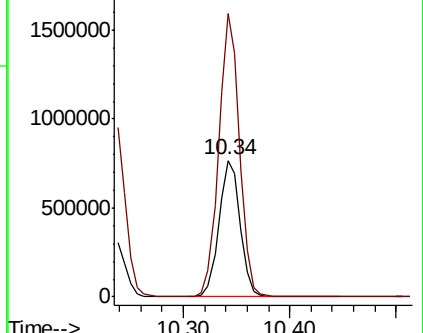




#69
o-Xylene
Concen: 8.622 ug/l
RT: 10.68 min Scan# 1574
Delta R.T. 0.00 min
Lab File: VX016903.D
Acq: 20 Jun 2020 03:14




Instrument :
MSVOA_X
ClientSampled :
TW-1


Tot Ion:106 Resp: 48383
Ion Ratio Lower Upper
106 100
91 212.3 107.9 323.7

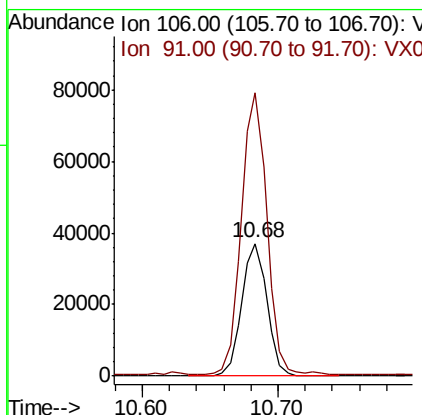

#70
Styrene
Concen: 0.361 ug/l
RT: 10.68 min Scan# 1574
Delta R.T. -0.01 min
Lab File: VX016903.D
Acq: 20 Jun 2020 03:14

Tgt Ion:104 Resp: 3439
Ion Ratio Lower Upper
104 100
78 219.2 39.6 59.4#
103 207.9 43.3 64.9#

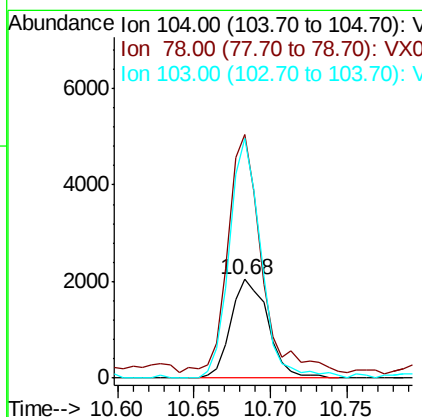



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. 0.00 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampled :

TW-1


Tot Ion:152 Resp: 266052

Ion Ratio Lower Upper

152 100

115 62.3 40.9 122.8




150 156.9 0.0 344.2



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

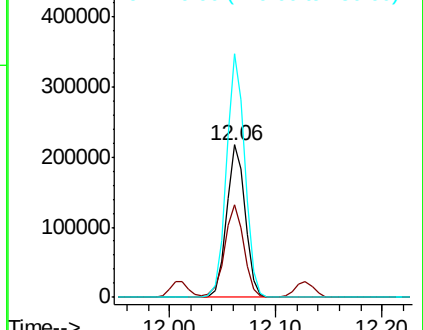

#73

Isopropylbenzene

Concen: 74.185 ug/l

RT: 11.00 min Scan# 1626

Delta R.T. 0.00 min

Lab File: VX016903.D


Acq: 20 Jun 2020 03:14

Tgt Ion:105 Resp: 1270785

Ion Ratio Lower Upper



105 100


120 26.5 13.2 39.6



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

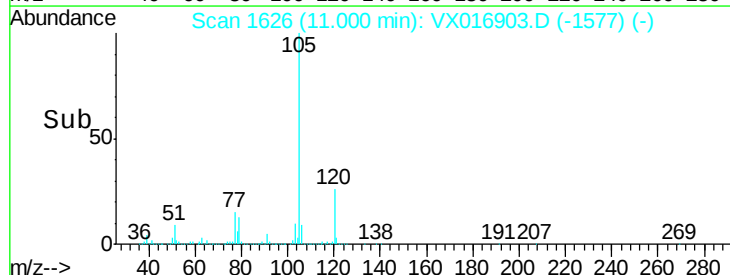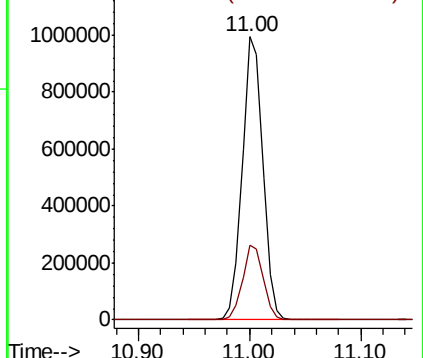

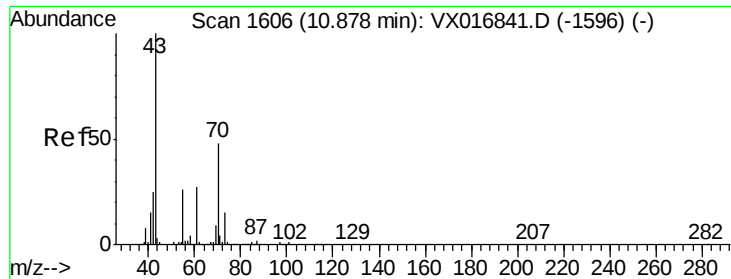

#74

N-amvl acetate

Concen: 0.205 ug/l

RT: 10.89 min Scan# 1608

Delta R.T. 0.01 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampled :

TW-1

Tot Ion: 43 Resp: 1224


Ion Ratio Lower Upper

43 100

70 210.7 39.9 59.9#

55 468.5 21.8 32.6#

61 0.0 22.2 33.4#



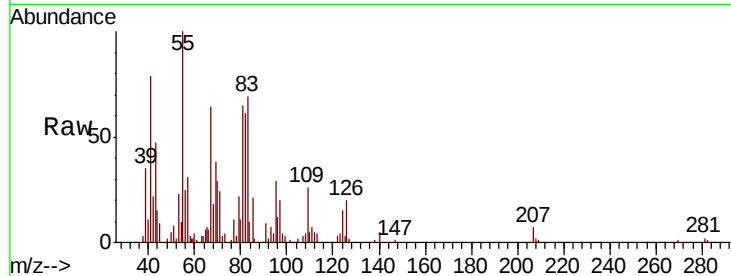


Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

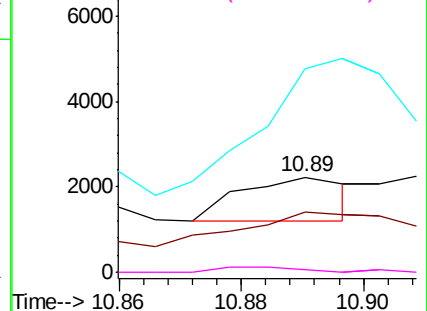

#75

1,1,2,2-Tetrachloroethane

Concen: 0.255 ug/l

RT: 11.26 min Scan# 1669

Delta R.T. 0.01 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14


Tgt Ion: 83 Resp: 1234

Ion Ratio Lower Upper

83 100

131 0.0 5.7 17.1#



85 27.3 32.6 97.8#




Abundance Ion 82.90 (82.60 to 83.60): VX0

Ion 130.80 (130.50 to 131.50): V

Ion 84.90 (84.60 to 85.60): VX0

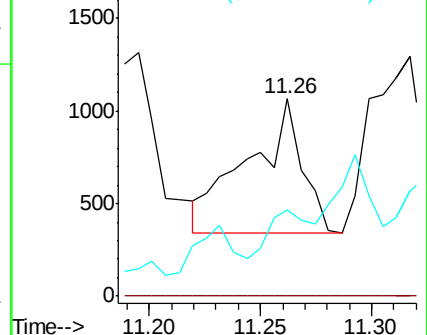

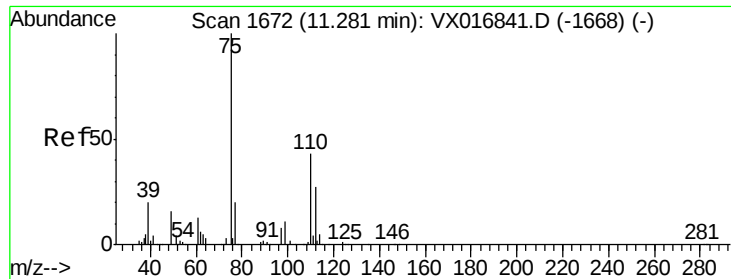

#76

1,2,3-Trichloropropane

Concen: 1.914 ug/l

RT: 11.34 min Scan# 1682

Delta R.T. 0.06 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampled :


TW-1

Tot Ion: 75 Resp: 9300

Ion Ratio Lower Upper

75 100

77 625.6 20.5 61.5#

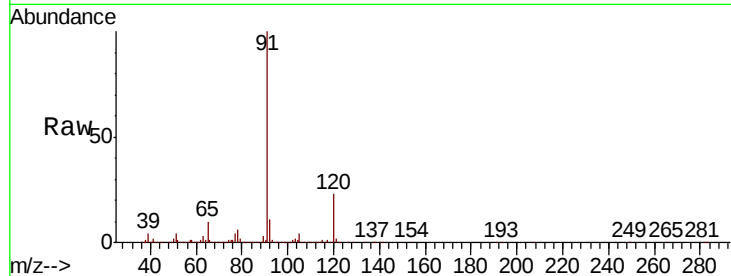

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

150000



100000

50000

0

11.30 11.35 11.40

Time-->



#78

n-propylbenzene

Concen: 80.446 ug/l

RT: 11.34 min Scan# 1682

Delta R.T. 0.00 min

Lab File: VX016903.D


Acq: 20 Jun 2020 03:14

Tgt Ion: 91 Resp: 1537918

Ion Ratio Lower Upper

91 100

120 23.6 11.9 35.5



Abundance Ion 91.00 (90.70 to 91.70): VX0

Ion 120.00 (119.70 to 120.70): V


1100000


500000

0

11.30 11.40

Time-->





#79

2-Chlorotoluene

Concen: 26.125 ug/l

RT: 11.42 min Scan# 1695

Delta R.T. 0.02 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampleId :


TW-1

Tot Ion: 91 Resp: 305575

Ion Ratio Lower Upper

91 100

126 0.5 17.2 51.5#

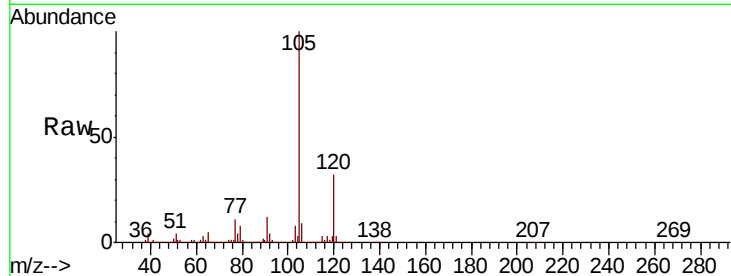

Abundance Ion 91.00 (90.70 to 91.70): VX016841.D (-1687) (-)

Ion 125.90 (125.60 to 126.60): VX016841.D (-1687) (-)

600000

500000

400000

300000

200000



100000

0

11.40

11.45

Time-->

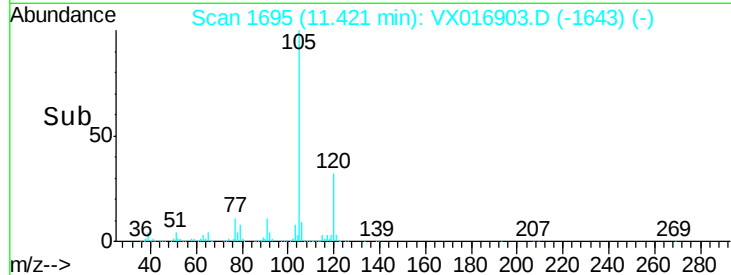

#80

1,3,5-Trimethylbenzene

Concen: 103.084 ug/l

RT: 11.49 min Scan# 1707

Delta R.T. 0.01 min

Lab File: VX016903.D


Acq: 20 Jun 2020 03:14

Tgt Ion: 105 Resp: 1523549

Ion Ratio Lower Upper

105 100

120 48.3 24.6 74.0

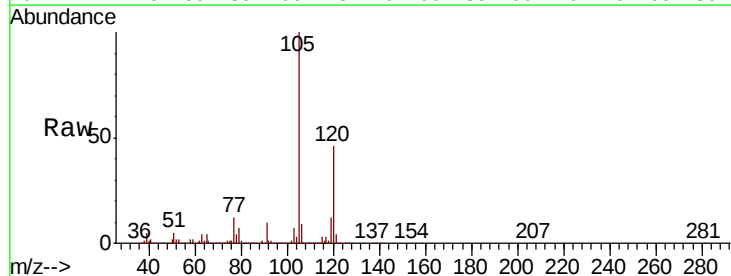

Abundance Ion 105.00 (104.70 to 105.70): VX016841.D (-1700) (-)

Ion 120.00 (119.70 to 120.70): VX016841.D (-1700) (-)

1500000

1000000

500000


0


11.49

11.50

11.60

Time-->




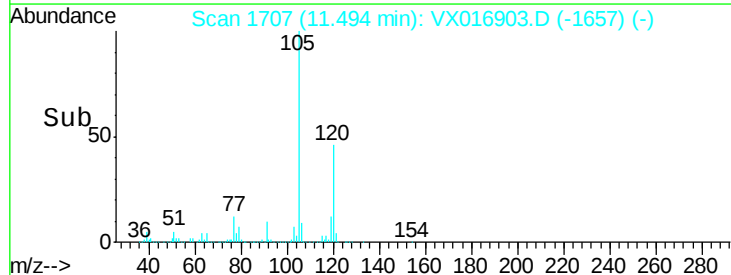


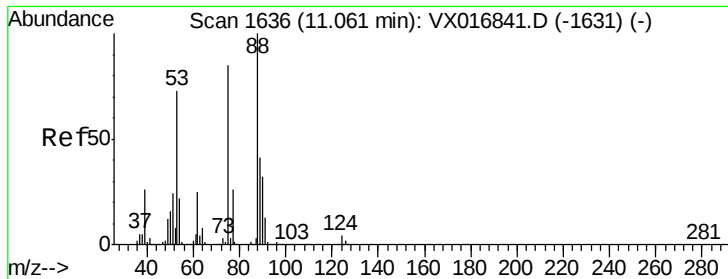

#81
trans-1,4-Dichloro-2-butene
Concen: 6.923 ug/l
RT: 11.00 min Scan# 1626
Delta R.T. -0.06 min
Lab File: VX016903.D
Acq: 20 Jun 2020 03:14




Instrument :
MSVOA_X
ClientSampleId :
TW-1


Tot Ion: 75 Resp: 13737
Ion Ratio Lower Upper
75 100
53 110.7 69.8 104.8#
89 112.1 38.3 57.5#

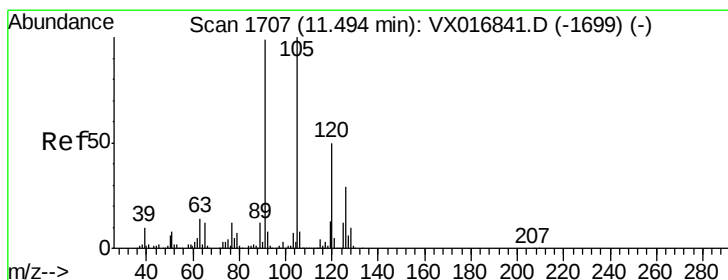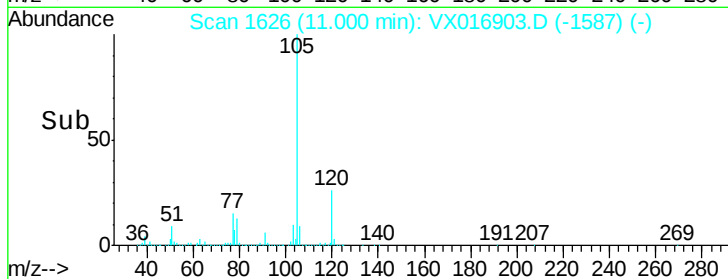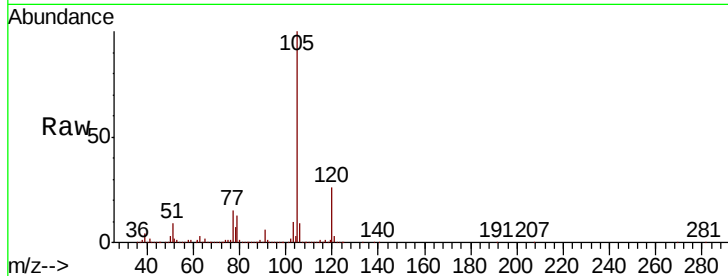

#82
4-Chlorotoluene
Concen: 11.128 ug/l
RT: 11.49 min Scan# 1707
Delta R.T. 0.00 min
Lab File: VX016903.D
Acq: 20 Jun 2020 03:14

Tgt Ion: 91 Resp: 156157
Ion Ratio Lower Upper
91 100
126 0.6 15.0 45.0#


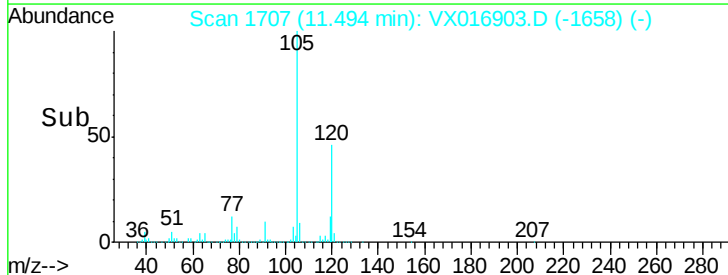

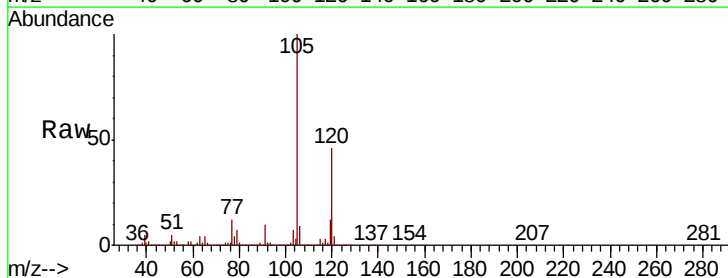




#83
 tert-Butylbenzene
 Concen: 36.356 ug/l
 RT: 11.79 min Scan# 1756
 Delta R.T. 0.04 min
 Lab File: VX016903.D
 Acq: 20 Jun 2020 03:14




Instrument :
 MSVOA_X
 ClientSampled :
 TW-1


Tot Ion:119 Resp: 531650
 Ion Ratio Lower Upper
 119 100
 91 81.9 28.5 85.5
 134 0.0 11.7 35.1#



#84
 1,2,4-Trimethylbenzene
 Concen: 272.126 ug/l
 RT: 11.79 min Scan# 1756
 Delta R.T. 0.00 min
 Lab File: VX016903.D
 Acq: 20 Jun 2020 03:14

Tgt Ion:105 Resp: 4143017
 Ion Ratio Lower Upper
 105 100
 120 46.7 22.3 66.9









#85
 sec-Butylbenzene
 Concen: 31.664 ug/l
 RT: 11.93 min Scan# 1779
 Delta R.T. 0.00 min
 Lab File: VX016903.D
 Acq: 20 Jun 2020 03:14




Instrument :
 MSVOA_X
 ClientSampleId :
 TW-1


Tot Ion:105 Resp: 537770
 Ion Ratio Lower Upper
 105 100
 134 16.4 10.4 31.2



#86
 p-Isopropyltoluene
 Concen: 9.632 ug/l
 RT: 12.05 min Scan# 1798
 Delta R.T. 0.00 min
 Lab File: VX016903.D
 Acq: 20 Jun 2020 03:14

Tgt Ion:119 Resp: 149876
 Ion Ratio Lower Upper
 119 100
 134 26.0 12.9 38.7
 91 22.7 11.6 34.8

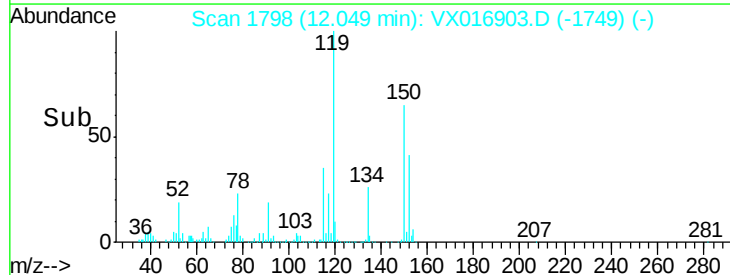



#87

1,3-Dichlorobenzene

Concen: 0.215 ug/l

RT: 12.01 min Scan# 1792

Delta R.T. 0.00 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampled :

TW-1





Tot Ion:146 Resp: 1833

Ion Ratio Lower Upper

146 100

111 60.6 19.4 58.2#

148 67.0 31.8 95.3

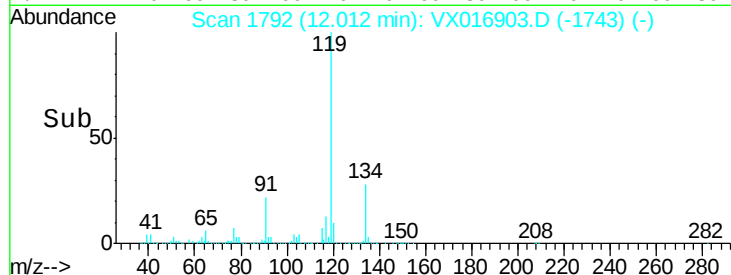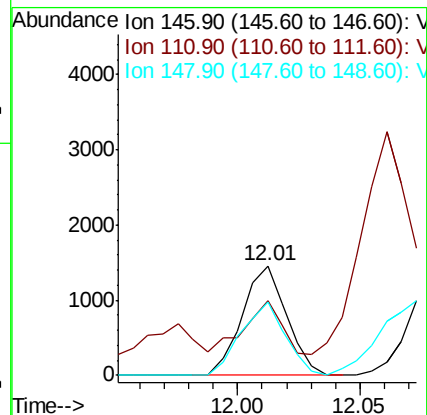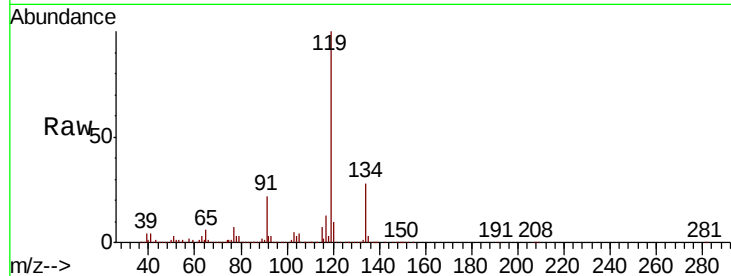

#88

1,4-Dichlorobenzene

Concen: 0.212 ug/l

RT: 12.01 min Scan# 1792

Delta R.T. -0.07 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14




Tgt Ion:146 Resp: 1833


Ion Ratio Lower Upper

146 100

111 44.8 19.0 57.0

148 67.0 31.6 95.0



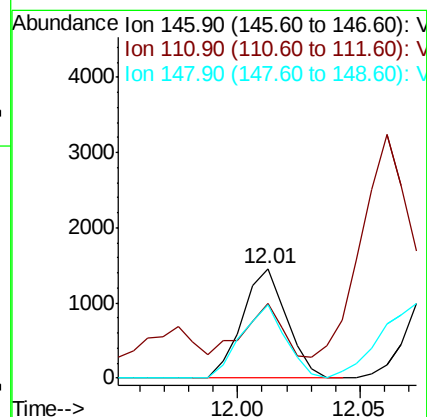





#89
n-Butylbenzene
Concen: 106.077 ug/l
RT: 12.37 min Scan# 1851
Delta R.T. 0.00 min
Lab File: VX016903.D
Acq: 20 Jun 2020 03:14




Instrument :
MSVOA_X
ClientSampled :
TW-1


Tot Ion: 91 Resp: 1415463
Ion Ratio Lower Upper
91 100
92 34.2 27.4 82.2
134 109.8 13.9 41.6#

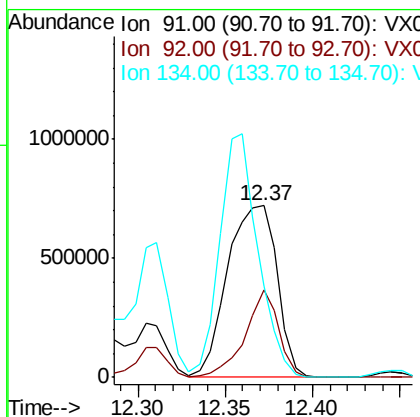

#90
Hexachloroethane
Concen: 57.355 ug/l
RT: 12.57 min Scan# 1884
Delta R.T. -0.01 min
Lab File: VX016903.D
Acq: 20 Jun 2020 03:14

Tgt Ion: 117 Resp: 160768
Ion Ratio Lower Upper
117 100
201 0.1 44.9 134.5#

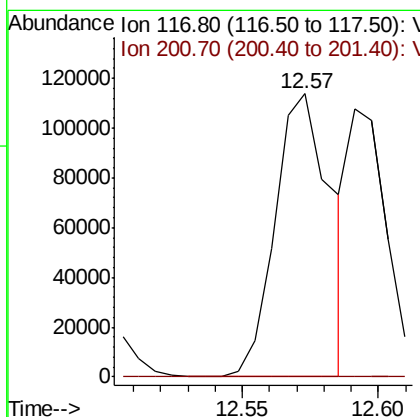



#92

1,2-Dibromo-3-Chloropropane

Concen: 11.262 ug/l

RT: 13.00 min Scan# 1954

Delta R.T. 0.02 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampleId :

TW-1


Tot Ion: 75 Resp: 12916

Ion Ratio Lower Upper

75 100

155 1.1 46.4 139.1#

157 0.0 58.6 175.8#



Abundance Ion 74.90 (74.60 to 75.60): VX016841.D (-1943) (-)



Ion 154.80 (154.50 to 155.50): VX016841.D (-1943) (-)

Ion 156.80 (156.50 to 157.50): VX016841.D (-1943) (-)

Time-->

13.00

13.05

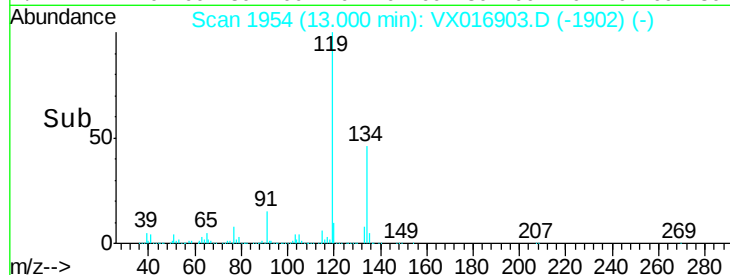

#93

1,2,4-Trichlorobenzene

Concen: 0.576 ug/l

RT: 13.63 min Scan# 2057

Delta R.T. 0.00 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14


Tgt Ion: 180 Resp: 3187

Ion Ratio Lower Upper

180 100

182 101.1 47.7 143.1

145 891.1 15.0 45.1#



Abundance Ion 179.80 (179.50 to 180.50): VX016841.D (-2050) (-)


Ion 181.80 (181.50 to 182.50): VX016841.D (-2050) (-)


Ion 144.80 (144.50 to 145.50): VX016841.D (-2050) (-)

Time-->

13.63

13.65





#94

Hexachlorobutadiene

Concen: 0.757 ug/l

RT: 13.77 min Scan# 2080

Delta R.T. 0.00 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14

Instrument :

MSVOA_X

ClientSampled :

TW-1


Tot Ion:225 Resp: 1890

Ion Ratio Lower Upper

225 100

223 74.5 32.1 96.5




227 65.2 32.3 96.8



Abundance Ion 224.70 (224.40 to 225.40): V

Ion 222.70 (222.40 to 223.40): V

Ion 226.70 (226.40 to 227.40): V

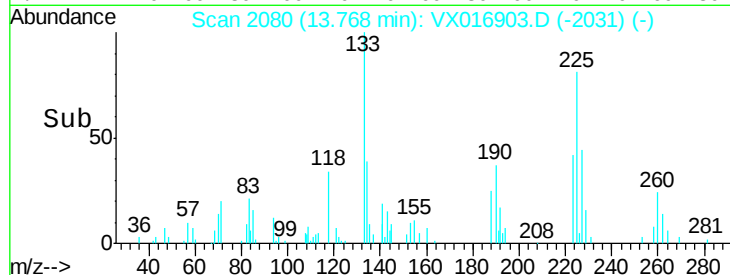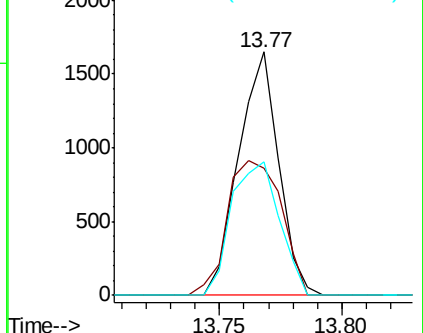

#95

Naphthalene

Concen: 17.898 ug/l

RT: 13.82 min Scan# 2088

Delta R.T. 0.00 min

Lab File: VX016903.D

Acq: 20 Jun 2020 03:14


Tgt Ion:128 Resp: 290735

Ion Ratio Lower Upper

128 100

127 13.2 10.4 15.6



129 12.4 8.6 13.0




Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

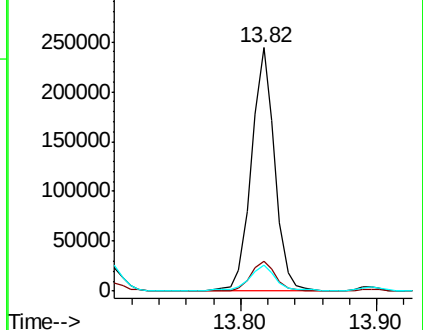



#96
 1,2,3-Trichlorobenzene
 Concen: 0.476 ug/l
 RT: 14.00 min Scan# 2118
 Delta R.T. 0.00 min
 Lab File: VX016903.D
 Acq: 20 Jun 2020 03:14

Instrument :
 MSVOA_X
 ClientSampleId :
 TW-1

Tot Ion	Ratio	Lower	Upper
180	100		
182	98.3	47.4	142.3
145	682.2	16.0	48.0

