

Data File : VX016878.D
Acq On : 19 Jun 2020 14:44
Operator : JC/SP
Sample : L3042-03RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OUTFALL001-200616RE

Quant Time: Jun 22 02:44:57 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061820W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 19 12:07:48 2020
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	218294	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	383935	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	361396	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	191215	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.03	65	131279	50.00	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.00%	
35) Dibromofluoromethane	5.47	113	110983	45.19	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.38%	
50) Toluene-d8	8.70	98	434803	44.25	ug/l	0.00
Spiked Amount 50.000			Recovery	=	88.50%	
62) 4-Bromofluorobenzene	11.12	95	209550	55.66	ug/l	0.00
Spiked Amount 50.000			Recovery	=	111.32%	
Target Compounds						
27) cis-1,2-Dichloroethene	4.57	96	6533	2.640	ug/l	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VX016878.D
Acq On : 19 Jun 2020 14:44
Operator : JC/SP
Sample : L3042-03RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OUTFALL001-200616RE

Quant Time: Jun 22 02:44:57 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061820W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 19 12:07:48 2020
Response via : Initial Calibration

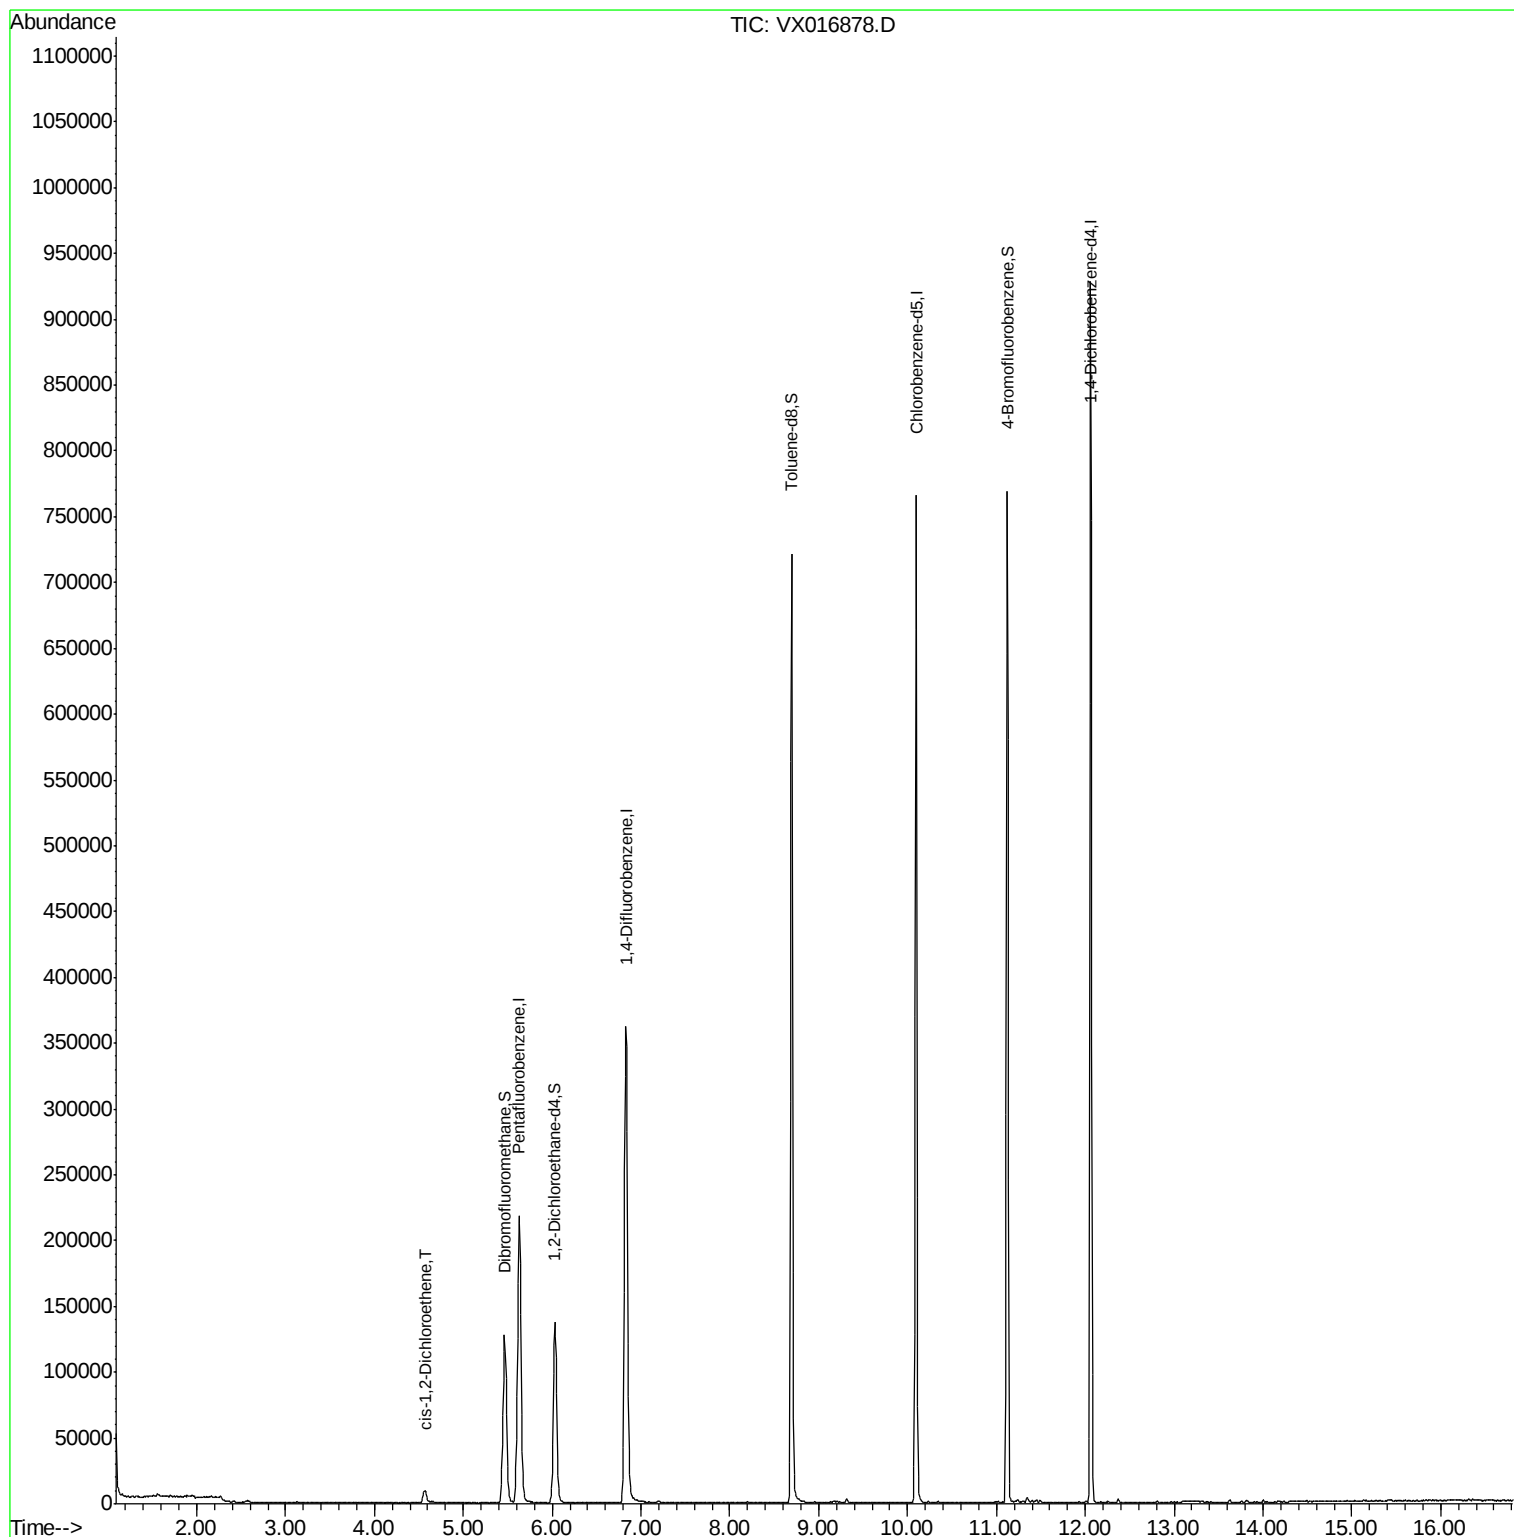

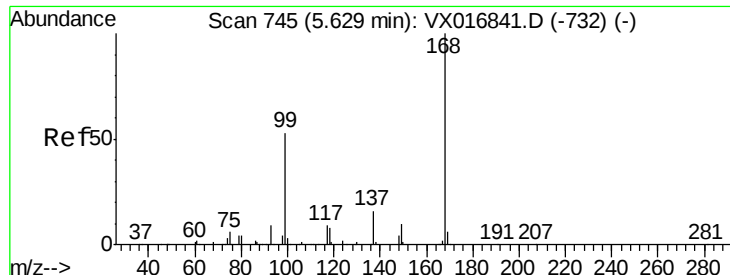

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.00 min

Lab File: VX016878.D

Acq: 19 Jun 2020 14:44

Instrument :

MSVOA_X

ClientSampleId :


OUTFALL001-200616RE

Tgt Ion:168 Resp: 218294

Ion Ratio Lower Upper




168 100

99 56.2 42.2 63.2

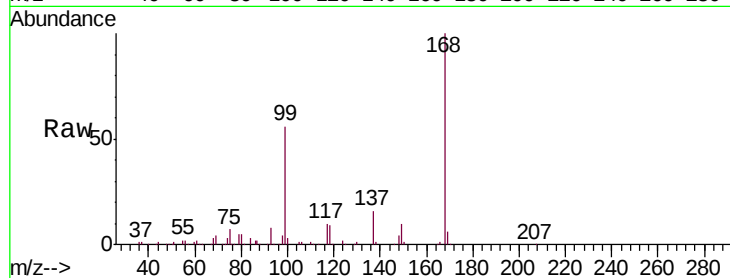

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

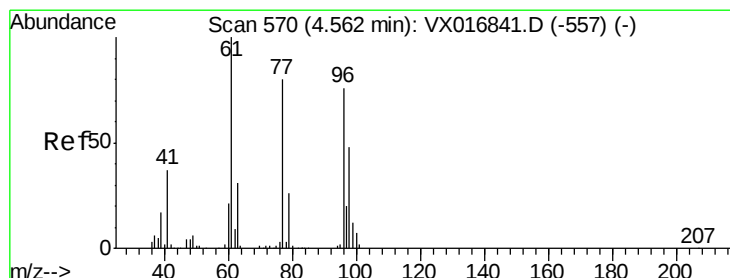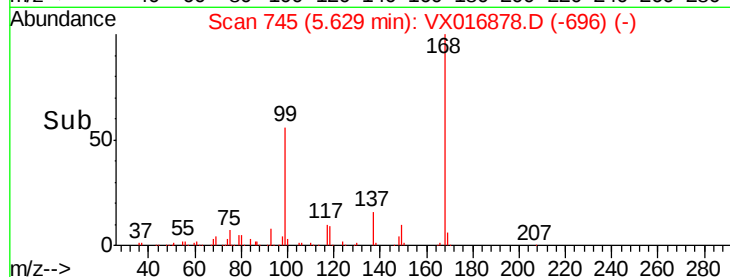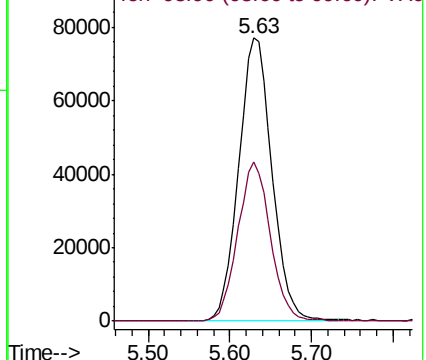

#27

cis-1,2-Dichloroethene

Concen: 2.640 ug/l

RT: 4.57 min Scan# 572

Delta R.T. 0.01 min

Lab File: VX016878.D

Acq: 19 Jun 2020 14:44


Tgt Ion: 96 Resp: 6533

Ion Ratio Lower Upper

96 100

61 122.4 0.0 273.8



98 63.3 0.0 129.0

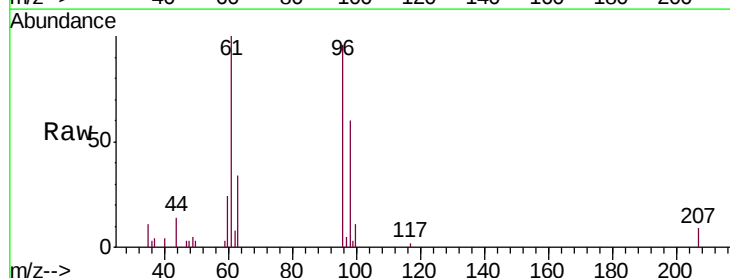


Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0



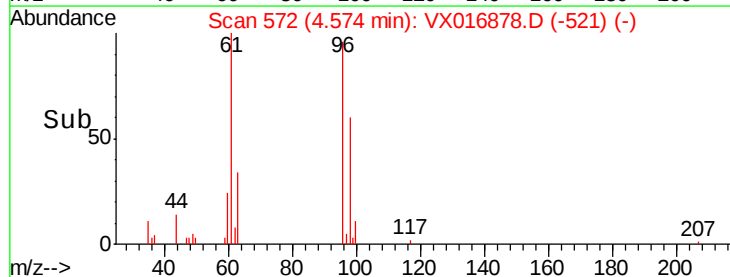
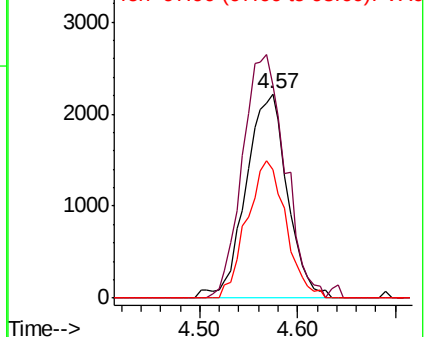


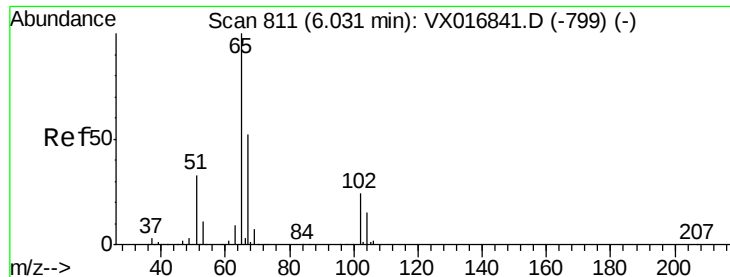

#33
 1,2-Dichloroethane-d4
 Concen: 50.004 ug/l
 RT: 6.03 min Scan# 811
 Delta R.T. -0.00 min
 Lab File: VX016878.D
 Acq: 19 Jun 2020 14:44




Instrument :
 MSVOA_X
 ClientSampleId :
 OUTFALL001-200616RE


Tgt Ion: 65 Resp: 131279
 Ion Ratio Lower Upper
 65 100
 67 52.5 0.0 102.6

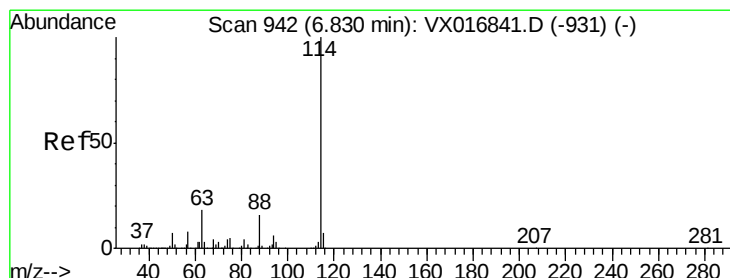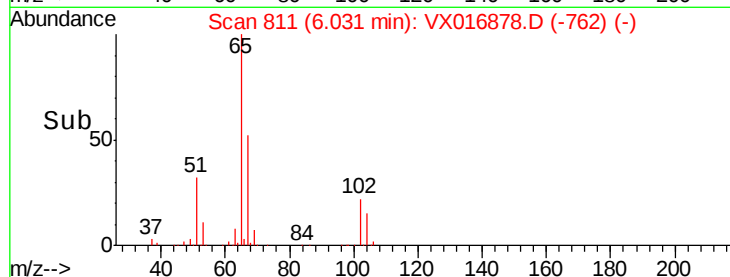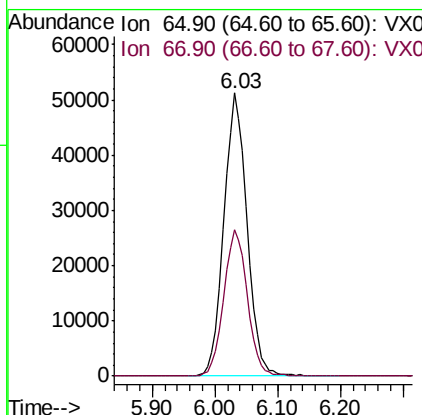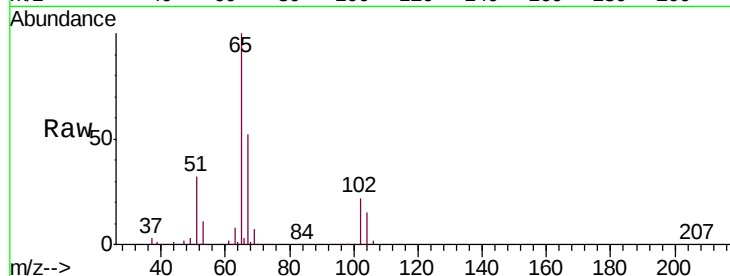

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.83 min Scan# 942
 Delta R.T. -0.00 min
 Lab File: VX016878.D
 Acq: 19 Jun 2020 14:44

Tgt Ion: 114 Resp: 383935
 Ion Ratio Lower Upper
 114 100
 63 20.4 0.0 37.0
 88 17.0 0.0 32.0


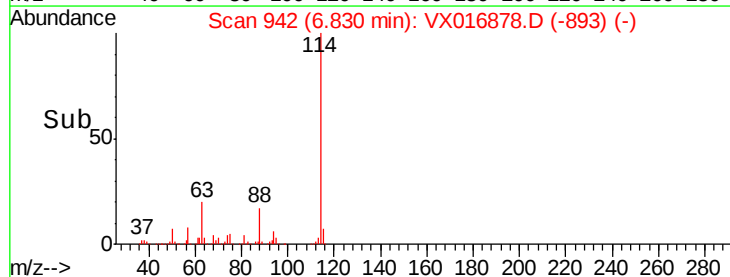
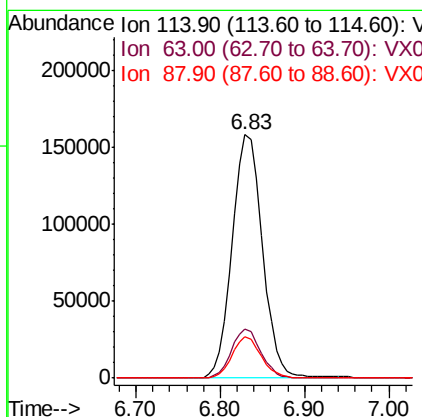
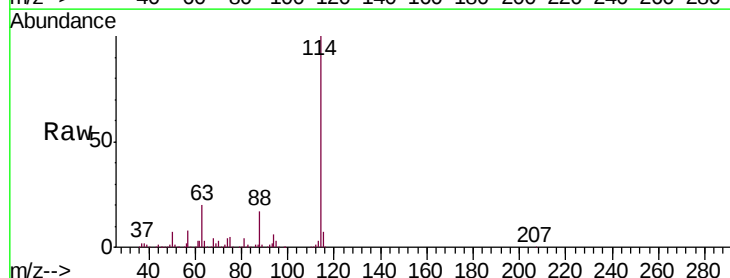


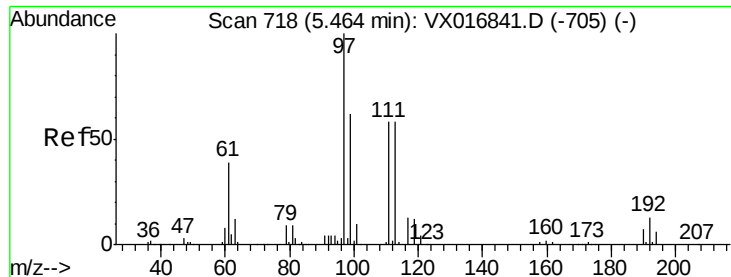

#35
 Dibromofluoromethane
 Concen: 45.188 ug/l
 RT: 5.47 min Scan# 719
 Delta R.T. 0.01 min
 Lab File: VX016878.D
 Acq: 19 Jun 2020 14:44




Instrument :
 MSVOA_X
 ClientSampleId :
 OUTFALL001-200616RE


Tgt Ion:113 Resp: 110983
 Ion Ratio Lower Upper
 113 100
 111 102.5 81.0 121.4
 192 23.5 18.5 27.7

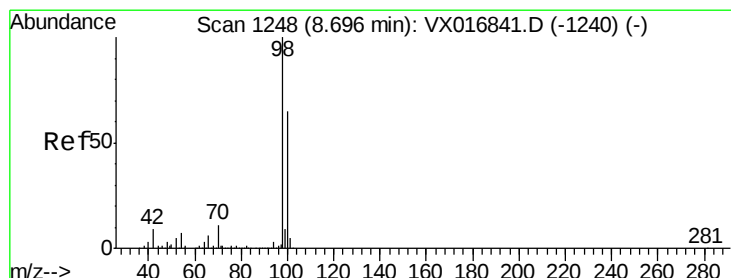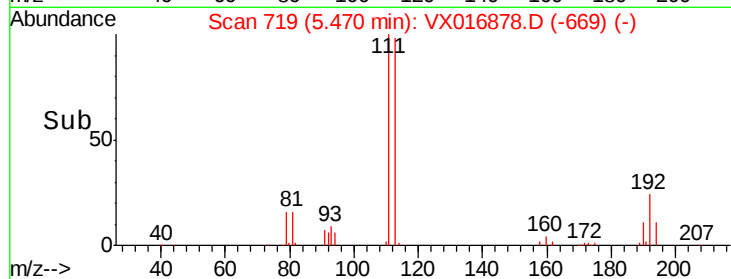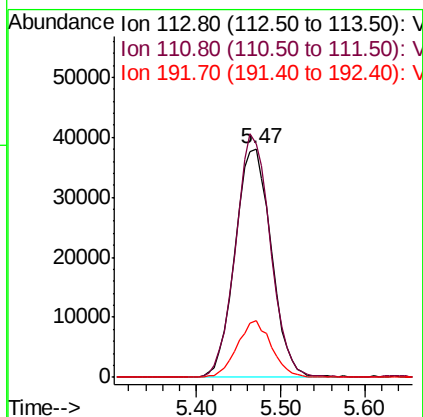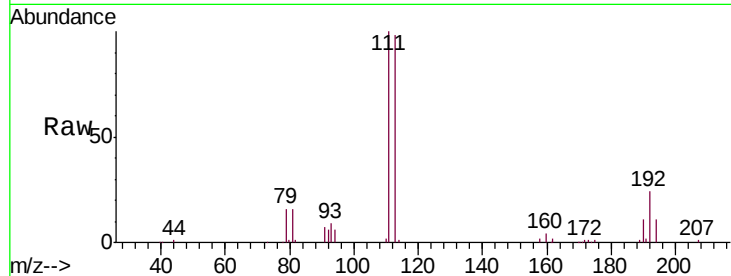

#50
 Toluene-d8
 Concen: 44.249 ug/l
 RT: 8.70 min Scan# 1248
 Delta R.T. -0.00 min
 Lab File: VX016878.D
 Acq: 19 Jun 2020 14:44

Tgt Ion: 98 Resp: 434803
 Ion Ratio Lower Upper
 98 100
 100 66.6 54.0 81.0

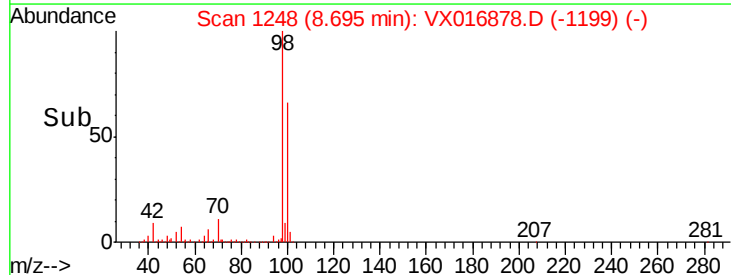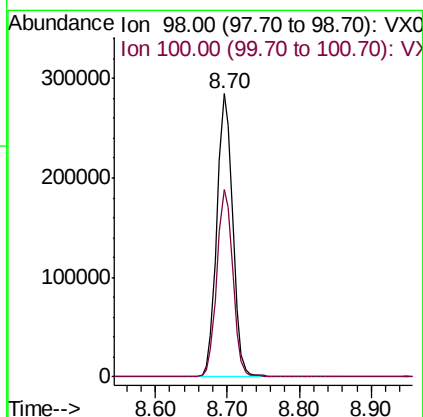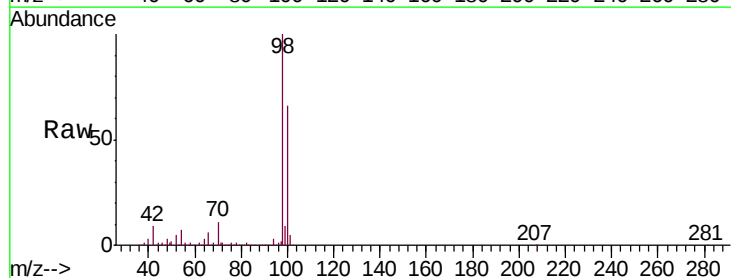

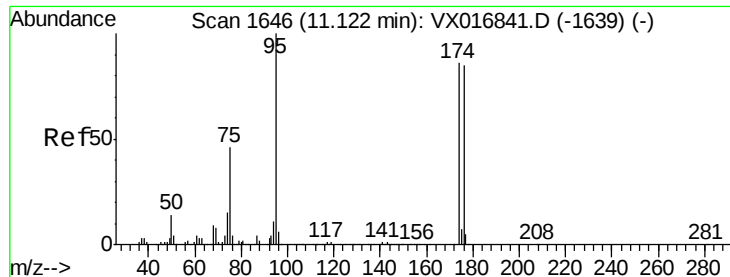

#62

4-Bromofluorobenzene

Concen: 55.660 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX016878.D

Acq: 19 Jun 2020 14:44

Instrument :

MSVOA_X

ClientSampleId :

OUTFALL001-200616RE


Tgt Ion: 95 Resp: 209550

Ion Ratio Lower Upper

95 100

174 86.5 0.0 174.2




176 80.8 0.0 170.0

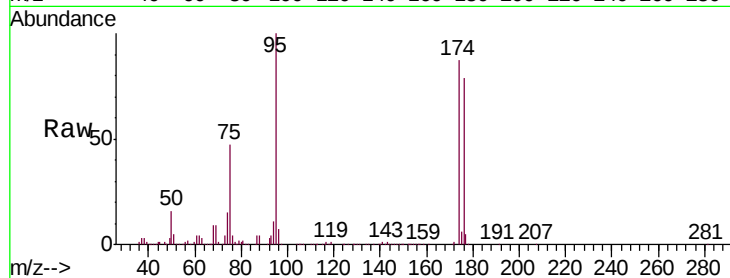

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

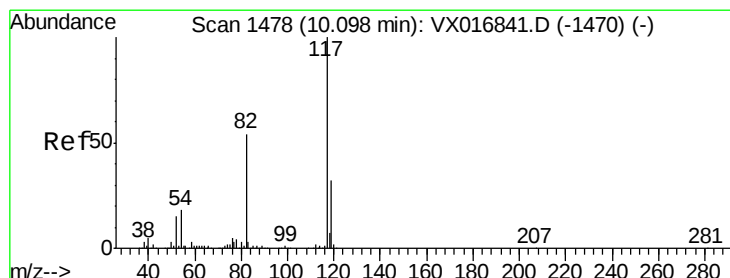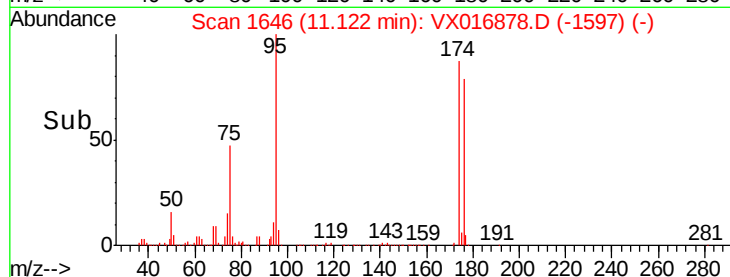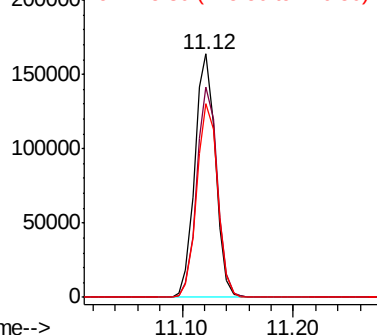

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.10 min Scan# 1478

Delta R.T. -0.00 min

Lab File: VX016878.D

Acq: 19 Jun 2020 14:44


Tgt Ion: 117 Resp: 361396

Ion Ratio Lower Upper

117 100

82 54.3 43.4 65.0



119 32.9 25.7 38.5

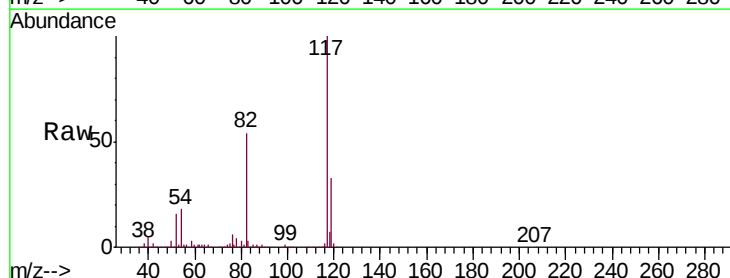


Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): V

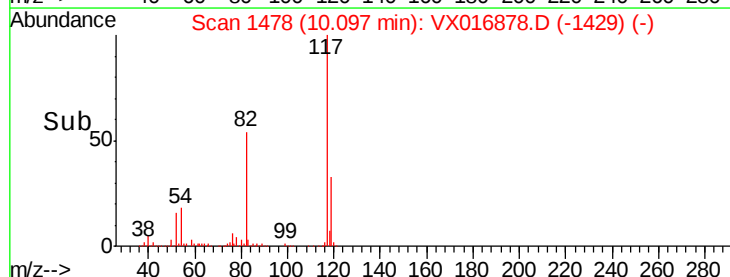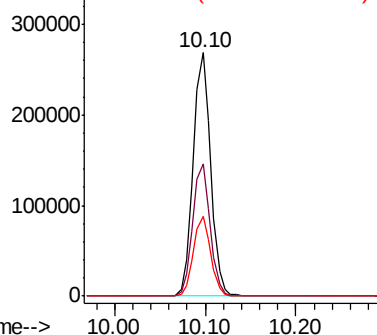

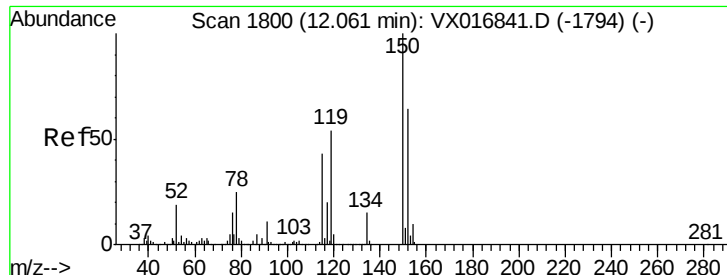

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX016878.D

Acq: 19 Jun 2020 14:44

Instrument :

MSVOA_X

ClientSampleId :

OUTFALL001-200616RE


Tgt Ion:152 Resp: 191215

Ion Ratio Lower Upper

152 100

115 59.3 40.9 122.8

150 156.3 0.0 344.2

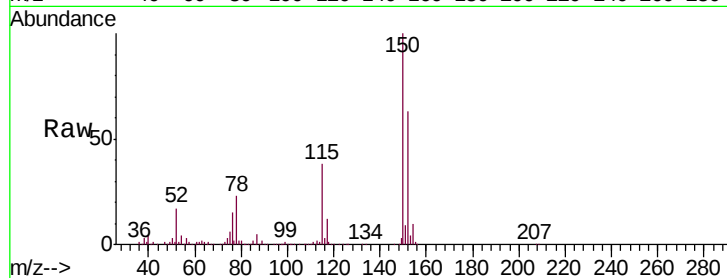

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

