

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX061920\
 Data File : VX016890.D
 Acq On : 19 Jun 2020 19:16
 Operator : JC/SP
 Sample : L3020-24
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-03_061720

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061820W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.465	703	718	729	rBV	134730	389561	29.70%	4.981%
2	5.629	734	745	760	rVB	243972	673773	51.37%	8.615%
3	6.032	801	811	824	rBV	142492	377739	28.80%	4.830%
4	6.830	932	942	954	rBV	414492	952372	72.61%	12.177%
5	8.696	1237	1248	1266	rBV	875924	1311557	100.00%	16.769%
6	10.098	1472	1478	1492	rVV	817802	1126979	85.93%	14.409%
7	10.232	1496	1500	1507	rVB	36911	50214	3.83%	0.642%
8	10.348	1513	1519	1526	rVB	16603	24477	1.87%	0.313%
9	11.122	1640	1646	1657	rBV	943335	1174639	89.56%	15.018%
10	11.342	1677	1682	1688	rVB	18856	25199	1.92%	0.322%
11	11.439	1693	1698	1703	rVV2	17122	24559	1.87%	0.314%
12	11.488	1703	1706	1714	rVB	16514	21965	1.67%	0.281%
13	11.793	1751	1756	1762	rVB	60813	75928	5.79%	0.971%
14	12.061	1795	1800	1807	rBV	1057429	1284321	97.92%	16.421%
15	12.128	1807	1811	1817	rVB	22693	28238	2.15%	0.361%
16	12.280	1831	1836	1844	rVV	23673	32142	2.45%	0.411%
17	12.360	1844	1849	1856	rVB4	11984	22683	1.73%	0.290%
18	12.652	1893	1897	1900	rBV	13359	16803	1.28%	0.215%
19	13.207	1981	1988	1992	rBV2	11654	15723	1.20%	0.201%
20	13.329	2004	2008	2014	rVB2	17097	23505	1.79%	0.301%
21	13.817	2083	2088	2093	rBV	58188	73791	5.63%	0.943%
22	14.676	2225	2229	2238	rVB	49345	62277	4.75%	0.796%
23	14.823	2248	2253	2262	rVB	24299	32873	2.51%	0.420%


Sum of corrected areas: 7821318

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX061920\
Data File : VX016890.D
Acq On : 19 Jun 2020 19:16
Operator : JC/SP
Sample : L3020-24
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-03_061720

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

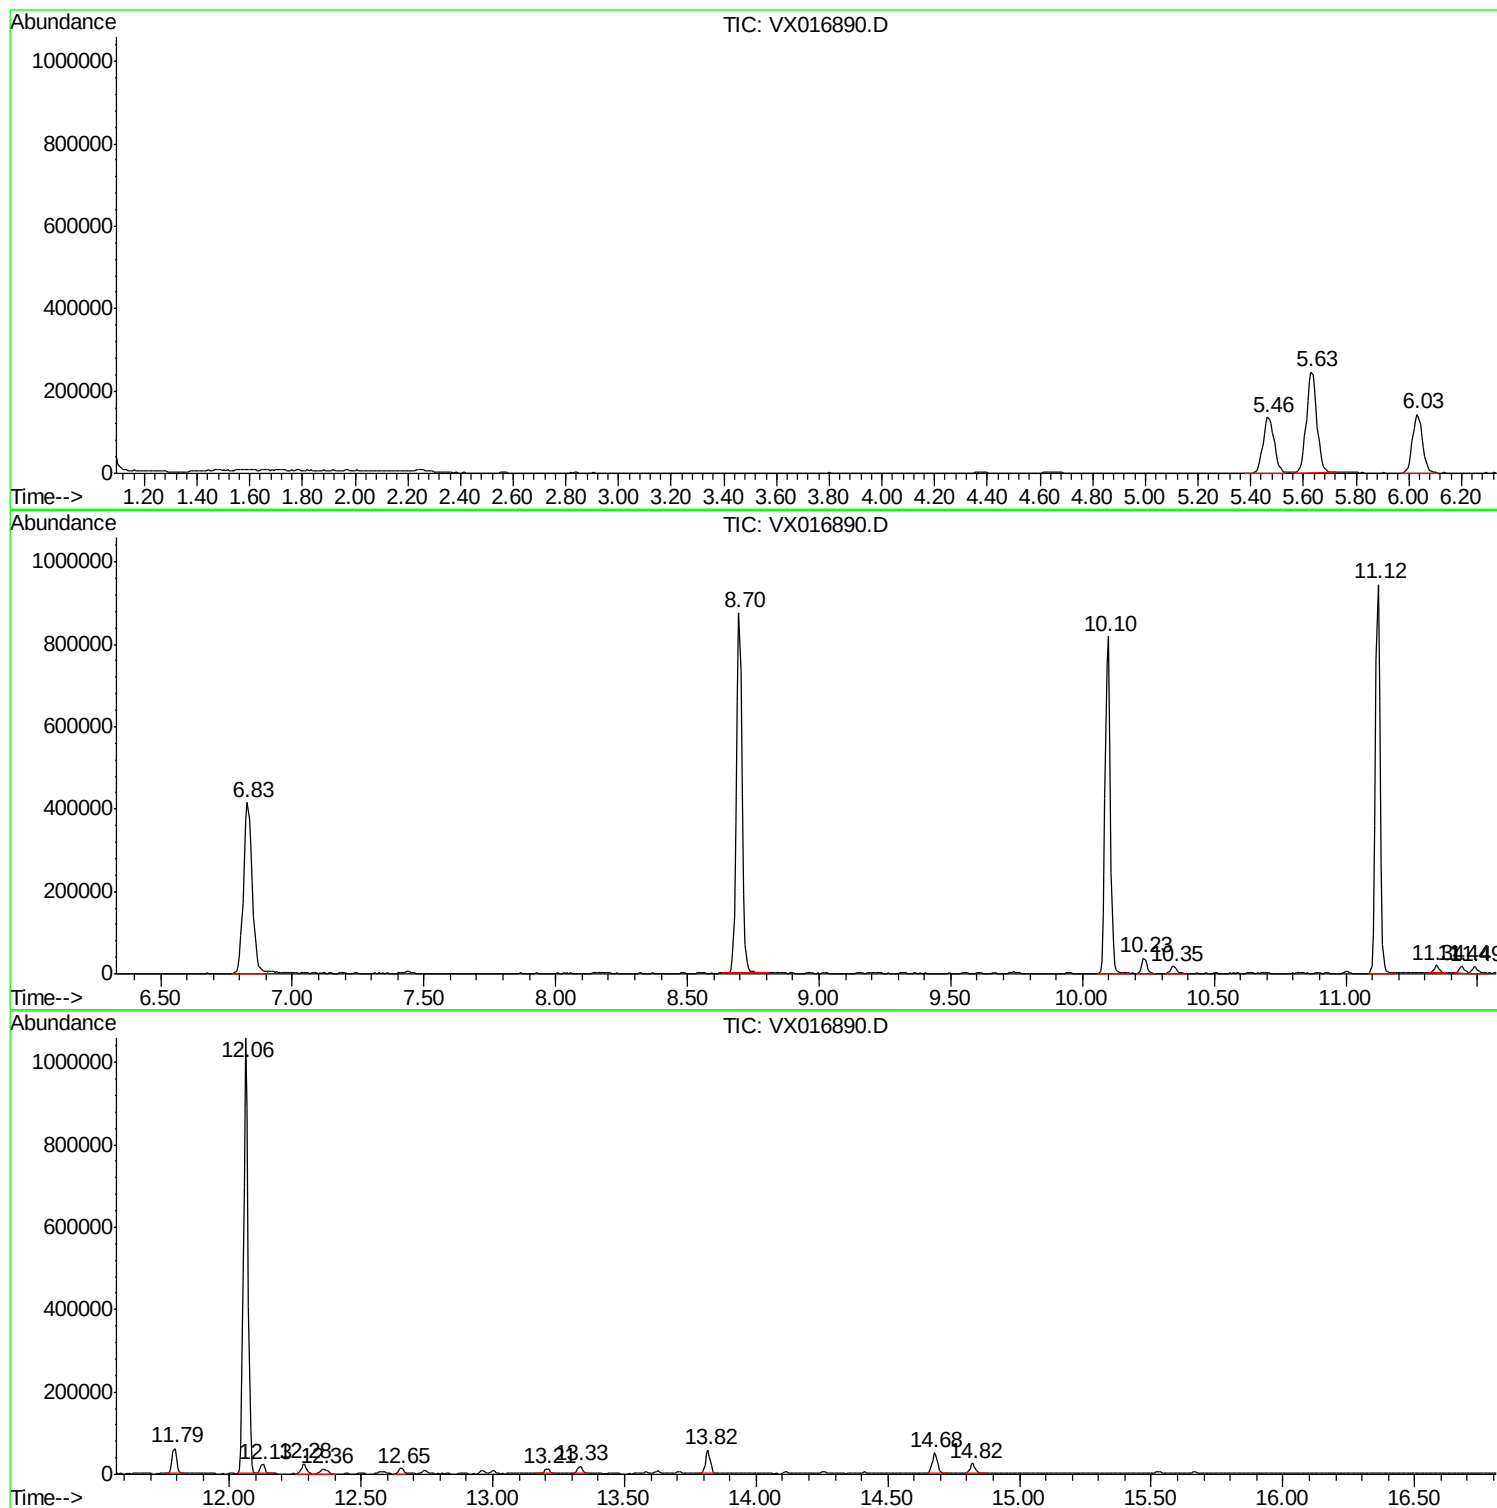

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX061920\
Data File : VX016890.D
Acq On : 19 Jun 2020 19:16
Operator : JC/SP
Sample : L3020-24
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-03_061720

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX061920\
Data File : VX016890.D
Acq On : 19 Jun 2020 19:16
Operator : JC/SP
Sample : L3020-24
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-03_061720

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc