


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX061920\
 Data File : VX016871.D
 Acq On : 19 Jun 2020 11:40
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061820W.M
 Title : SW846 8260
 Last Update : Fri Jun 19 12:07:48 2020

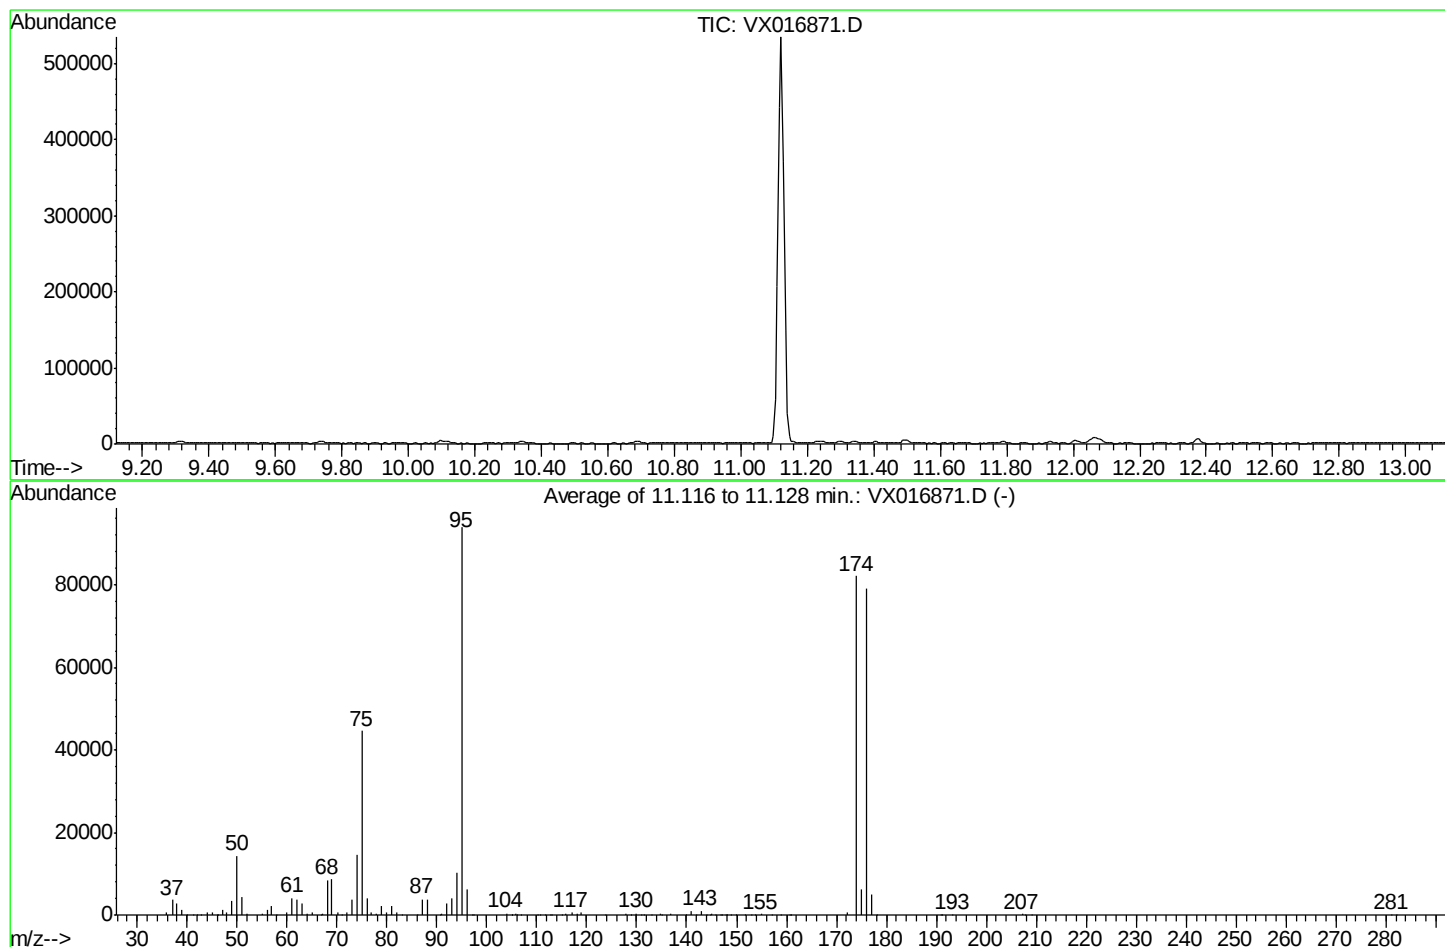

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	14330	PASS
75	95	30	60	47.4	44520	PASS
95	95	100	100	100.0	93925	PASS
96	95	5	9	6.5	6120	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.4	82112	PASS
175	174	5	9	7.6	6215	PASS
176	174	95	101	96.2	78965	PASS
177	176	5	9	6.2	4883	PASS