


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX061920\
Data File : VX016898.D
Acq On : 19 Jun 2020 22:40
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061820W.M
Title : SW846 8260
Last Update : Fri Jun 19 12:07:48 2020

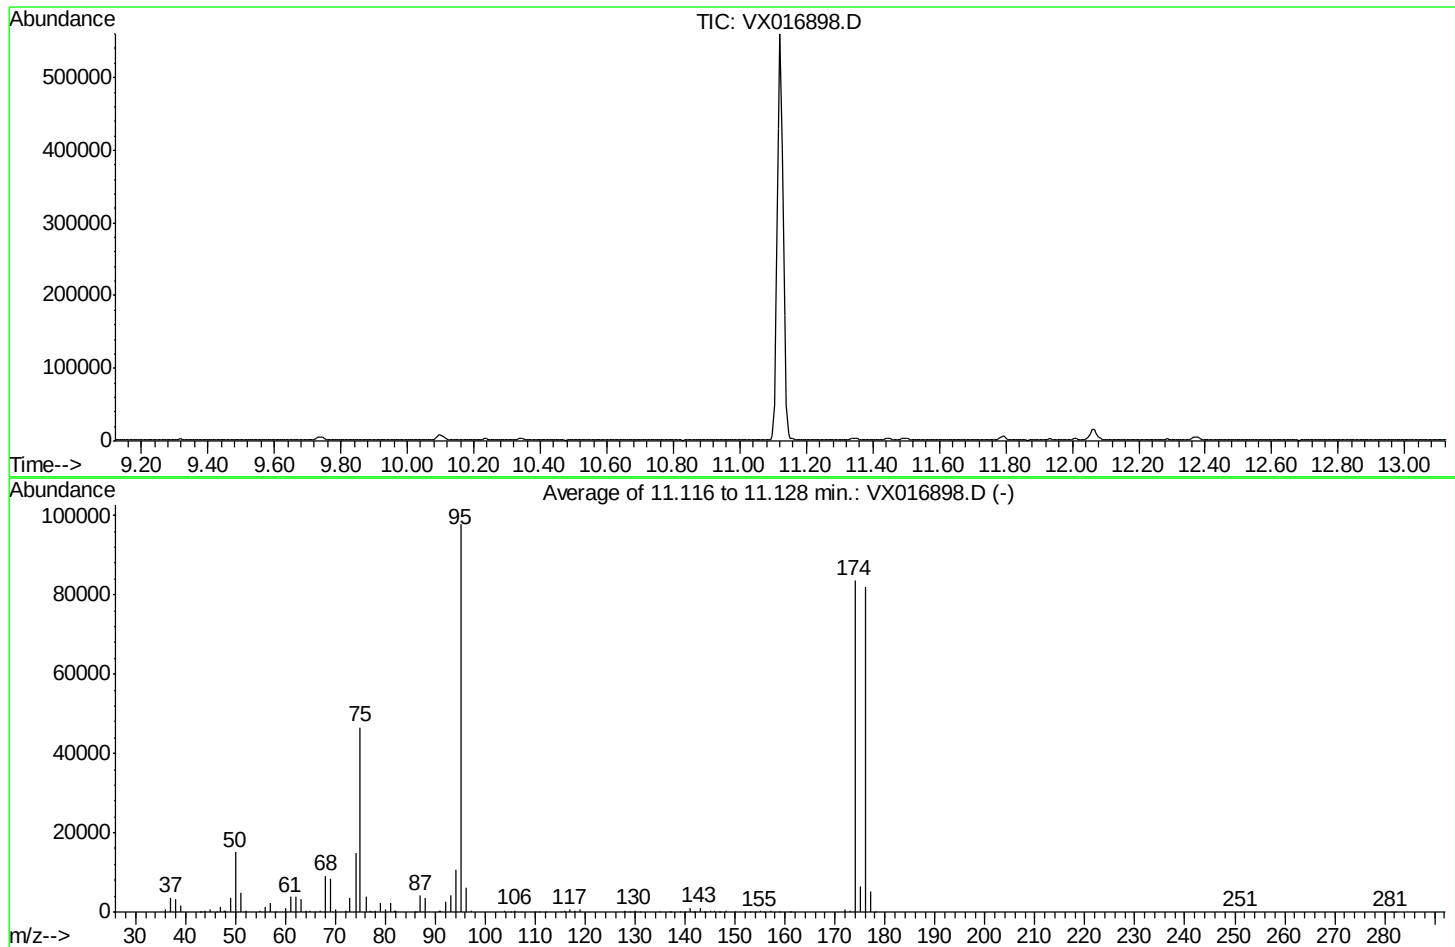

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	15031	PASS
75	95	30	60	47.7	46642	PASS
95	95	100	100	100.0	97778	PASS
96	95	5	9	6.1	5984	PASS
173	174	0.00	2	0.3	289	PASS
174	95	50	100	85.4	83485	PASS
175	174	5	9	7.7	6440	PASS
176	174	95	101	98.3	82058	PASS
177	176	5	9	6.2	5104	PASS