

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061923\
 Data File : VX036200.D
 Acq On : 19 Jun 2023 12:48
 Operator : JC/MD
 Sample : VX0619MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0619MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
 Title : SW846 8260

Signal : TIC: VX036200.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	17	rVB2	8037	7917	1.47%	0.268%
2	2.794	273	280	283	rBV2	2905	5385	1.00%	0.182%
3	4.562	562	570	584	rBV	4892	17218	3.20%	0.582%
4	5.385	691	705	720	rBV	51829	155833	29.00%	5.268%
5	5.550	721	732	747	rVB	123409	344370	64.08%	11.641%
6	5.952	786	798	811	rBV2	71103	190145	35.38%	6.427%
7	6.757	921	930	946	rBV	194485	460874	85.75%	15.579%
8	8.647	1233	1240	1249	rBV	297129	457571	85.14%	15.467%
9	10.055	1465	1471	1486	rBV	386734	537438	100.00%	18.167%
10	11.079	1634	1639	1651	rVB	230783	294927	54.88%	9.969%
11	12.018	1788	1793	1807	rBV	382631	486661	90.55%	16.450%




Sum of corrected areas: 2958339

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061923\
Data File : VX036200.D
Acq On : 19 Jun 2023 12:48
Operator : JC/MD
Sample : VX0619MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0619MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

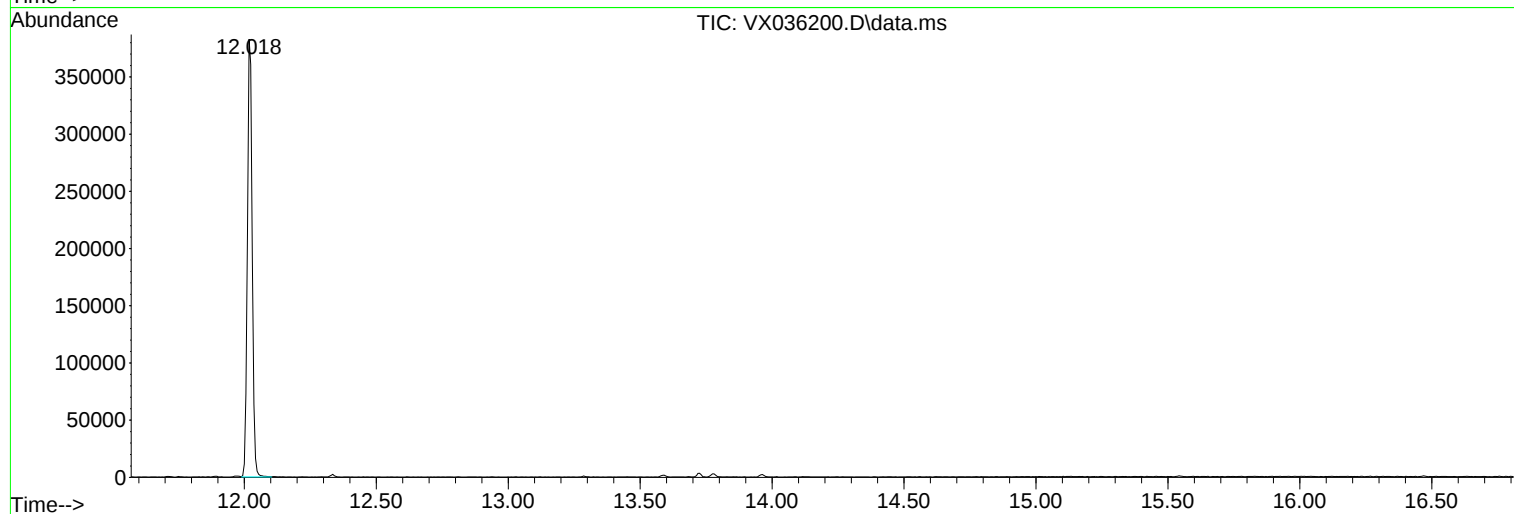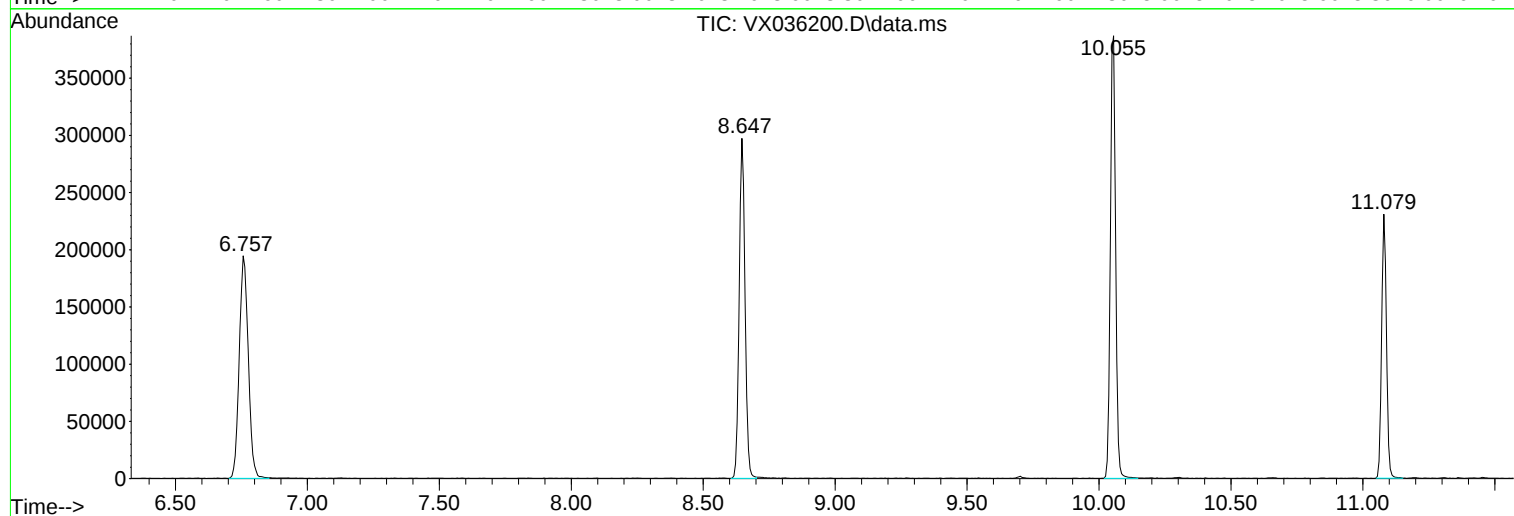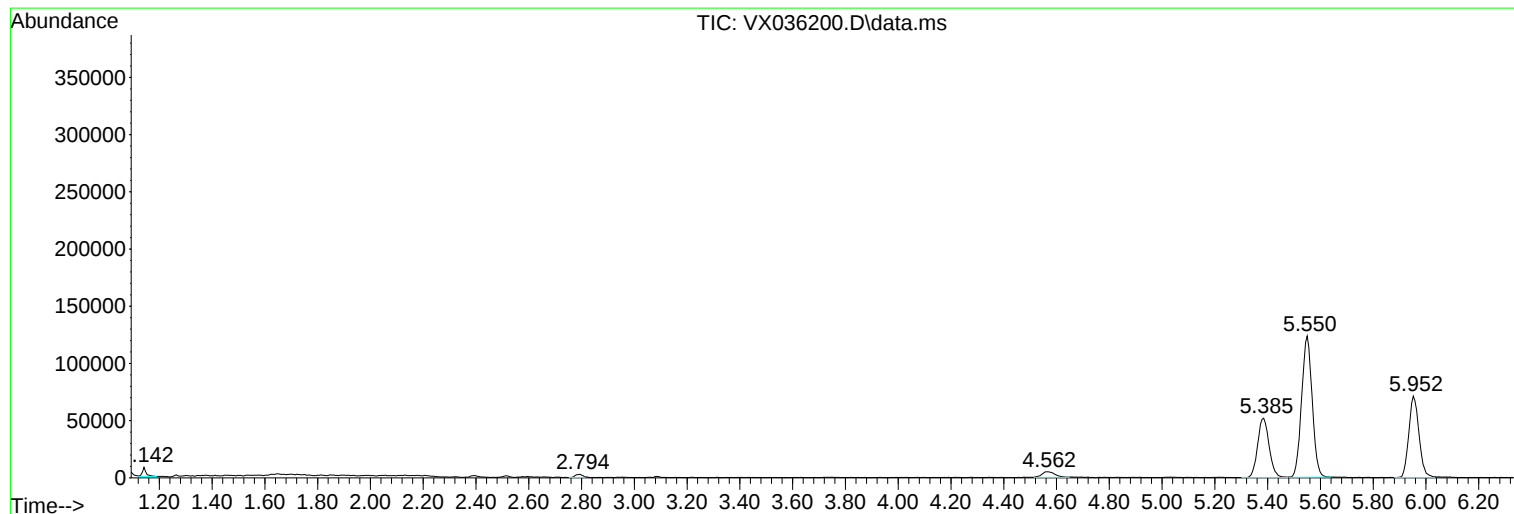

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061923\
Data File : VX036200.D
Acq On : 19 Jun 2023 12:48
Operator : JC/MD
Sample : VX0619MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0619MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061923\
Data File : VX036200.D
Acq On : 19 Jun 2023 12:48
Operator : JC/MD
Sample : VX0619MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0619MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc