

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061925\
 Data File : VX046771.D
 Acq On : 19 Jun 2025 15:45
 Operator : JC/MD
 Sample : Q2351-01 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FAIRLAWN-SUMP

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M

Title : SW846 8260

Signal : TIC: VX046771.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.306	521	528	538	rBV3	3120	9161	1.38%	0.251%
2	5.391	695	706	722	rBV4	69384	225251	33.85%	6.171%
3	5.556	722	733	752	rVB	116926	366683	55.11%	10.046%
4	5.958	789	799	821	rBV	79514	227062	34.12%	6.221%
5	6.763	922	931	949	rBV	186189	488242	73.38%	13.376%
6	7.372	1022	1031	1040	rBV4	4565	11626	1.75%	0.319%
7	8.646	1234	1240	1257	rVB	412641	665385	100.00%	18.229%
8	10.049	1465	1470	1487	rBV	417406	573935	86.26%	15.724%
9	11.079	1634	1639	1652	rBV	334787	432330	64.97%	11.844%
10	12.018	1788	1793	1806	rBV	446861	550714	82.77%	15.088%
11	14.310	2165	2169	2173	rBV6	4081	7210	1.08%	0.198%
12	14.792	2244	2248	2251	rVB5	4561	6862	1.03%	0.188%
13	14.956	2268	2275	2282	rBV5	10382	27731	4.17%	0.760%
14	15.212	2314	2317	2320	rBV5	7050	9963	1.50%	0.273%
15	15.414	2346	2350	2355	rVB4	14800	21369	3.21%	0.585%
16	15.737	2400	2403	2409	rVB4	17810	26569	3.99%	0.728%




Sum of corrected areas: 3650093

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061925\
Data File : VX046771.D
Acq On : 19 Jun 2025 15:45
Operator : JC/MD
Sample : Q2351-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FAIRLAWN-SUMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

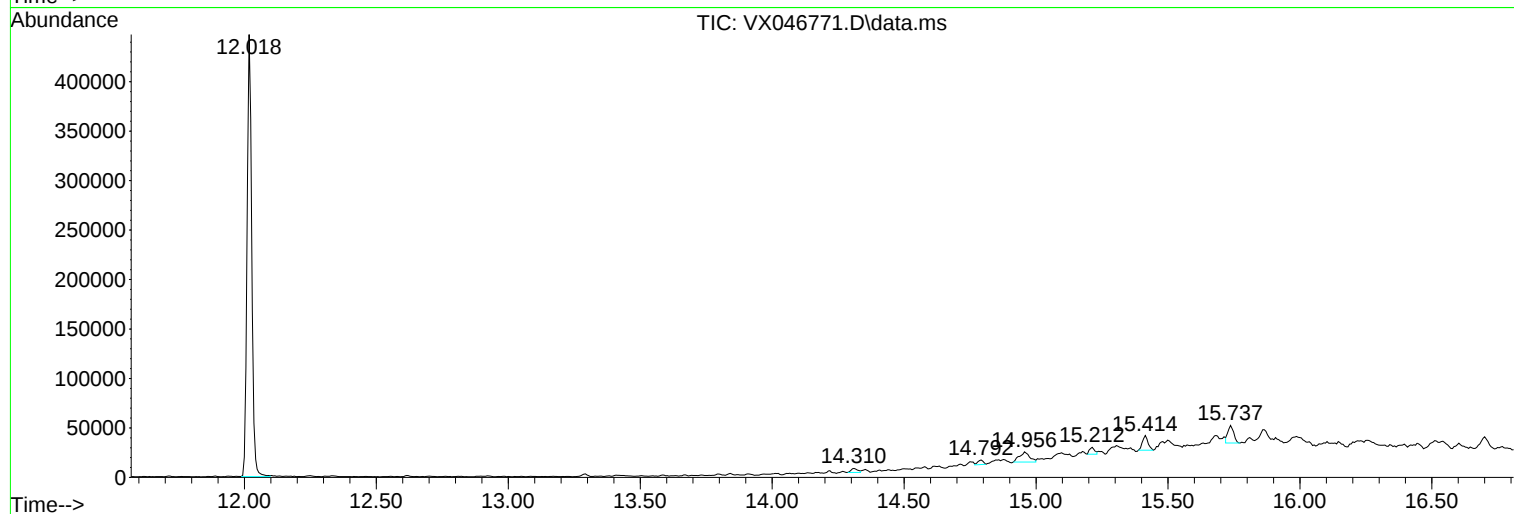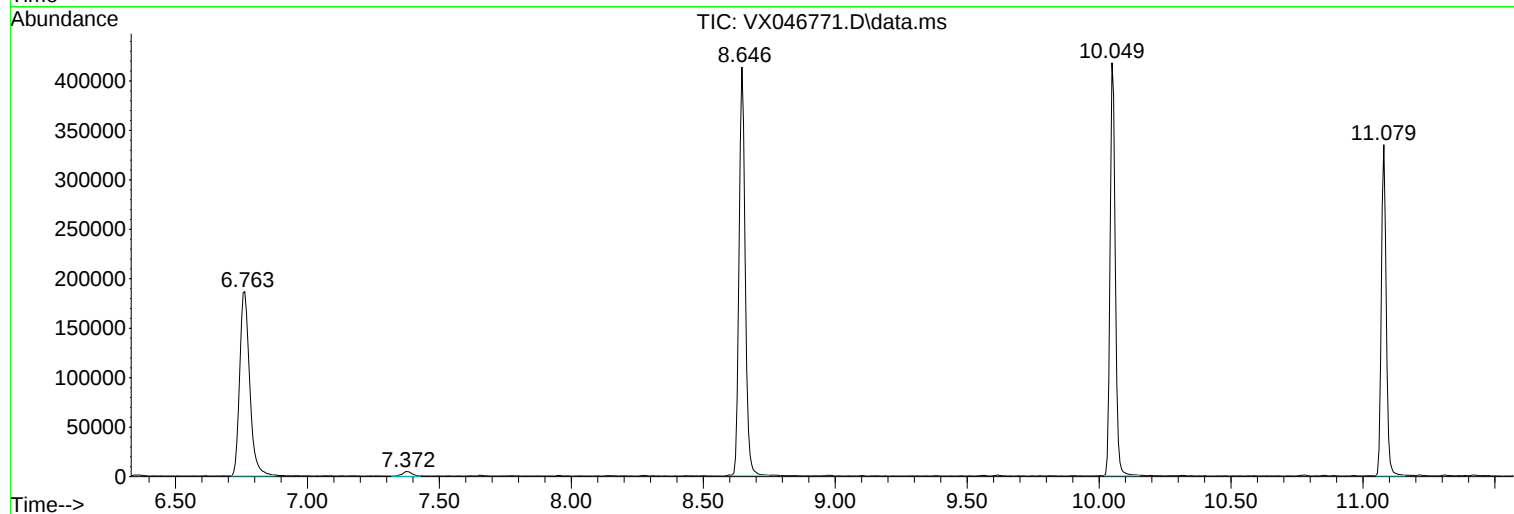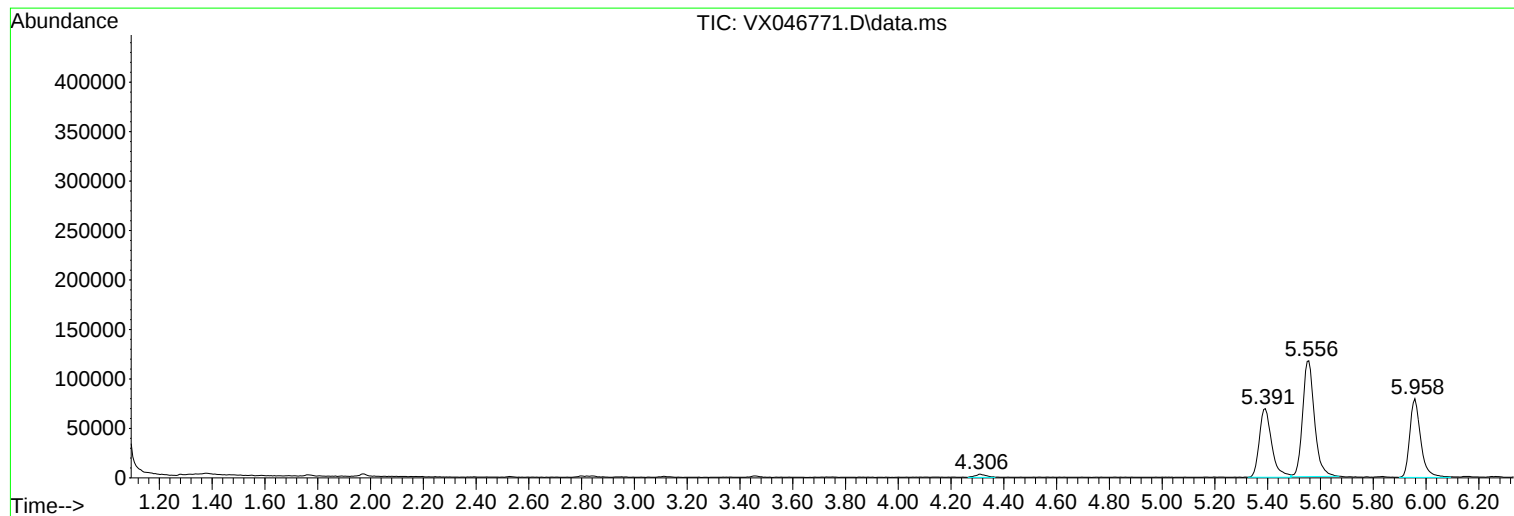

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061925\
Data File : VX046771.D
Acq On : 19 Jun 2025 15:45
Operator : JC/MD
Sample : Q2351-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FAIRLAWN-SUMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061925\
Data File : VX046771.D
Acq On : 19 Jun 2025 15:45
Operator : JC/MD
Sample : Q2351-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FAIRLAWN-SUMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc