

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062019\  
Data File : VX010371.D  
Acq On : 20 Jun 2019 20:41  
Operator : JC/SP  
Sample : K3469-14 40X  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
DUP-061919-01

## Integration Parameters: RTEINT.P

Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X061919W.M  
Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.276       | 16            | 20          | 31           | rBV      | 42668          | 60140         | 4.27%           | 0.803%        |
| 2         | 5.501       | 702           | 713         | 727          | rBV2     | 170094         | 488159        | 34.68%          | 6.515%        |
| 3         | 5.665       | 727           | 740         | 752          | rVV      | 293111         | 828335        | 58.85%          | 11.055%       |
| 4         | 6.061       | 795           | 805         | 820          | rBV      | 161979         | 426075        | 30.27%          | 5.686%        |
| 5         | 6.860       | 926           | 936         | 951          | rBV      | 431920         | 1021034       | 72.54%          | 13.627%       |
| 6         | 8.713       | 1232          | 1240        | 1249         | rBV      | 905735         | 1407475       | 100.00%         | 18.784%       |
| 7         | 10.109      | 1462          | 1469        | 1479         | rBV      | 858473         | 1197454       | 85.08%          | 15.981%       |
| 8         | 11.134      | 1631          | 1637        | 1652         | rBV      | 723439         | 945340        | 67.17%          | 12.616%       |
| 9         | 12.079      | 1785          | 1792        | 1800         | rBV      | 891945         | 1118911       | 79.50%          | 14.933%       |


Sum of corrected areas: 7492923

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062019\  
Data File : VX010371.D  
Acq On : 20 Jun 2019 20:41  
Operator : JC/SP  
Sample : K3469-14 40X  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
DUP-061919-01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X061919W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

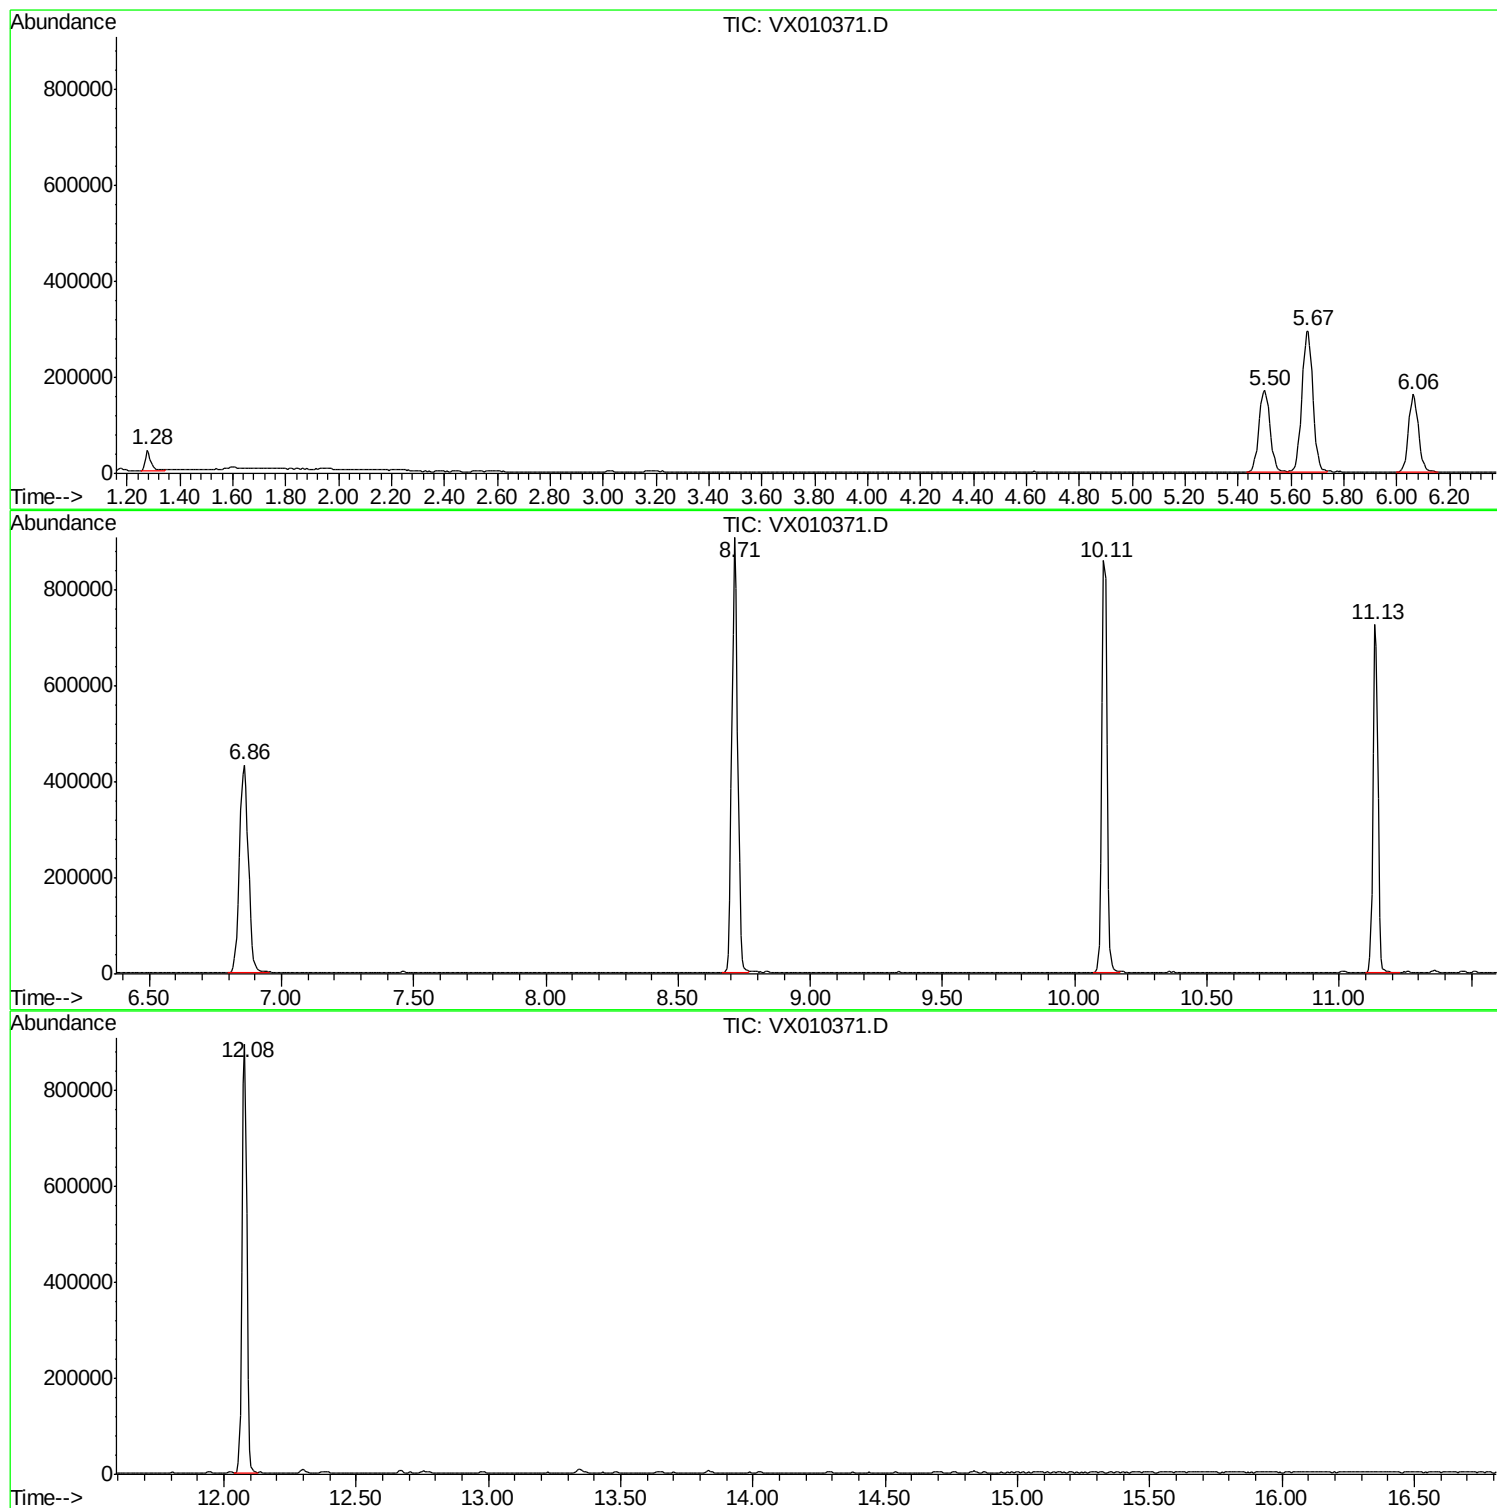

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX062019\  
Data File : VX010371.D  
Acq On : 20 Jun 2019 20:41  
Operator : JC/SP  
Sample : K3469-14 40X  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
DUP-061919-01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X061919W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX062019\  
Data File : VX010371.D  
Acq On : 20 Jun 2019 20:41  
Operator : JC/SP  
Sample : K3469-14 40X  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
DUP-061919-01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X061919W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |