


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX062019\
 Data File : VX010350.D
 Acq On : 20 Jun 2019 09:31
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
 Title : SW846 8260
 Last Update : Thu Jun 20 03:31:56 2019

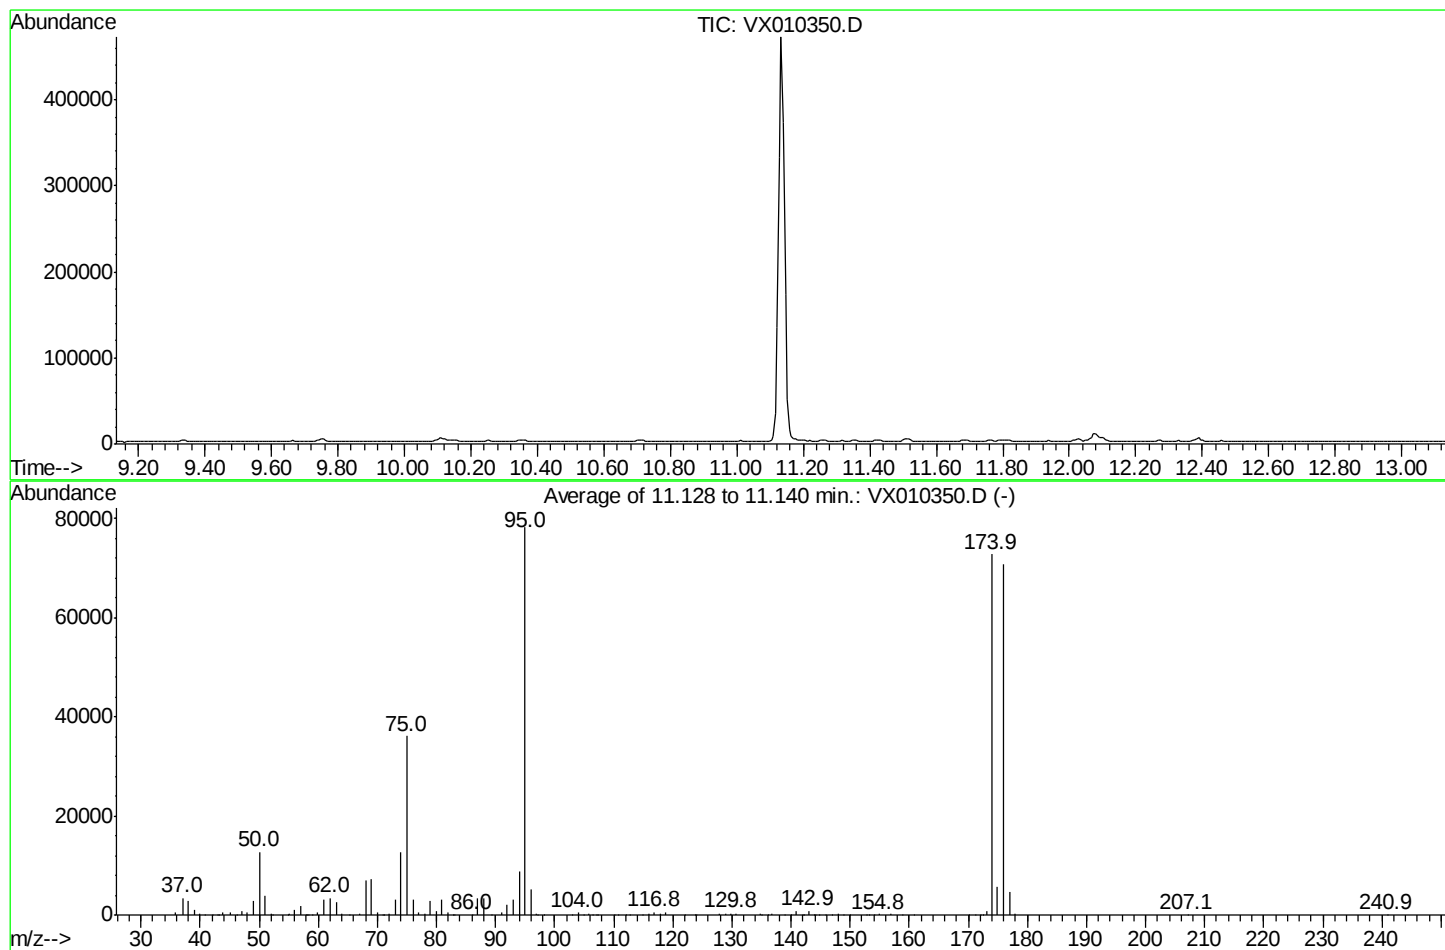

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	12742	PASS
75	95	30	60	46.2	36157	PASS
95	95	100	100	100.0	78237	PASS
96	95	5	9	6.6	5192	PASS
173	174	0.00	2	1.1	824	PASS
174	95	50	100	93.0	72789	PASS
175	174	5	9	7.7	5608	PASS
176	174	95	101	97.4	70896	PASS
177	176	5	9	6.5	4636	PASS